
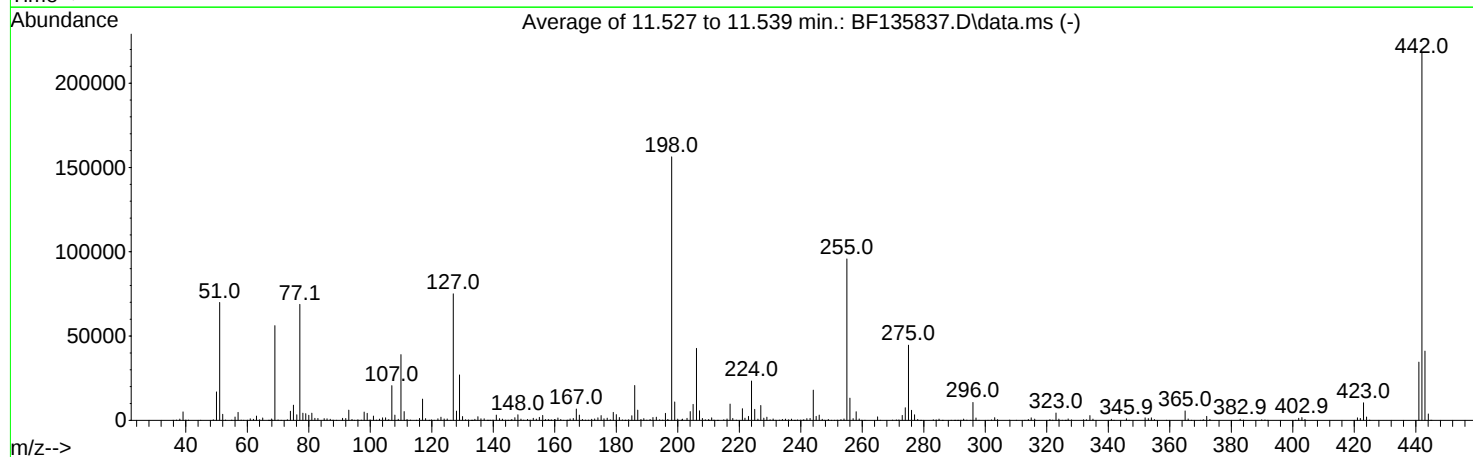


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135837.D
Acq On : 18 Oct 2023 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 17 01:22:00 2023

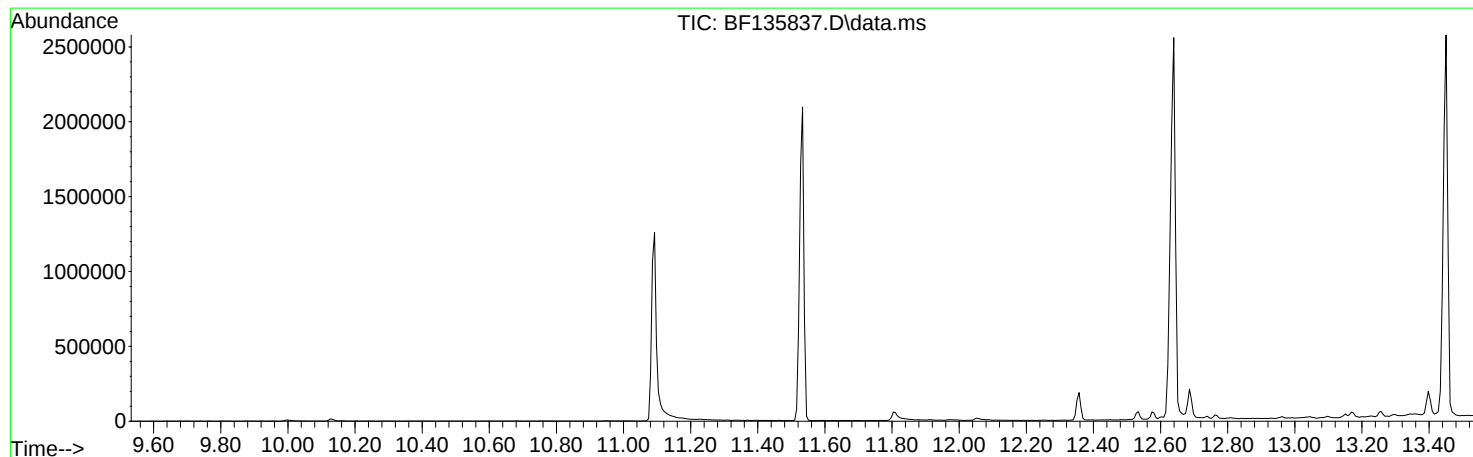




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	69913	PASS
68	69	0.00	2	1.6	878	PASS
69	198	0.00	100	35.9	56177	PASS
70	69	0.00	2	0.5	296	PASS
127	198	10	80	48.0	75083	PASS
197	198	0.00	2	0.3	493	PASS
198	198	100	100	100.0	156296	PASS
199	198	5	9	7.0	10960	PASS
275	198	10	60	28.5	44568	PASS
365	198	1	100	3.6	5620	PASS
441	198	0.01	100	22.1	34576	PASS
442	442	50	100	100.0	218197	PASS
443	442	15	24	18.8	41099	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
Data File : BF135837.D
Acq On : 18 Oct 2023 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 18 11:45:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

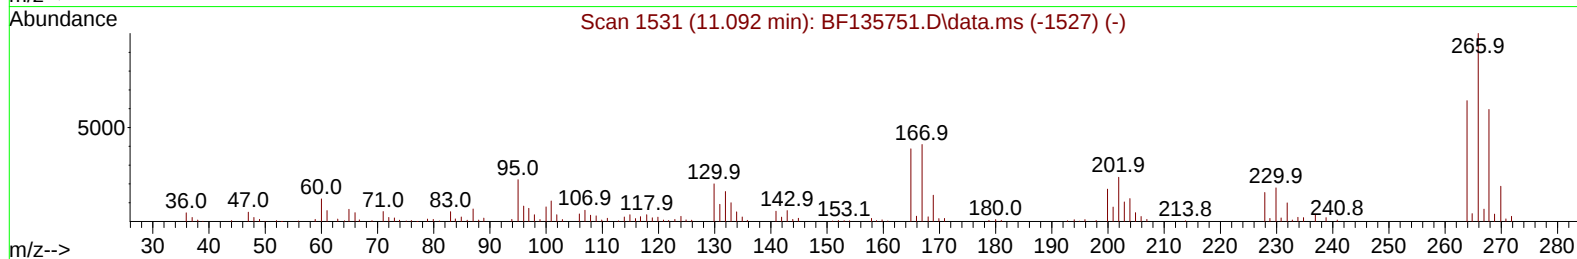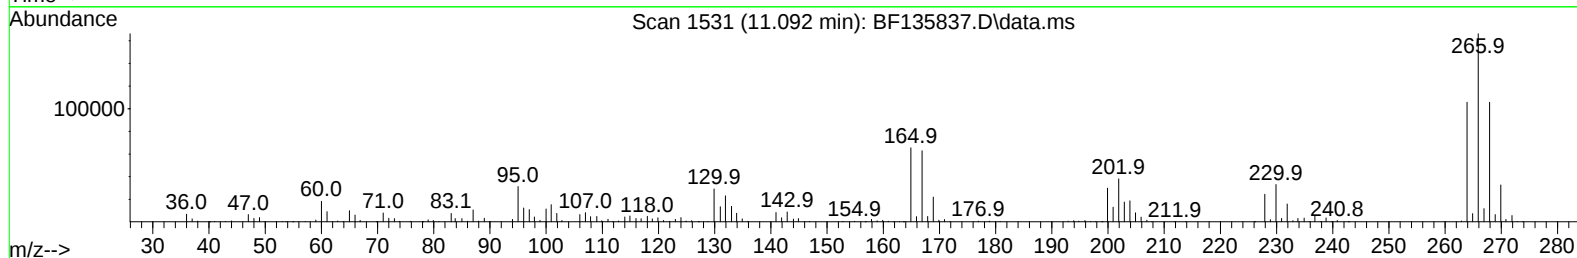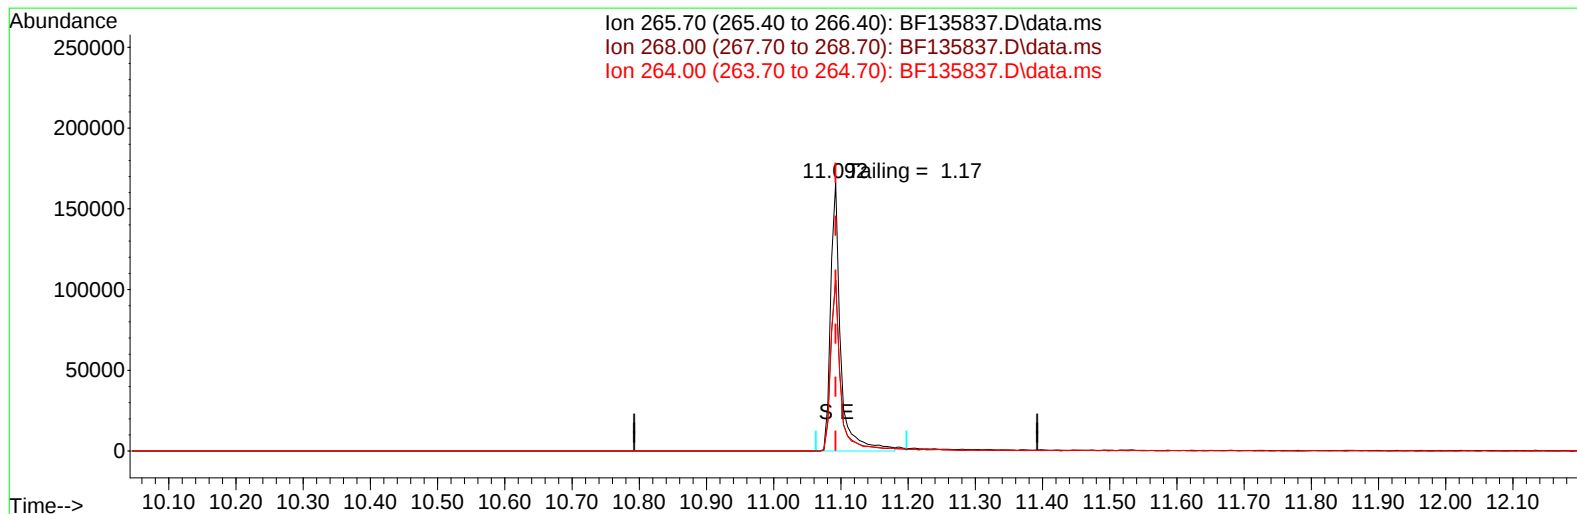

TIC: BF135837.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.000) 376475.00 ng




response 174514

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	63.61
264.00	64.30	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101823\
 Data File : BF135837.D
 Acq On : 18 Oct 2023 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 18 11:45:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 17 01:22:00 2023
 Response via : Initial Calibration

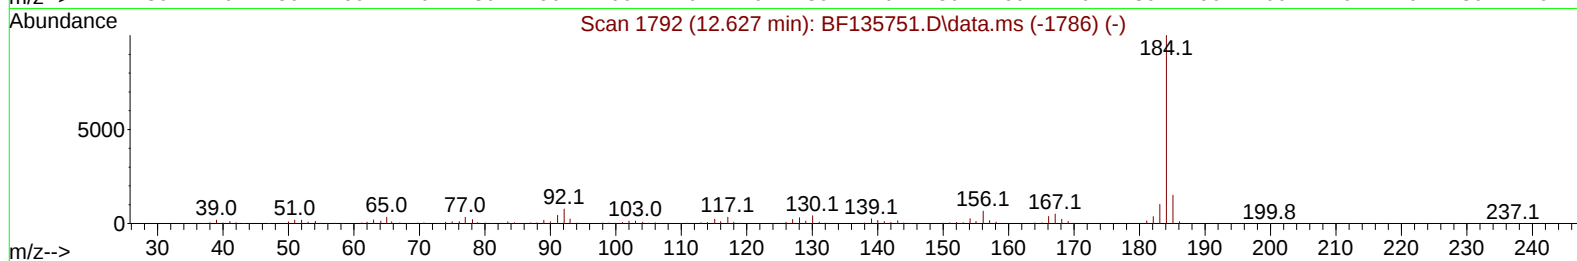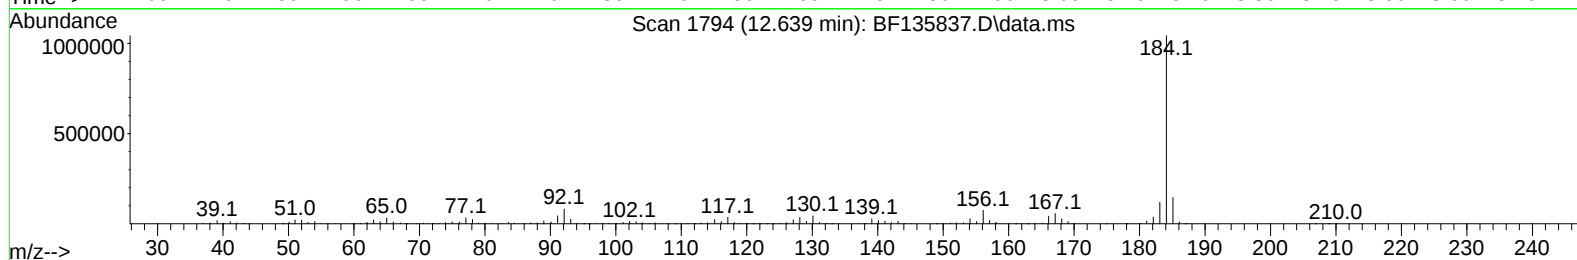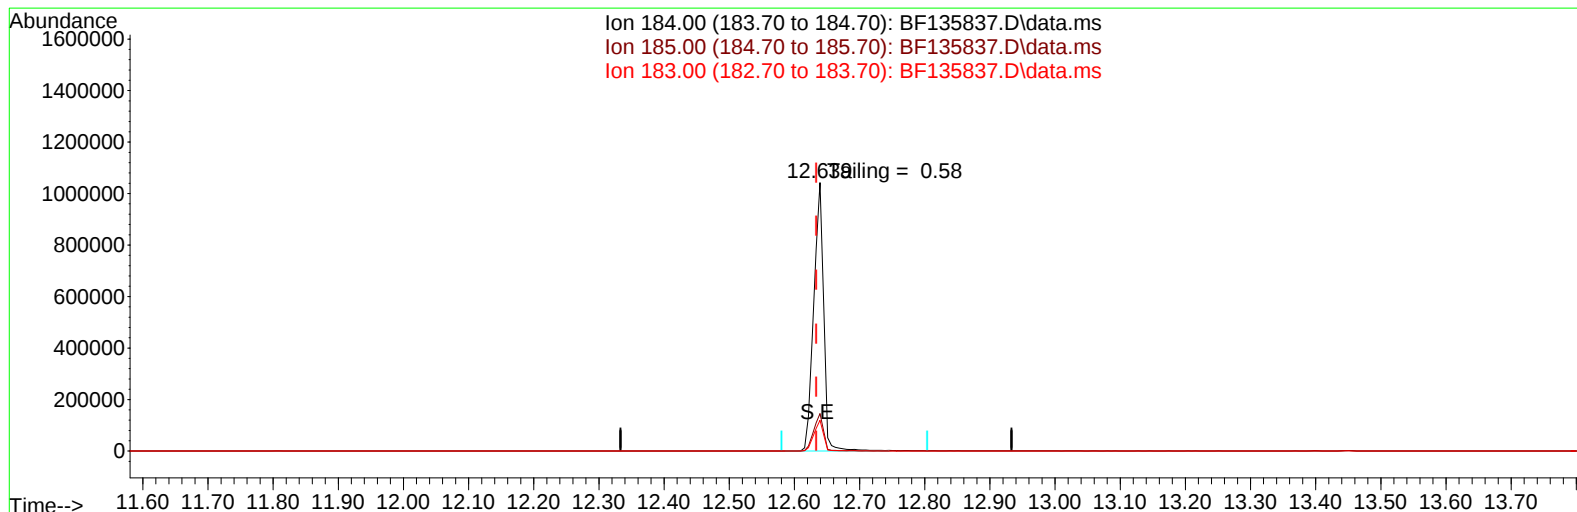

TIC: BF135837.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 117941.08 ng

response 1111788

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.00
183.00	10.20	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/18/2023	BNA_F	<u>BF135837.D</u>
Compound Name	Response	Retention Time
DDT	472142	13.451
DDD	11030	13.169
DDE	1014	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12044	484186	2.49

Instrument :
BNA_F
ClientSampleId :
DFTPP