

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101918\
 Data File : BF110011.D
 Acq On : 19 Oct 2018 19:09
 Operator : JU/SJ
 Sample : J5593-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 20 00:08:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 16 14:58:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	207950	20.00	ng	-0.01
21) Naphthalene-d8	8.25	136	865106	20.00	ng	-0.02
39) Acenaphthene-d10	10.01	164	412034	20.00	ng	-0.02
64) Phenanthrene-d10	11.50	188	763049	20.00	ng	-0.01
76) Chrysene-d12	14.14	240	526806	20.00	ng	-0.02
87) Perylene-d12	15.66	264	382034	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	544383	41.50	ng	-0.01
7) Phenol-d6	6.58	99	428839	26.33	ng	-0.02
23) Nitrobenzene-d5	7.53	82	1275526	99.32	ng	-0.02
42) 2,4,6-Tribromophenol	10.80	330	330516	92.65	ng	-0.01
45) 2-Fluorobiphenyl	9.33	172	2219736	85.96	ng	-0.01
79) Terphenyl-d14	13.09	244	2046614	81.58	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.53	70	171719	16.418	ng	# 78
25) Isophorone	7.53	82	1272924	50.445	ng	# 67
51) 2,6-Dinitrotoluene	10.01	165	51613	9.314	ng	# 22
57) 2,4-Dinitrotoluene	10.01	165	51613	11.252	ng	# 19
65) 4,6-Dinitro-2-methylphenol	10.80	198	623	8.093	ng	# 1
67) 4-Bromophenyl-phenylether	10.80	248	20751	2.509	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101918\
Data File : BF110011.D
Acq On : 19 Oct 2018 19:09
Operator : JU/SJ
Sample : J5593-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 20 00:08:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

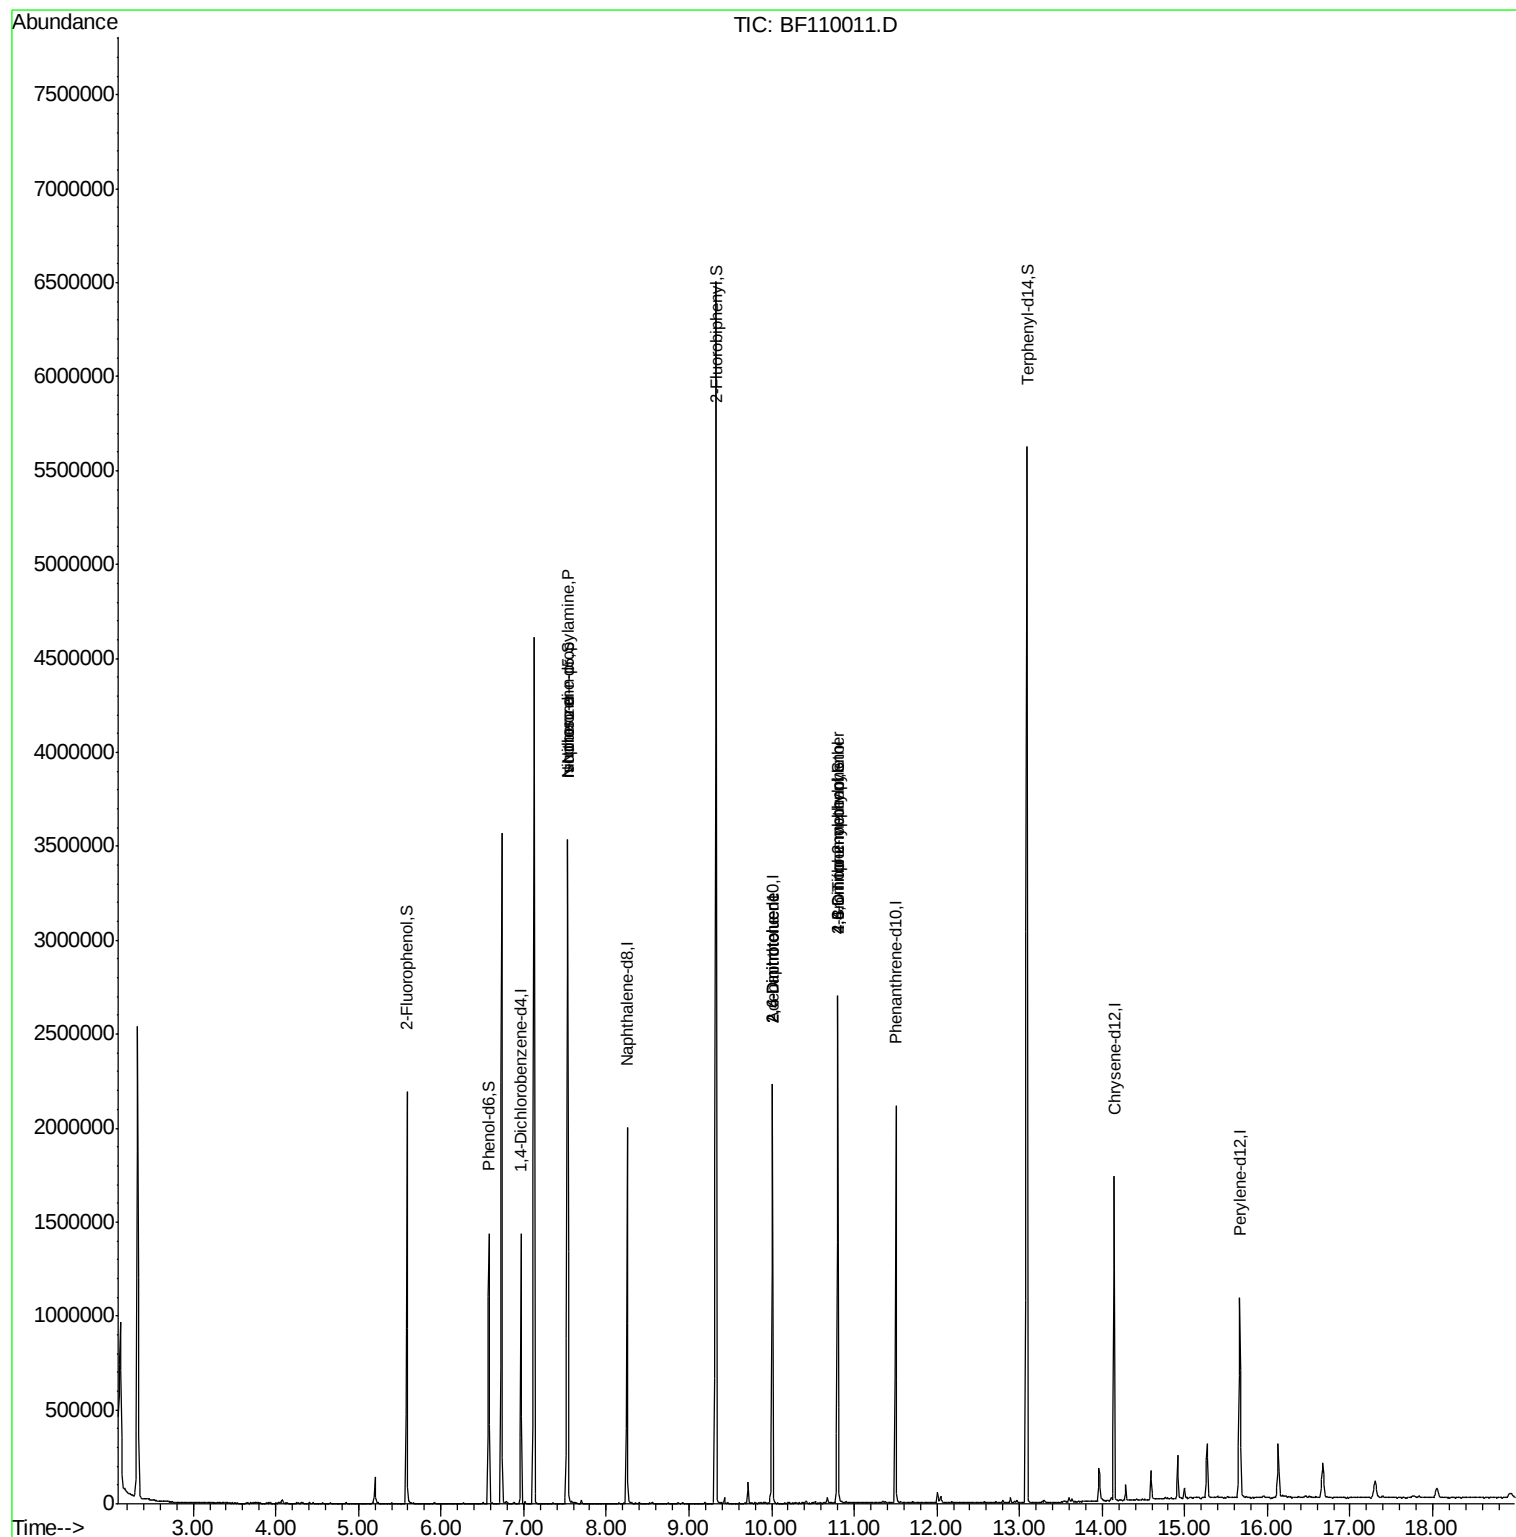

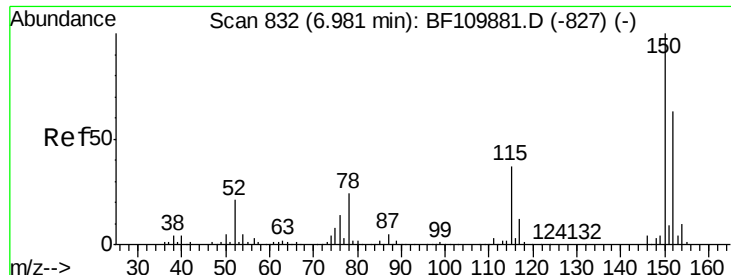


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 830
Delta R.T. -0.01 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Instrument :
BNA_F
ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.5	122.7	184.1
115	60.5	49.1	73.7



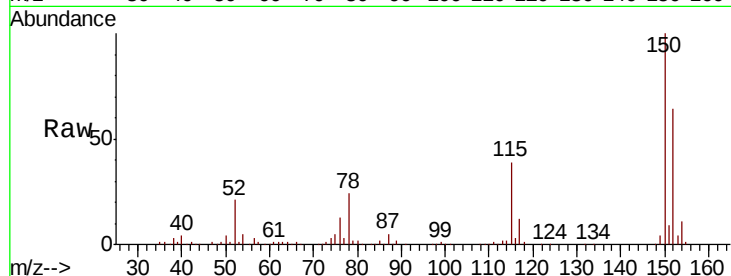


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

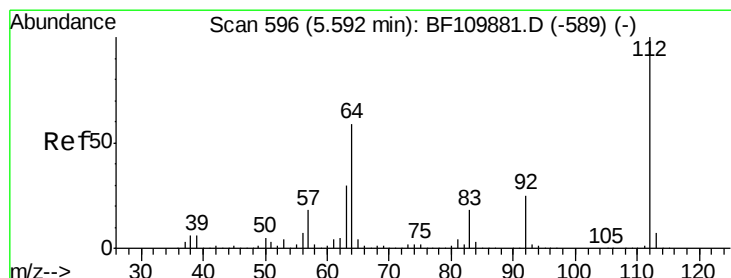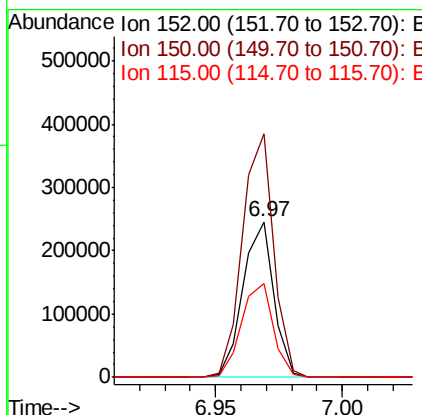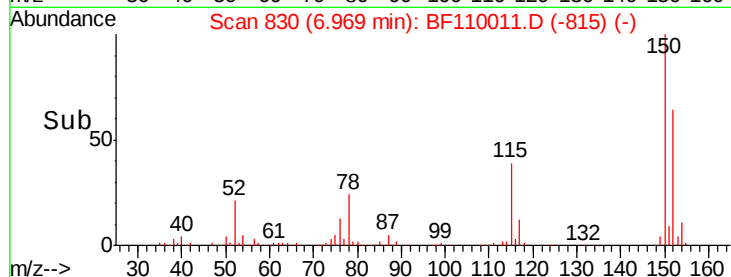

#5

2-Fluorophenol
Concen: 41.497 ng
RT: 5.59 min Scan# 595
Delta R.T. -0.01 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.3	44.1	66.1
63	30.4	23.7	35.5


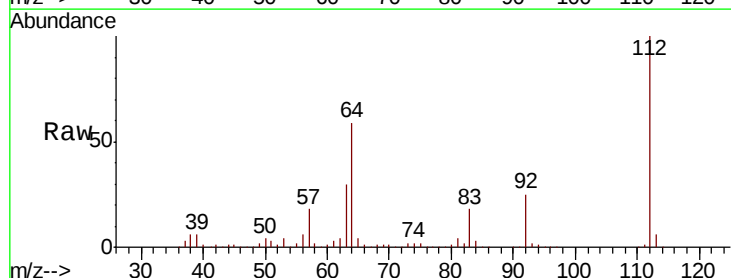



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

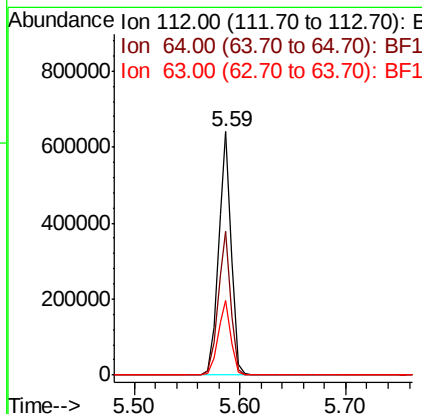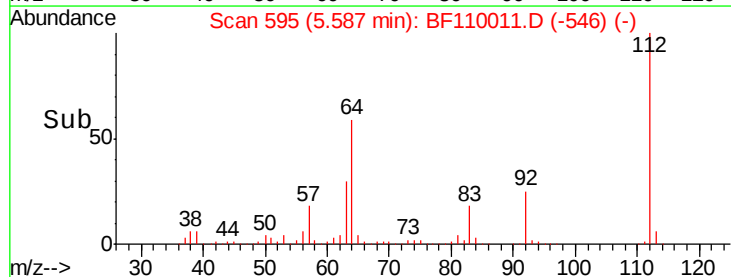

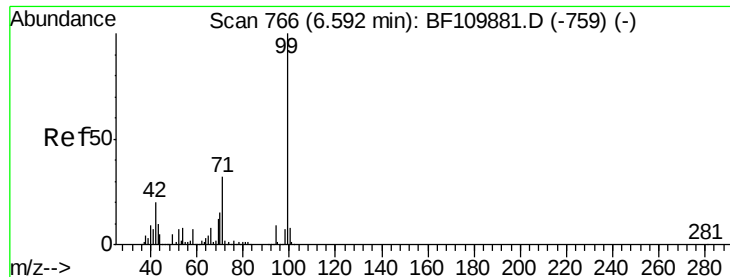

#7

Phenol-d6

Concen: 26.325 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.02 min

Lab File: BF110011.D

Acq: 19 Oct 2018 19:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 428839

Ion Ratio Lower Upper

99 100

42 18.0 15.8 23.6




71 32.1 28.0 42.0

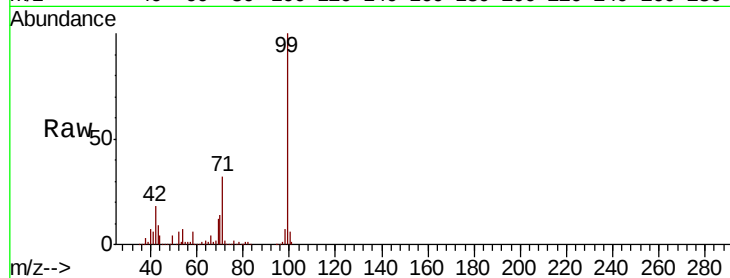

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

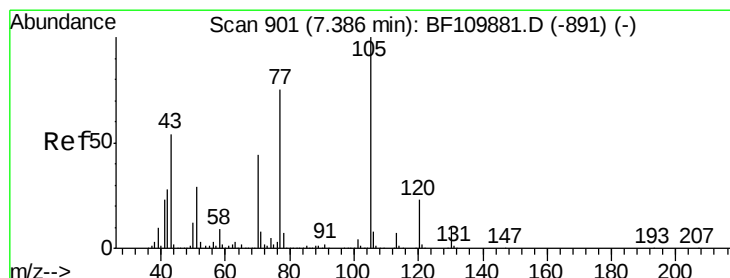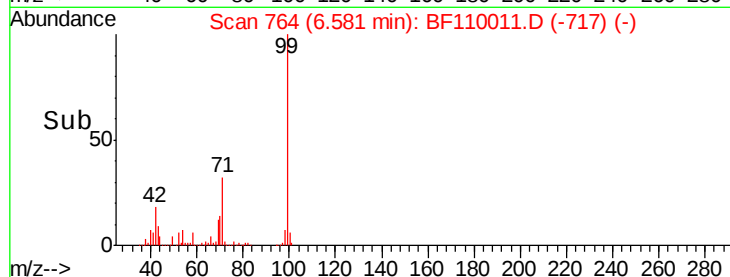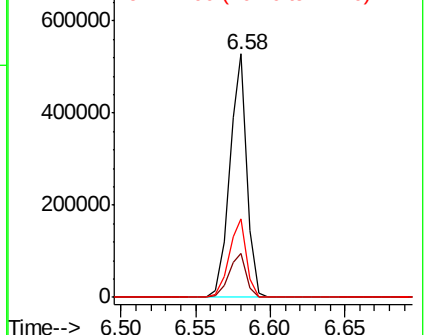

#19

n-Nitroso-di-n-propylamine

Concen: 16.418 ng

RT: 7.53 min Scan# 926

Delta R.T. 0.14 min

Lab File: BF110011.D

Acq: 19 Oct 2018 19:09

Tgt Ion: 70 Resp: 171719


Ion Ratio Lower Upper

70 100

42 47.7 47.4 71.2

101 0.0 7.3 10.9#

130 2.0 16.2 24.2#


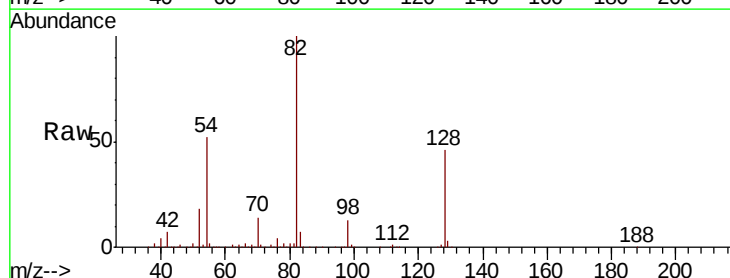



Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

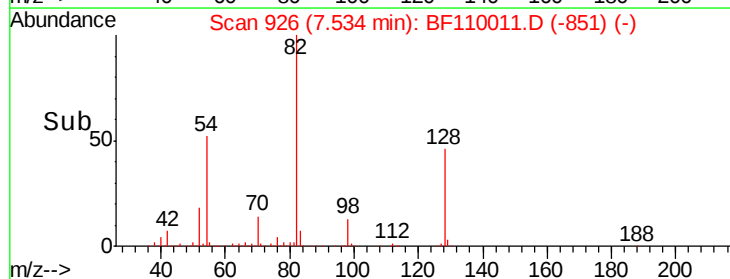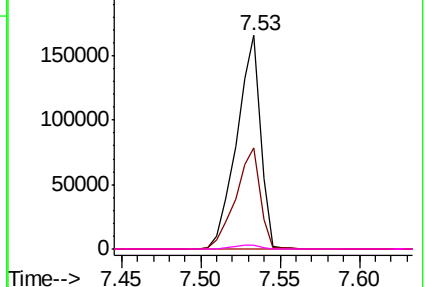

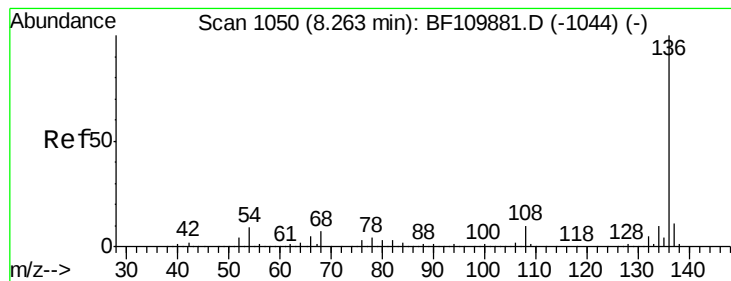

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1048

Delta R.T. -0.02 min

Lab File: BF110011.D

Acq: 19 Oct 2018 19:09

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 865106



Ion Ratio Lower Upper

136 100

137 11.1 8.8 13.2

54 8.2 5.4 8.2

68 5.6 4.2 6.2

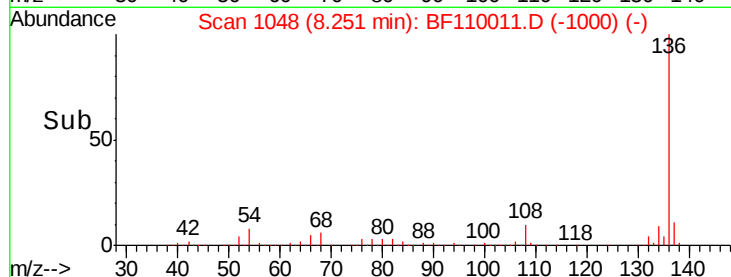
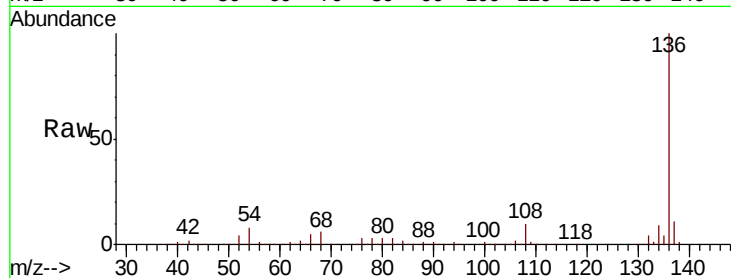


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

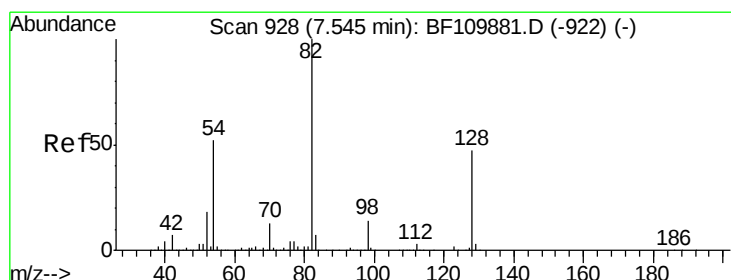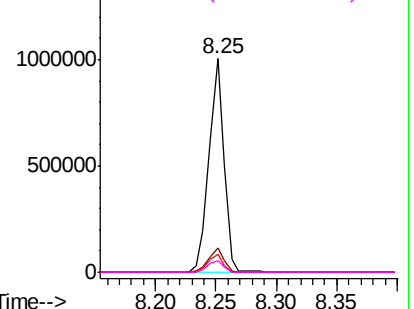

#23

Nitrobenzene-d5

Concen: 99.322 ng

RT: 7.53 min Scan# 926

Delta R.T. -0.02 min

Lab File: BF110011.D

Acq: 19 Oct 2018 19:09



Tgt Ion: 82 Resp: 1275526

Ion Ratio Lower Upper

82 100

128 46.2 34.2 51.2


54 52.2 38.6 58.0

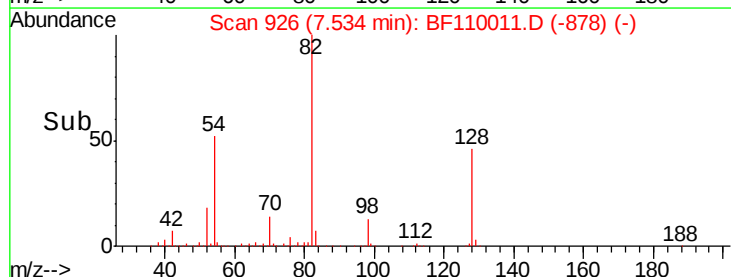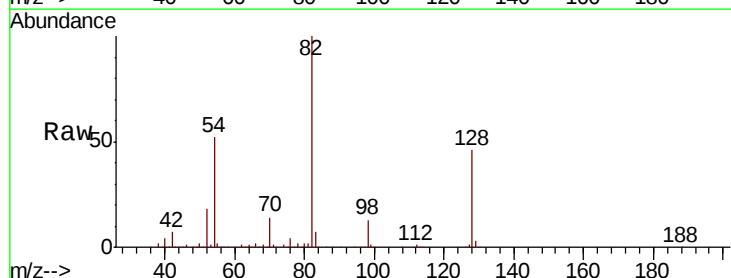


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

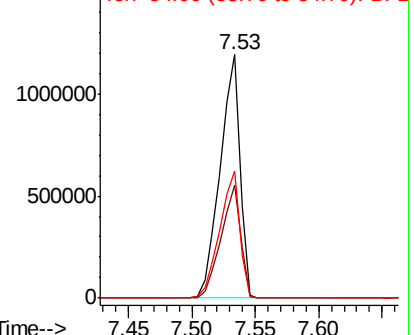


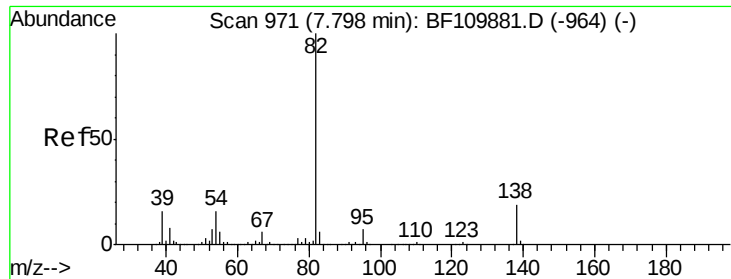




#25
Isophorone
Concen: 50.445 ng
RT: 7.53 min Scan# 926
Delta R.T. -0.27 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 82 Resp: 1272924
Ion Ratio Lower Upper
82 100
95 0.0 5.7 8.5#
138 0.0 13.2 19.8#

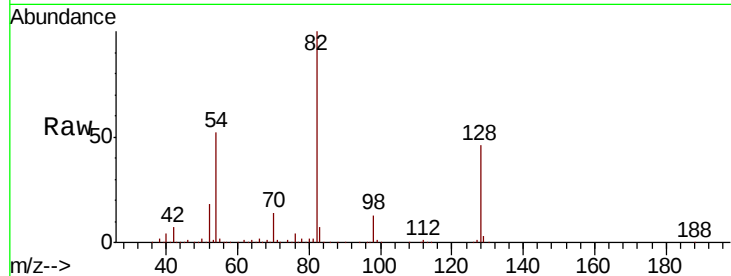


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): E

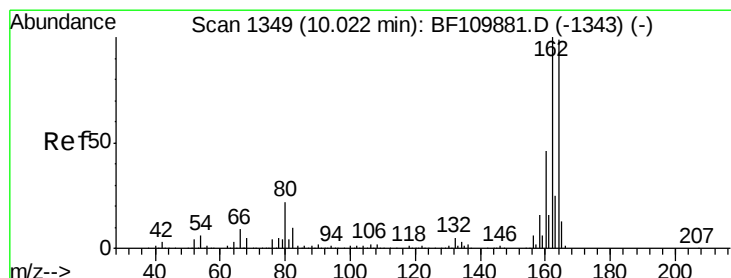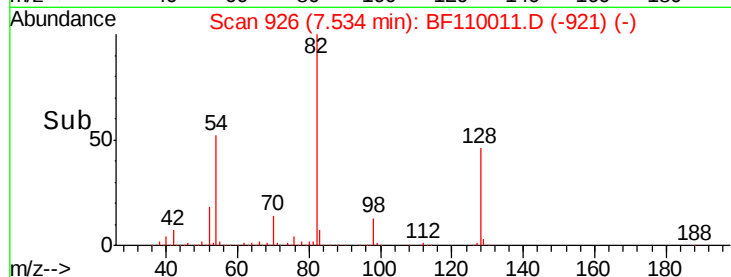
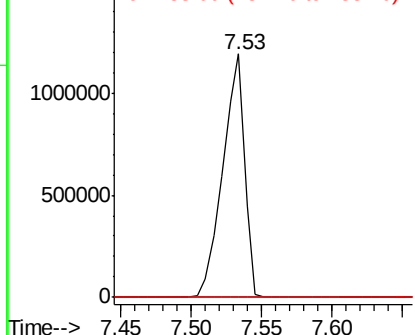



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.01 min Scan# 1347
Delta R.T. -0.02 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Tgt Ion:164 Resp: 412034
Ion Ratio Lower Upper
164 100
162 103.3 83.0 124.6
160 46.3 37.0 55.6

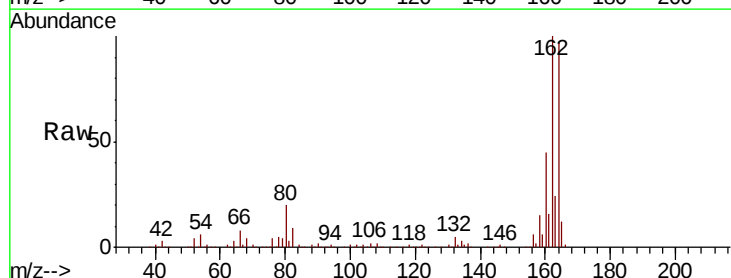

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

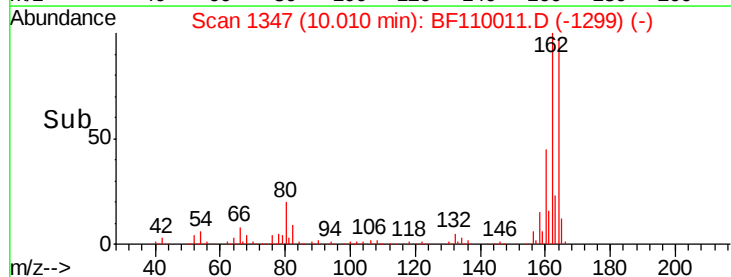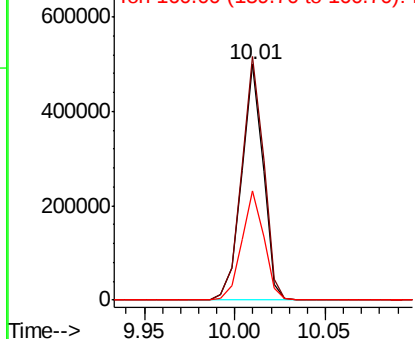


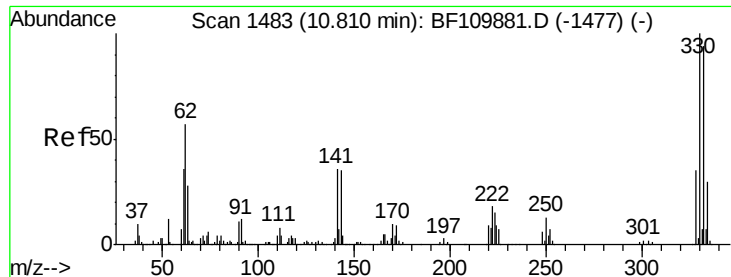

#42
 2,4,6-Tribromophenol
 Concen: 92.652 ng
 RT: 10.80 min Scan# 1482
 Delta R.T. -0.01 min
 Lab File: BF110011.D
 Acq: 19 Oct 2018 19:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.2	77.1	115.7
141	36.9	27.0	40.4



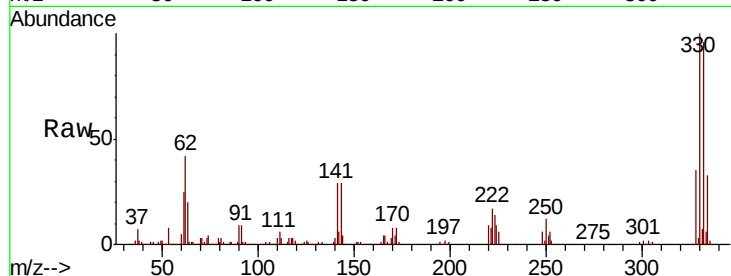


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

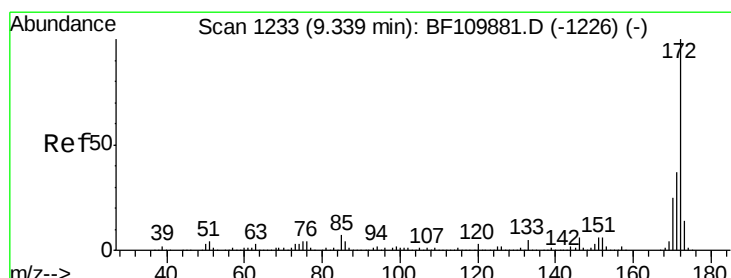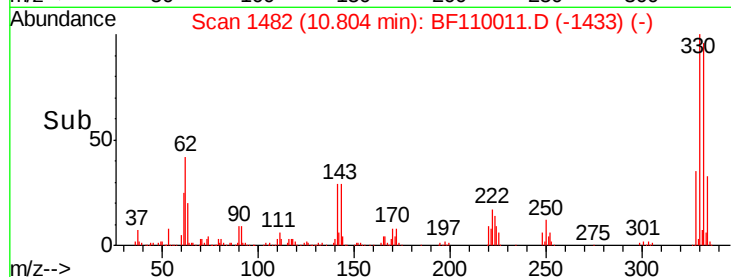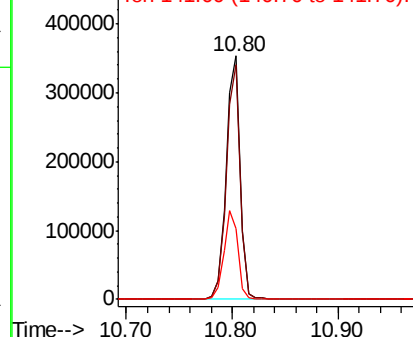

#45
 2-Fluorobiphenyl
 Concen: 85.962 ng
 RT: 9.33 min Scan# 1231
 Delta R.T. -0.01 min
 Lab File: BF110011.D
 Acq: 19 Oct 2018 19:09

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	28.6	43.0
170	24.6	19.7	29.5


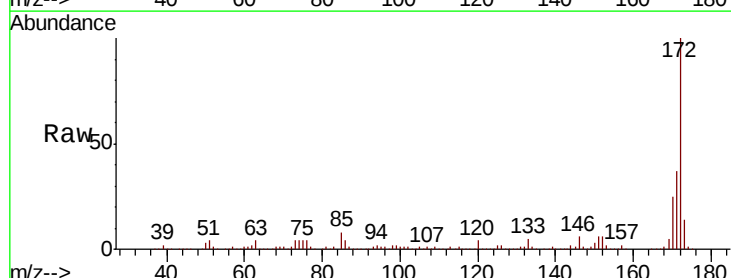



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



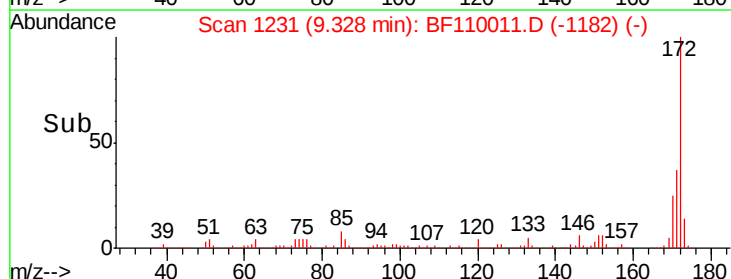
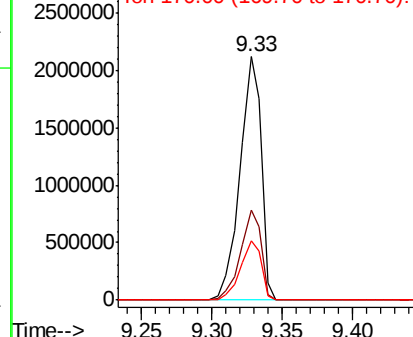


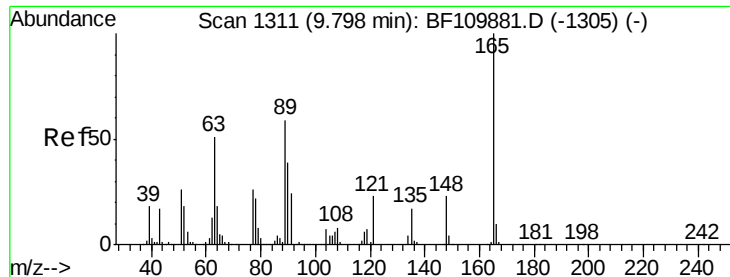

#51
2,6-Dinitrotoluene
Concen: 9.314 ng
RT: 10.01 min Scan# 1347
Delta R.T. 0.21 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.0	48.9	73.3#
89	1.2	46.6	69.8#

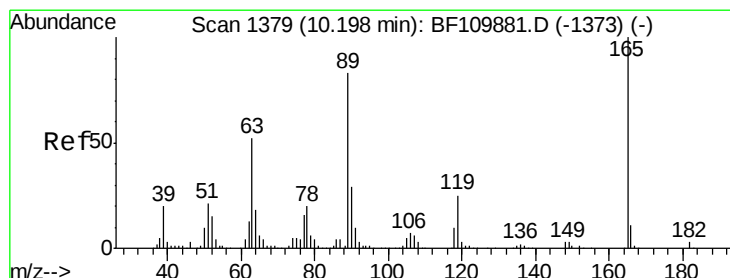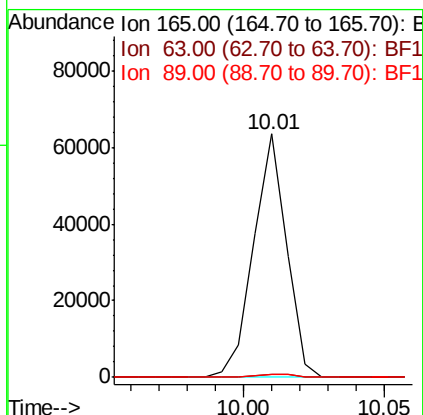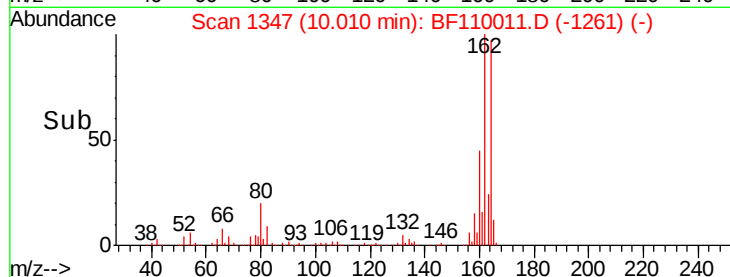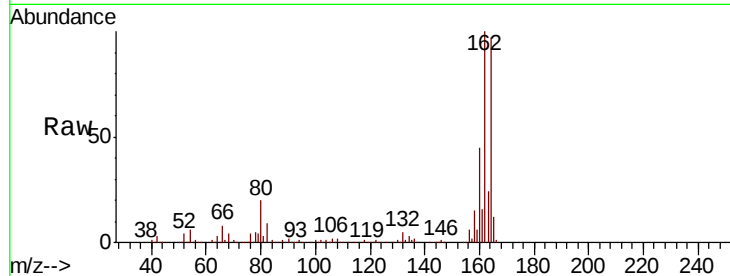

#57
2,4-Dinitrotoluene
Concen: 11.252 ng
RT: 10.01 min Scan# 1347
Delta R.T. -0.20 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.0	44.8	67.2#
89	1.2	62.2	93.4#
182	0.0	2.1	3.1#


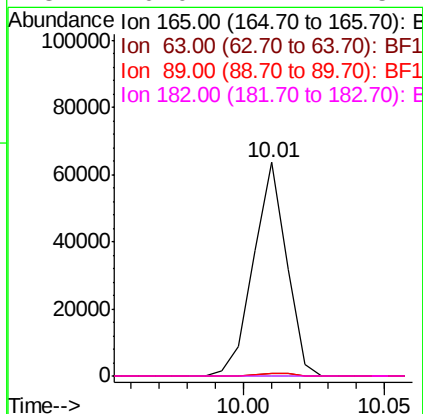
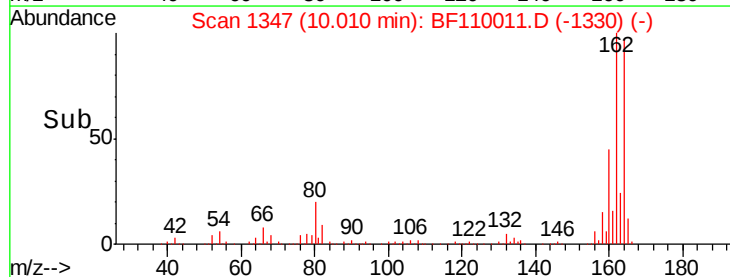
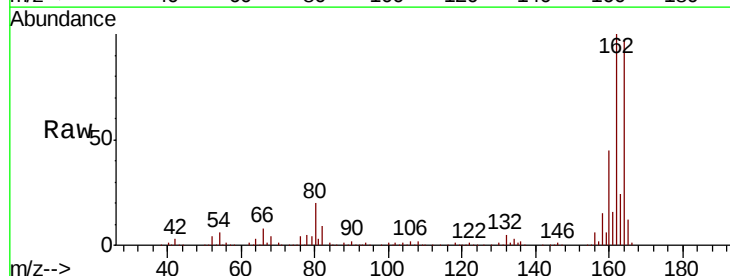


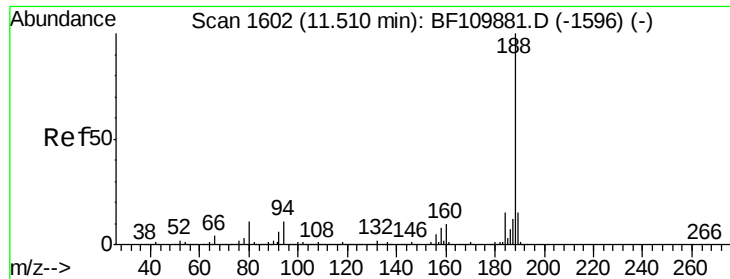

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1601
Delta R.T. -0.01 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 763049
Ion Ratio Lower Upper
188 100
94 9.4 7.2 10.8
80 9.7 7.9 11.9

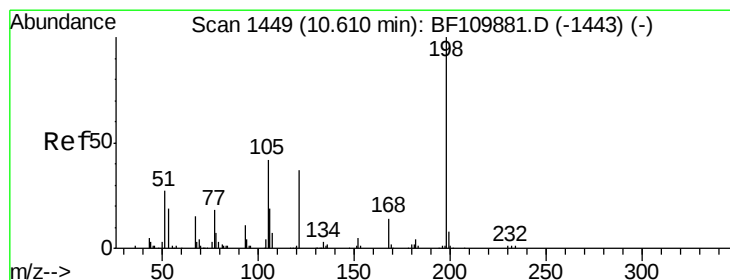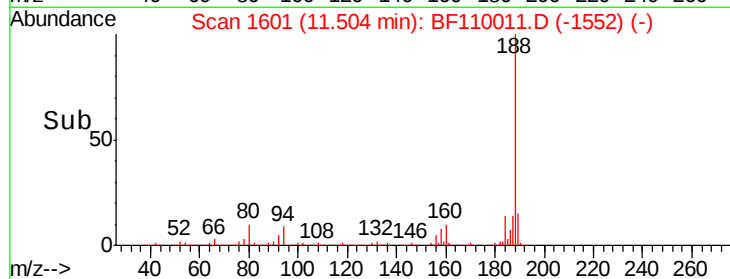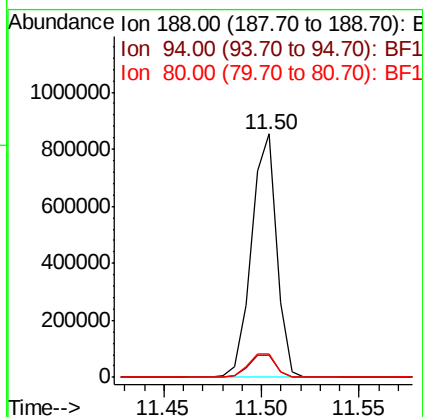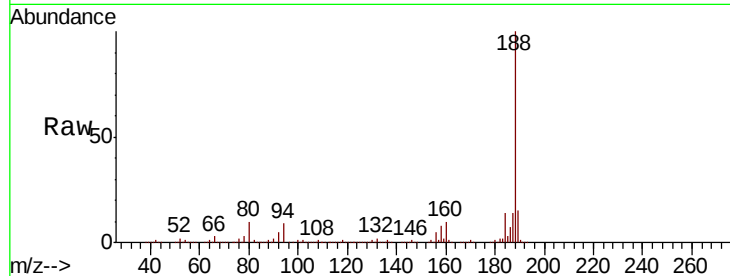

#65
4,6-Dinitro-2-methylphenol
Concen: 8.093 ng
RT: 10.80 min Scan# 1482
Delta R.T. 0.18 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Tgt Ion:198 Resp: 623
Ion Ratio Lower Upper
198 100
51 215.4 22.8 62.8#
105 194.4 23.6 63.6#

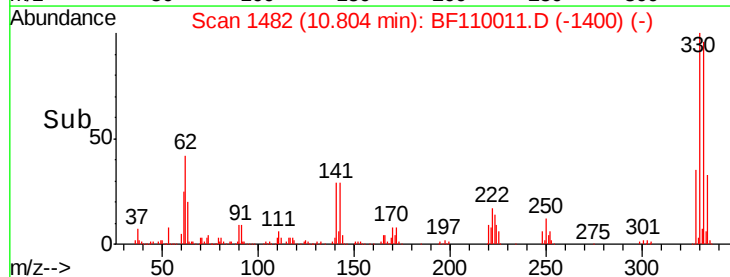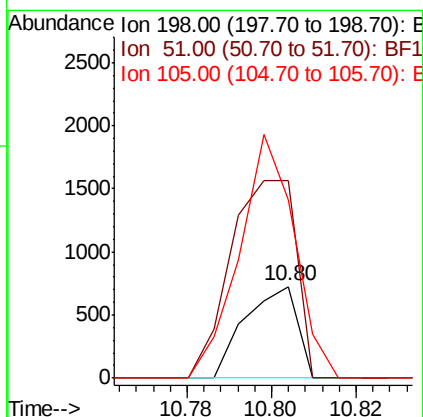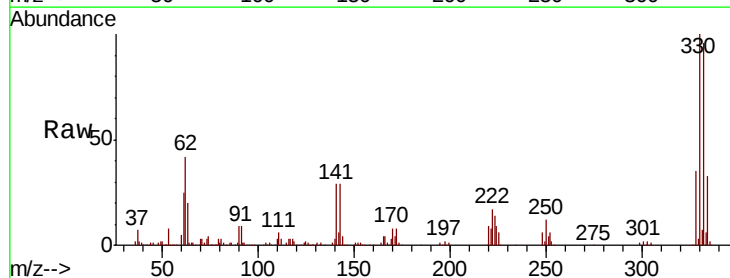


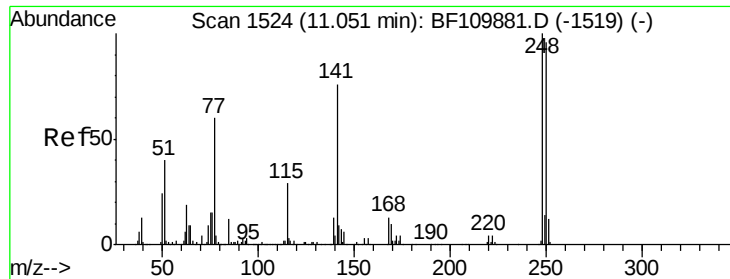




#67
 4-Bromophenyl-phenylether
 Concen: 2.509 ng
 RT: 10.80 min Scan# 1482
 Delta R.T. -0.25 min
 Lab File: BF110011.D
 Acq: 19 Oct 2018 19:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 20751
 Ion Ratio Lower Upper
 248 100
 250 199.5 79.4 119.2#
 141 488.2 55.9 83.9#

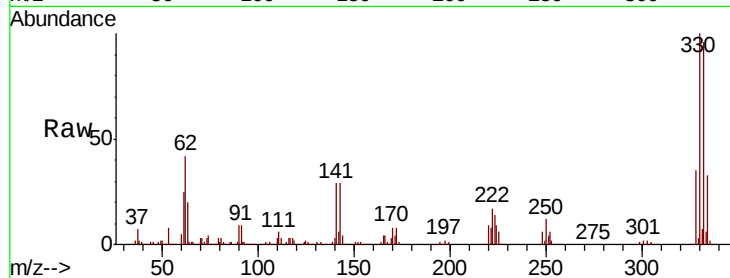


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

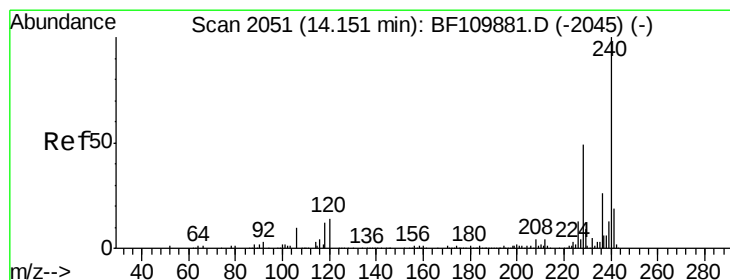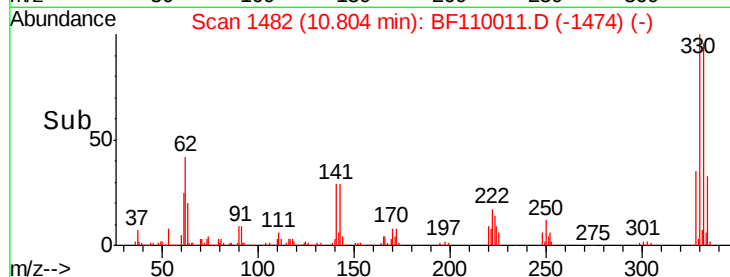
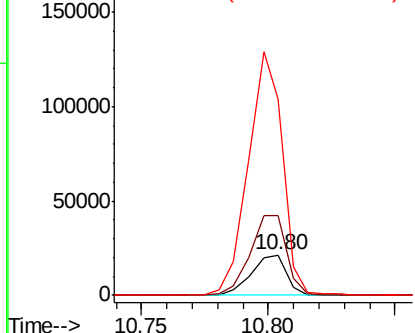



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.14 min Scan# 2050
 Delta R.T. -0.02 min
 Lab File: BF110011.D
 Acq: 19 Oct 2018 19:09

Tgt Ion:240 Resp: 526806
 Ion Ratio Lower Upper
 240 100
 120 11.8 8.3 12.5
 236 24.5 21.2 31.8

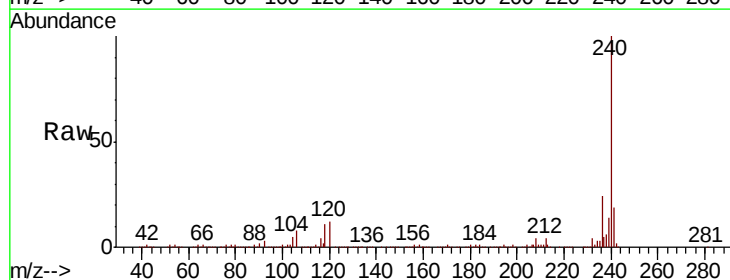

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

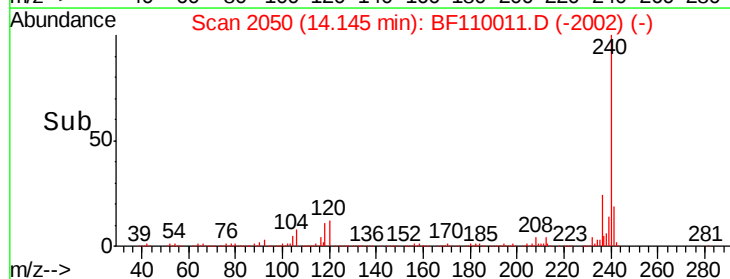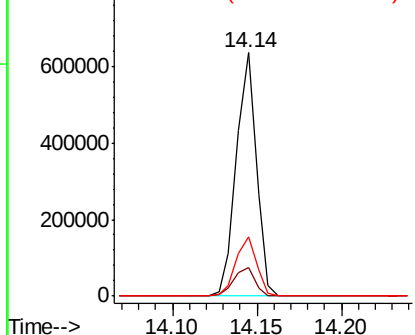


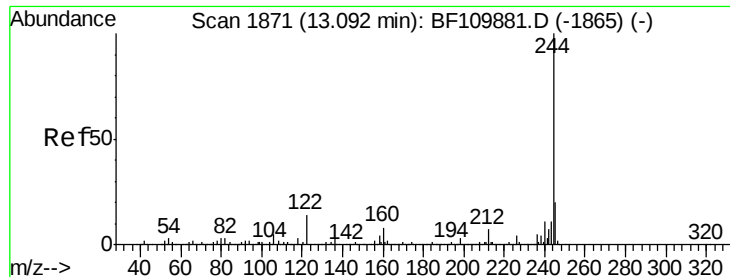




#79
Terphenyl-d14
Concen: 81.581 ng
RT: 13.09 min Scan# 1871
Delta R.T. -0.01 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:244 Resp: 2046614
Ion Ratio Lower Upper
244 100
212 7.0 5.8 8.8
122 12.0 8.7 13.1

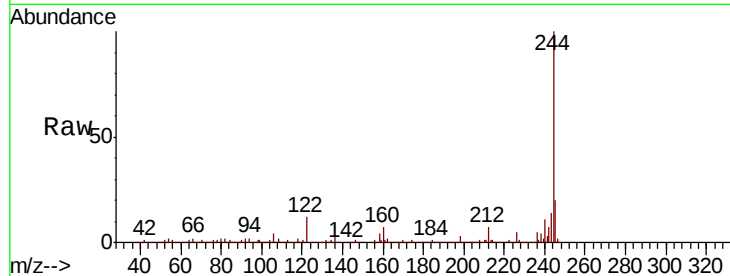


Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

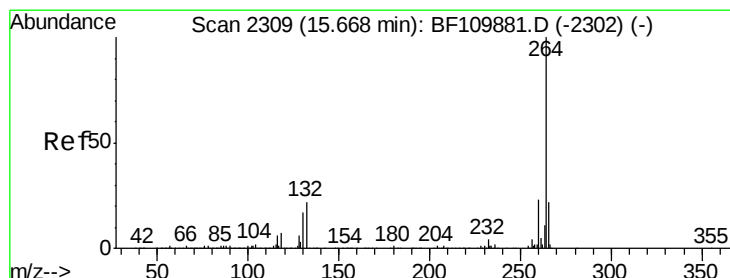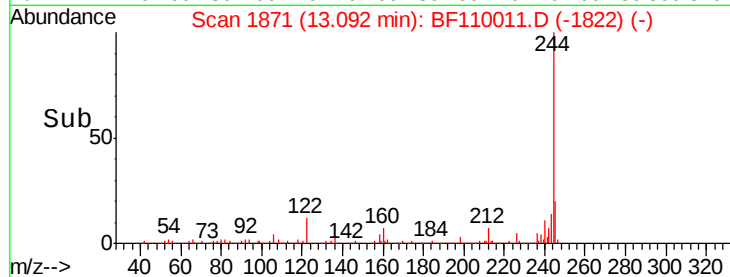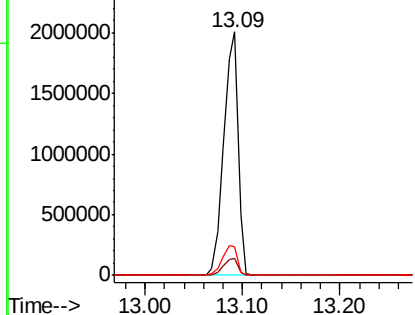

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.66 min Scan# 2308
Delta R.T. -0.03 min
Lab File: BF110011.D
Acq: 19 Oct 2018 19:09

Tgt Ion:264 Resp: 382034
Ion Ratio Lower Upper
264 100
260 23.1 18.7 28.1
265 21.5 16.7 25.1

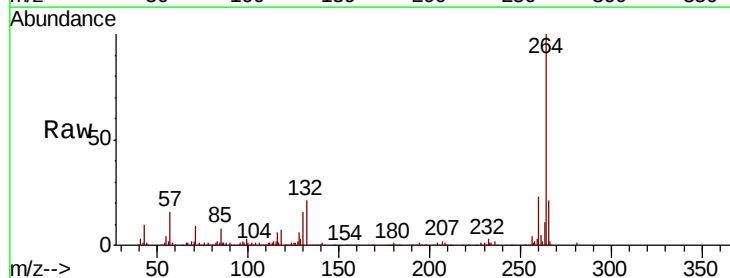

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

