

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101918\
 Data File : BF110032.D
 Acq On : 20 Oct 2018 5:35
 Operator : JU/SJ
 Sample : J5593-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 20 06:47:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 20 01:53:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	215022	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	807106	20.00	ng	0.00
39) Acenaphthene-d10	10.01	164	344233	20.00	ng	0.00
64) Phenanthrene-d10	11.50	188	534256	20.00	ng	0.00
76) Chrysene-d12	14.14	240	364829	20.00	ng	0.00
87) Perylene-d12	15.67	264	312043	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	497112	36.65	ng	0.00
7) Phenol-d6	6.58	99	378149	22.45	ng	-0.01
23) Nitrobenzene-d5	7.53	82	1237537	103.29	ng	0.00
42) 2,4,6-Tribromophenol	10.80	330	240786	80.79	ng	0.00
45) 2-Fluorobiphenyl	9.33	172	1897086	87.94	ng	0.00
79) Terphenyl-d14	13.09	244	1462810	84.20	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.53	70	165097	15.265	ng	# 80
25) Isophorone	7.53	82	1237527	52.567	ng	# 67
50) Dimethylphthalate	9.72	163	48968	2.009	ng	# 97
51) 2,6-Dinitrotoluene	10.01	165	43513	9.399	ng	# 23
57) 2,4-Dinitrotoluene	10.01	165	43513	11.313	ng	# 19
65) 4,6-Dinitro-2-methylphenol	10.80	198	461	8.103	ng	# 1
67) 4-Bromophenyl-phenylether	10.80	248	16628	2.872	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101918\
Data File : BF110032.D
Acq On : 20 Oct 2018 5:35
Operator : JU/SJ
Sample : J5593-17
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 20 06:47:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 20 01:53:35 2018
Response via : Initial Calibration




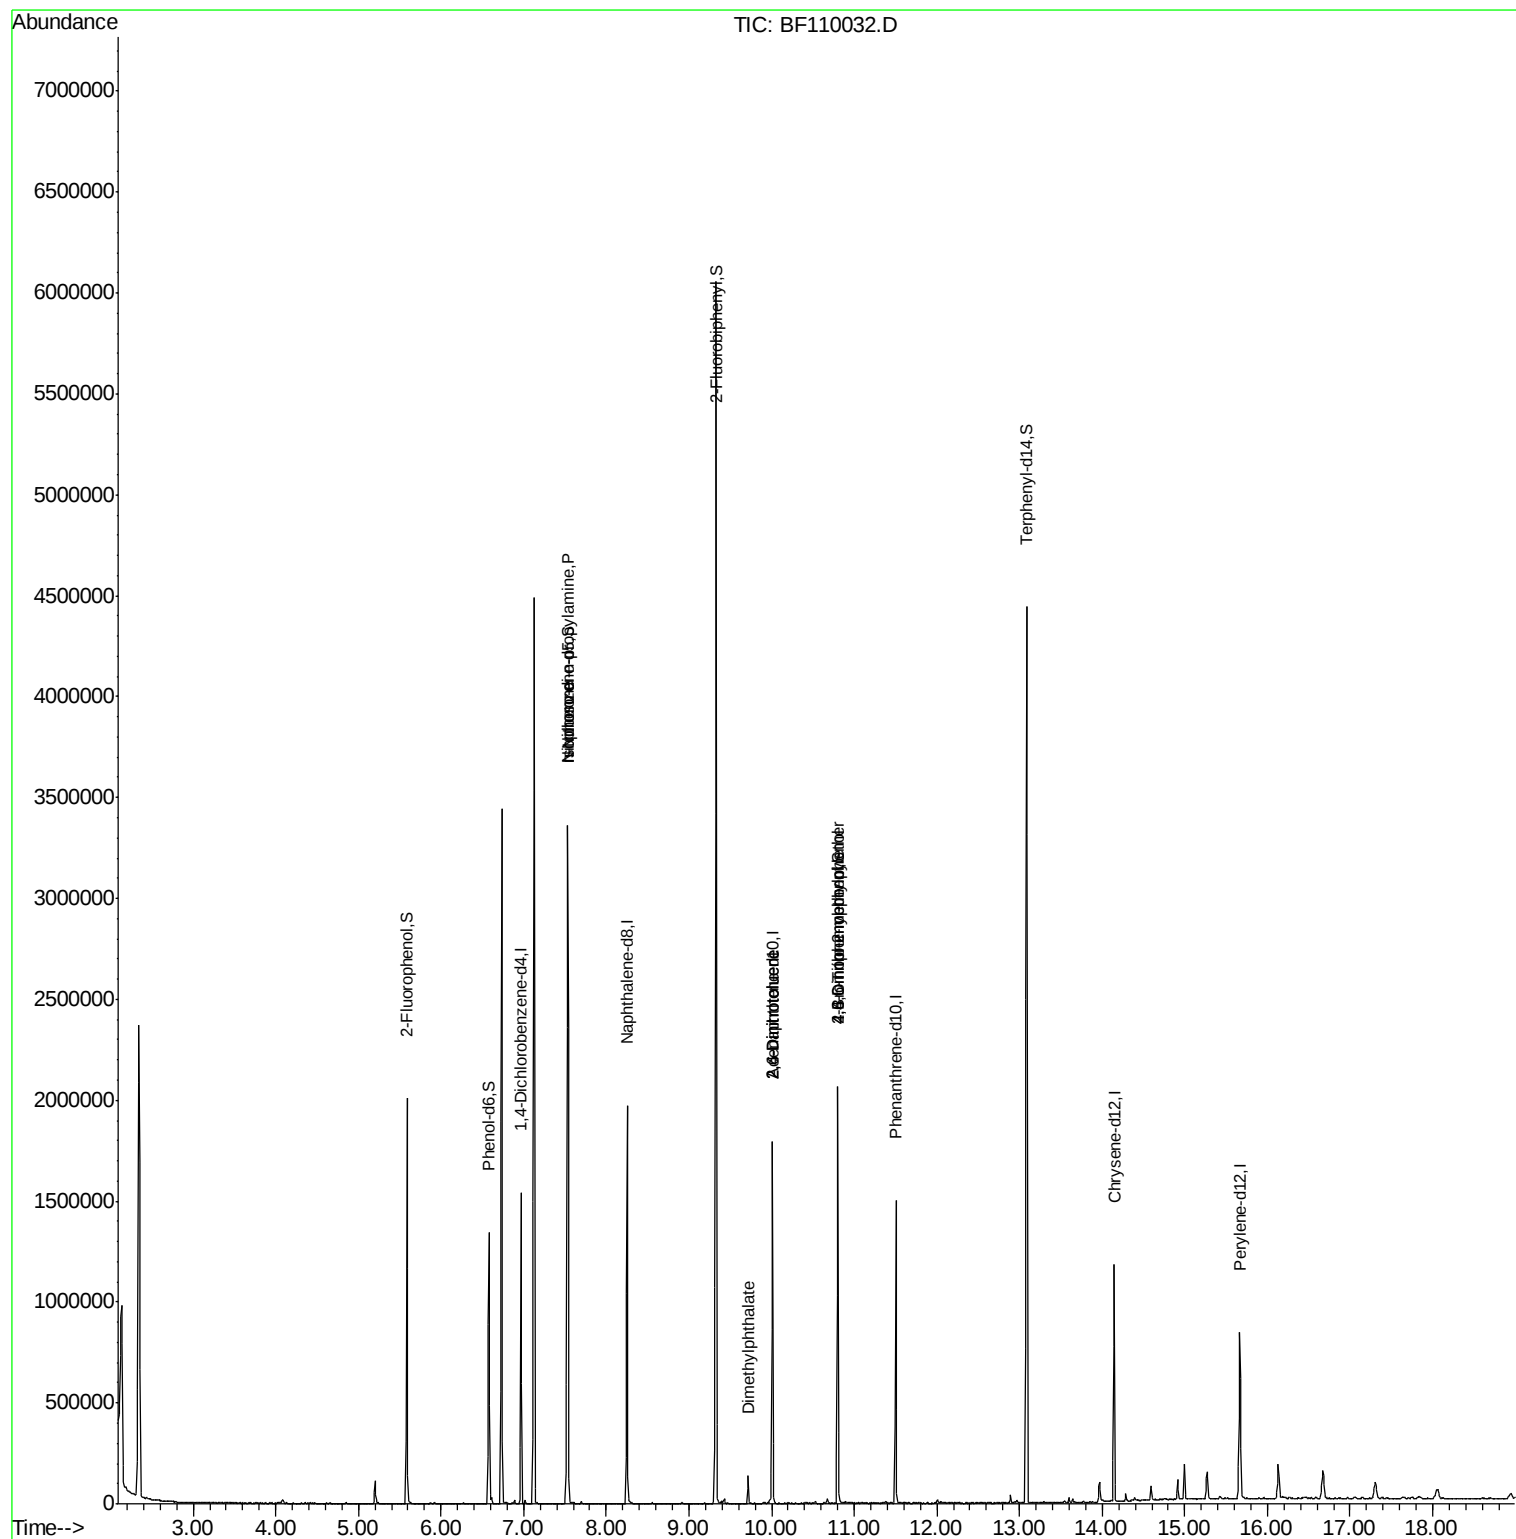


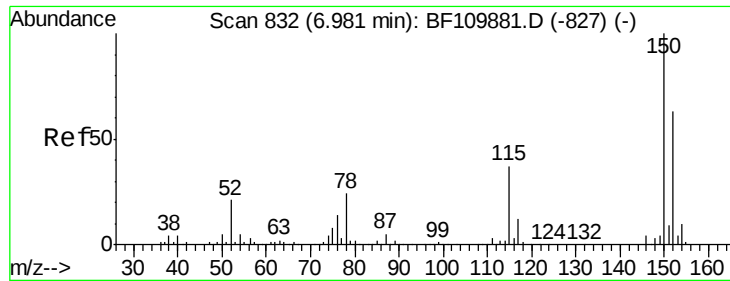

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.97 min Scan# 830
 Delta R.T. -0.00 min
 Lab File: BF110032.D
 Acq: 20 Oct 2018 5:35




Instrument :
 BNA_F
 ClientSampled :




Tot Ion:152 Resp: 215022
 Ion Ratio Lower Upper
 152 100
 150 156.3 122.7 184.1
 115 62.2 49.1 73.7

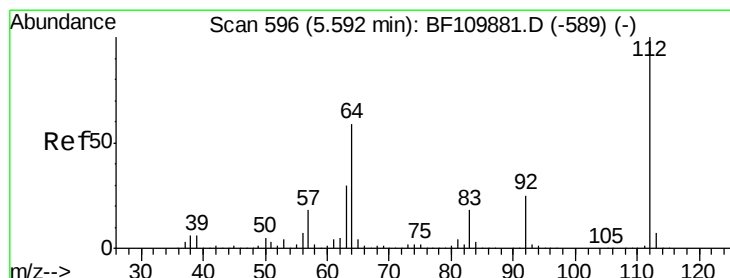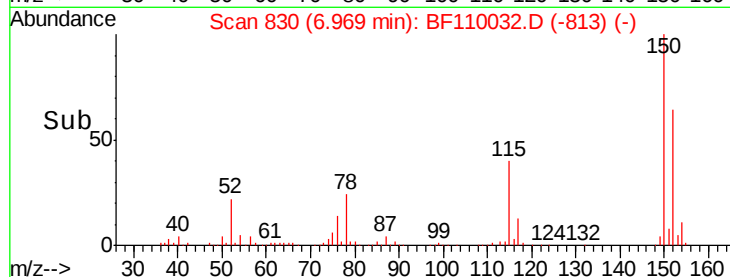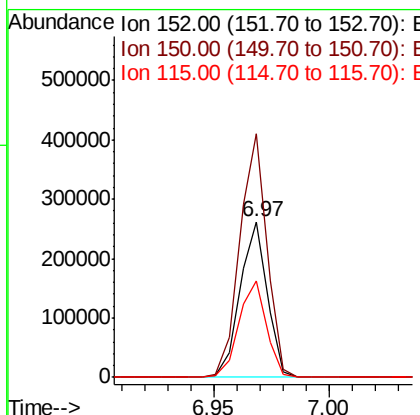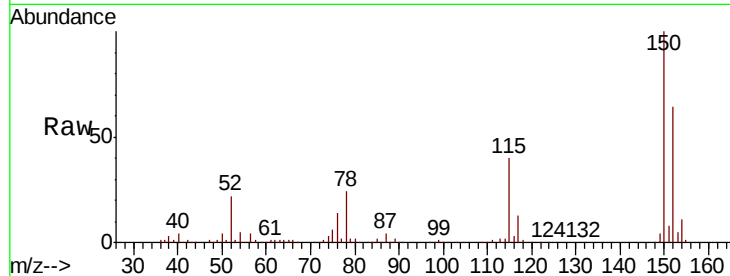

#5
 2-Fluorophenol
 Concen: 36.647 ng
 RT: 5.59 min Scan# 595
 Delta R.T. -0.00 min
 Lab File: BF110032.D
 Acq: 20 Oct 2018 5:35

Tgt Ion:112 Resp: 497112
 Ion Ratio Lower Upper
 112 100
 64 60.3 44.1 66.1
 63 31.1 23.7 35.5

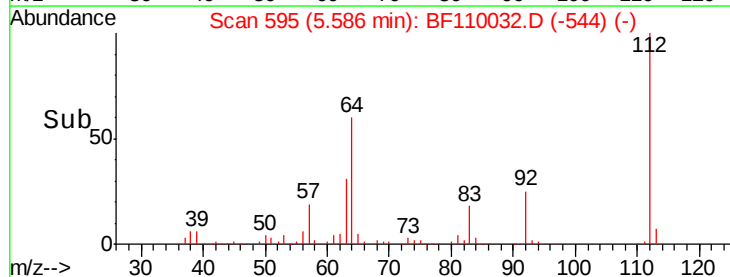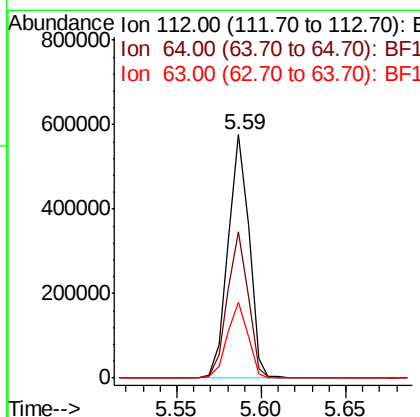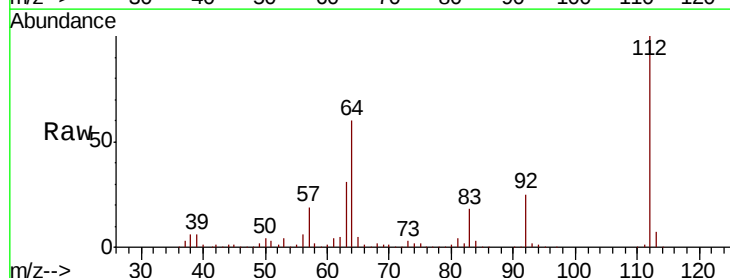

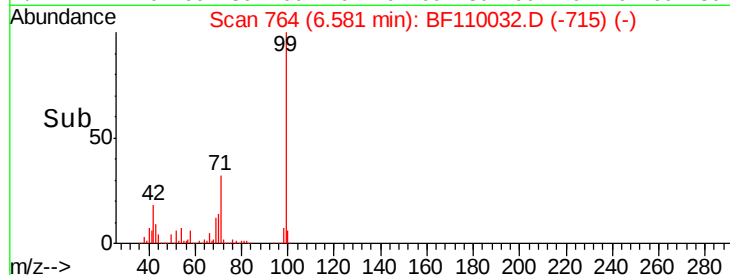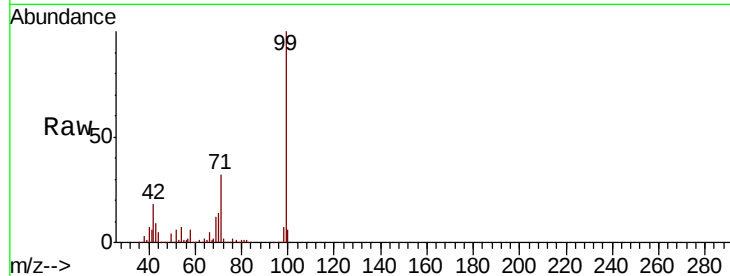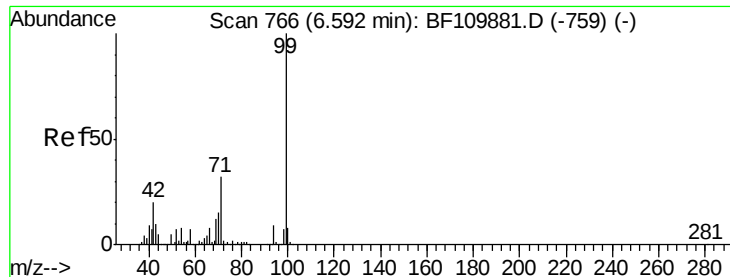

#7

Phenol-d6

Concen: 22.450 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.01 min

Lab File: BF110032.D

Acq: 20 Oct 2018 5:35

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 378149

Ion Ratio Lower Upper

99 100

42 18.1 15.8 23.6

71 31.9 28.0 42.0

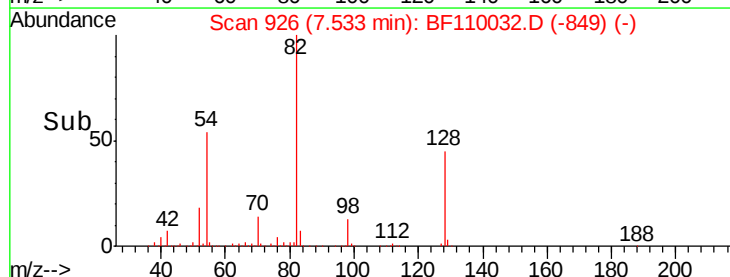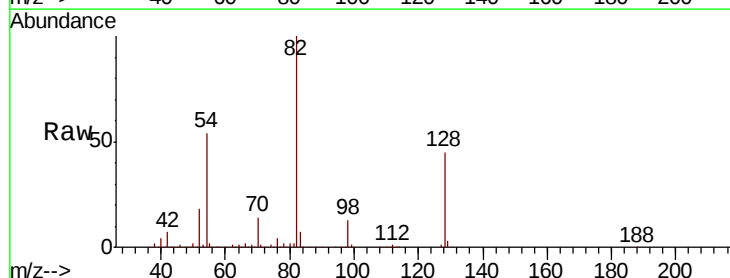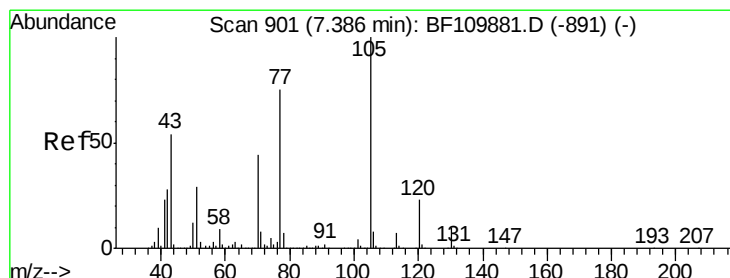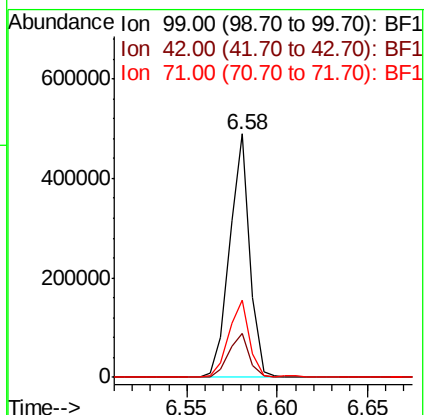

#19

n-Nitroso-di-n-propylamine

Concen: 15.265 ng

RT: 7.53 min Scan# 926

Delta R.T. 0.15 min

Lab File: BF110032.D

Acq: 20 Oct 2018 5:35

Tgt Ion: 70 Resp: 165097


Ion Ratio Lower Upper


70 100

42 49.8 47.4 71.2

101 0.0 7.3 10.9#

130 2.2 16.2 24.2#

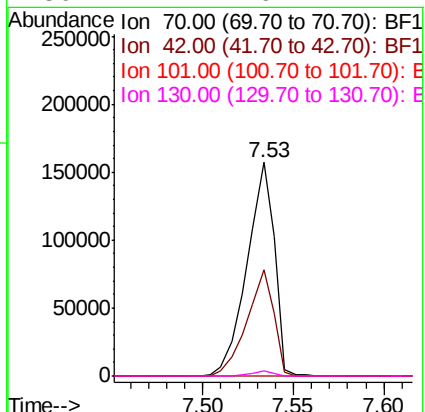

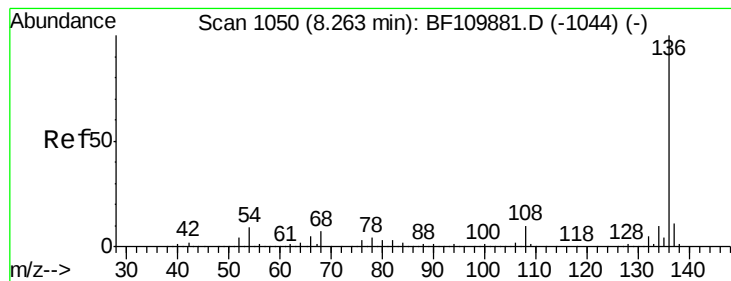

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1048

Delta R.T. -0.01 min

Lab File: BF110032.D

Acq: 20 Oct 2018 5:35

Instrument :

BNA_F

ClientSampled :

Tot Ion:136 Resp: 807106



Ion Ratio Lower Upper

136 100

137 11.3 8.8 13.2

54 8.2 5.4 8.2#

68 5.8 4.2 6.2


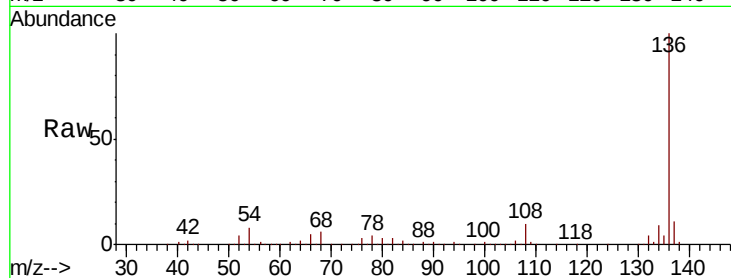


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

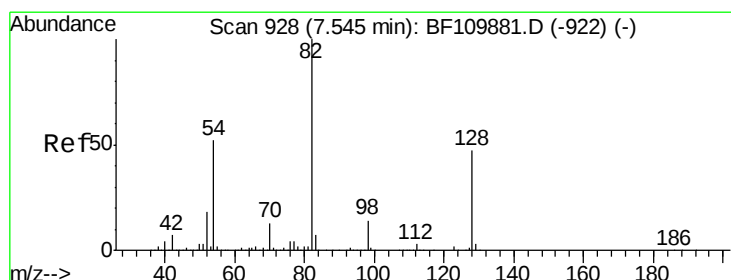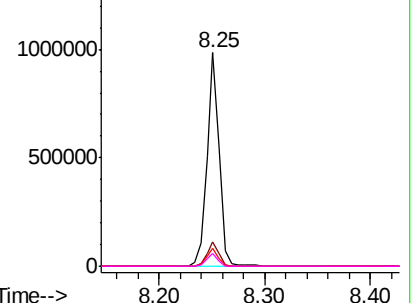

#23

Nitrobenzene-d5

Concen: 103.289 ng

RT: 7.53 min Scan# 926

Delta R.T. -0.01 min

Lab File: BF110032.D

Acq: 20 Oct 2018 5:35



Tgt Ion: 82 Resp: 1237537

Ion Ratio Lower Upper

82 100

128 45.4 34.2 51.2


54 53.6 38.6 58.0

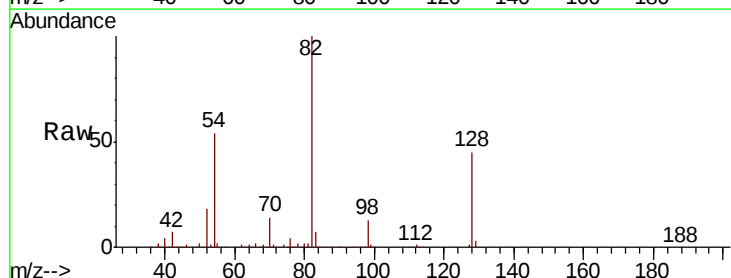


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

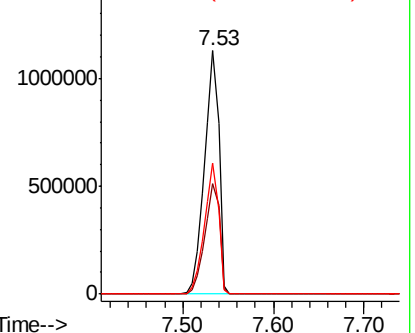

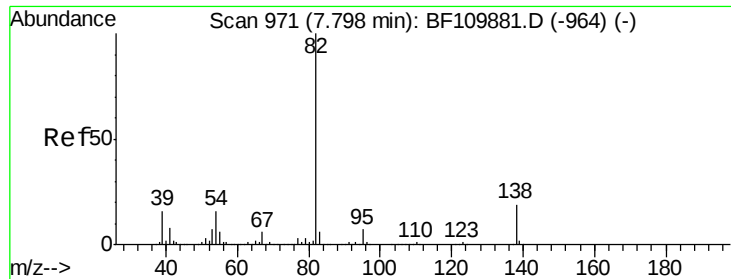

#25

Isophorone

Concen: 52.567 ng

RT: 7.53 min Scan# 926

Delta R.T. -0.26 min

Lab File: BF110032.D

Acq: 20 Oct 2018 5:35

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 1237527

Ion Ratio Lower Upper




82 100

95 0.0 5.7 8.5#

138 0.0 13.2 19.8#

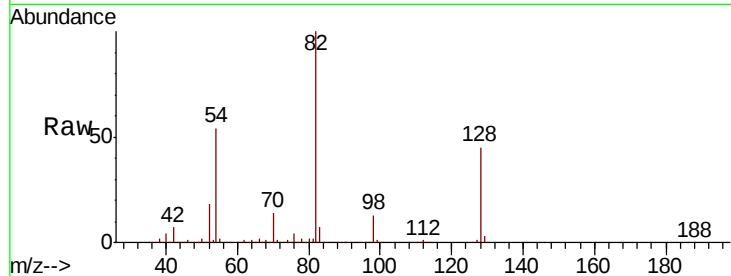

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): E

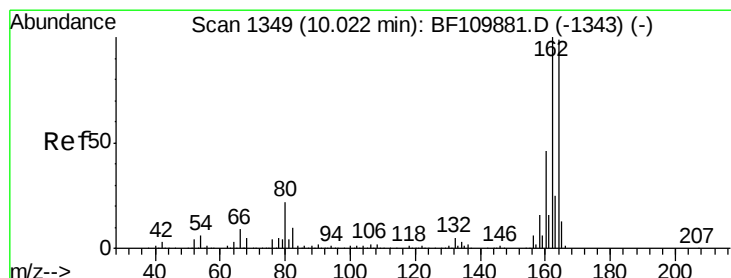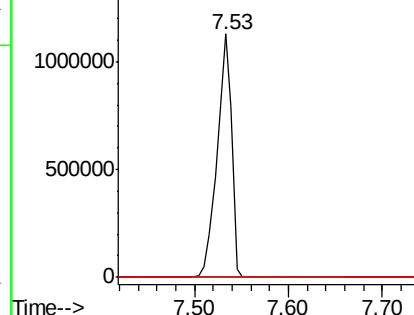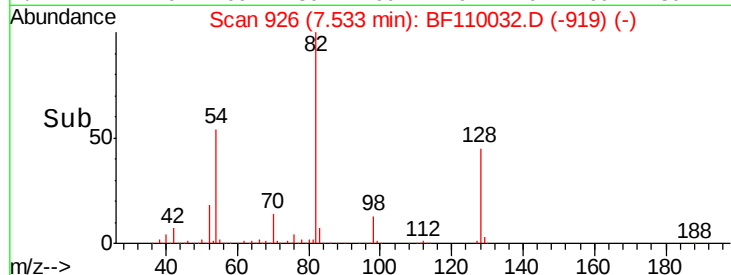

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1347

Delta R.T. -0.01 min

Lab File: BF110032.D

Acq: 20 Oct 2018 5:35


Tgt Ion:164 Resp: 344233

Ion Ratio Lower Upper



164 100


162 102.2 83.0 124.6

160 45.3 37.0 55.6

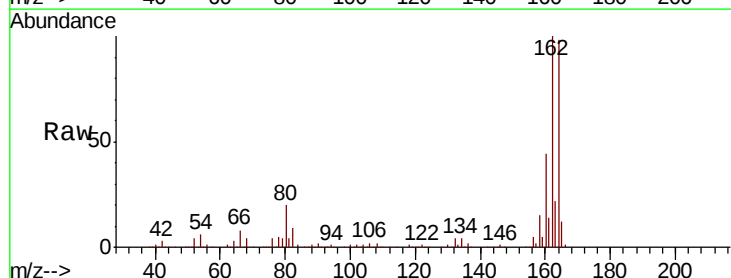

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

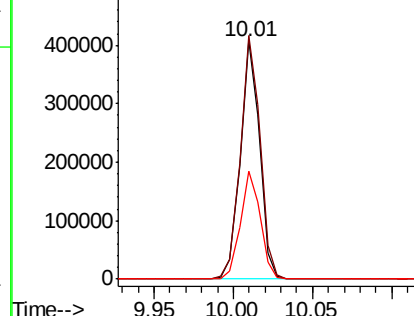


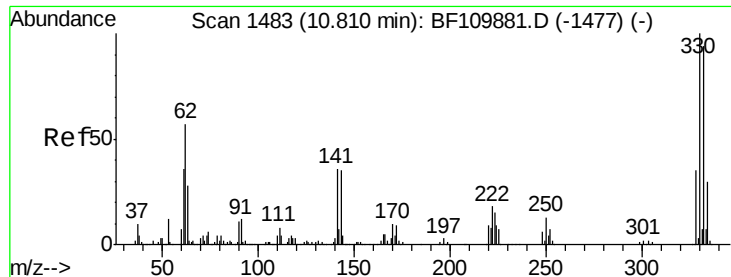

#42
 2,4,6-Tribromophenol
 Concen: 80.793 ng
 RT: 10.80 min Scan# 1482
 Delta R.T. -0.00 min
 Lab File: BF110032.D
 Acq: 20 Oct 2018 5:35

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	77.1	115.7
141	36.7	27.0	40.4



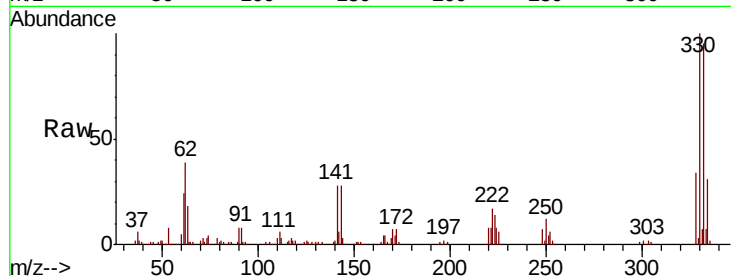


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

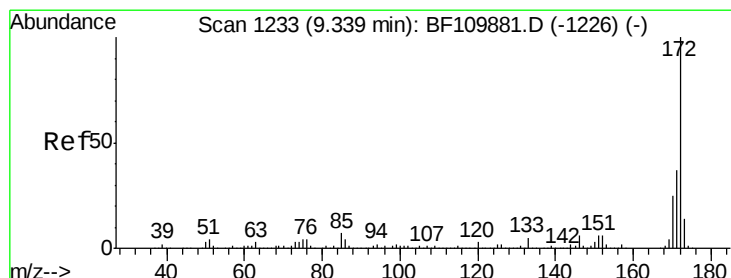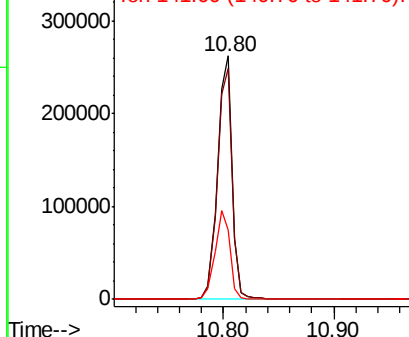

#45
 2-Fluorobiphenyl
 Concen: 87.937 ng
 RT: 9.33 min Scan# 1231
 Delta R.T. -0.01 min
 Lab File: BF110032.D
 Acq: 20 Oct 2018 5:35

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	28.6	43.0
170	24.8	19.7	29.5


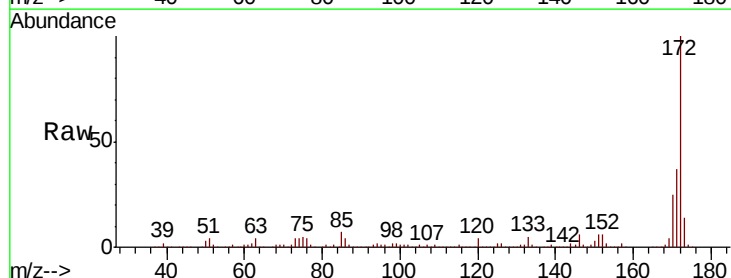



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

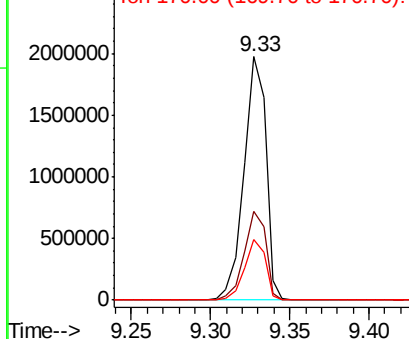







#50
Dimethylphthalate
Concen: 2.009 ng
RT: 9.72 min Scan# 1297
Delta R.T. -0.01 min
Lab File: BF110032.D
Acq: 20 Oct 2018 5:35

Instrument :
BNA_F
ClientSampleId :

Tot Ion	163	Resp	48968
Ion Ratio	100	Lower	Upper
163	100		
194	3.0	3.2	4.8#
164	11.1	8.1	12.1

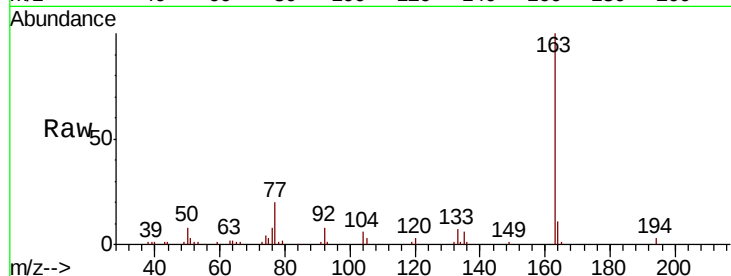


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

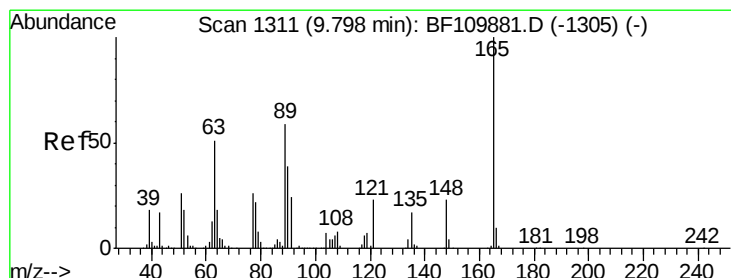
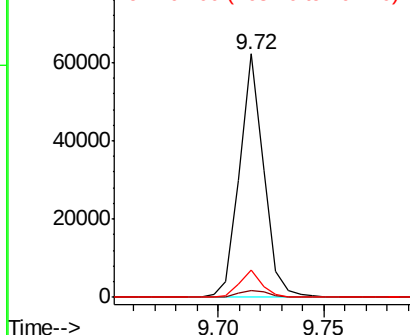



#51
2,6-Dinitrotoluene
Concen: 9.399 ng
RT: 10.01 min Scan# 1347
Delta R.T. 0.22 min
Lab File: BF110032.D
Acq: 20 Oct 2018 5:35

Tgt Ion	165	Resp	43513
Ion Ratio	100	Lower	Upper
165	100		
63	1.4	48.9	73.3#
89	1.2	46.6	69.8#

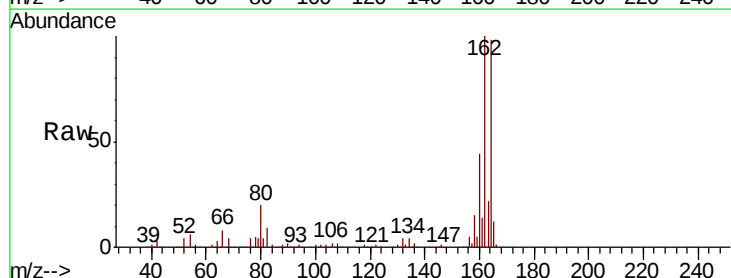

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1




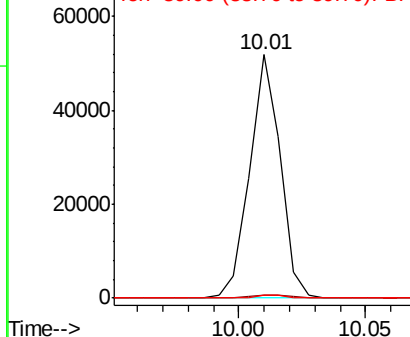


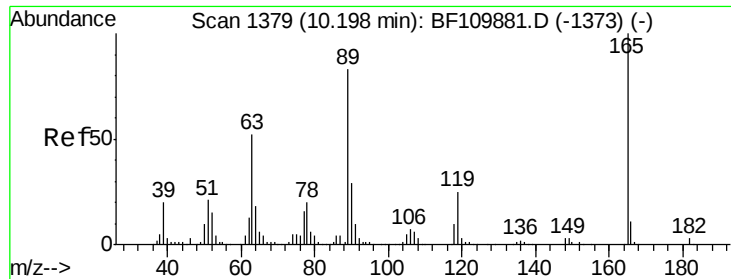

#57
2,4-Dinitrotoluene
Concen: 11.313 ng
RT: 10.01 min Scan# 1347
Delta R.T. -0.19 min
Lab File: BF110032.D
Acq: 20 Oct 2018 5:35




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.4	44.8	67.2#
89	1.2	62.2	93.4#
182	0.0	2.1	3.1#

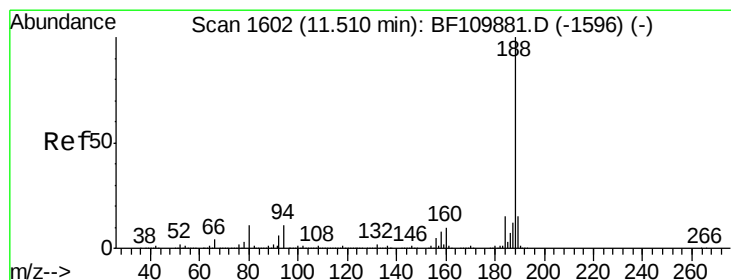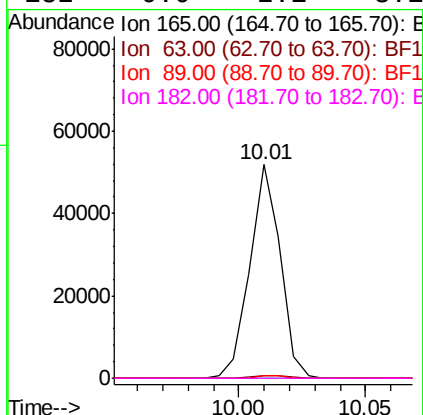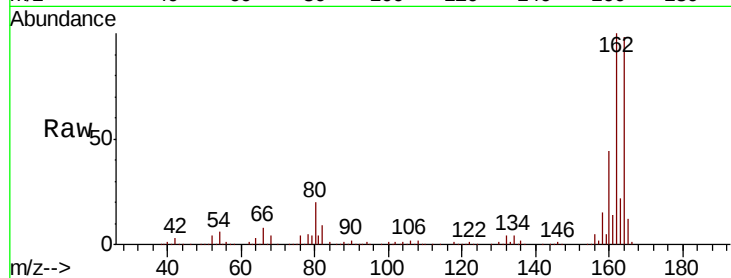

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1601
Delta R.T. -0.00 min
Lab File: BF110032.D
Acq: 20 Oct 2018 5:35

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.2	7.2	10.8
80	9.4	7.9	11.9

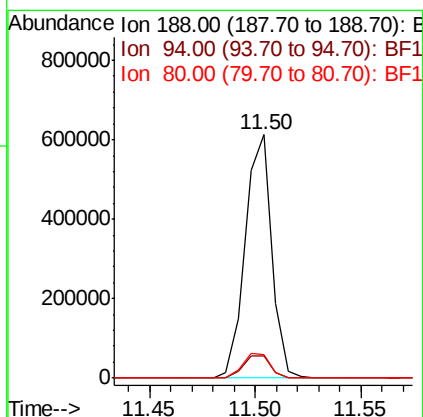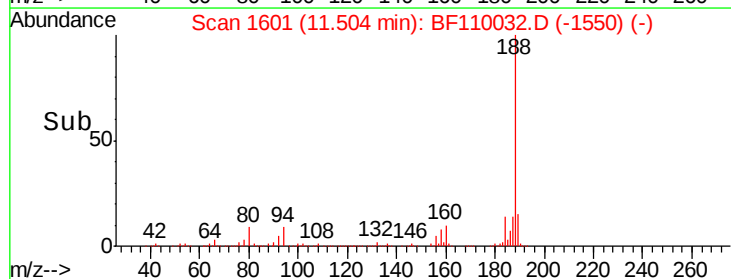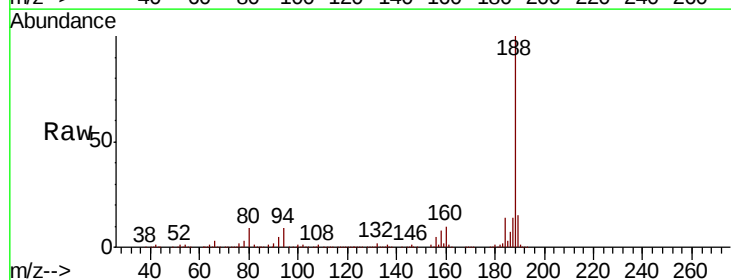


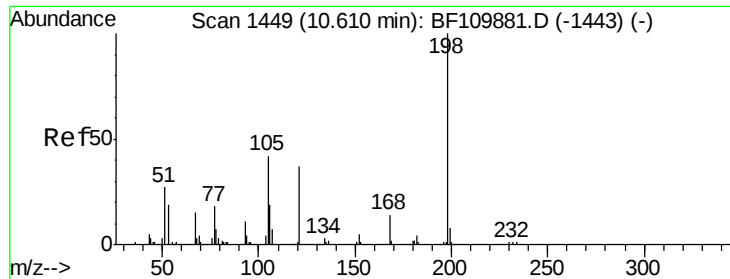




#65
 4,6-Dinitro-2-methylphenol
 Concen: 8.103 ng
 RT: 10.80 min Scan# 1481
 Delta R.T. 0.19 min
 Lab File: BF110032.D
 Acq: 20 Oct 2018 5:35

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:198 Resp: 461
 Ion Ratio Lower Upper
 198 100
 51 191.2 22.8 62.8#
 105 160.8 23.6 63.6#

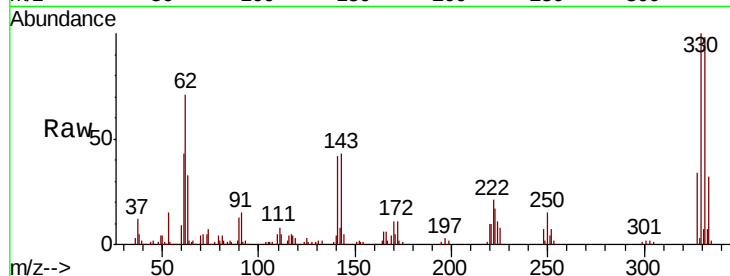


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

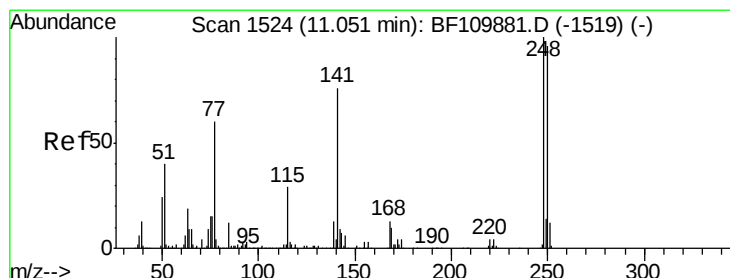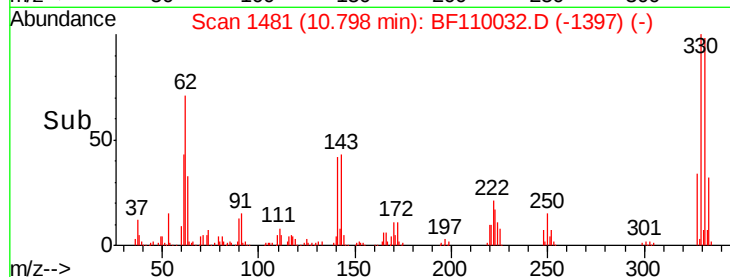
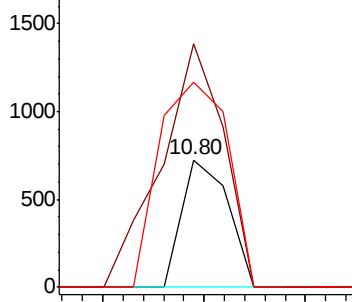



#67
 4-Bromophenyl-phenylether
 Concen: 2.872 ng
 RT: 10.80 min Scan# 1482
 Delta R.T. -0.24 min
 Lab File: BF110032.D
 Acq: 20 Oct 2018 5:35

Tgt Ion:248 Resp: 16628
 Ion Ratio Lower Upper
 248 100
 250 179.0 79.4 119.2#
 141 431.2 55.9 83.9#

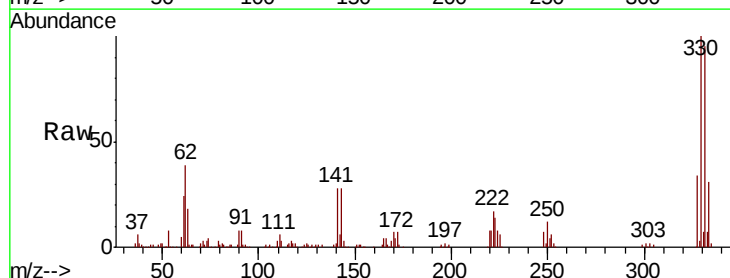

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E



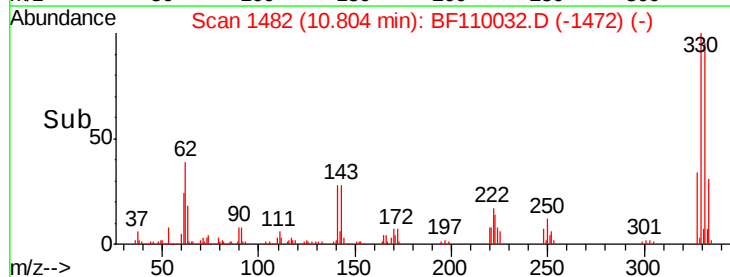
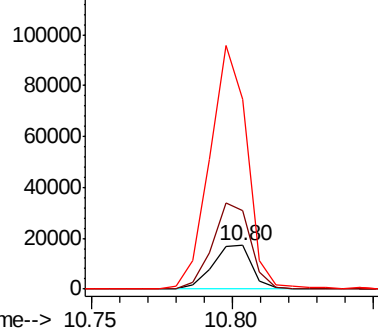


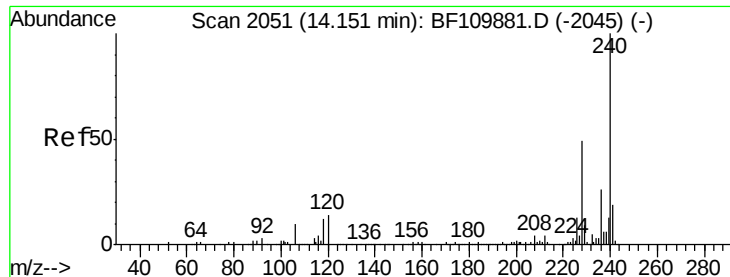

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.14 min Scan# 2050
Delta R.T. -0.01 min
Lab File: BF110032.D
Acq: 20 Oct 2018 5:35




Instrument :
BNA_F
ClientSampleId :


Tot Ion:240 Resp: 364829
Ion Ratio Lower Upper
240 100
120 12.9 8.3 12.5#
236 25.5 21.2 31.8

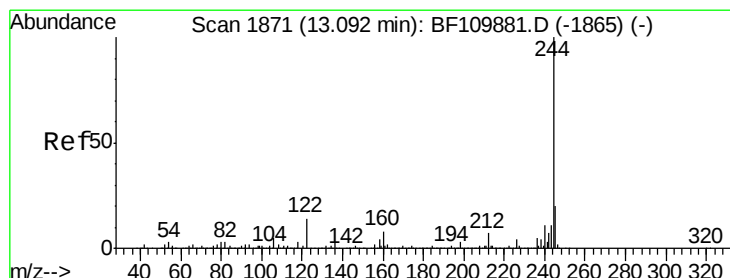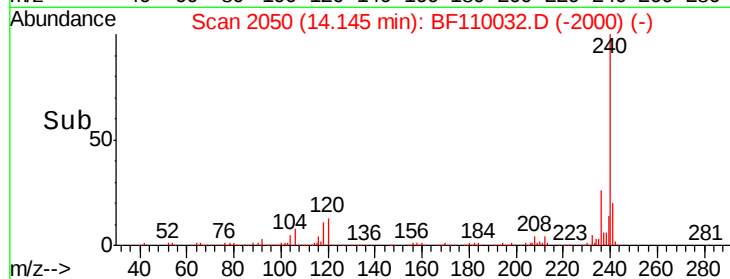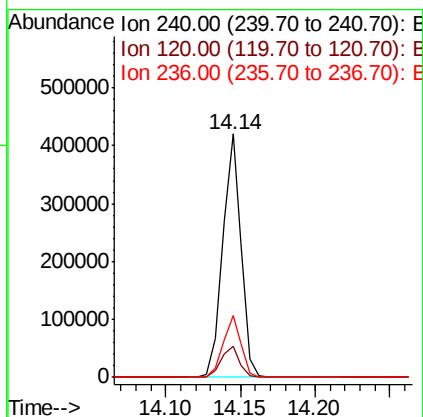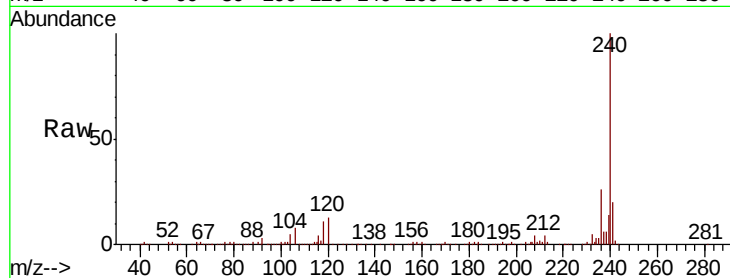

#79
Terphenyl-d14
Concen: 84.198 ng
RT: 13.09 min Scan# 1870
Delta R.T. -0.00 min
Lab File: BF110032.D
Acq: 20 Oct 2018 5:35

Tgt Ion:244 Resp: 1462810
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.8
122 13.5 8.7 13.1#

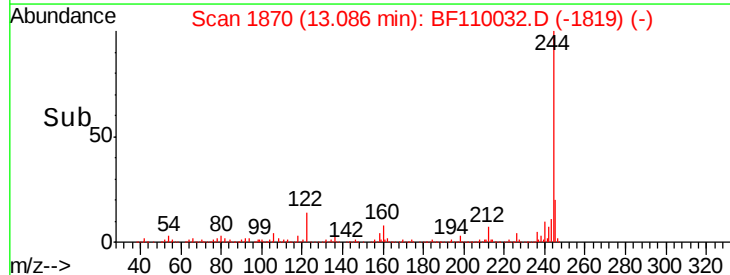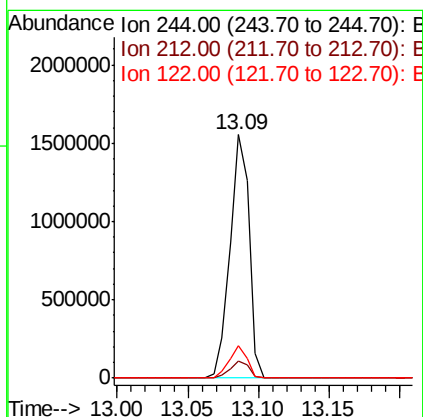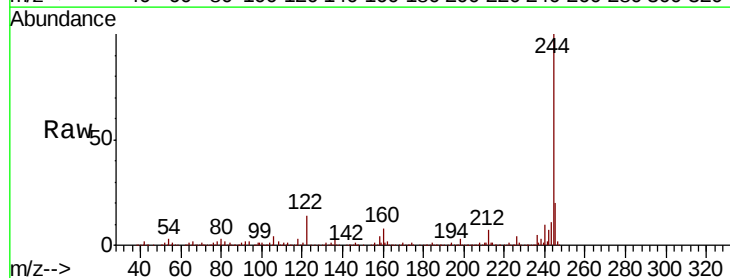



#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.67 min Scan# 2309
 Delta R.T. -0.00 min
 Lab File: BF110032.D
 Acq: 20 Oct 2018 5:35

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.7	28.1
265	21.2	16.7	25.1

