
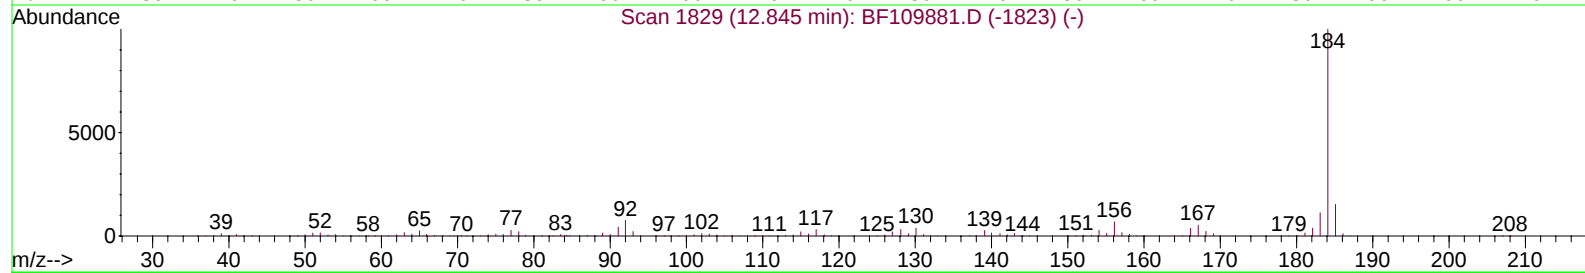
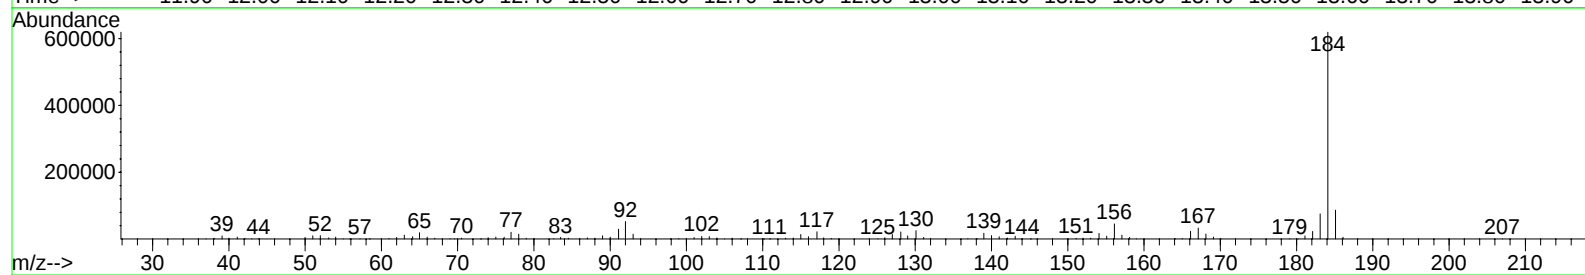


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101918\  
Data File   : BF109996.D  
Acq On      : 19 Oct 2018  12:18  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Oct 22 07:08:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

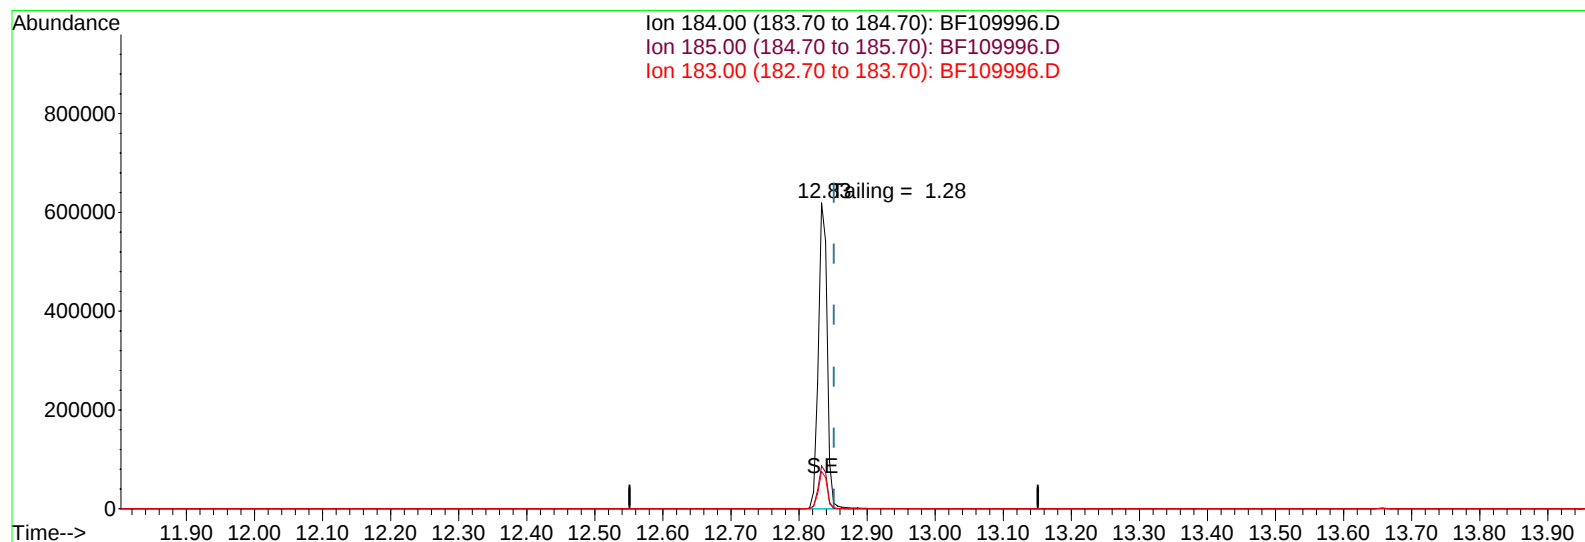

TIC: BF109996.D

(77) Benzidine




12.833min (-0.018) 0.00ng

response 557455

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.01
183.00	11.80	12.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101918\
Data File : BF109996.D
Acq On : 19 Oct 2018 12:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 07:08:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

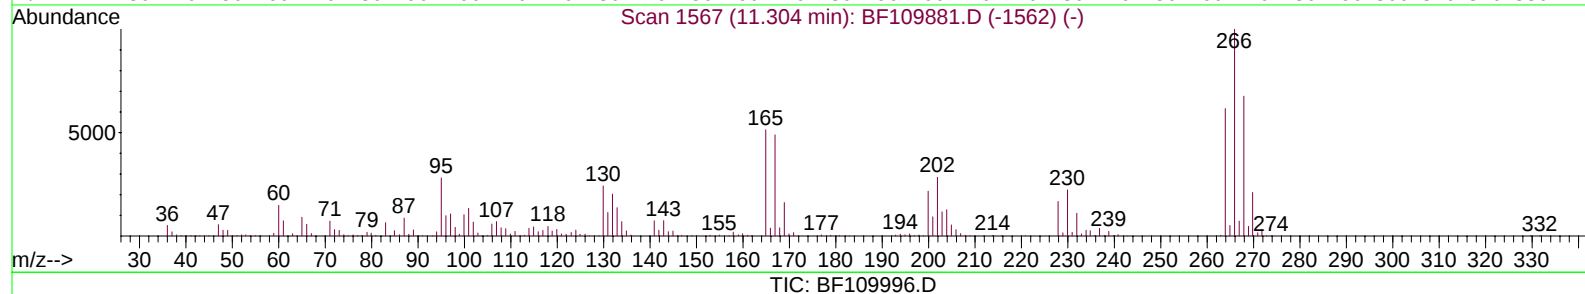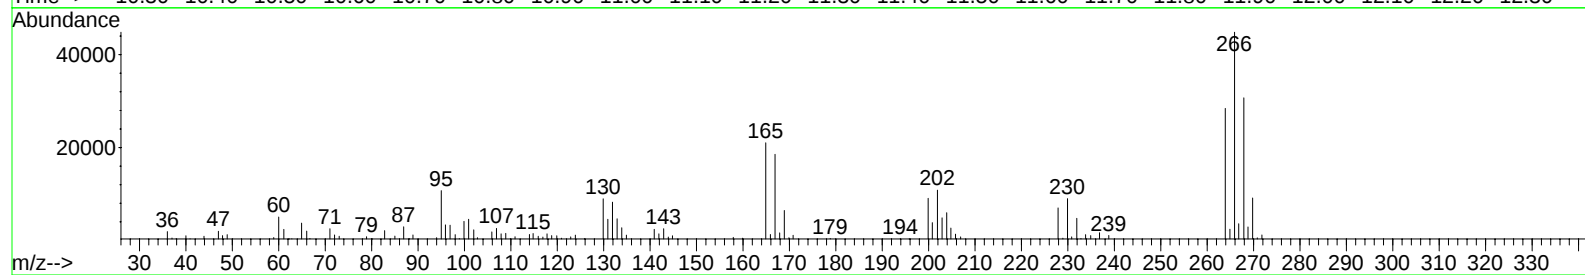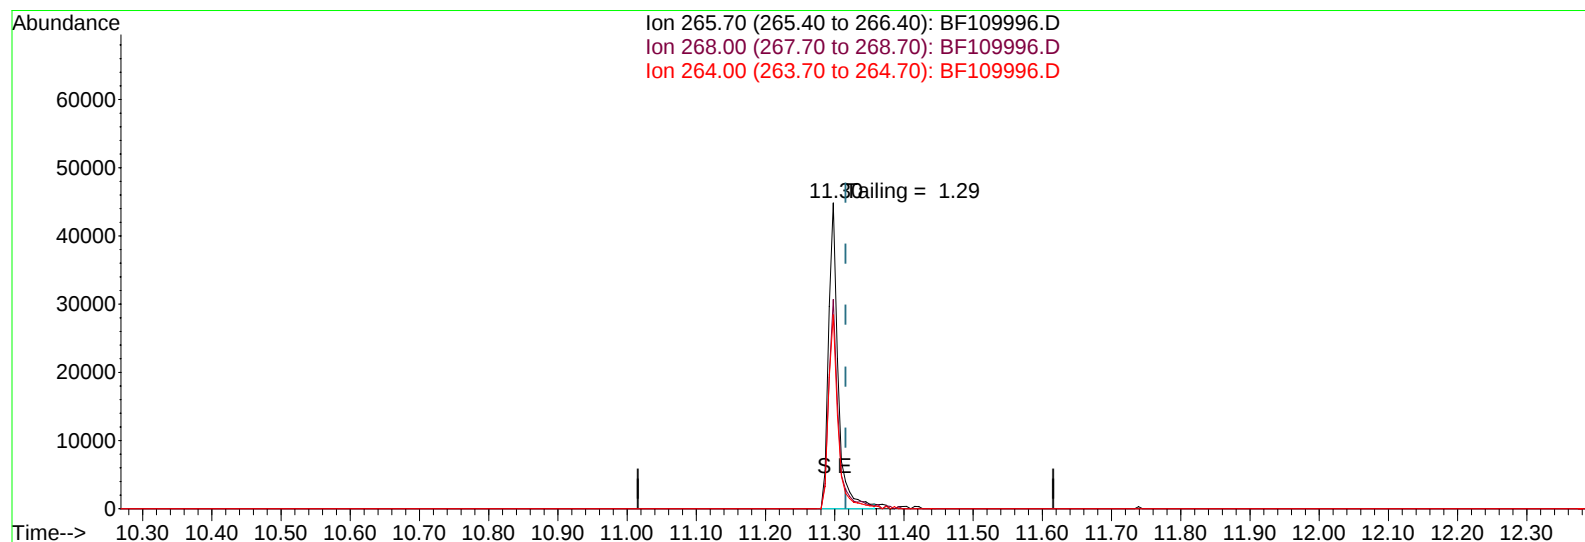

(70) Pentachlorophenol (C)

11.298min (-0.018) 15217.55ng

response 43537

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	68.47
264.00	63.20	63.44
0.00	0.00	0.00