


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101918\
Data File : BF109996.D
Acq On : 19 Oct 2018 12:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 16 14:58:24 2018

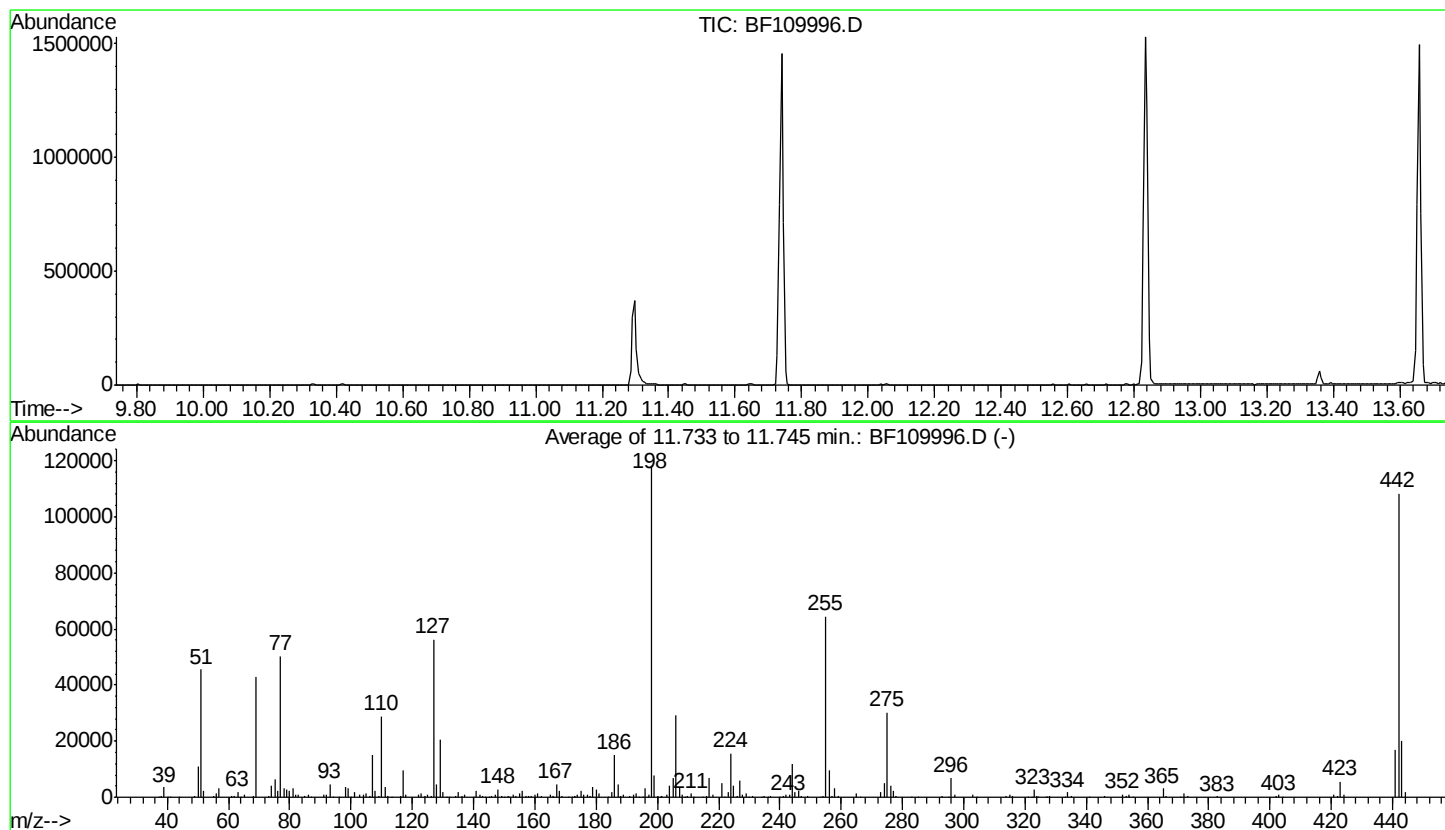

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	45501	PASS
68	69	0.00	2	1.1	466	PASS
69	198	0.00	100	36.2	42856	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	56285	PASS
197	198	0.00	2	0.7	807	PASS
198	198	100	100	100.0	118253	PASS
199	198	5	9	6.6	7819	PASS
275	198	10	60	25.6	30320	PASS
365	198	1	100	2.7	3183	PASS
441	198	0.01	100	14.1	16703	PASS
442	198	50	100	91.7	108386	PASS
443	442	15	24	18.6	20113	PASS