


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101918\
 Data File : BF110022.D
 Acq On : 20 Oct 2018 00:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 14:58:24 2018

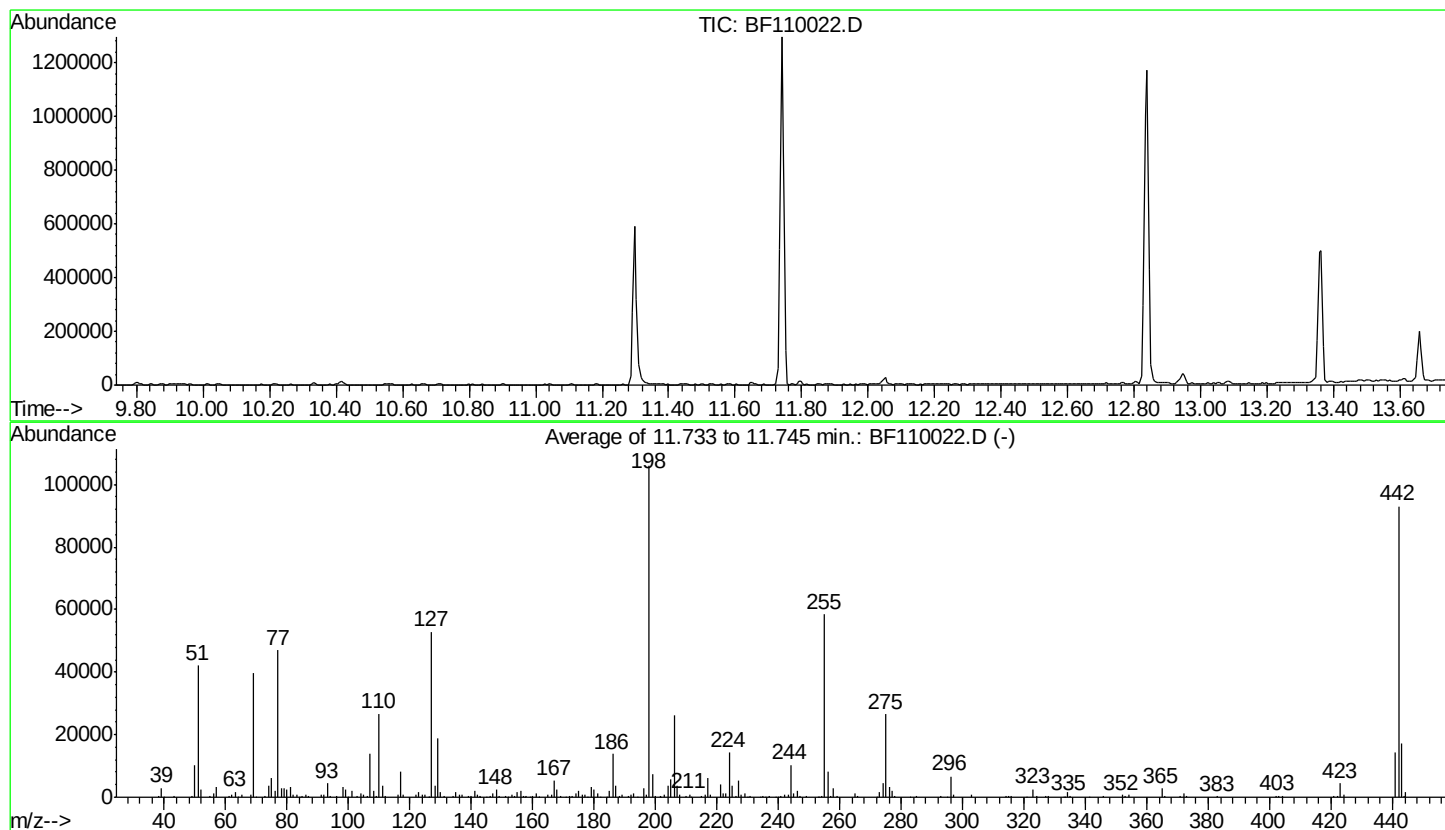

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	42013	PASS
68	69	0.00	2	1.6	630	PASS
69	198	0.00	100	37.6	39805	PASS
70	69	0.00	2	0.3	116	PASS
127	198	10	80	49.9	52850	PASS
197	198	0.00	2	0.9	950	PASS
198	198	100	100	100.0	106005	PASS
199	198	5	9	6.9	7280	PASS
275	198	10	60	25.1	26566	PASS
365	198	1	100	2.5	2693	PASS
441	198	0.01	100	13.5	14353	PASS
442	198	50	100	87.7	92960	PASS
443	442	15	24	18.3	17005	PASS