
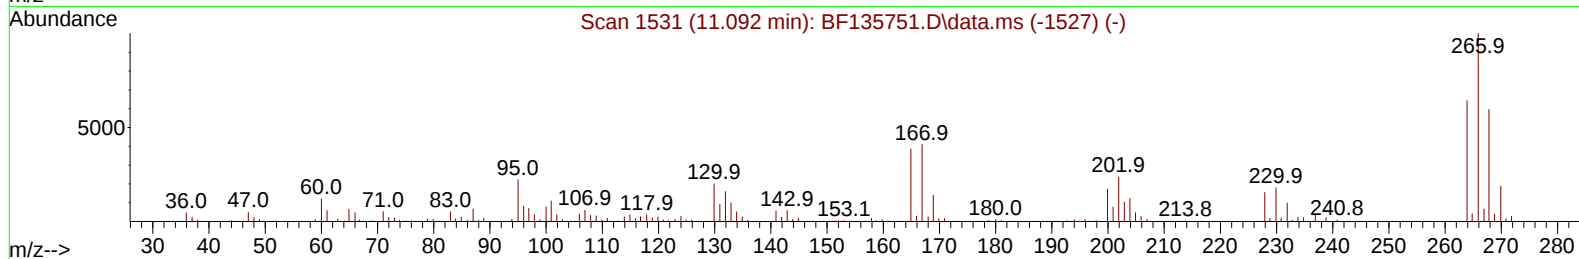
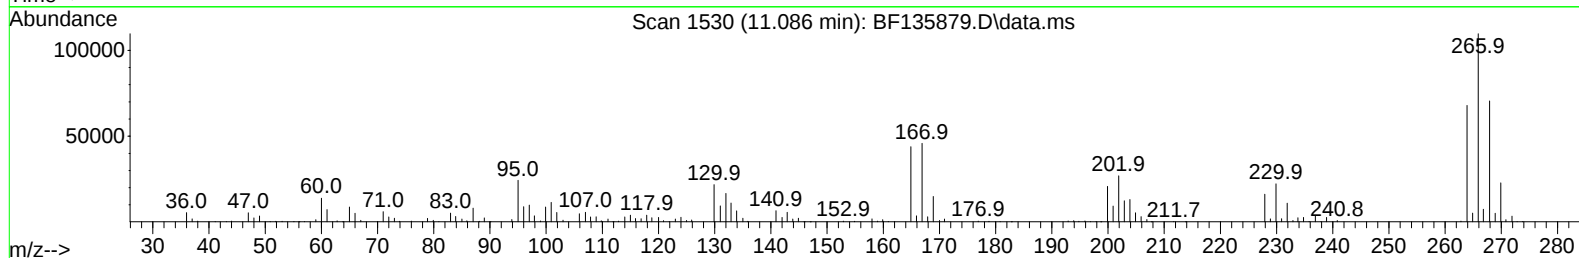


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101923\
Data File : BF135879.D
Acq On : 19 Oct 2023 11:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 12:41:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

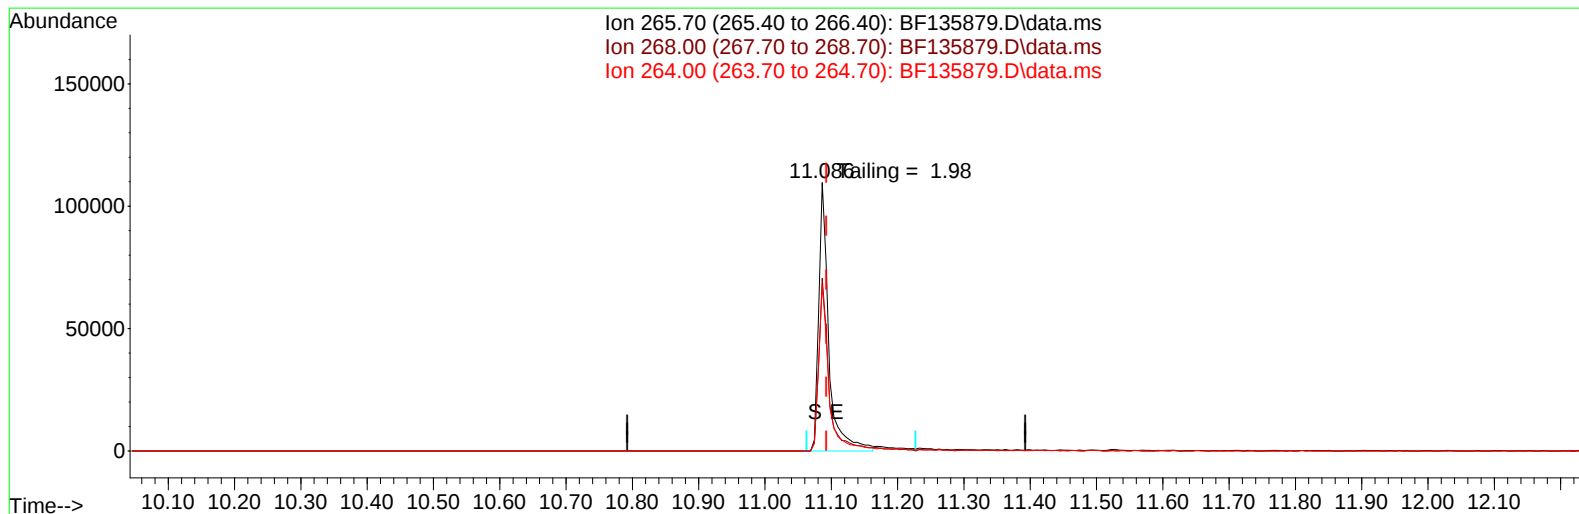

TIC: BF135879.D\data.ms

(70) Pentachlorophenol (C)




11.086min (-0.006) 71225.96 ng

response 122305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	64.33
264.00	64.30	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101923\
Data File : BF135879.D
Acq On : 19 Oct 2023 11:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 12:41:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

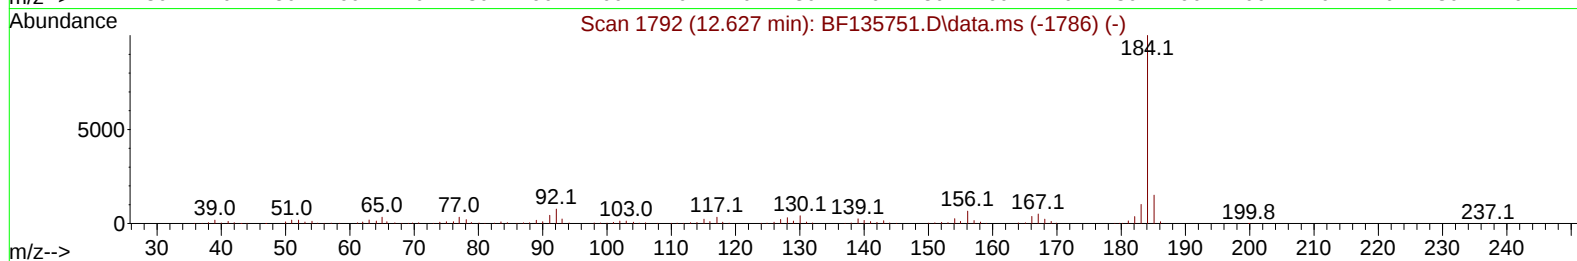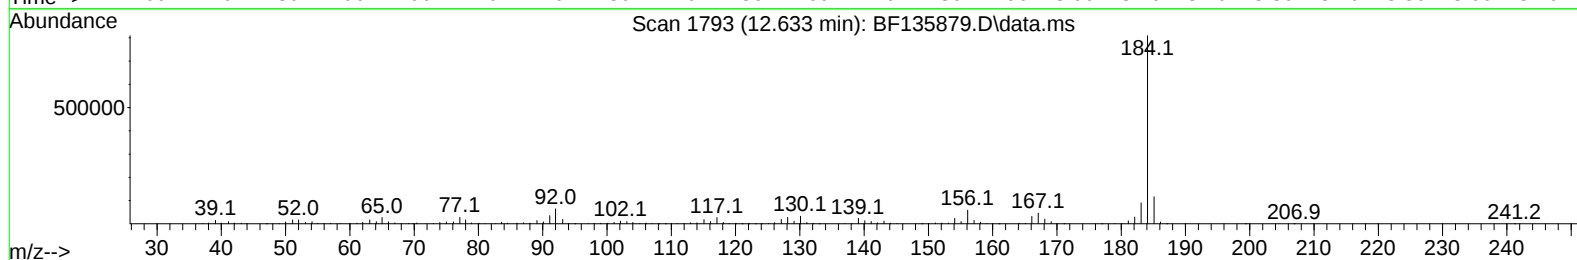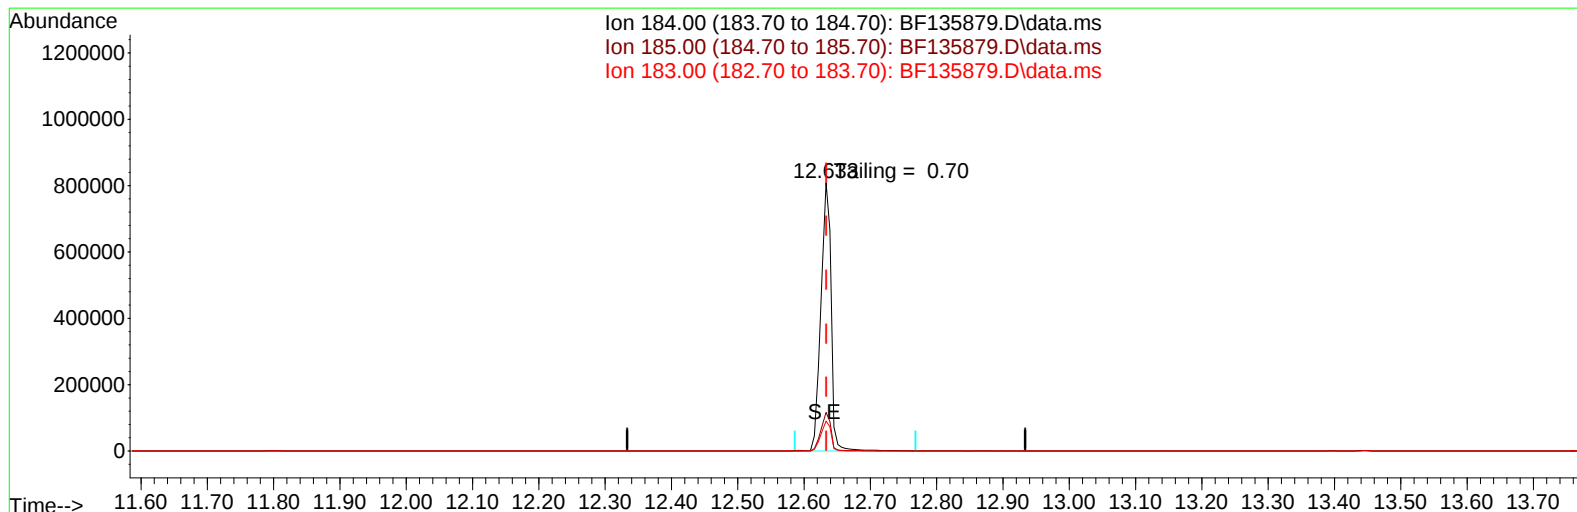

TIC: BF135879.D\data.ms

(77) Benzidine

12.633min (-0.000) 12217.23 ng

response 871487

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.38
183.00	10.20	11.19
0.00	0.00	0.00