
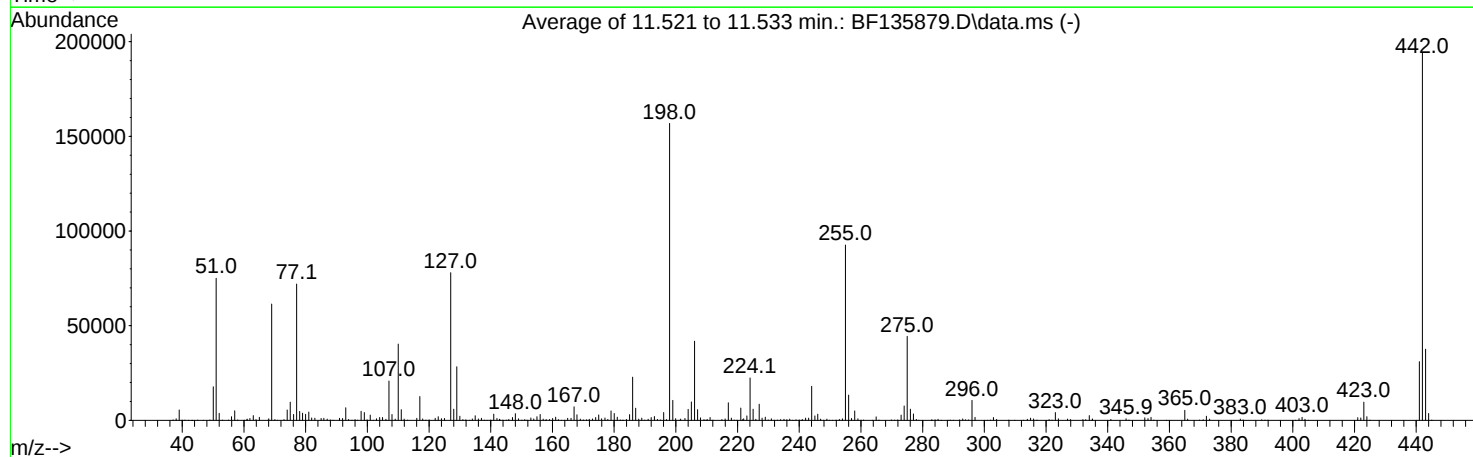


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101923\  
Data File : BF135879.D  
Acq On : 19 Oct 2023 11:24  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF101323.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Oct 17 01:22:00 2023

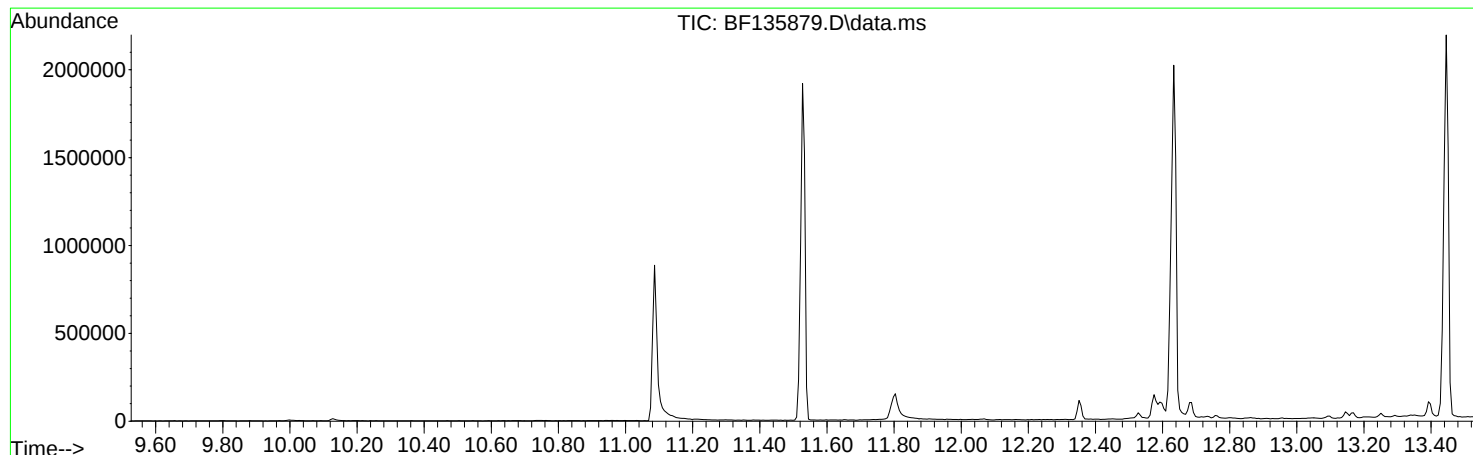




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 47.9         | 75059      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.4          | 834        | PASS                |
| 69             | 198             | 0.00            | 100             | 39.2         | 61411      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 396        | PASS                |
| 127            | 198             | 10              | 80              | 49.7         | 77976      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 405        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 156821     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 10537      | PASS                |
| 275            | 198             | 10              | 60              | 28.3         | 44360      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 5304       | PASS                |
| 441            | 198             | 0.01            | 100             | 19.8         | 30994      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 194291     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 37633      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101923\  
Data File : BF135879.D  
Acq On : 19 Oct 2023 11:24  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Oct 19 12:41:45 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF101323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 17 01:22:00 2023  
Response via : Initial Calibration

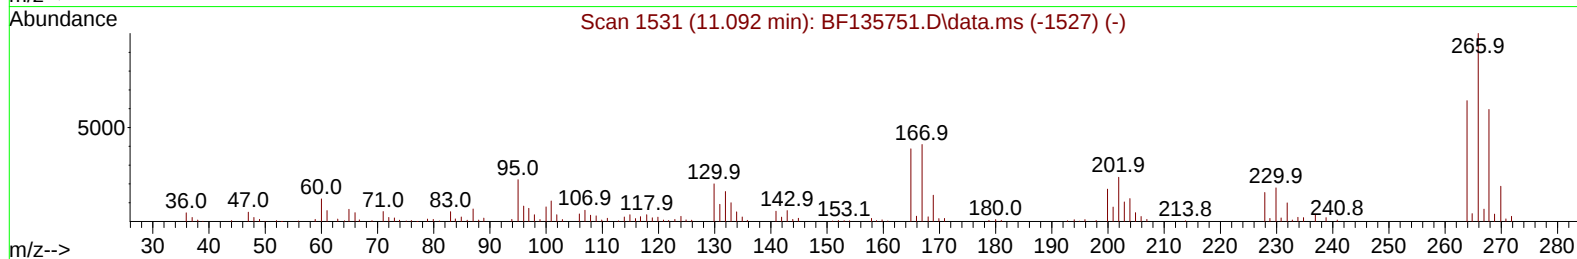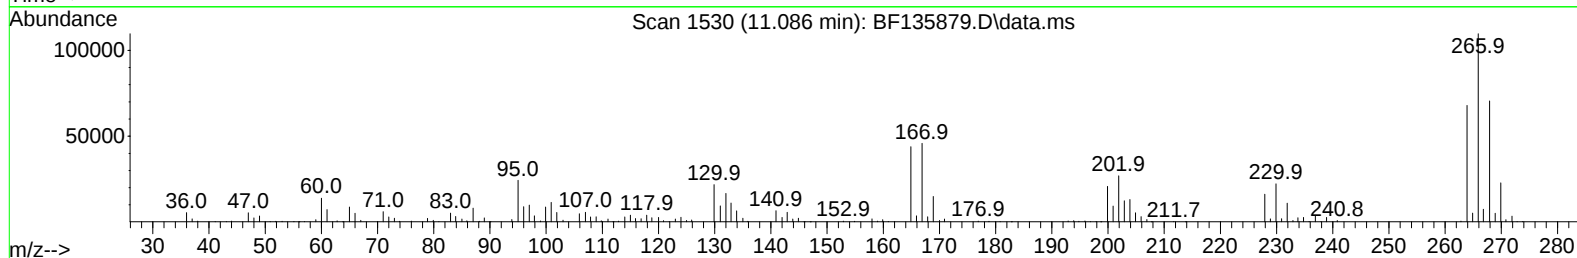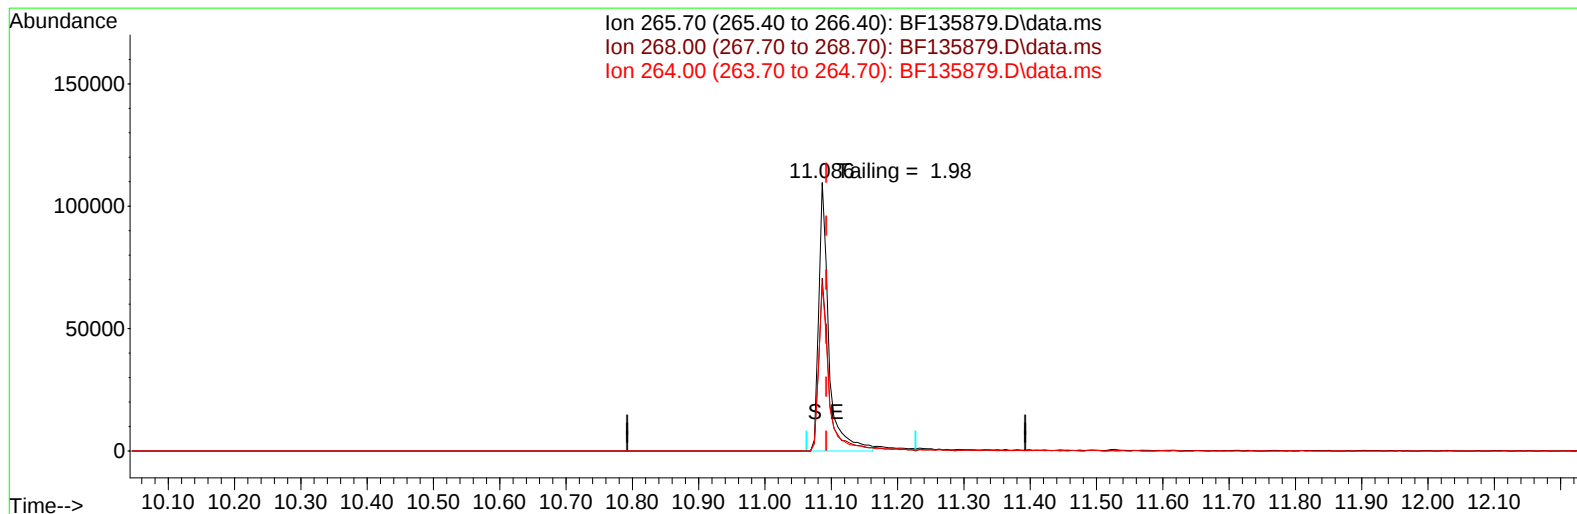

TIC: BF135879.D\data.ms

**(70) Pentachlorophenol (C)**

11.086min (-0.006) 71225.96 ng




response 122305

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 59.60  | 64.33  |
| 264.00 | 64.30  | 61.90  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF101923\  
 Data File : BF135879.D  
 Acq On : 19 Oct 2023 11:24  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Oct 19 12:41:45 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF101323.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Oct 17 01:22:00 2023  
 Response via : Initial Calibration

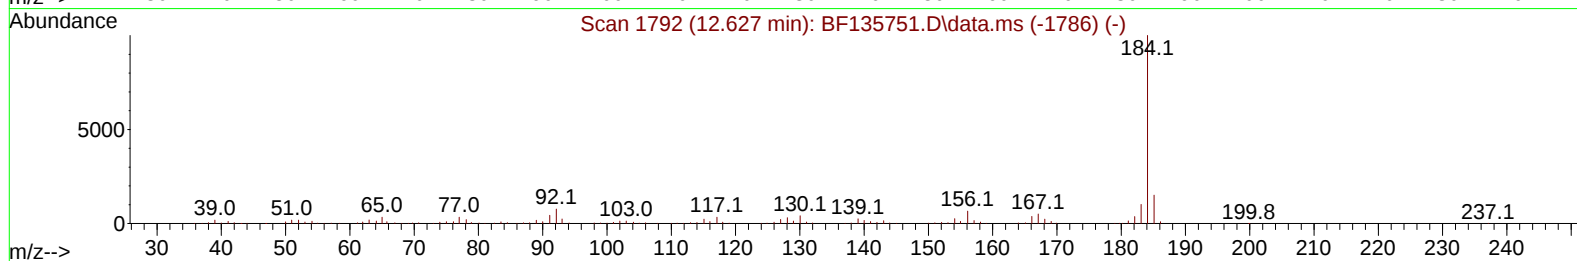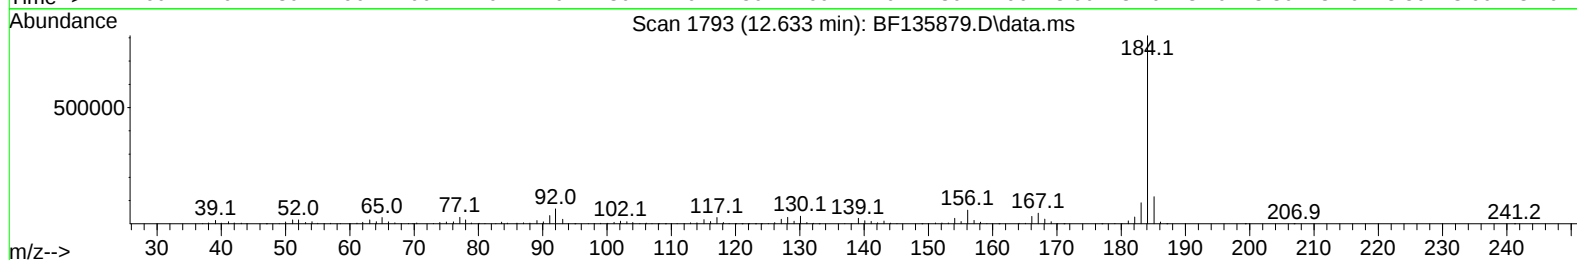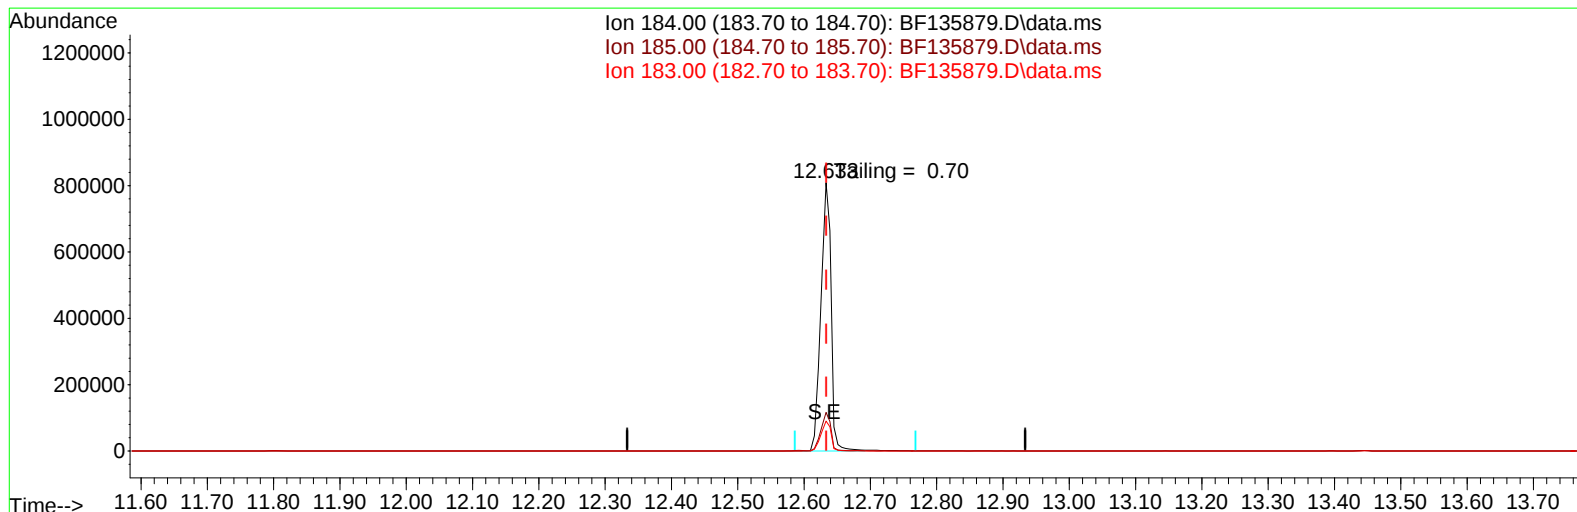

TIC: BF135879.D\data.ms

**(77) Benzidine**

12.633min (-0.000) 12217.23 ng

response 871487

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.38  |
| 183.00 | 10.20  | 11.19  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/19/2023    | BNA_F            | <u>BF135879.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 414507           | 13.445             |
| DDD           | 12631            | 13.145             |
| DDE           | 633              | 12.804             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13264         | 427771           | 3.10               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP