
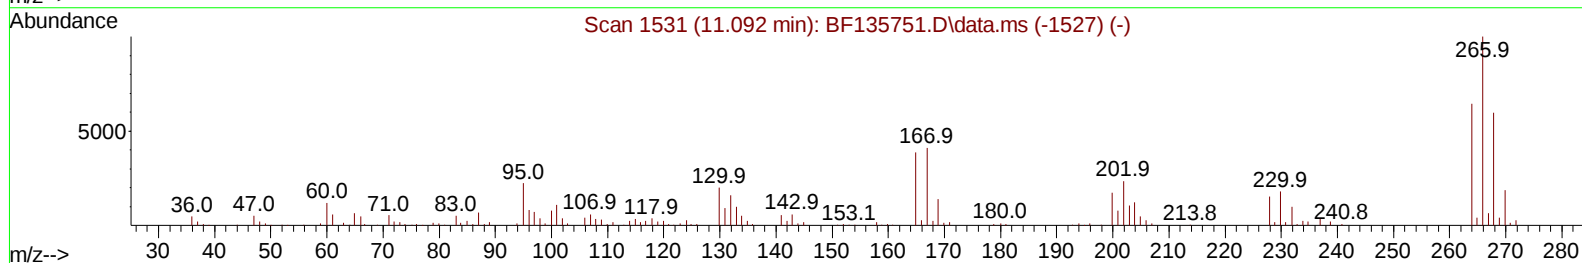
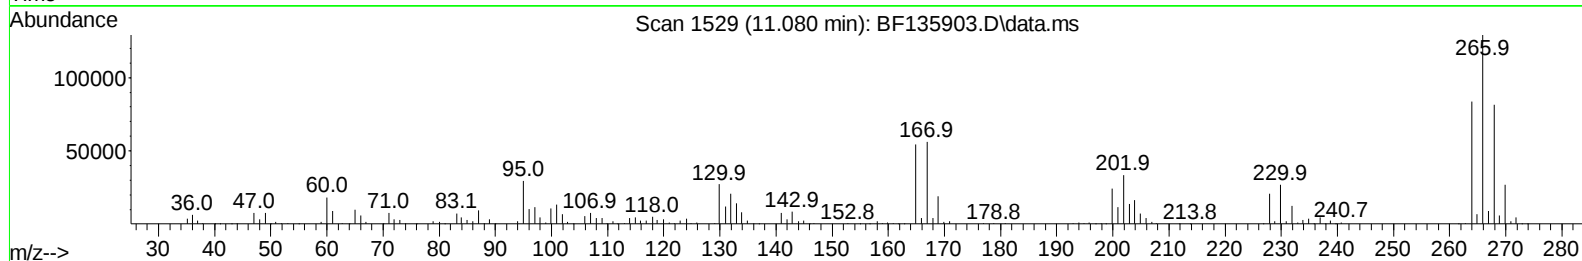


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102023\
Data File : BF135903.D
Acq On : 20 Oct 2023 12:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 14:17:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

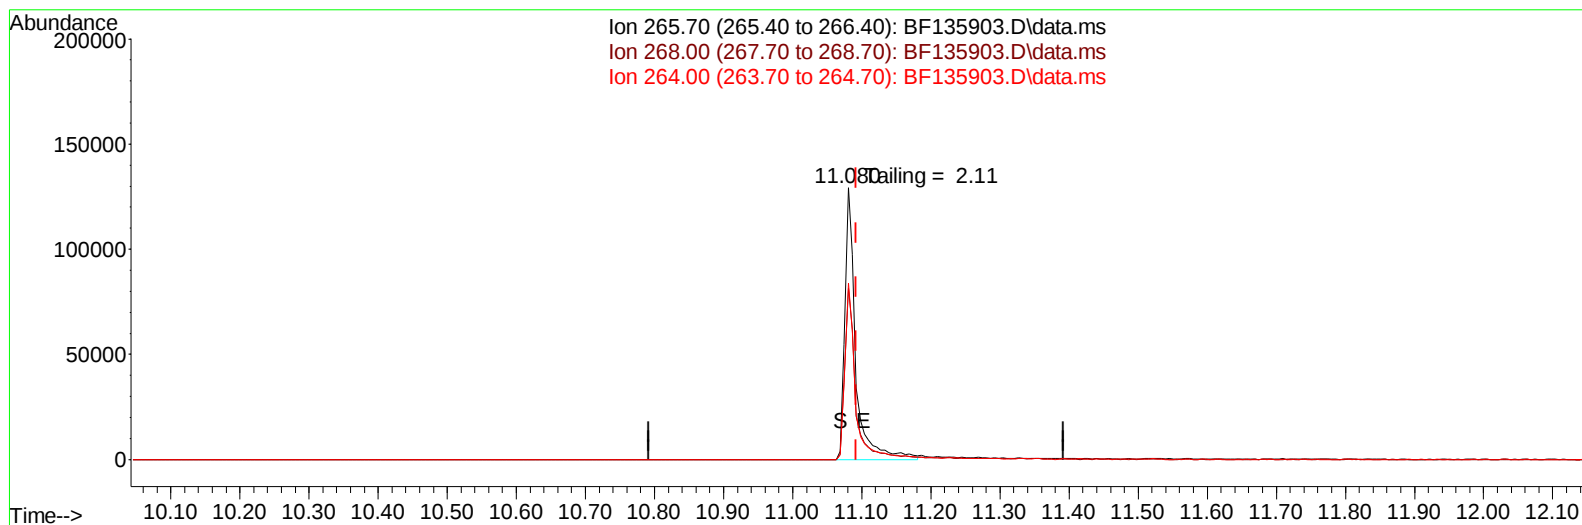

TIC: BF135903.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.012) 51269.40 ng

response 136395

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	63.02
264.00	64.30	64.86
0.00	0.00	0.00

Abundance

1200000

1000000

800000

600000

400000

200000

0

Time--> 11.60 11.70 11.80 11.90 12.00 12.10 12.20 12.30 12.40 12.50 12.60 12.70 12.80 12.90 13.00 13.10 13.20 13.30 13.40 13.50 13.60 13.70

Ion 184.00 (183.70 to 184.70): BF135903.D\data.ms



Ion 185.00 (184.70 to 185.70): BF135903.D\data.ms

Ion 183.00 (182.70 to 183.70): BF135903.D\data.ms

12.62

Tailing = 0.72

SE

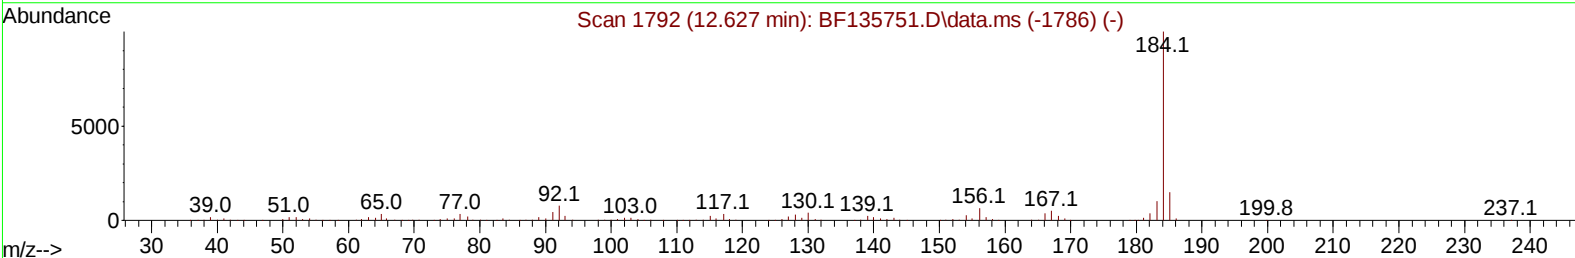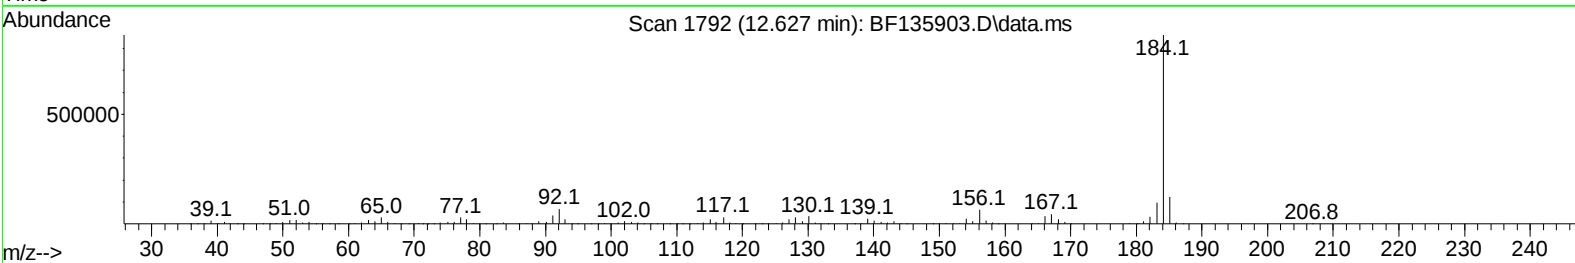

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.16
183.00	10.20	11.15
0.00	0.00	0.00