
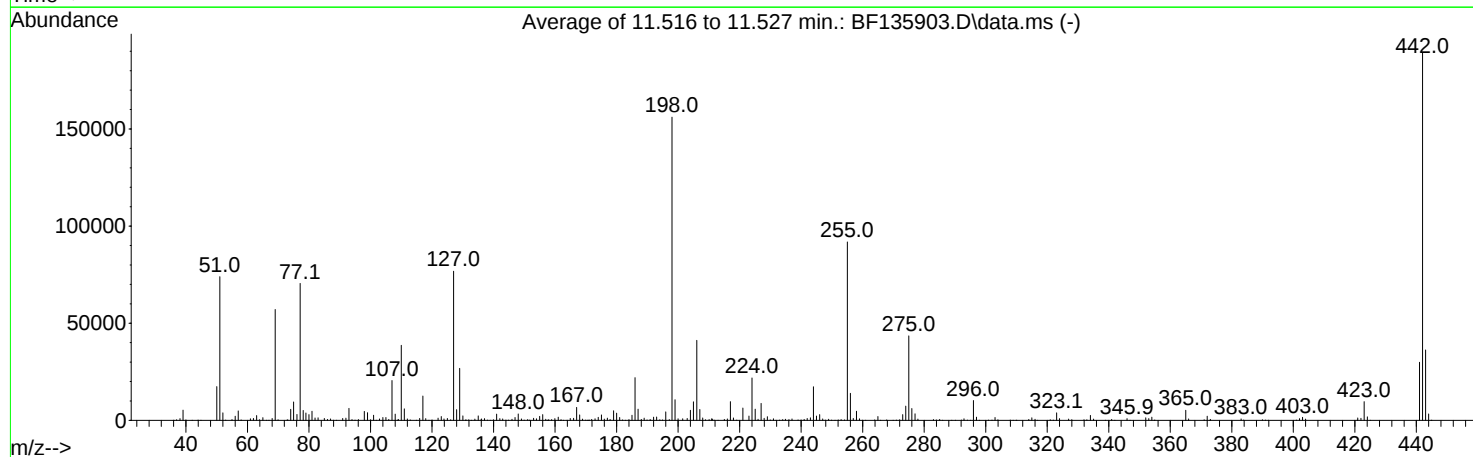


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102023\
Data File : BF135903.D
Acq On : 20 Oct 2023 12:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 17 01:22:00 2023

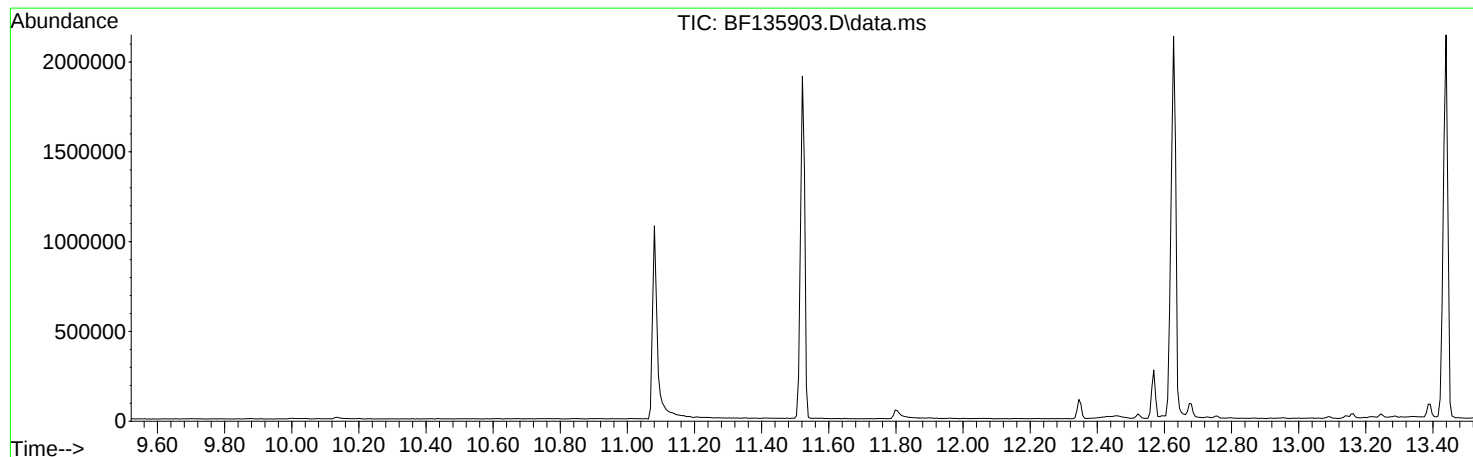




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	73930	PASS
68	69	0.00	2	1.8	1018	PASS
69	198	0.00	100	36.6	57093	PASS
70	69	0.00	2	0.6	334	PASS
127	198	10	80	49.2	76741	PASS
197	198	0.00	2	0.3	441	PASS
198	198	100	100	100.0	156107	PASS
199	198	5	9	6.8	10613	PASS
275	198	10	60	27.9	43485	PASS
365	198	1	100	3.3	5214	PASS
441	198	0.01	100	19.1	29889	PASS
442	442	50	100	100.0	189368	PASS
443	442	15	24	19.1	36254	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102023\
Data File : BF135903.D
Acq On : 20 Oct 2023 12:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 20 14:17:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

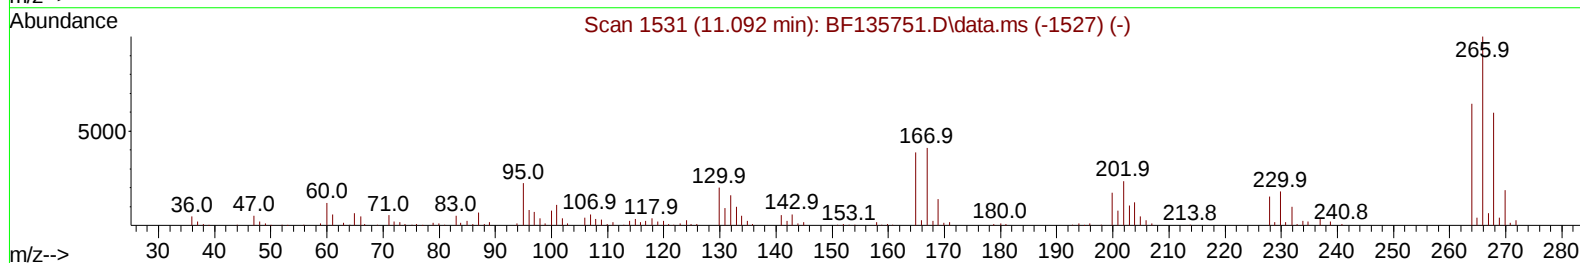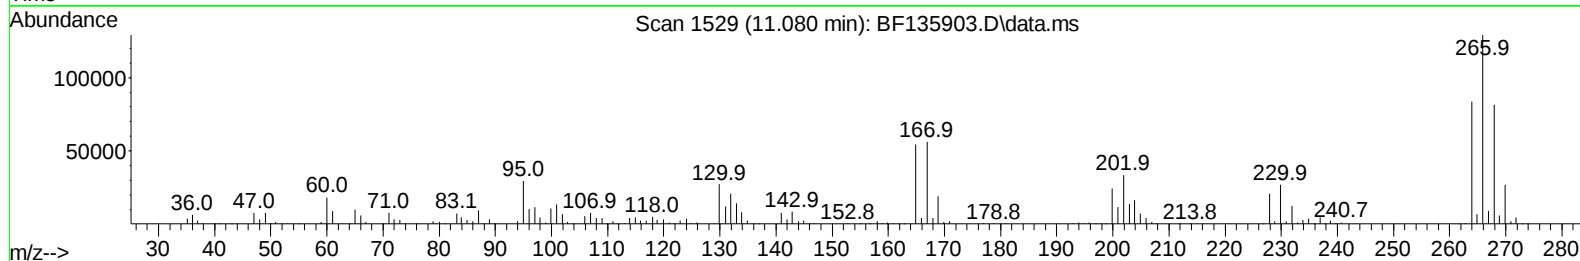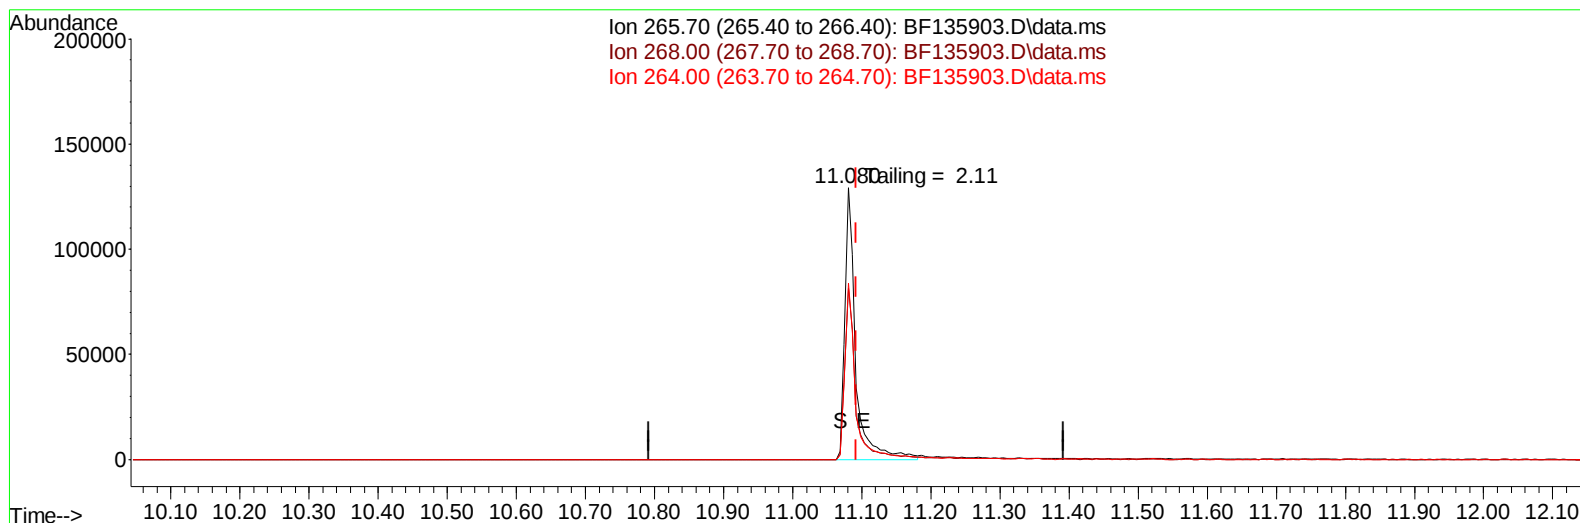

TIC: BF135903.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.012) 51269.40 ng

response 136395

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	63.02
264.00	64.30	64.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2023	BNA_F	<u>BF135903.D</u>
Compound Name	Response	Retention Time
DDT	401037	13.439
DDD	8348	13.162
DDE	600	12.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8948	409985	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP