
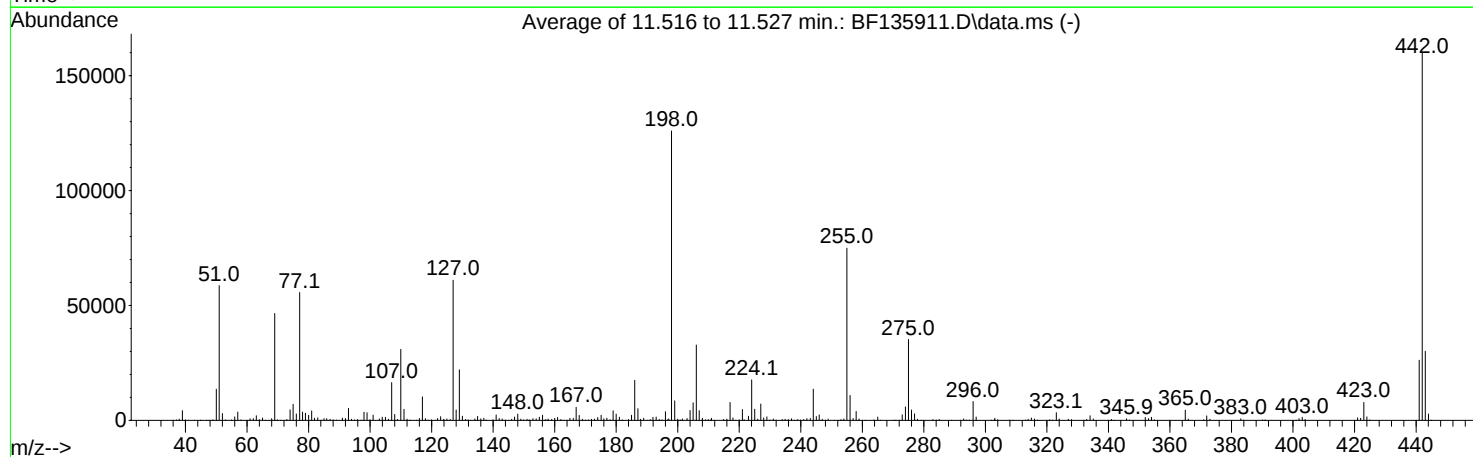


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102023\
Data File : BF135911.D
Acq On : 20 Oct 2023 16:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 17 01:22:00 2023

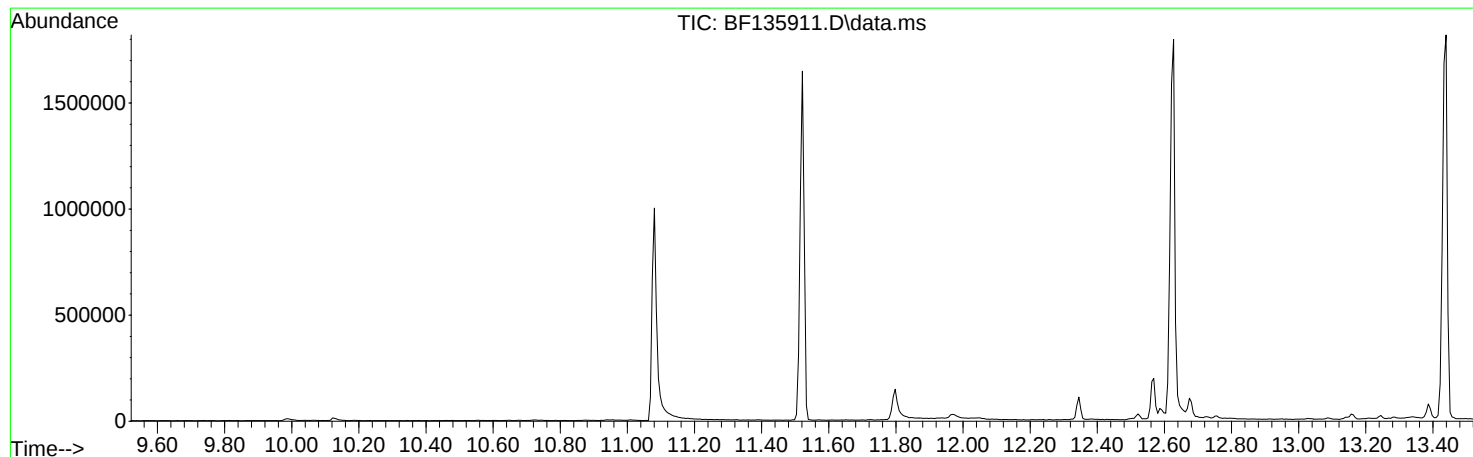




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	58603	PASS
68	69	0.00	2	1.6	765	PASS
69	198	0.00	100	37.0	46555	PASS
70	69	0.00	2	0.5	239	PASS
127	198	10	80	48.4	61000	PASS
197	198	0.00	2	0.5	643	PASS
198	198	100	100	100.0	125944	PASS
199	198	5	9	6.7	8500	PASS
275	198	10	60	28.0	35221	PASS
365	198	1	100	3.6	4483	PASS
441	198	0.01	100	20.8	26195	PASS
442	442	50	100	100.0	160091	PASS
443	442	15	24	18.8	30096	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102023\
Data File : BF135911.D
Acq On : 20 Oct 2023 16:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 20 17:36:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

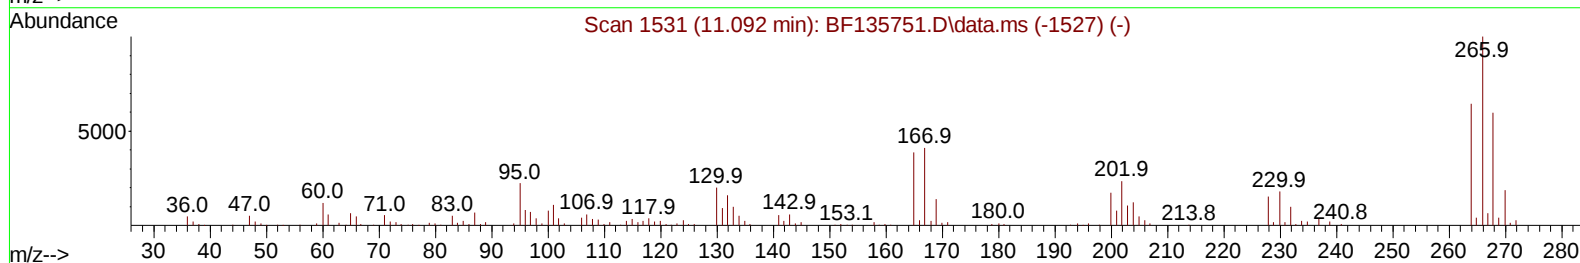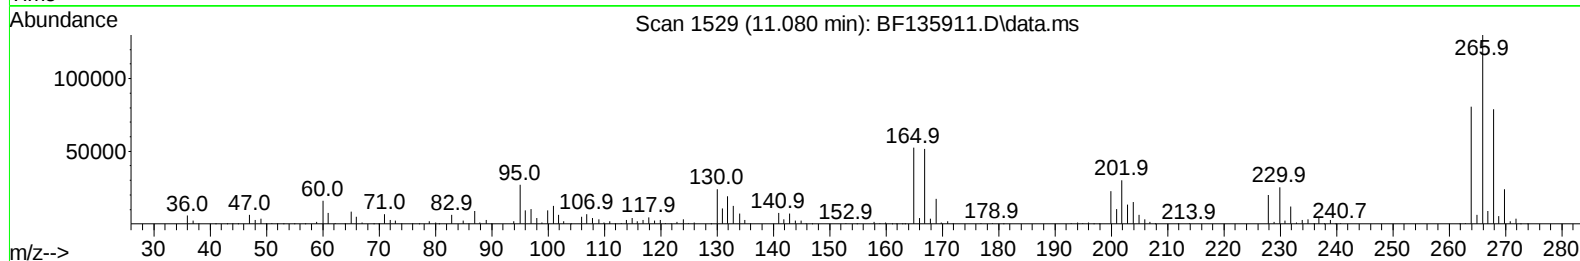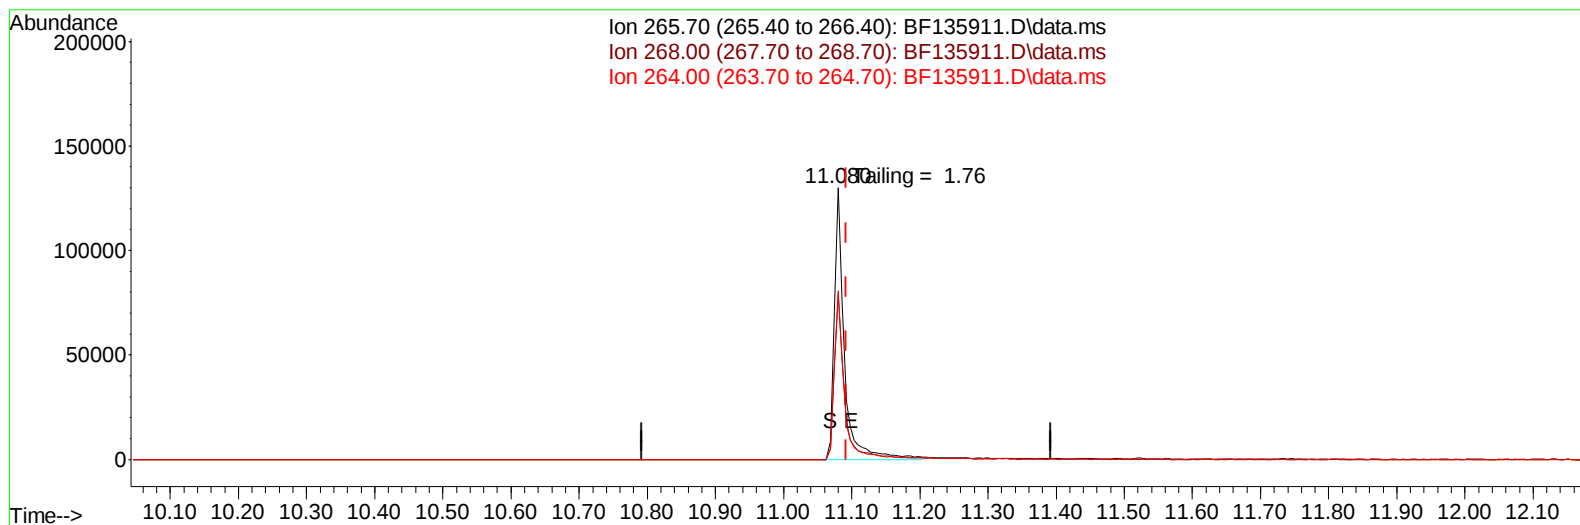

TIC: BF135911.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.012) 65802.31 ng




response 133150

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.60	60.83
264.00	64.30	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102023\
Data File : BF135911.D
Acq On : 20 Oct 2023 16:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 20 17:36:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 01:22:00 2023
Response via : Initial Calibration

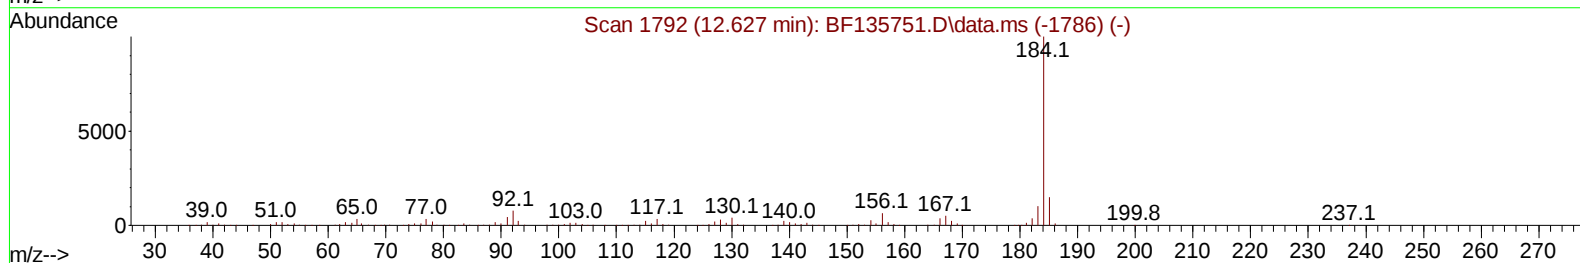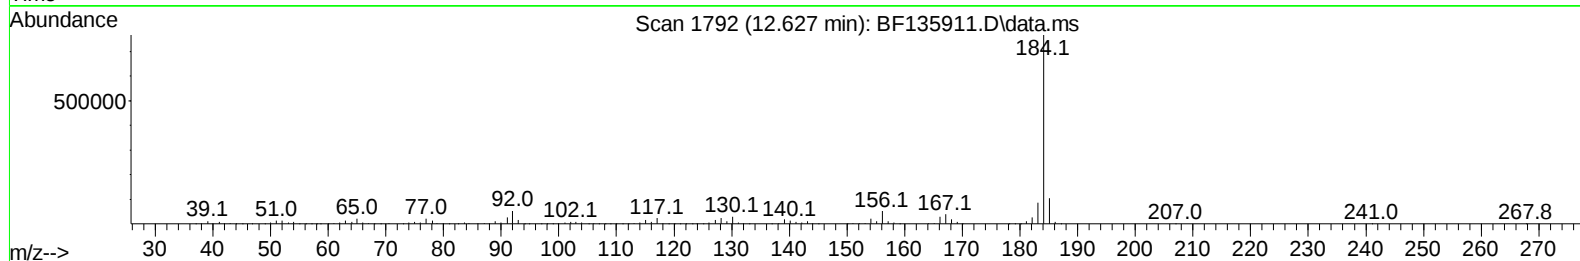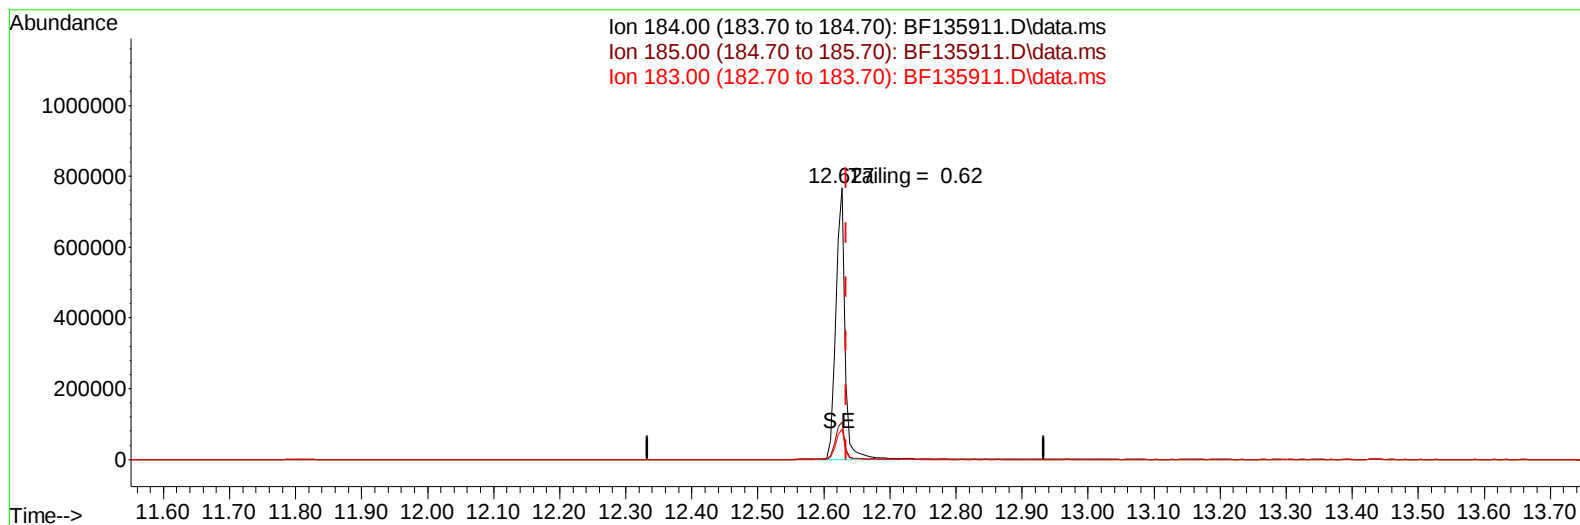

TIC: BF135911.D\data.ms

(77) Benzidine

12.627min (-0.006) 0.00 ng

response 749315

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.76
183.00	10.20	11.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2023	BNA_F	<u>BF135911.D</u>
Compound Name	Response	Retention Time
DDT	356424	13.439
DDD	6788	13.162
DDE	526	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7314	363738	2.01

Instrument :
BNA_F
ClientSampleId :
DFTPP