


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102025\
Data File : BF143996.D
Acq On : 20 Oct 2025 12:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

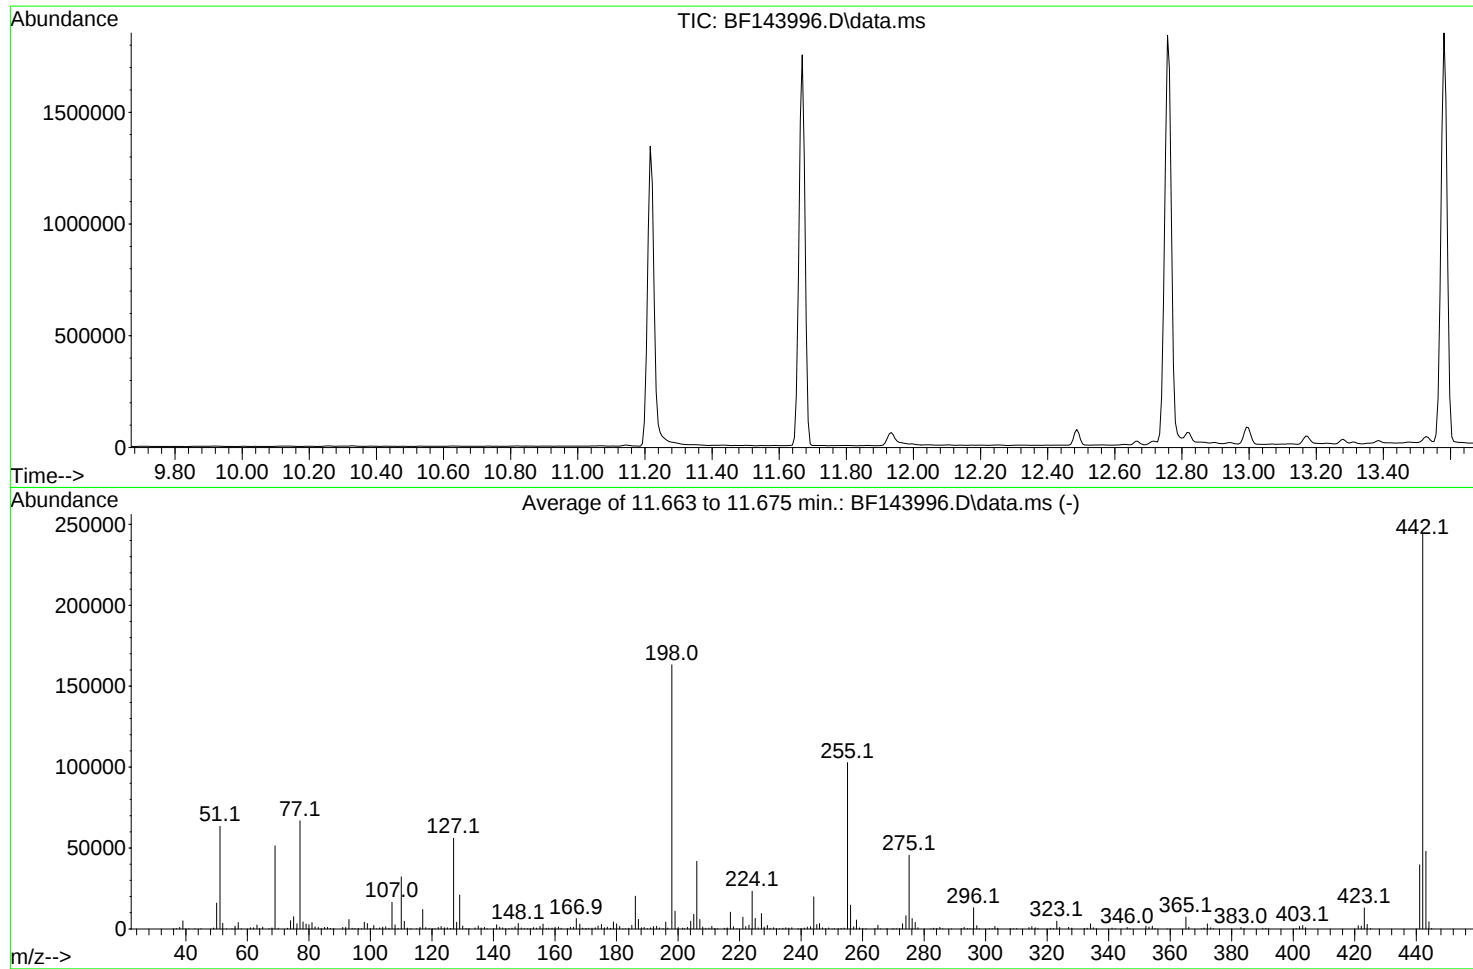




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.3	676	PASS
69	69	100	100	100.0	51413	PASS
70	69	0.00	2	0.8	426	PASS
197	198	0.00	2	0.4	599	PASS
198	198	100	100	100.0	163200	PASS
199	198	5	9	6.8	11025	PASS
365	198	1	100	4.5	7333	PASS
441	443	0.01	150	82.5	39595	PASS
442	442	100	100	100.0	243989	PASS
443	442	15	24	19.7	47997	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102025\
Data File : BF143996.D
Acq On : 20 Oct 2025 12:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 20 17:03:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

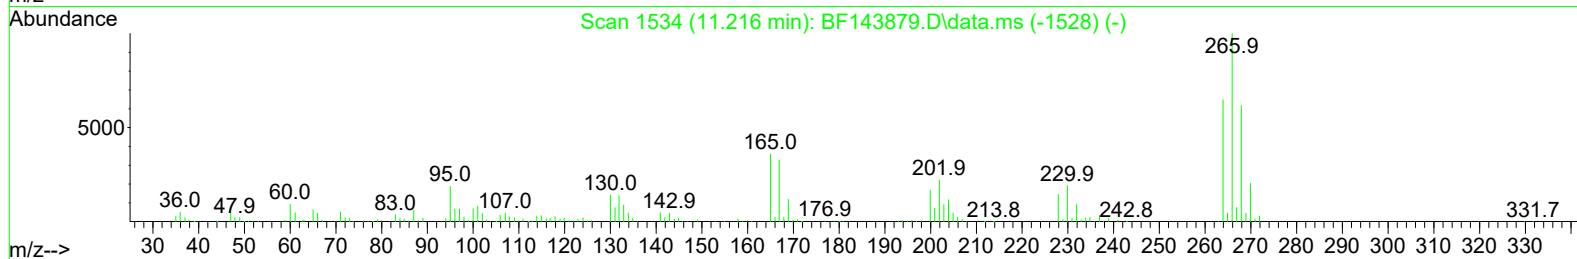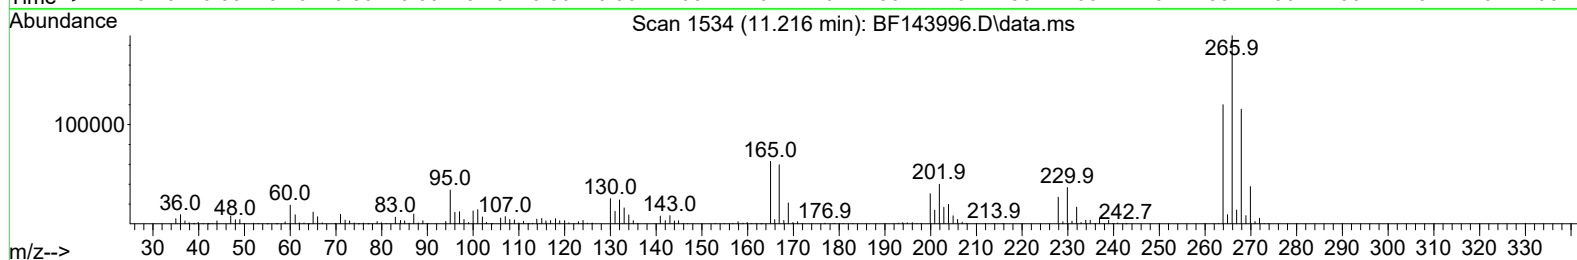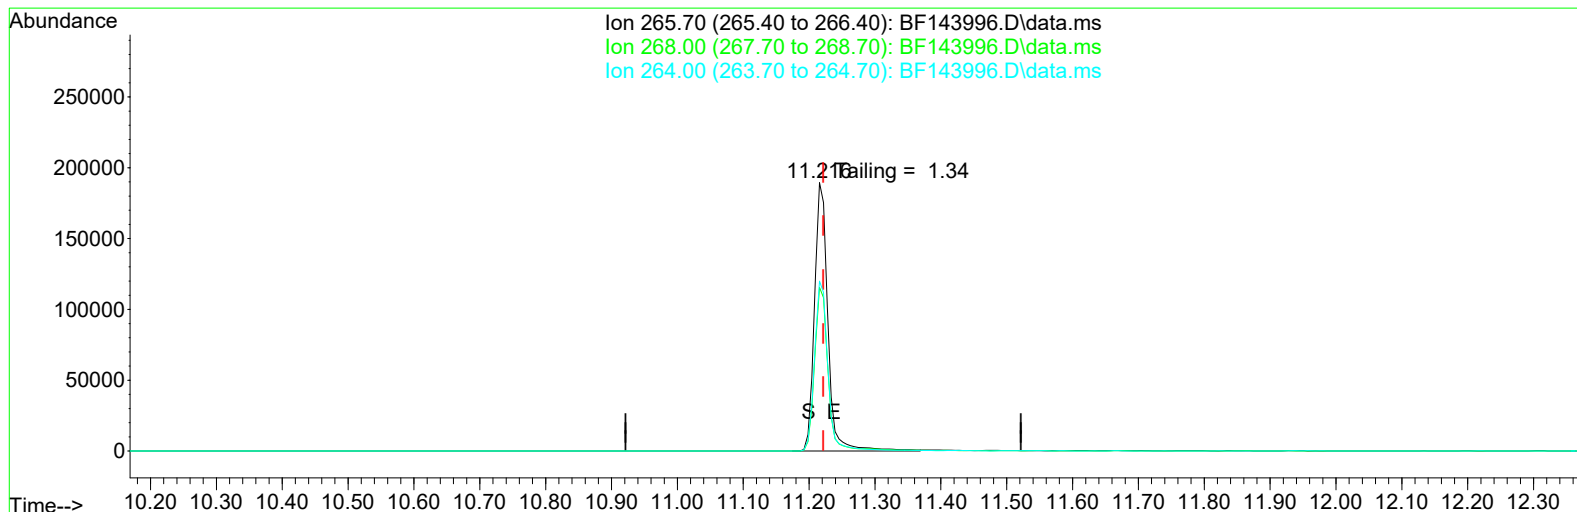

TIC: BF143996.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 91778.74 ng




response 268416

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.01
264.00	64.70	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102025\
Data File : BF143996.D
Acq On : 20 Oct 2025 12:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 20 17:03:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

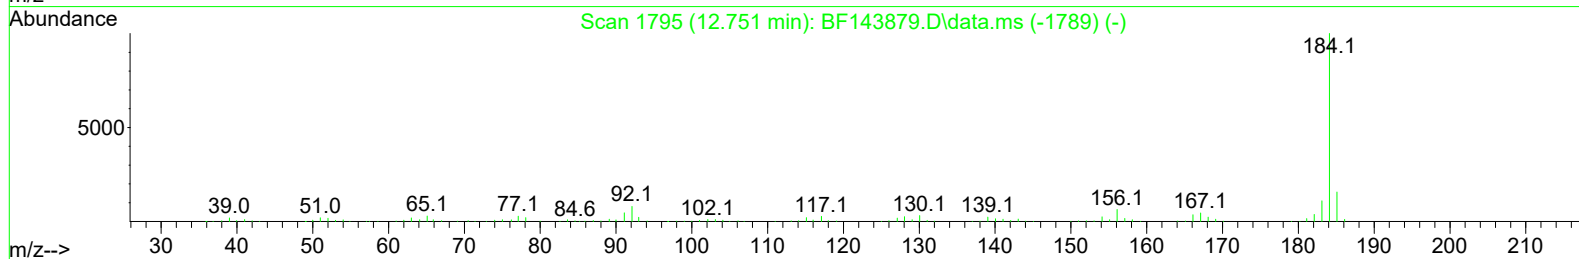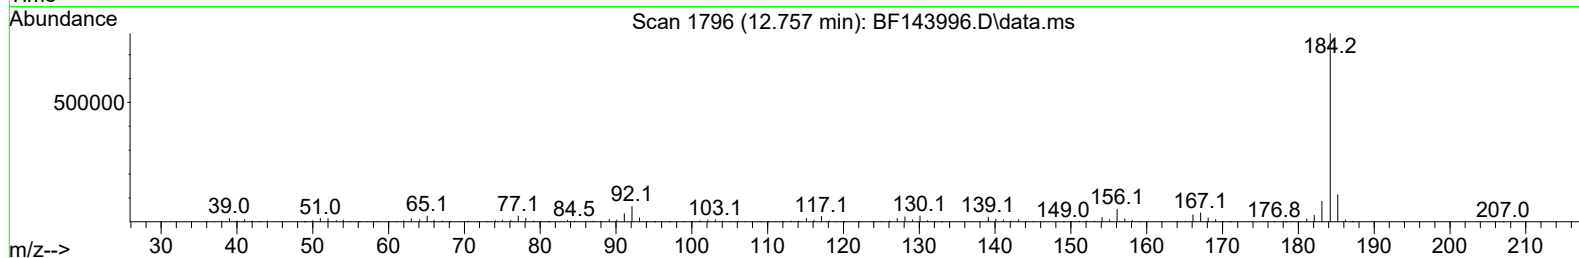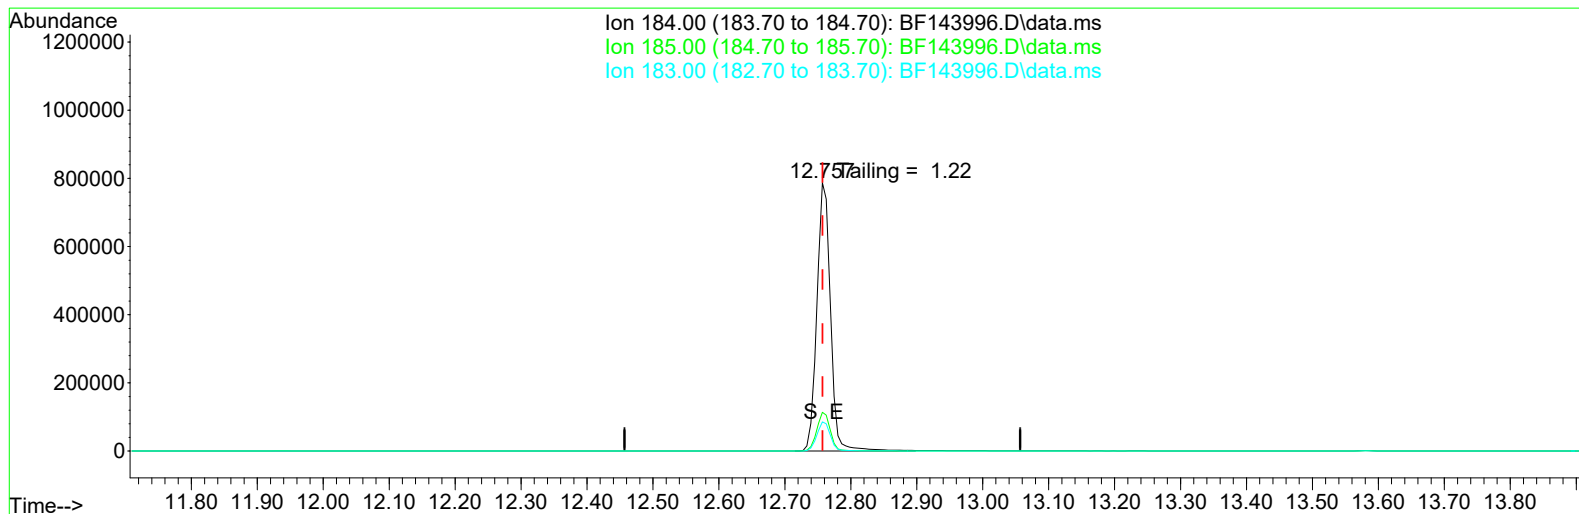

TIC: BF143996.D\data.ms

(77) Benzidine

12.757min (-0.000) 58721.78 ng

response 1131625

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.43
183.00	11.00	10.88
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
10/20/2025	BNA_F	<u>BF143996.D</u>
Compound Name	Response	Retention Time
DDT	497907	13.58
DDD	9211	13.28
DDE	3438	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12649	510556	2.48