
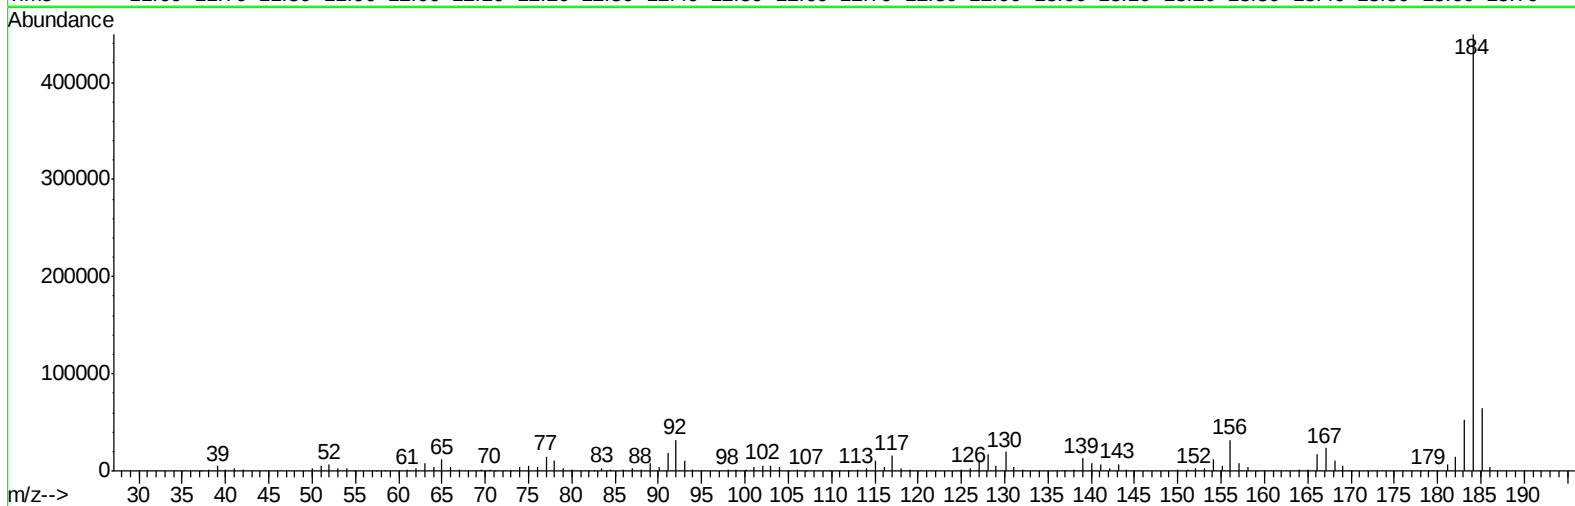


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102119\
Data File : BF117448.D
Acq On : 21 Oct 2019 14:58
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 05:34:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

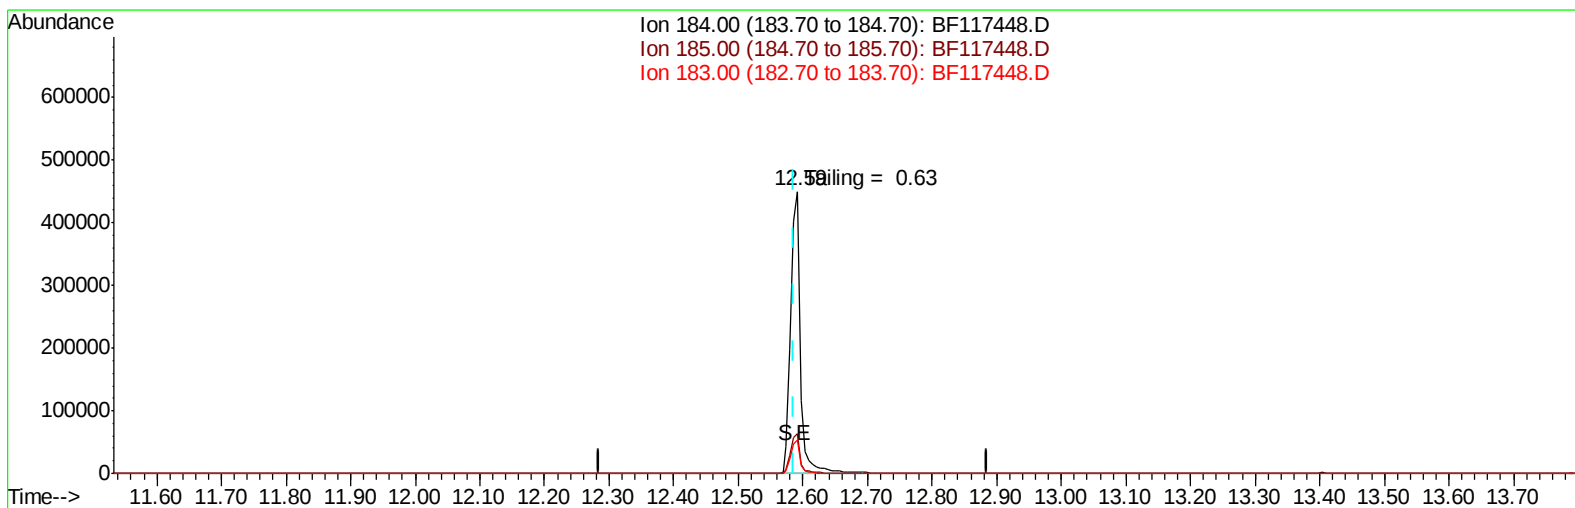

TIC: BF117448.D

(77) Benzidine

12.592min (+0.006) 0.00ng

response 475291

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.31
183.00	12.00	11.79
0.00	0.00	0.00