
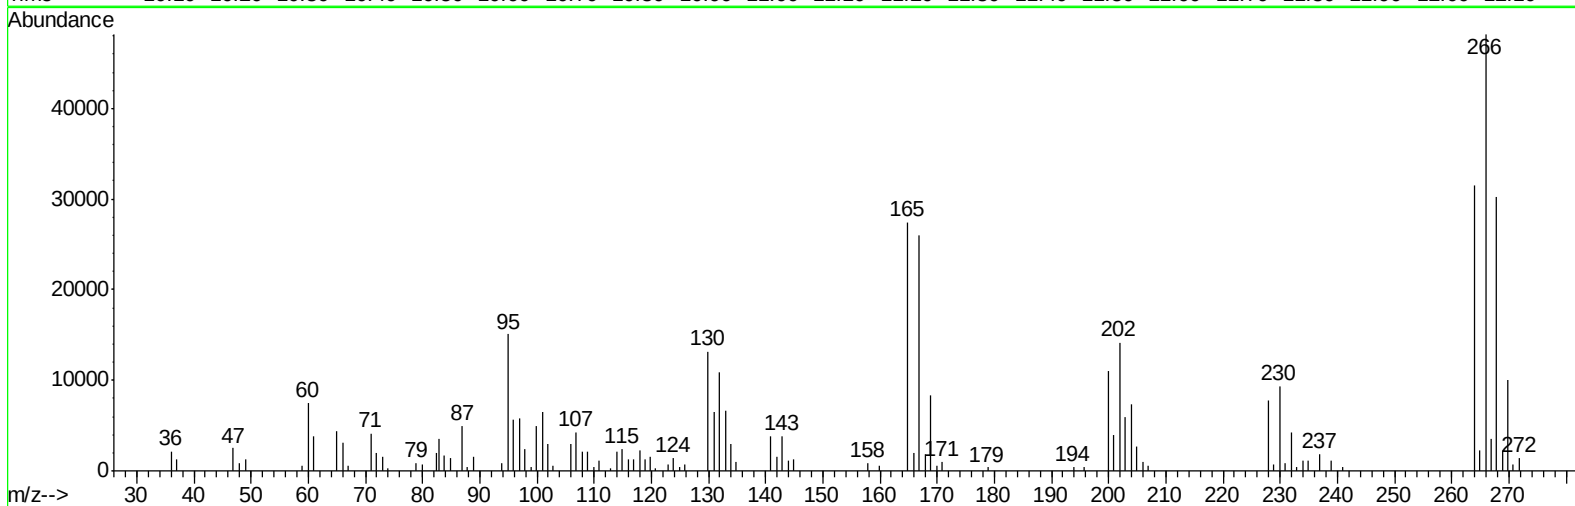


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102119\
Data File : BF117448.D
Acq On : 21 Oct 2019 14:58
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 05:34:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

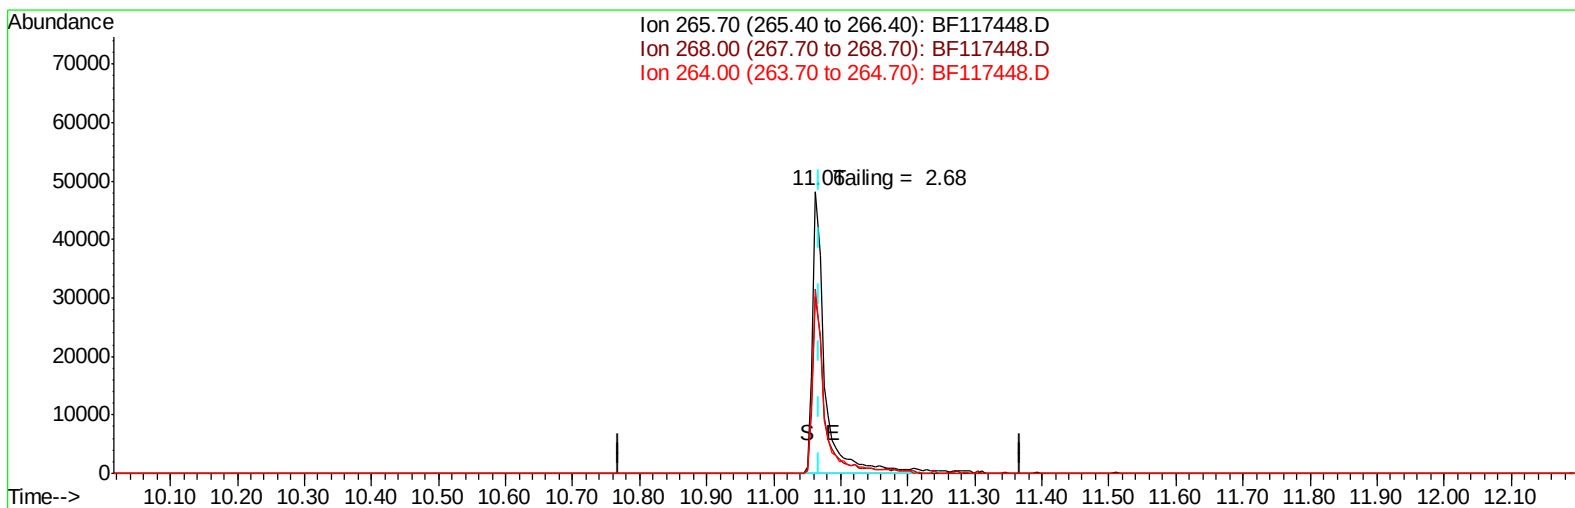

TIC: BF117448.D

(70) Pentachlorophenol (C)



11.063min (-0.006) 62815.56ng

response 57998

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.76
264.00	64.30	65.39
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102119\
 Data File : BF117448.D
 Acq On : 21 Oct 2019 14:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 05:34:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 18:53:31 2019
 Response via : Initial Calibration

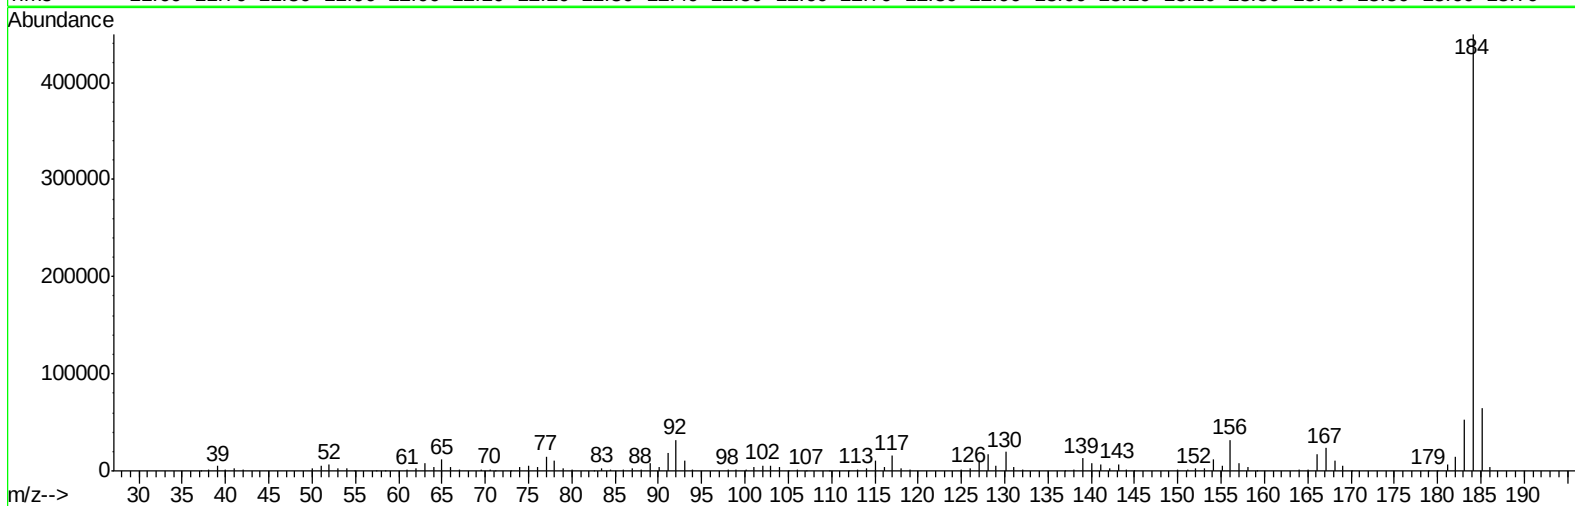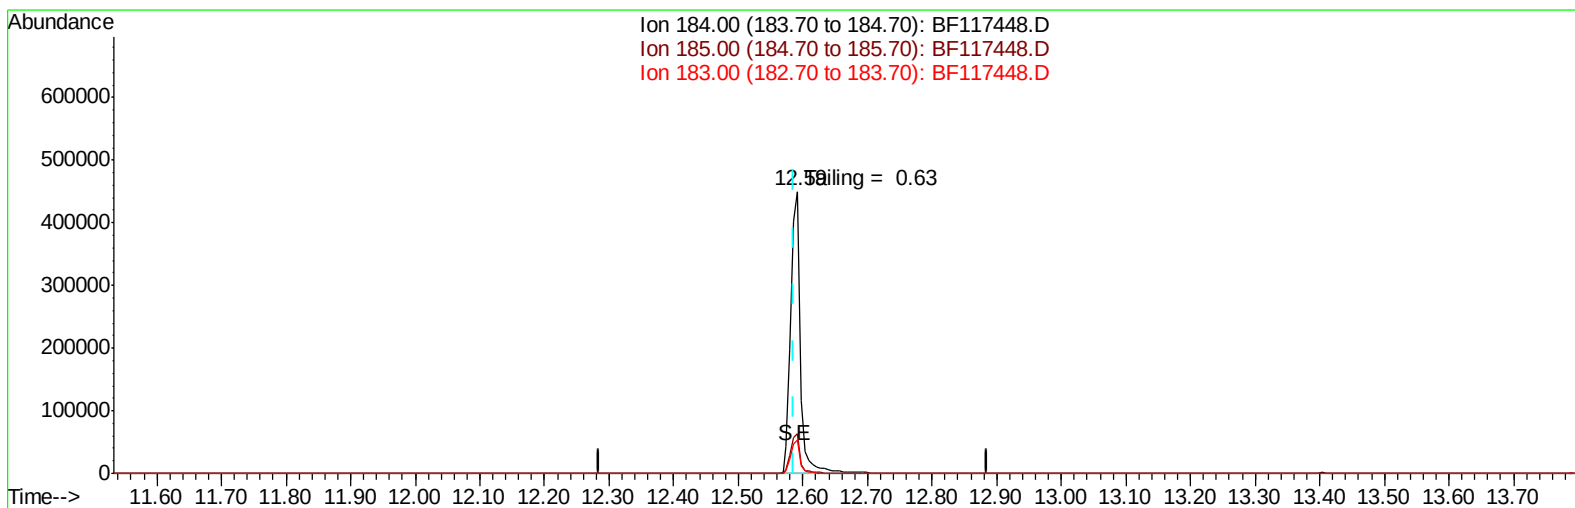

TIC: BF117448.D

(77) Benzidine

12.592min (+0.006) 0.00ng

response 475291

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.31
183.00	12.00	11.79
0.00	0.00	0.00