


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102119\
 Data File : BF117448.D
 Acq On : 21 Oct 2019 14:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

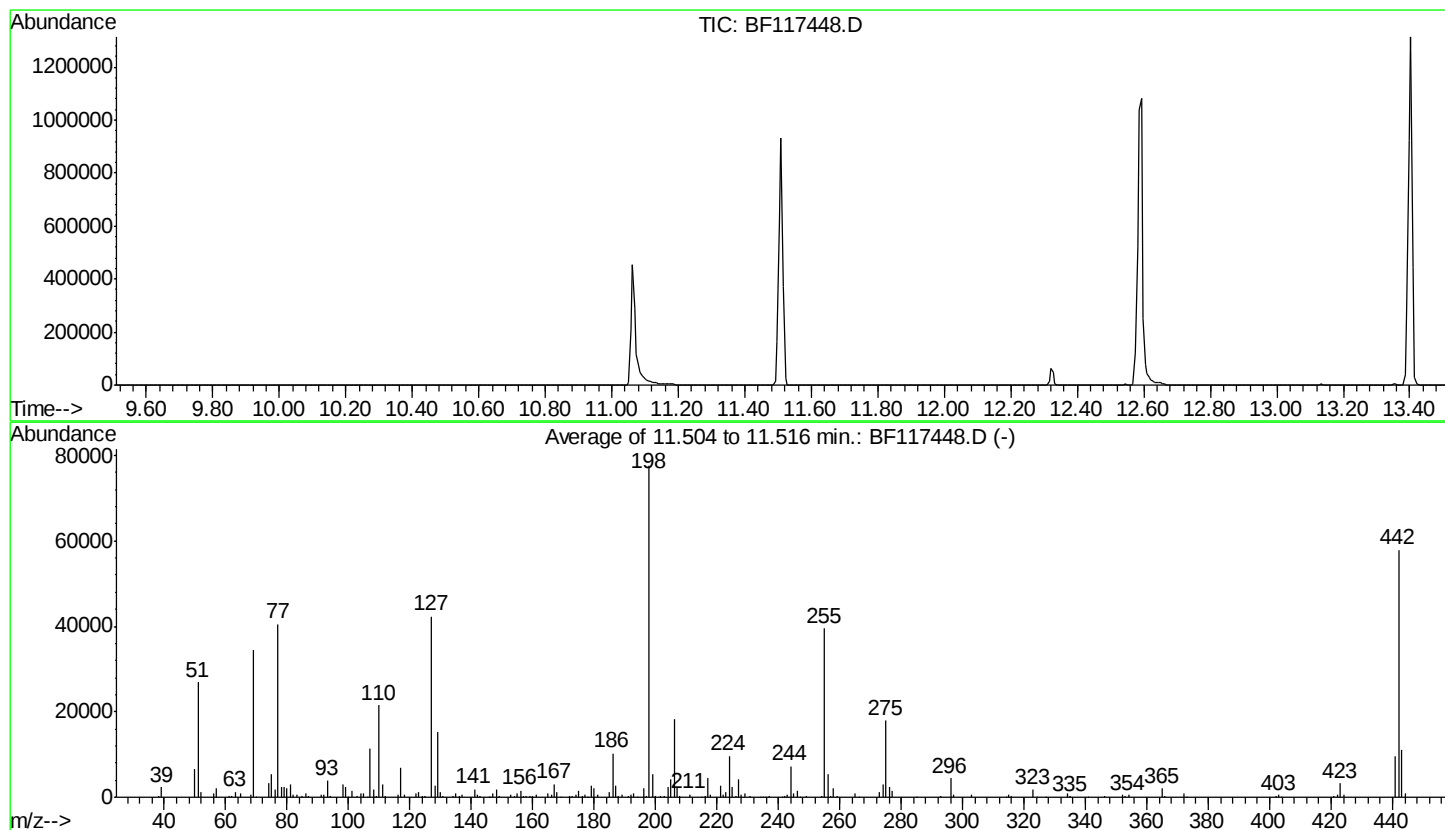

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	26935	PASS
68	69	0.00	2	1.6	548	PASS
69	198	0.00	100	44.2	34315	PASS
70	69	0.00	2	0.3	106	PASS
127	198	10	80	54.5	42264	PASS
197	198	0.00	2	0.2	162	PASS
198	198	100	100	100.0	77600	PASS
199	198	5	9	7.0	5430	PASS
275	198	10	60	23.2	17971	PASS
365	198	1	100	2.7	2080	PASS
441	198	0.01	100	12.3	9583	PASS
442	198	50	100	74.6	57858	PASS
443	442	15	24	19.3	11165	PASS