
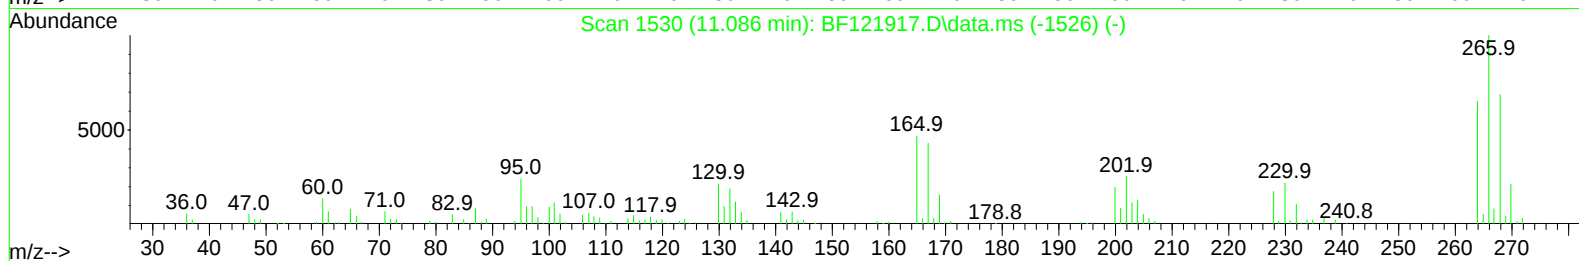
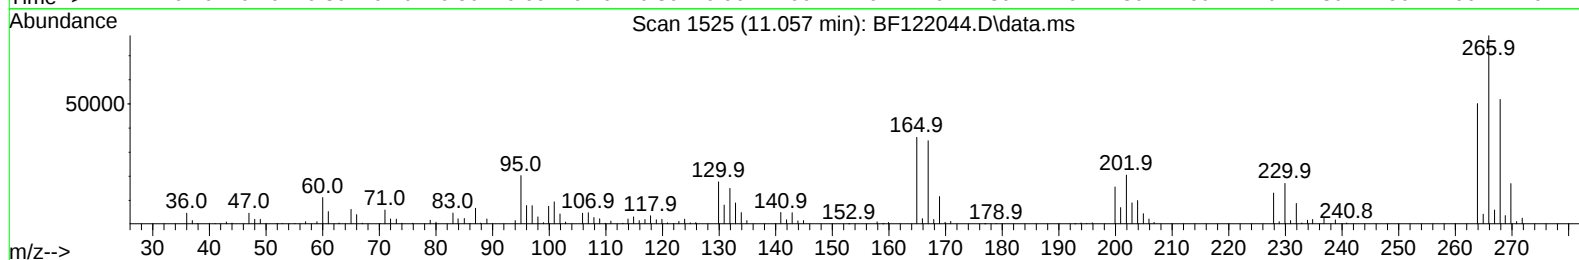


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102120\
Data File : BF122044.D
Acq On : 21 Oct 2020 9:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 02:17:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 12:04:42 2020
Response via : Initial Calibration

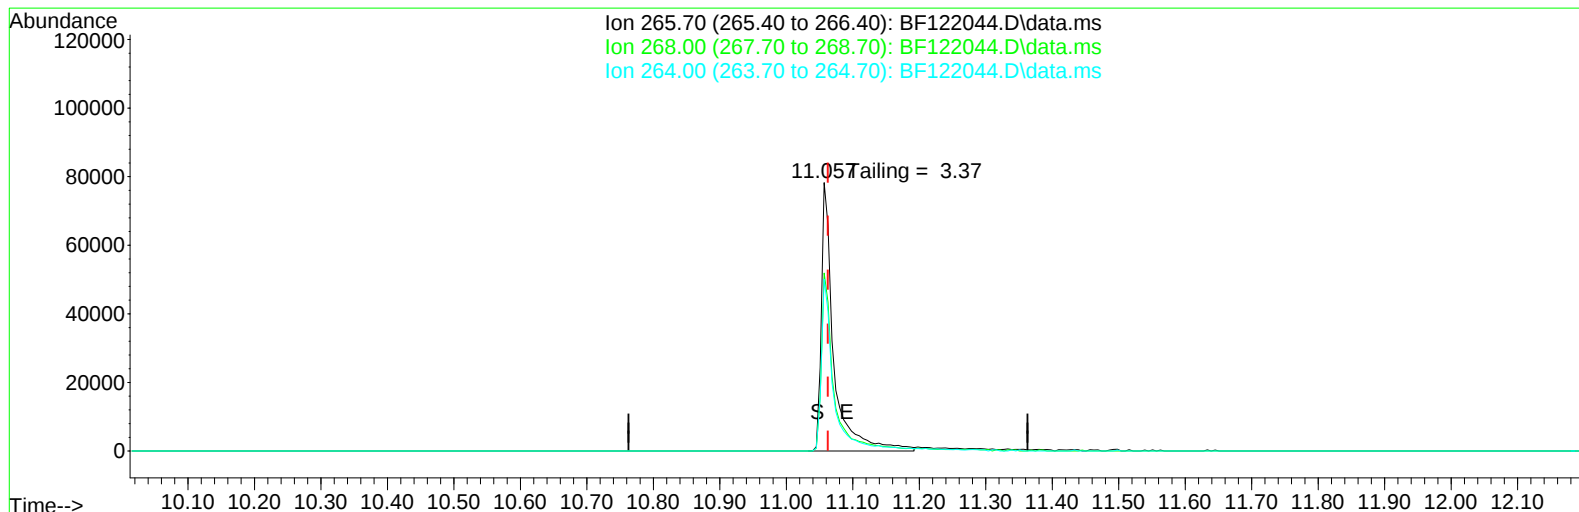

TIC: BF122044.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.006) 41651.97 ng

response 102696

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	66.30
264.00	62.40	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102120\
Data File : BF122044.D
Acq On : 21 Oct 2020 9:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 02:17:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 12:04:42 2020
Response via : Initial Calibration

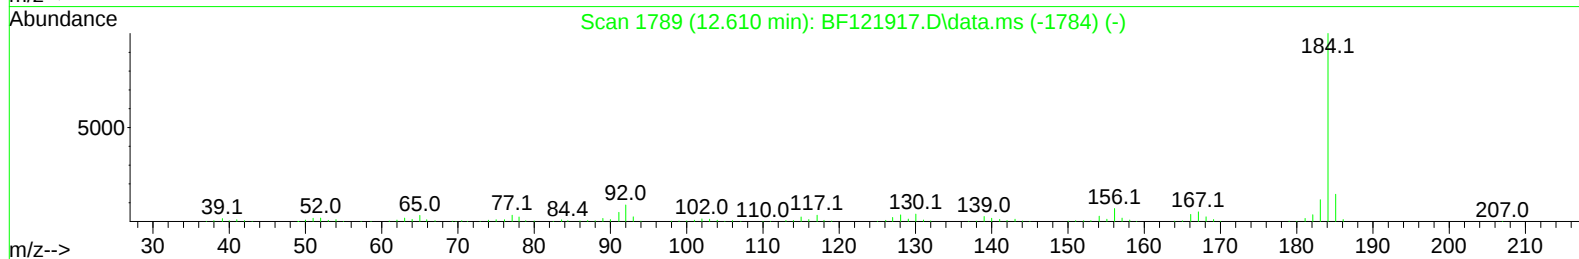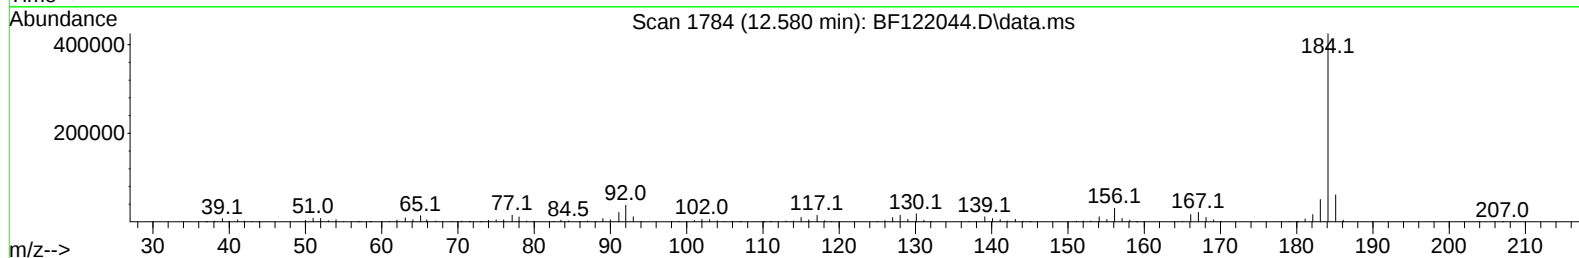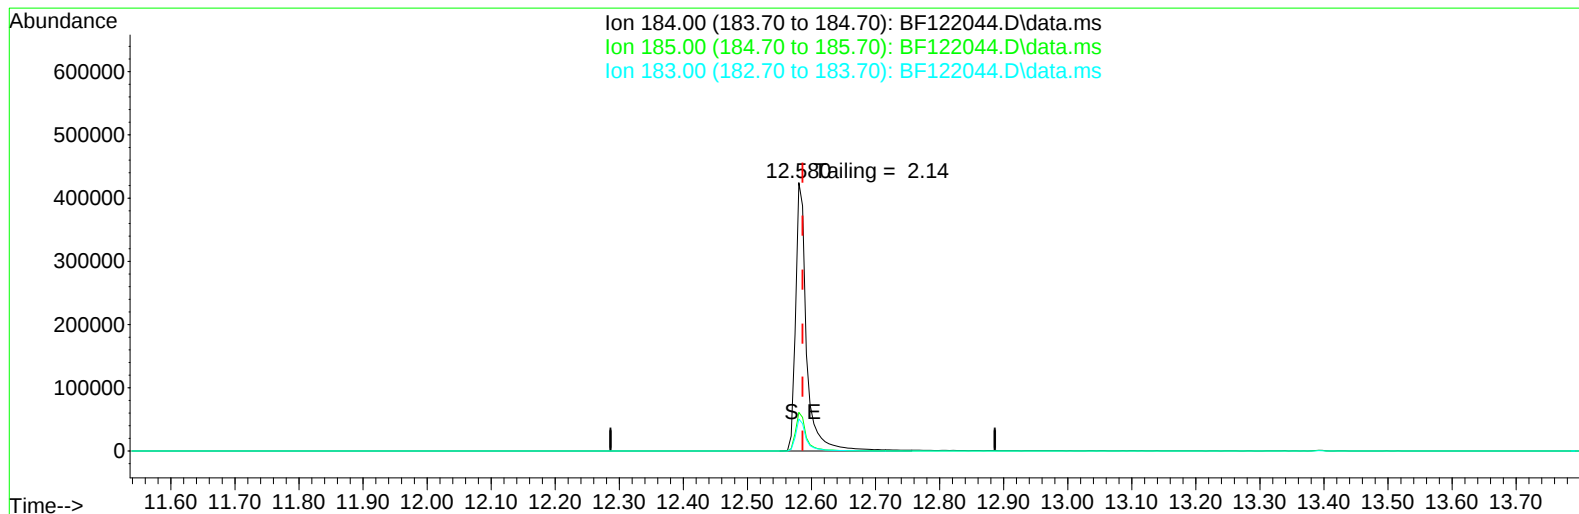

TIC: BF122044.D\data.ms

(77) Benzidine

12.580min (-0.006) 0.00 ng

response 510965

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.36
183.00	11.70	11.93
0.00	0.00	0.00