

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102120\
 Data File : BF122050.D
 Acq On : 21 Oct 2020 12:30
 Operator : JU/CG
 Sample : PB132200BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB132200BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	490	493	503	rBV	39588	71427	1.31%	0.238%
2	5.363	553	557	588	rBV	3455582	3782303	69.31%	12.612%
3	6.381	725	730	747	rBV	3285649	3797135	69.58%	12.661%
4	6.728	785	789	800	rBV	806545	752649	13.79%	2.510%
5	7.298	881	886	889	rBV	2503078	2683952	49.18%	8.949%
6	8.010	1002	1007	1025	rBV	1037666	1028560	18.85%	3.430%
7	9.087	1183	1190	1193	rBV	4510998	4682525	85.81%	15.613%
8	9.757	1299	1304	1314	rBV	1297780	1219913	22.36%	4.068%
9	10.551	1434	1439	1467	rBV	2844824	3076964	56.39%	10.260%
10	11.245	1552	1557	1566	rBV	1279831	1293924	23.71%	4.314%
11	12.833	1819	1827	1830	rBV	4922811	5456875	100.00%	18.195%
12	13.880	2001	2005	2020	rBV	1137677	1167393	21.39%	3.893%
13	15.310	2243	2248	2266	rBV	605002	977013	17.90%	3.258%




Sum of corrected areas: 29990633

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102120\
Data File : BF122050.D
Acq On : 21 Oct 2020 12:30
Operator : JU/CG
Sample : PB132200BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132200BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

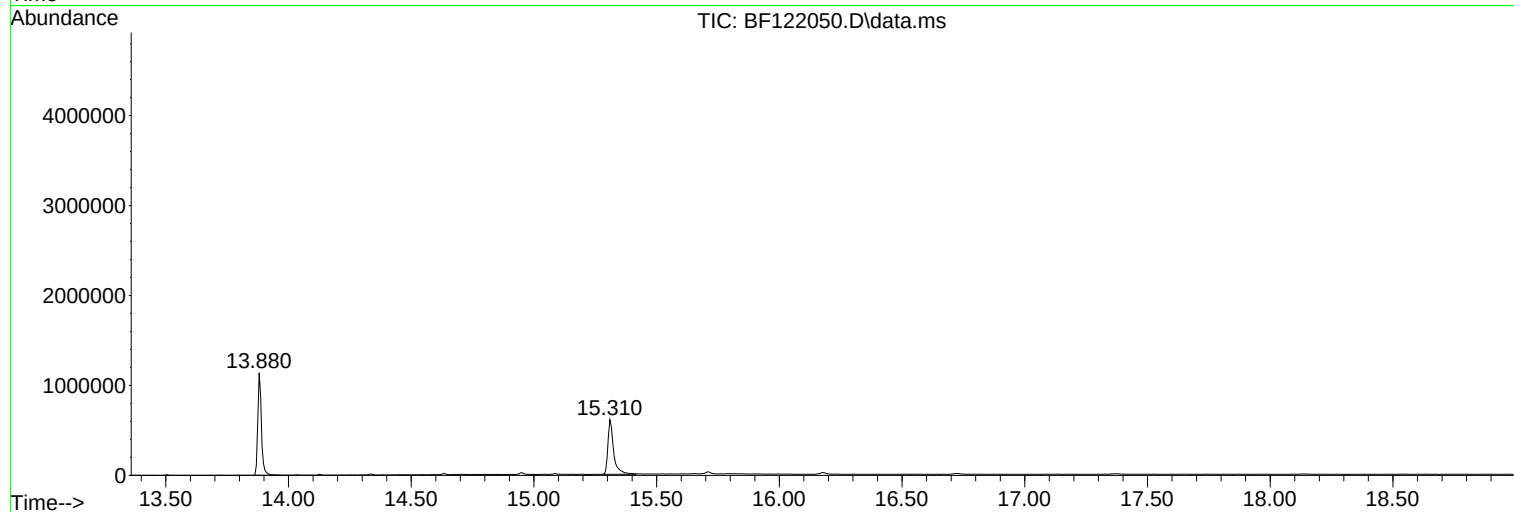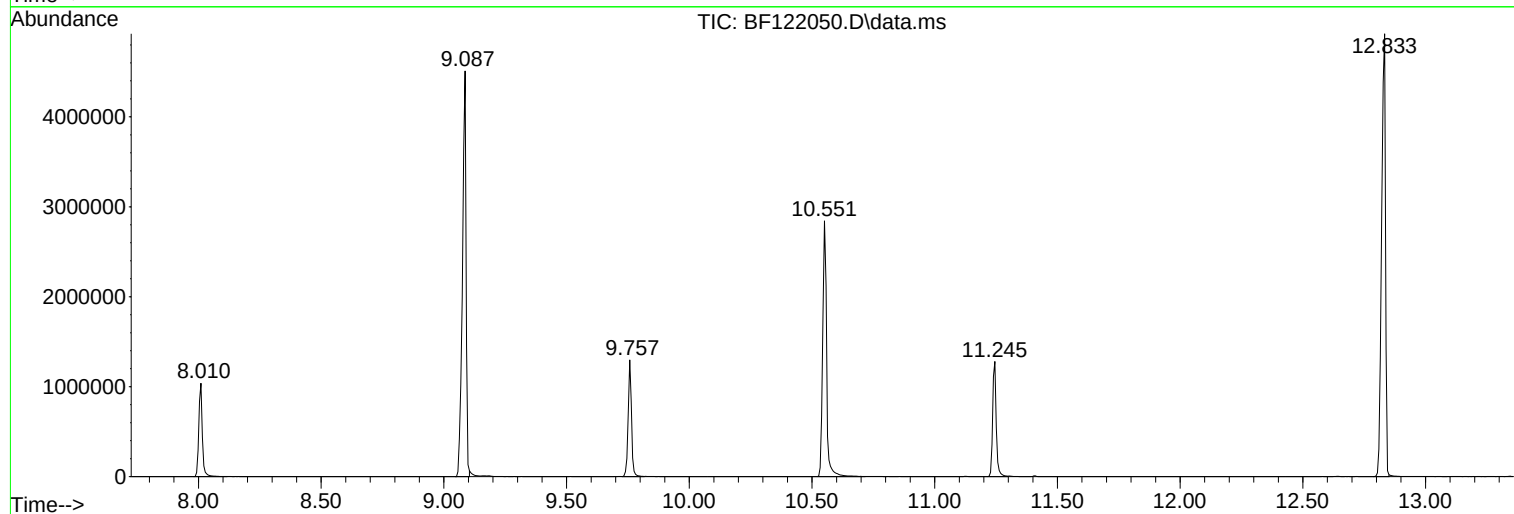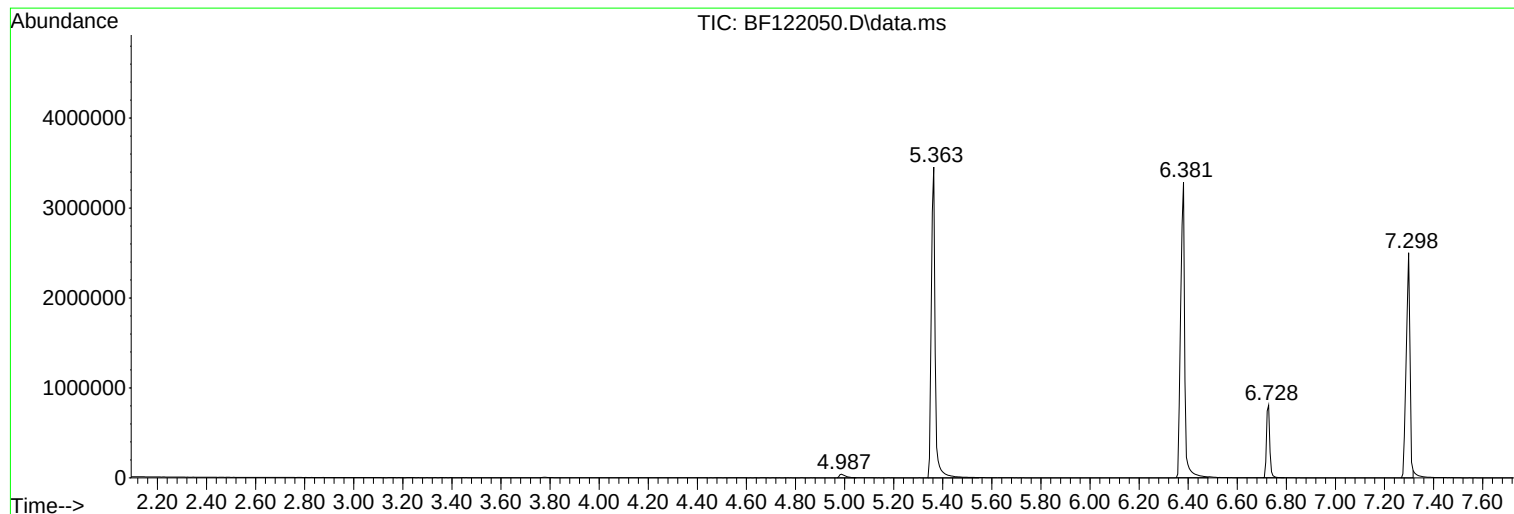

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102120\
Data File : BF122050.D
Acq On : 21 Oct 2020 12:30
Operator : JU/CG
Sample : PB132200BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132200BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102120\
Data File : BF122050.D
Acq On : 21 Oct 2020 12:30
Operator : JU/CG
Sample : PB132200BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132200BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------