
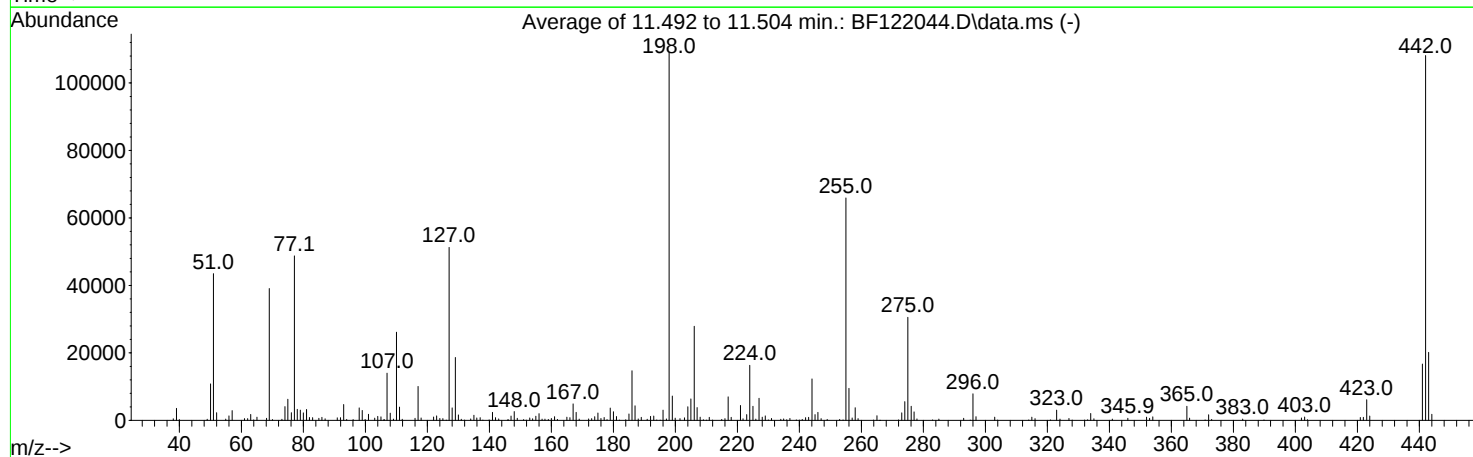


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102120\
Data File : BF122044.D
Acq On : 21 Oct 2020 9:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 21 12:04:42 2020

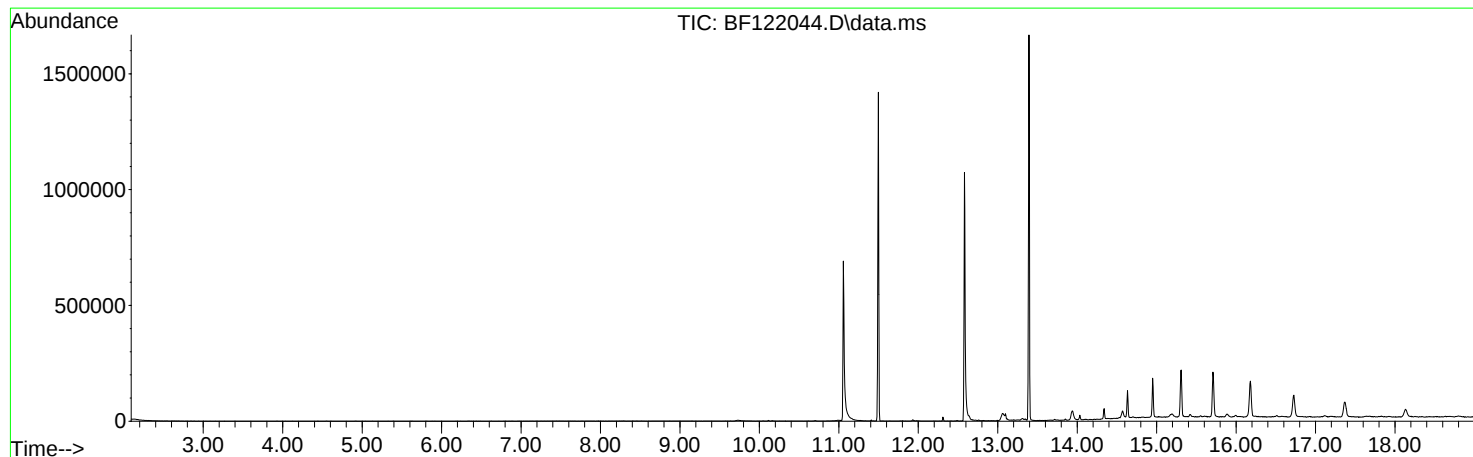

Spectrum Information: Average of 11.492 to 11.504 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	43494	PASS
68	69	0.00	2	1.6	606	PASS
69	198	0.00	100	35.8	39086	PASS
70	69	0.00	2	0.6	239	PASS
127	198	10	80	47.0	51275	PASS
197	198	0.00	2	0.4	423	PASS
198	198	100	100	100.0	109027	PASS
199	198	5	9	6.6	7210	PASS
275	198	10	60	28.0	30552	PASS
365	198	1	100	3.8	4164	PASS
441	198	0.01	100	15.3	16708	PASS
442	198	50	100	99.2	108136	PASS
443	442	15	24	18.6	20149	PASS