
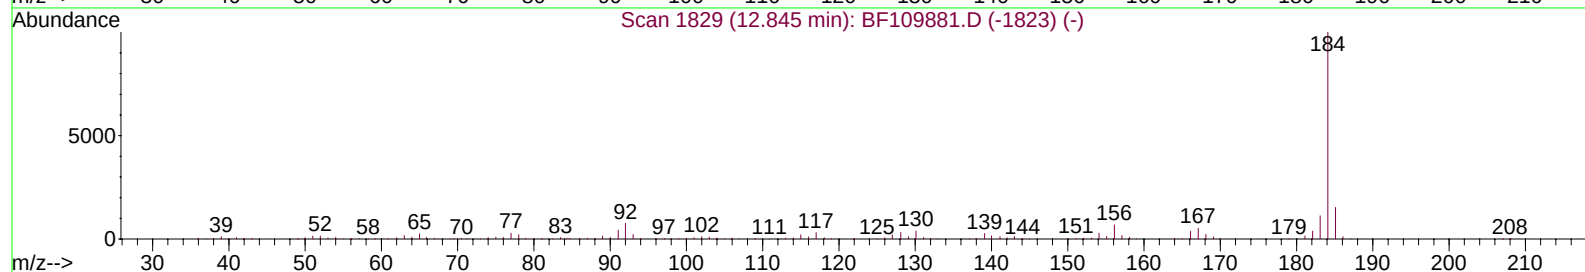
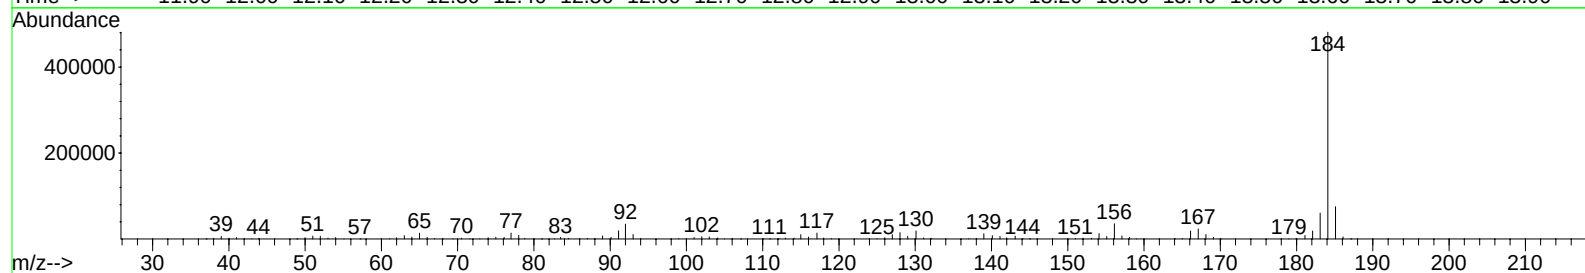


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102218\
Data File : BF110065.D
Acq On : 22 Oct 2018 23:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 08:38:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

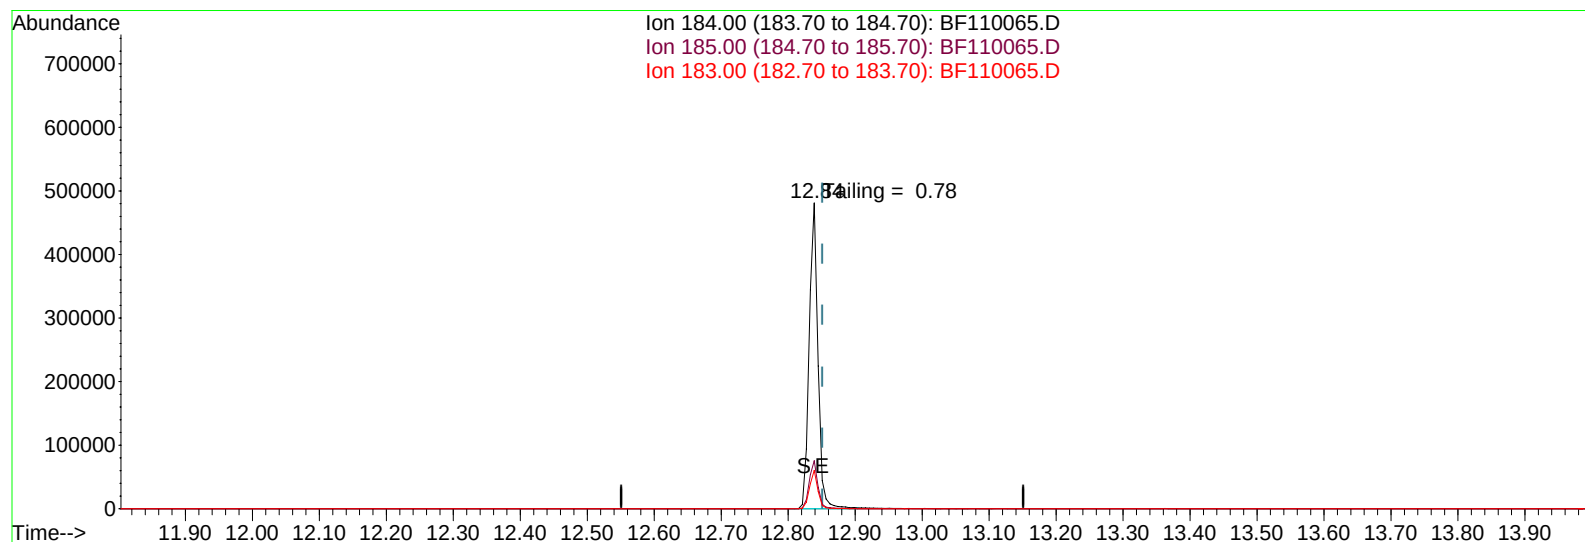

TIC: BF110065.D

(77) Benzidine




12.839min (-0.012) 0.00ng

response 440873

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.69
183.00	11.80	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102218\
Data File : BF110065.D
Acq On : 22 Oct 2018 23:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 08:38:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

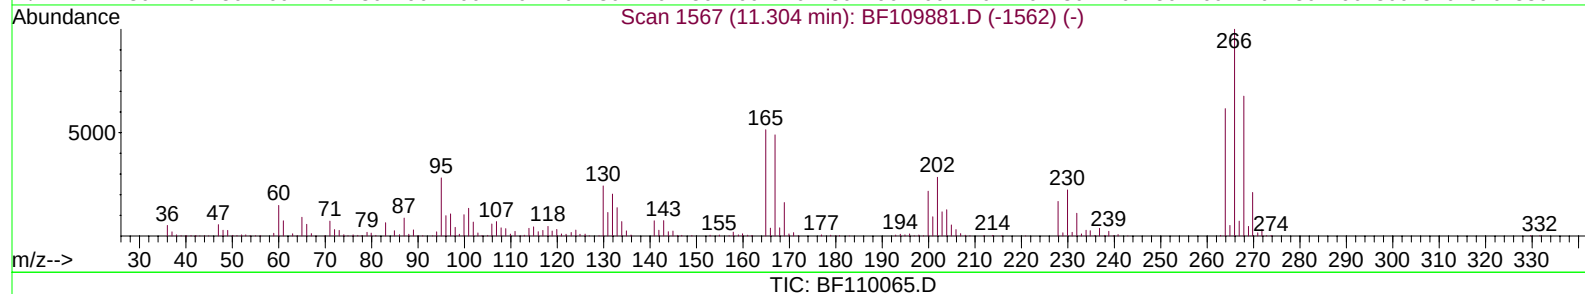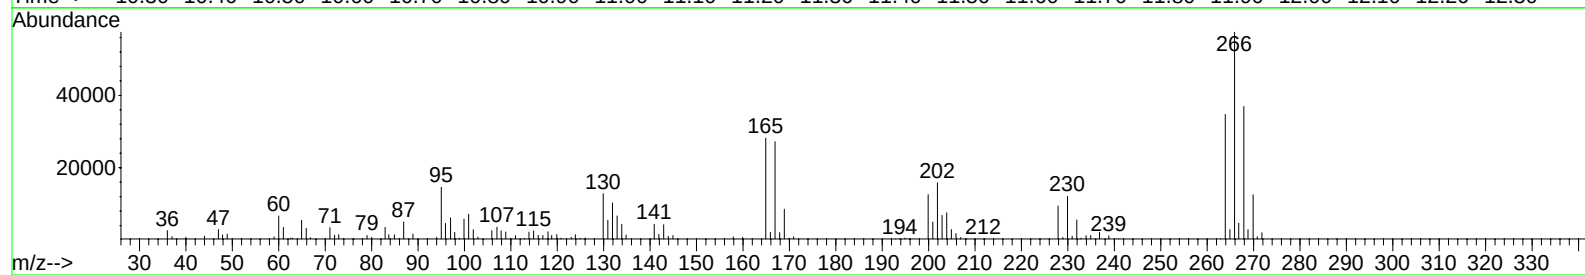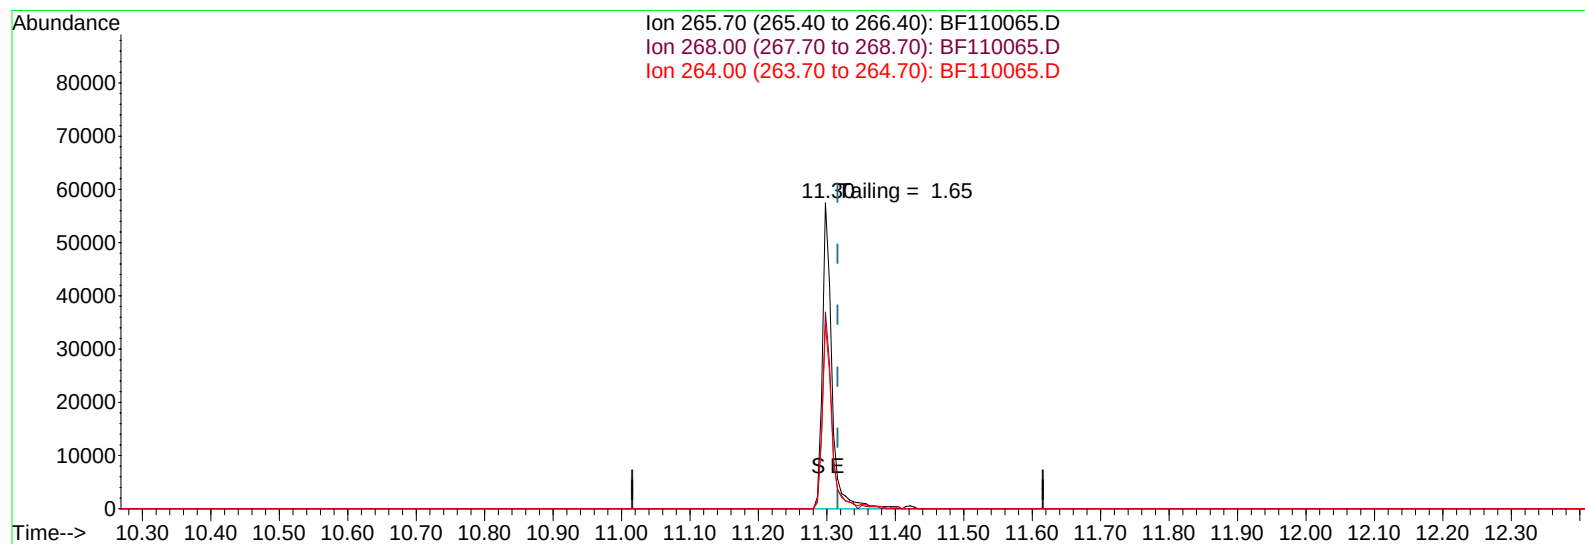

(70) Pentachlorophenol (C)

11.298min (-0.018) 18993.70ng

response 55090

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	64.29
264.00	63.20	60.42
0.00	0.00	0.00