

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102218\
 Data File : BF110051.D
 Acq On : 22 Oct 2018 16:17
 Operator : JU/SJ
 Sample : J5601-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 101818-SIDI-E-D-B

Quant Time: Oct 23 03:52:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 16 14:58:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	194954	20.00	ng	-0.01
21) Naphthalene-d8	8.25	136	710941	20.00	ng	-0.02
39) Acenaphthene-d10	10.01	164	282253	20.00	ng	-0.02
64) Phenanthrene-d10	11.50	188	454378	20.00	ng	-0.01
76) Chrysene-d12	14.15	240	341185	20.00	ng	-0.01
87) Perylene-d12	15.68	264	265573	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	458306	37.26	ng	-0.01
7) Phenol-d6	6.58	99	364286	23.85	ng	-0.02
23) Nitrobenzene-d5	7.53	82	1033811	97.96	ng	-0.02
42) 2,4,6-Tribromophenol	10.80	330	195057	79.82	ng	-0.01
45) 2-Fluorobiphenyl	9.33	172	1717944	97.12	ng	-0.01
79) Terphenyl-d14	13.09	244	1337046	82.29	ng	-0.02
Target Compounds						
10) Phenol	6.59	94	34243	2.077	ng	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102218\
Data File : BF110051.D
Acq On : 22 Oct 2018 16:17
Operator : JU/SJ
Sample : J5601-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
101818-SIDI-E-D-B

Quant Time: Oct 23 03:52:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

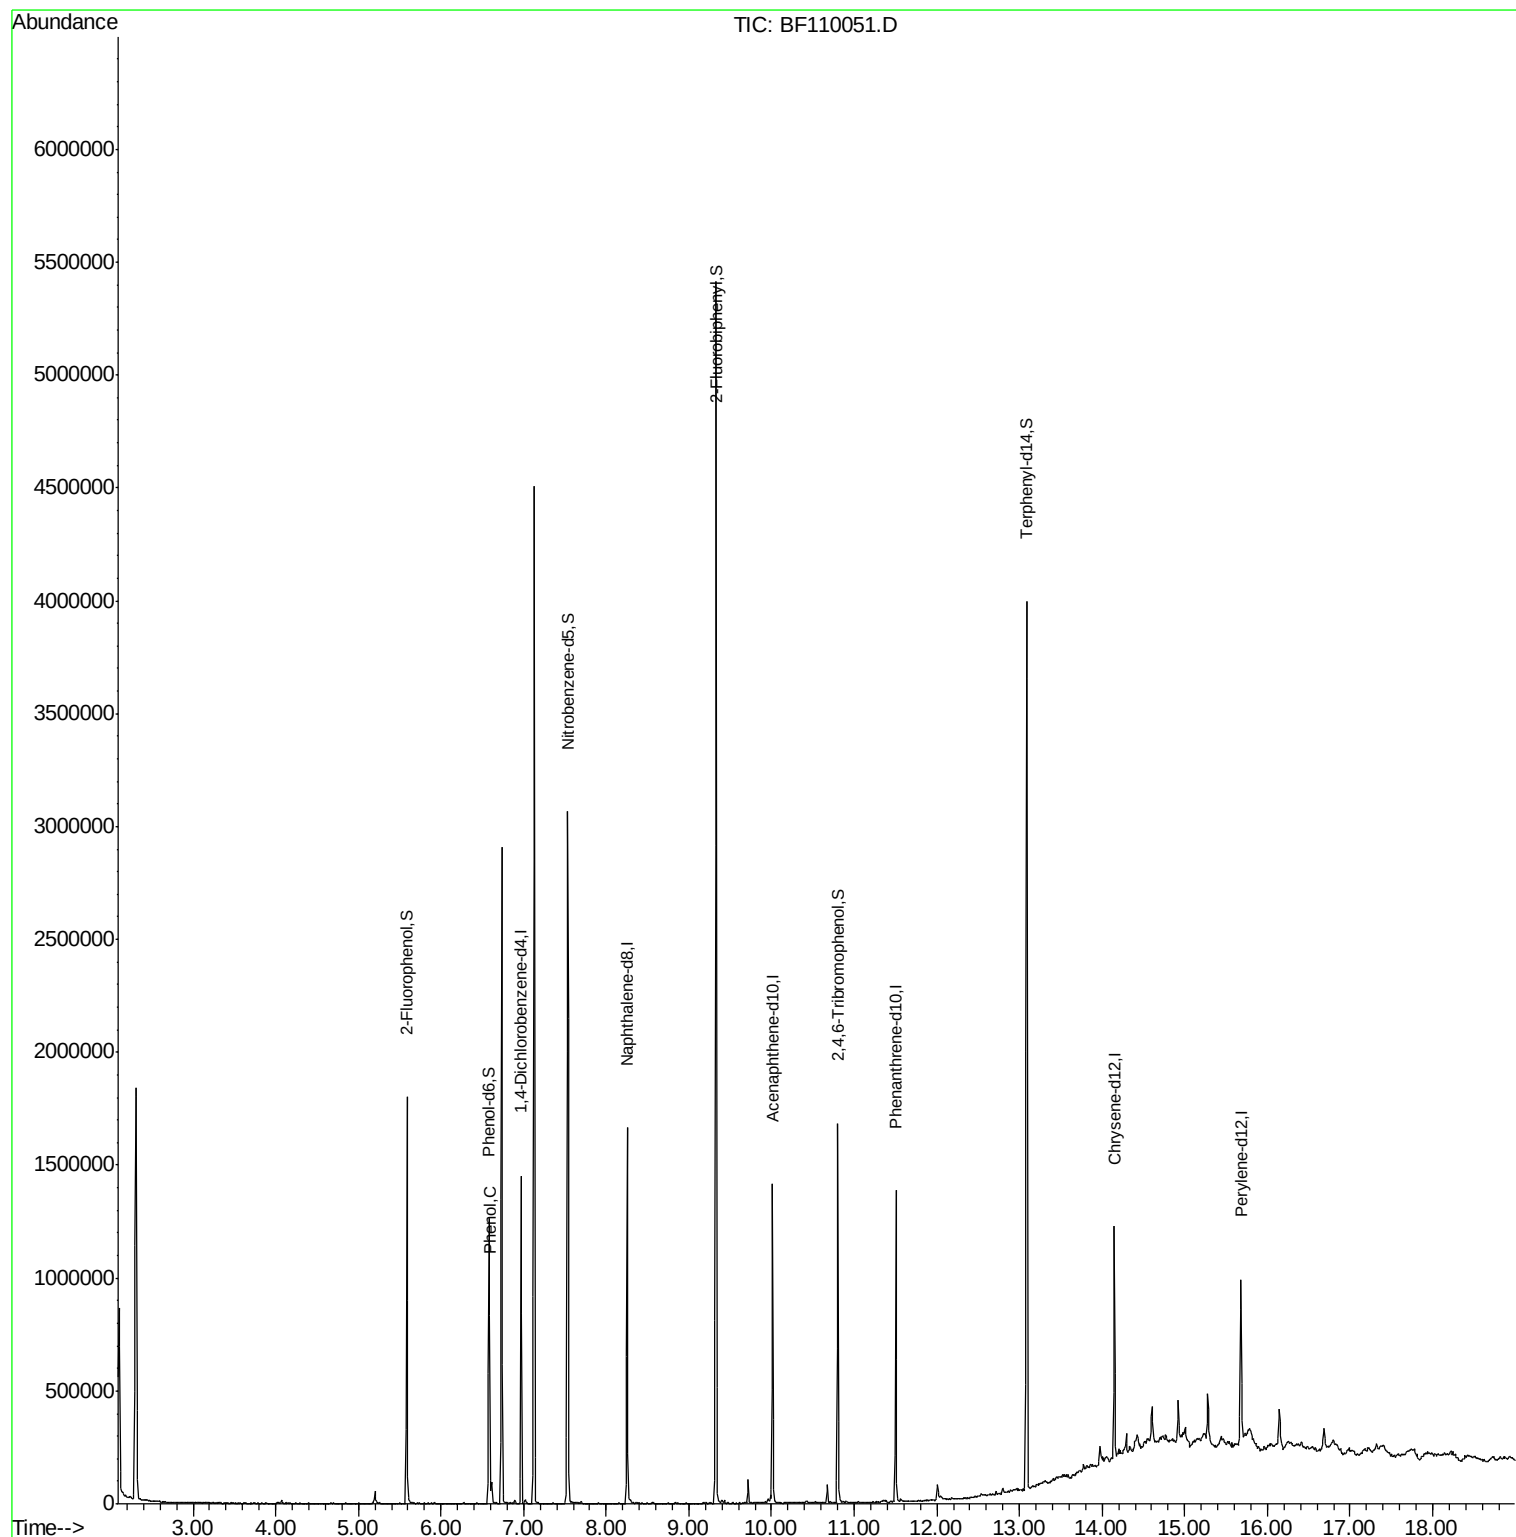

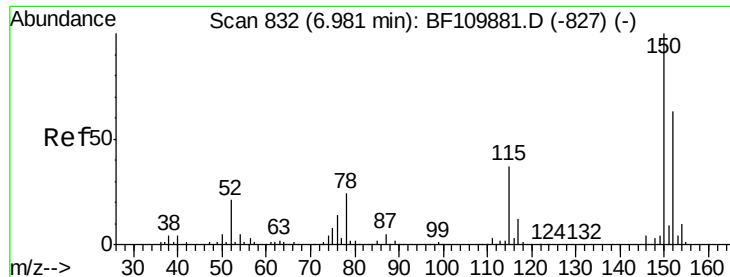


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 830
Delta R.T. -0.01 min
Lab File: BF110051.D
Acq: 22 Oct 2018 16:17

Instrument :
BNA_F
ClientSampleId :
101818-SIDI-E-D-B

Tot Ion:152 Resp: 194954
Ion Ratio Lower Upper
152 100
150 157.1 122.7 184.1
115 62.1 49.1 73.7

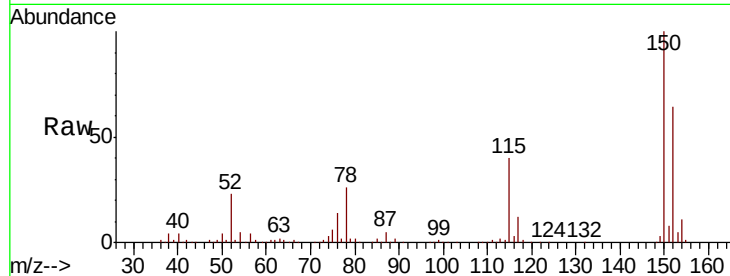


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

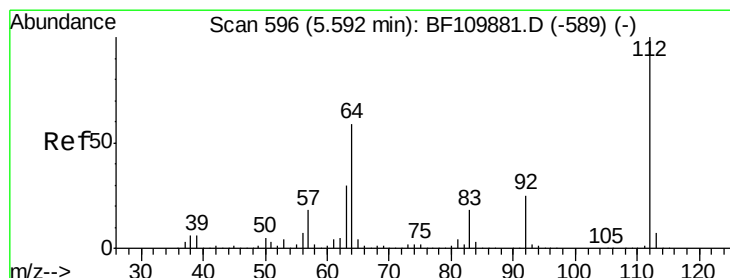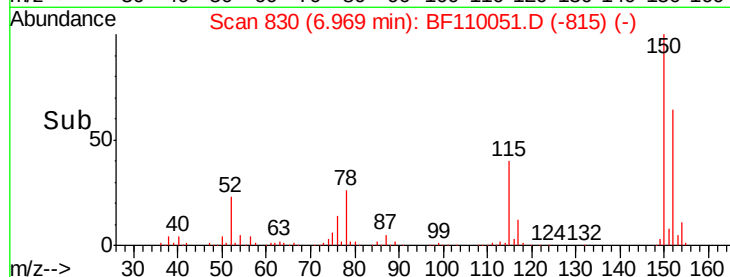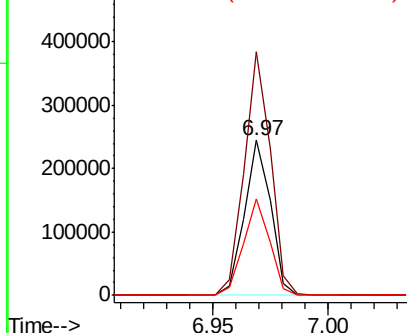



#5


2-Fluorophenol
Concen: 37.264 ng
RT: 5.59 min Scan# 595
Delta R.T. -0.01 min
Lab File: BF110051.D
Acq: 22 Oct 2018 16:17

Tgt Ion:112 Resp: 458306
Ion Ratio Lower Upper
112 100
64 59.3 44.1 66.1
63 30.6 23.7 35.5

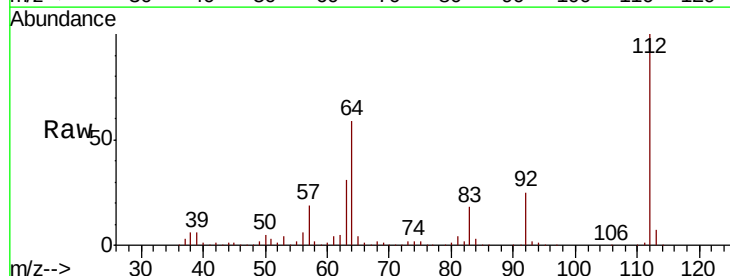

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

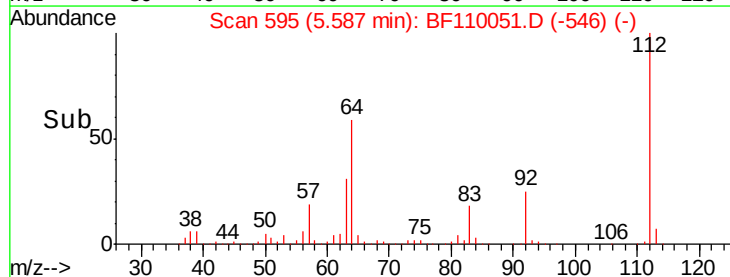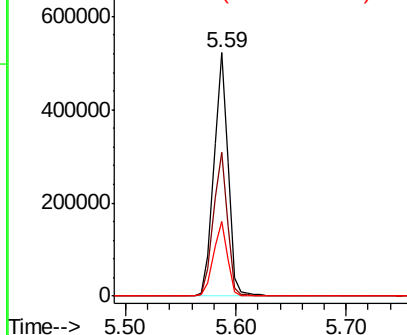

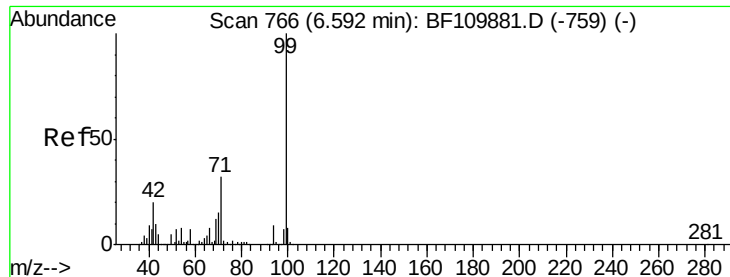

#7

Phenol-d6

Concen: 23.853 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.02 min

Lab File: BF110051.D

Acq: 22 Oct 2018 16:17

Instrument :

BNA_F

ClientSampleId :

101818-SIDI-E-D-B


Tot Ion: 99 Resp: 364286

Ion Ratio Lower Upper




99 100

42 19.6 15.8 23.6

71 34.5 28.0 42.0

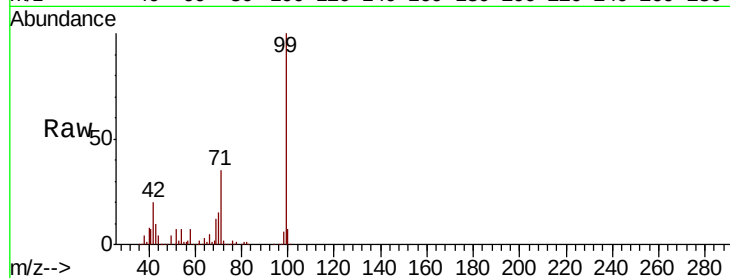

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

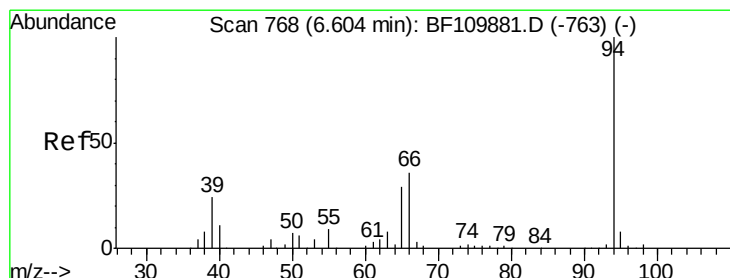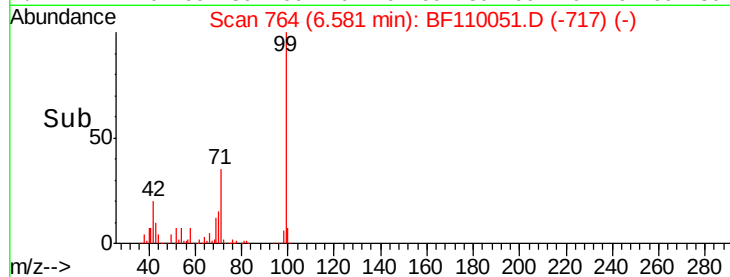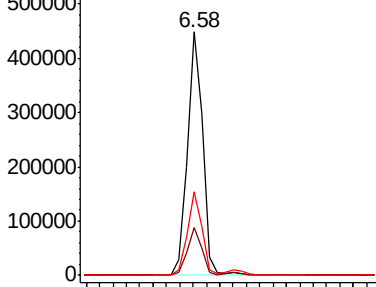

#10

Phenol

Concen: 2.077 ng

RT: 6.59 min Scan# 766

Delta R.T. -0.02 min

Lab File: BF110051.D

Acq: 22 Oct 2018 16:17


Tgt Ion: 94 Resp: 34243

Ion Ratio Lower Upper



94 100


65 29.4 25.3 65.3

66 39.8 54.5 94.5#

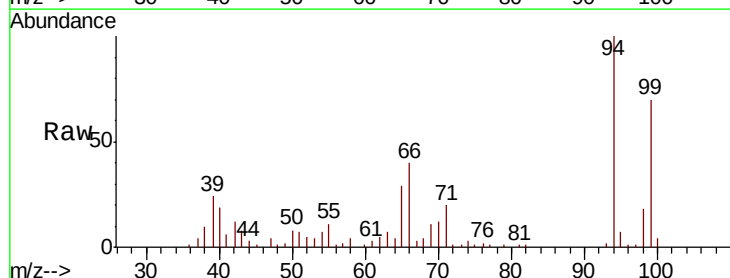

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

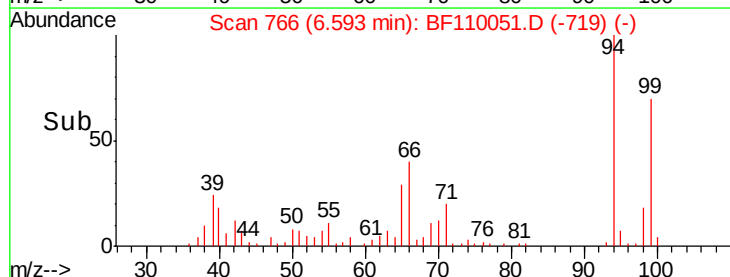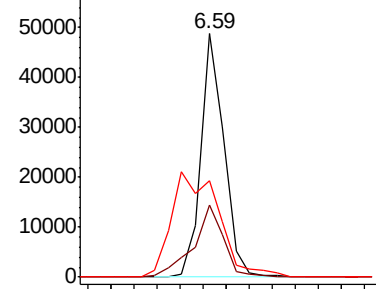

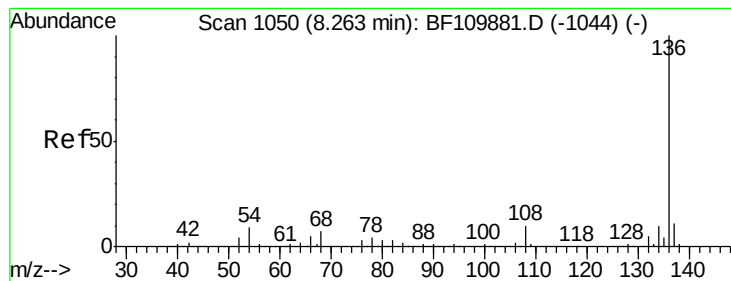

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1048

Delta R.T. -0.02 min

Lab File: BF110051.D

Acq: 22 Oct 2018 16:17

Instrument :

BNA_F

ClientSampleId :

101818-SIDI-E-D-B

Tot Ion:136 Resp: 710941



Ion Ratio Lower Upper

136 100

137 11.1 8.8 13.2

54 8.9 5.4 8.2#

68 6.0 4.2 6.2


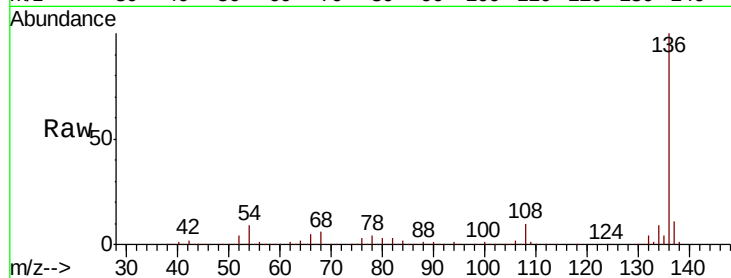


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

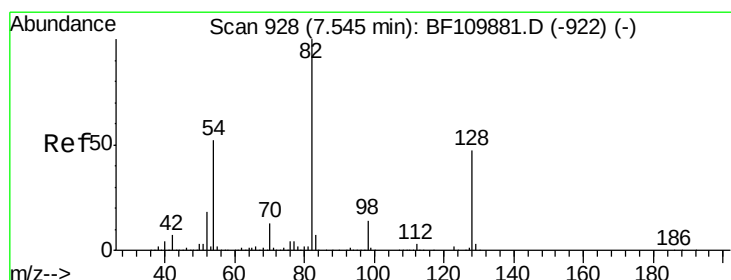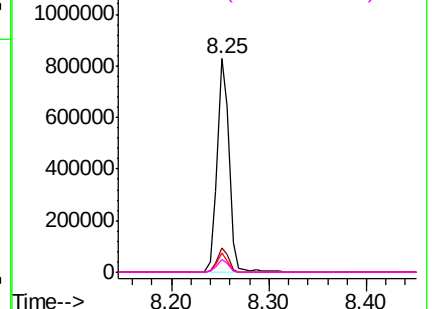

#23

Nitrobenzene-d5

Concen: 97.957 ng

RT: 7.53 min Scan# 926

Delta R.T. -0.02 min

Lab File: BF110051.D

Acq: 22 Oct 2018 16:17



Tgt Ion: 82 Resp: 1033811

Ion Ratio Lower Upper

82 100

128 46.1 34.2 51.2


54 53.9 38.6 58.0

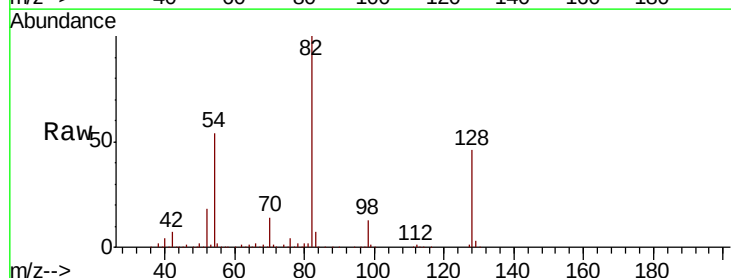


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

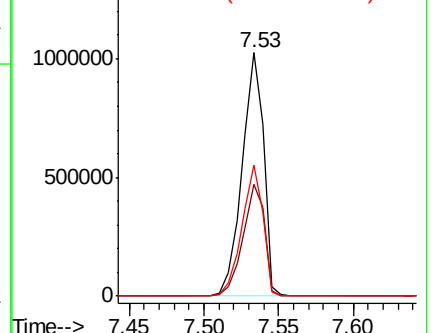







#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.01 min Scan# 1347
Delta R.T. -0.02 min
Lab File: BF110051.D
Acq: 22 Oct 2018 16:17

Instrument :
BNA_F
ClientSampleId :
101818-SIDI-E-D-B

Tot Ion:164 Resp: 282253
Ion Ratio Lower Upper
164 100
162 103.6 83.0 124.6
160 45.8 37.0 55.6

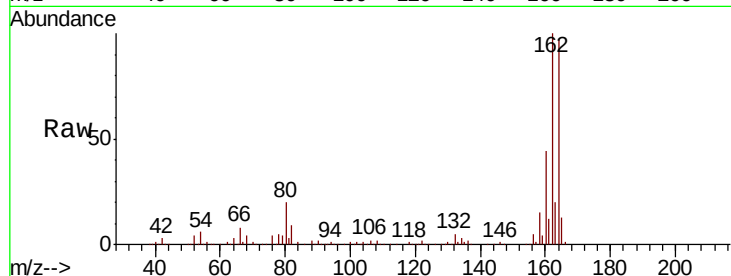


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

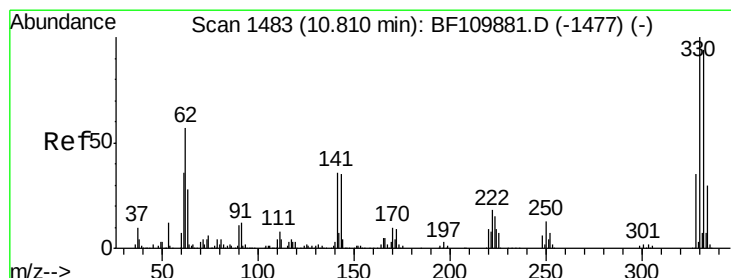
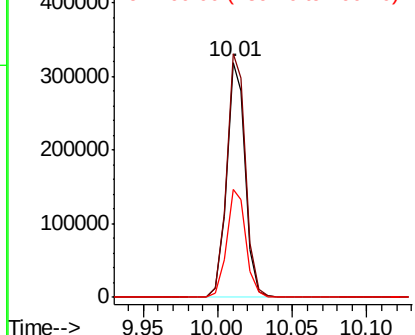



#42
2,4,6-Tribromophenol
Concen: 79.821 ng
RT: 10.80 min Scan# 1482
Delta R.T. -0.01 min
Lab File: BF110051.D
Acq: 22 Oct 2018 16:17

Tgt Ion:330 Resp: 195057
Ion Ratio Lower Upper
330 100
332 96.2 77.1 115.7
141 37.5 27.0 40.4

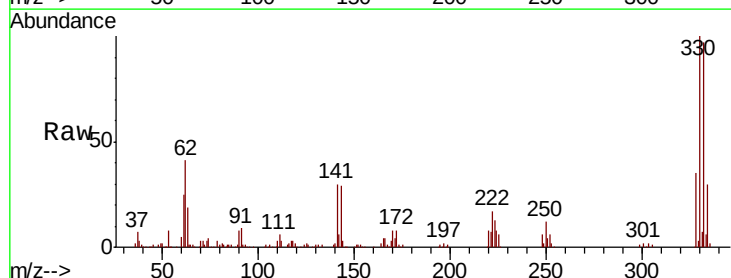

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

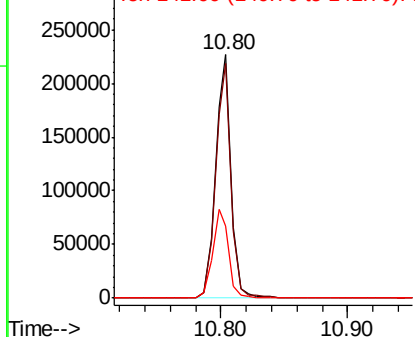




#45
 2-Fluorobiphenyl
 Concen: 97.120 ng
 RT: 9.33 min Scan# 1231
 Delta R.T. -0.01 min
 Lab File: BF110051.D
 Acq: 22 Oct 2018 16:17




Instrument :
 BNA_F
 ClientSampleId :
 101818-SIDI-E-D-B

Tot Ion:172 Resp: 1717944

Ion	Ratio	Lower	Upper
172	100		
171	36.9	28.6	43.0
170	24.7	19.7	29.5

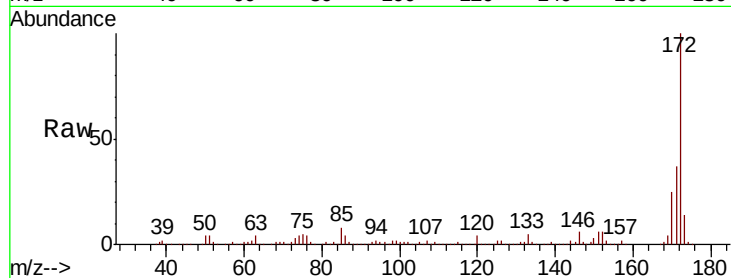


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

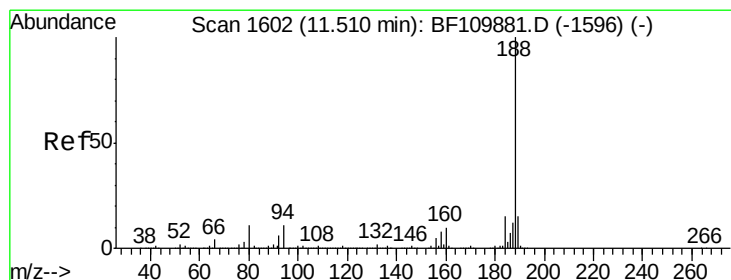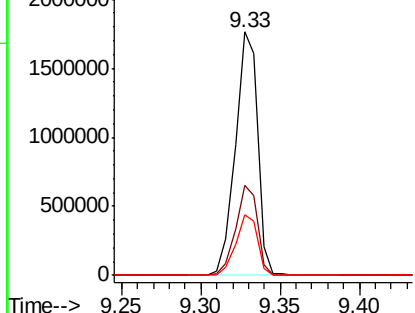



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.50 min Scan# 1601
 Delta R.T. -0.01 min
 Lab File: BF110051.D
 Acq: 22 Oct 2018 16:17


Tgt Ion:188 Resp: 454378

Ion	Ratio	Lower	Upper
188	100		
94	9.4	7.2	10.8
80	10.0	7.9	11.9

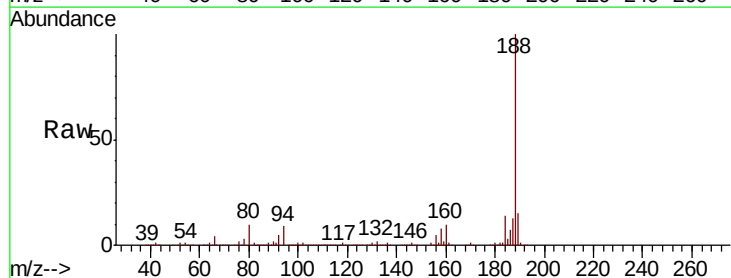

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

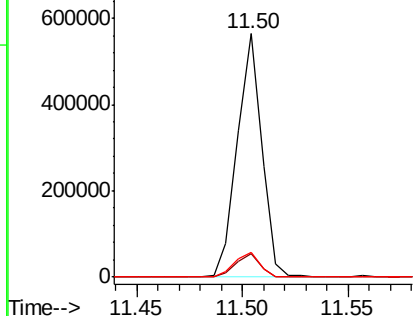

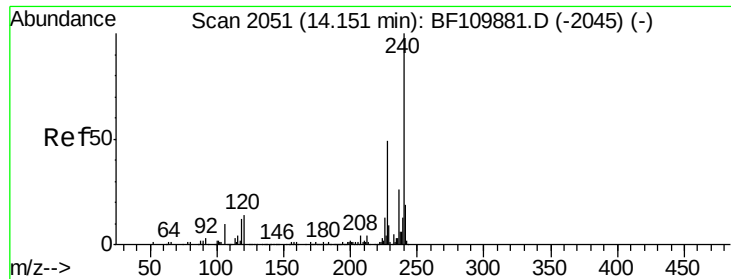

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2051

Delta R.T. -0.01 min

Lab File: BF110051.D

Acq: 22 Oct 2018 16:17

Instrument :

BNA_F

ClientSampleId :

101818-SIDI-E-D-B


Tot Ion:240 Resp: 341185

Ion Ratio Lower Upper

240 100

120 10.4 8.3 12.5

236 25.5 21.2 31.8



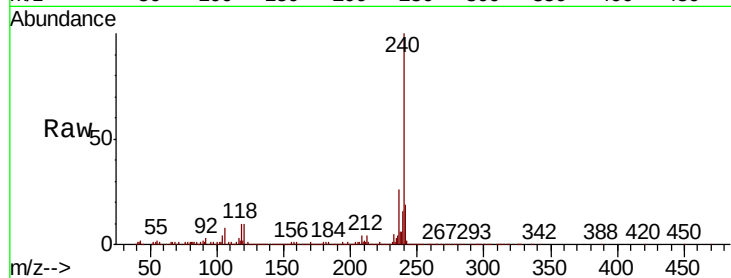


Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

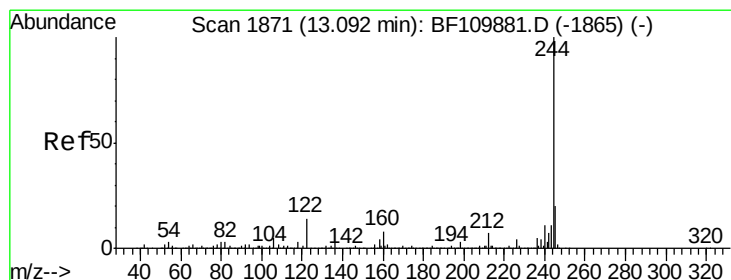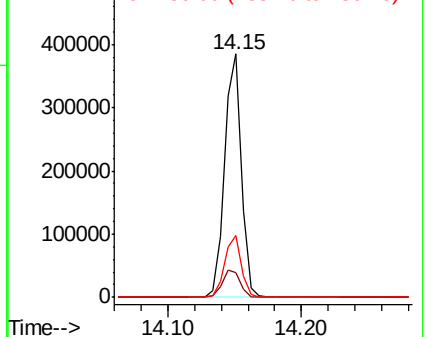

#79

Terphenyl-d14

Concen: 82.293 ng

RT: 13.09 min Scan# 1870

Delta R.T. -0.02 min

Lab File: BF110051.D

Acq: 22 Oct 2018 16:17


Tgt Ion:244 Resp: 1337046

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.8

122 13.1 8.7 13.1#


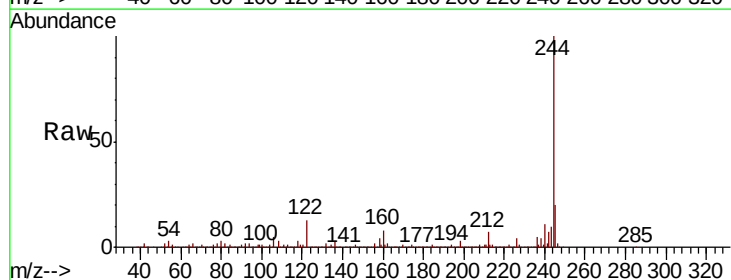



Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

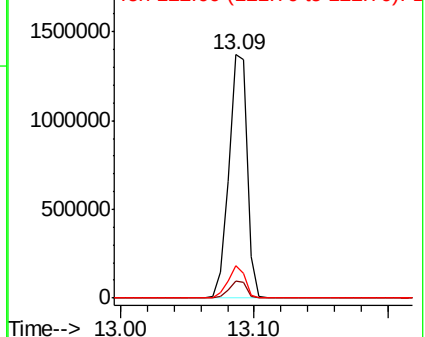

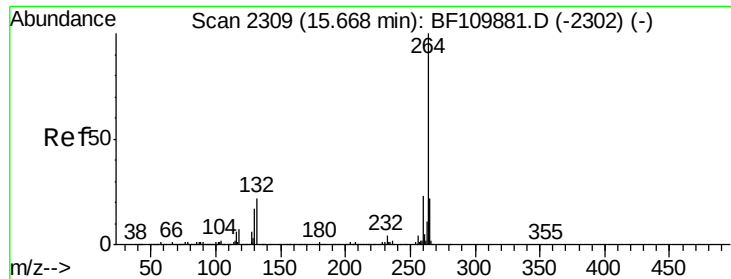

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.68 min Scan# 2311
Delta R.T. -0.01 min
Lab File: BF110051.D
Acq: 22 Oct 2018 16:17

Instrument :
BNA_F
ClientSampleId :
101818-SIDI-E-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	18.7	28.1
265	22.3	16.7	25.1

