


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102218\
 Data File : BF110039.D
 Acq On : 22 Oct 2018 10:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 14:58:24 2018

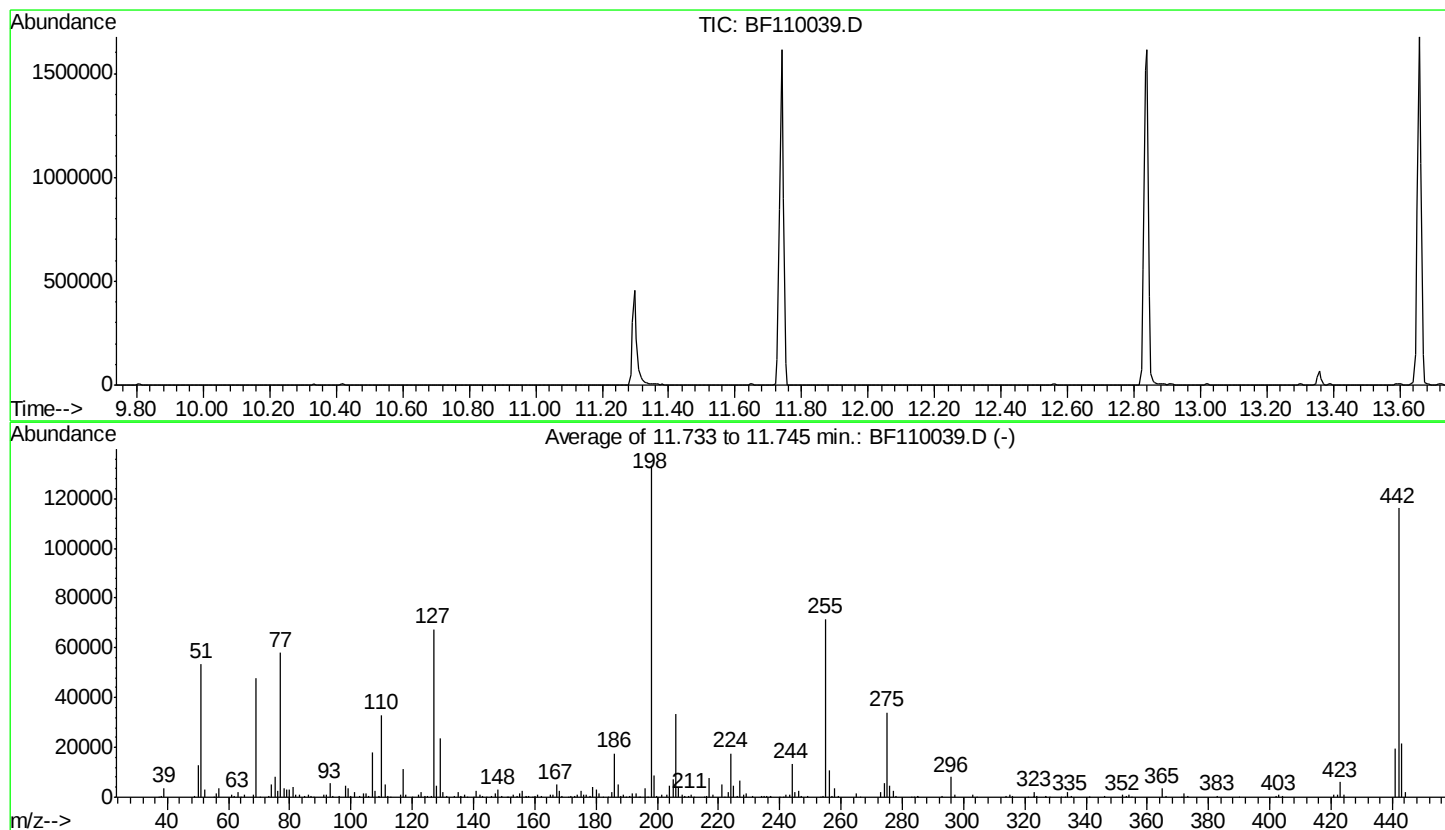

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	53522	PASS
68	69	0.00	2	1.9	886	PASS
69	198	0.00	100	35.8	47746	PASS
70	69	0.00	2	0.3	153	PASS
127	198	10	80	50.6	67453	PASS
197	198	0.00	2	0.2	265	PASS
198	198	100	100	100.0	133237	PASS
199	198	5	9	6.5	8692	PASS
275	198	10	60	25.5	34032	PASS
365	198	1	100	2.7	3561	PASS
441	198	0.01	100	14.5	19312	PASS
442	198	50	100	87.1	116069	PASS
443	442	15	24	18.5	21470	PASS