


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102218\
 Data File : BF110065.D
 Acq On : 22 Oct 2018 23:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 14:58:24 2018

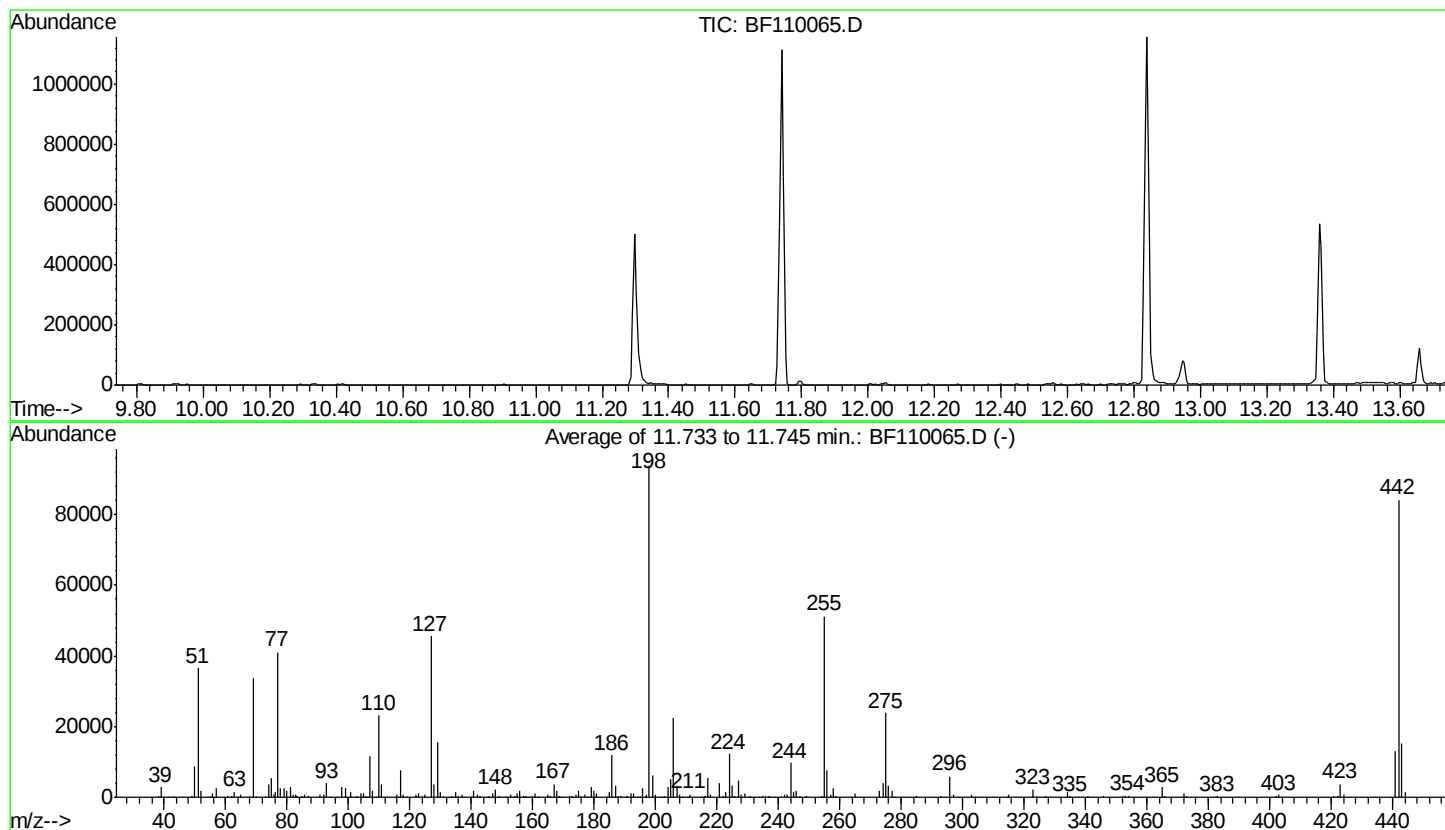

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	36536	PASS
68	69	0.00	2	1.5	499	PASS
69	198	0.00	100	35.7	33544	PASS
70	69	0.00	2	0.3	101	PASS
127	198	10	80	48.6	45589	PASS
197	198	0.00	2	0.7	648	PASS
198	198	100	100	100.0	93856	PASS
199	198	5	9	6.6	6161	PASS
275	198	10	60	25.5	23887	PASS
365	198	1	100	3.0	2815	PASS
441	198	0.01	100	14.0	13182	PASS
442	198	50	100	89.7	84144	PASS
443	442	15	24	18.3	15375	PASS