
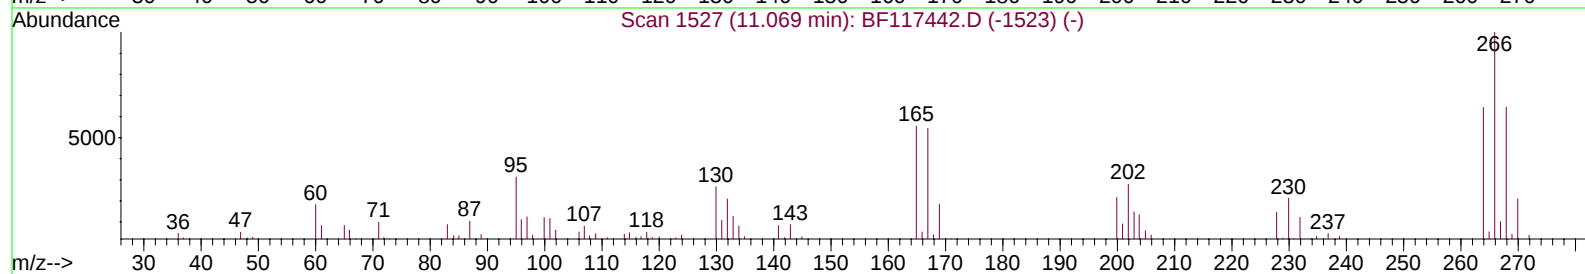
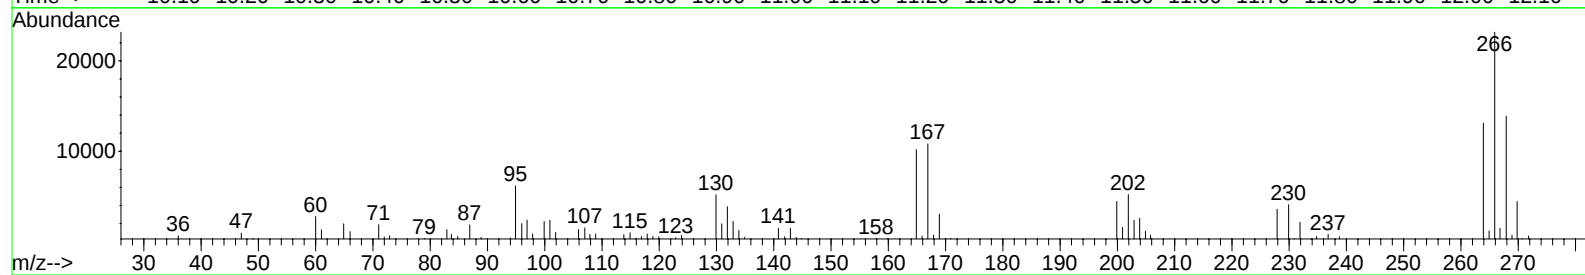


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102219\
Data File : BF117472.D
Acq On : 22 Oct 2019 12:16
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 18:46:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

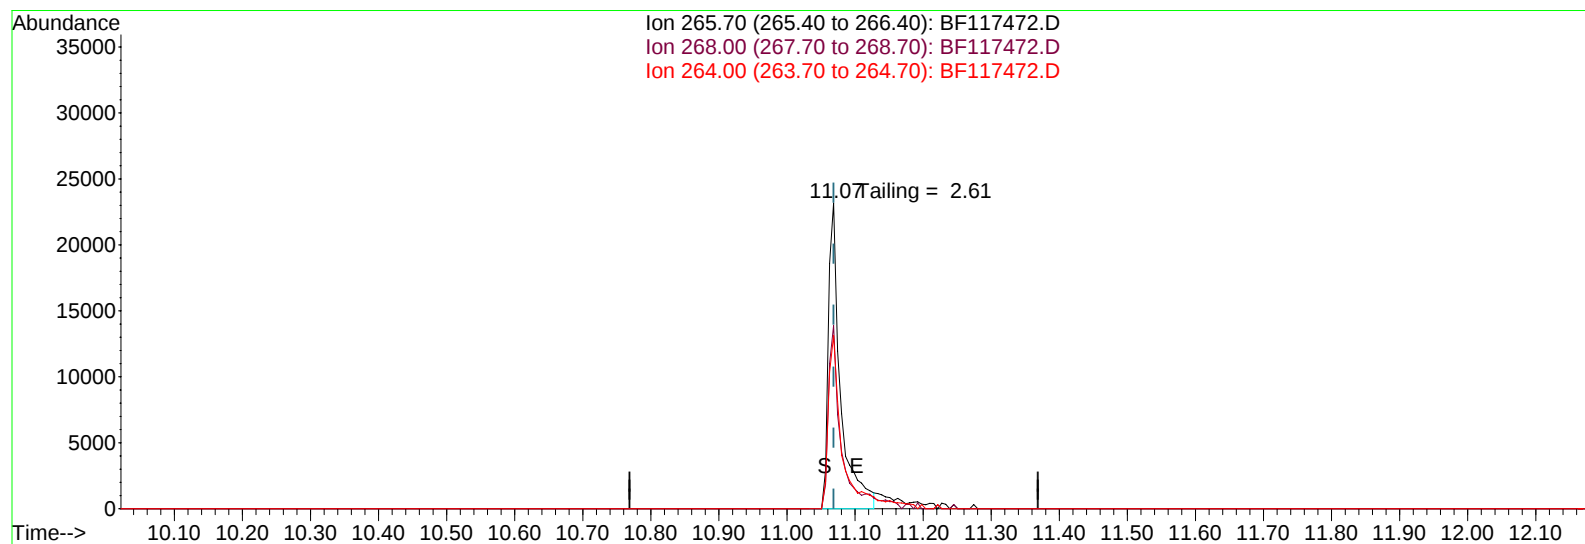

TIC: BF117472.D

(70) Pentachlorophenol (C)




11.069min (-0.000) 63156.11ng

response 31231

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	59.98
264.00	64.30	56.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102219\
Data File : BF117472.D
Acq On : 22 Oct 2019 12:16
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 18:46:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

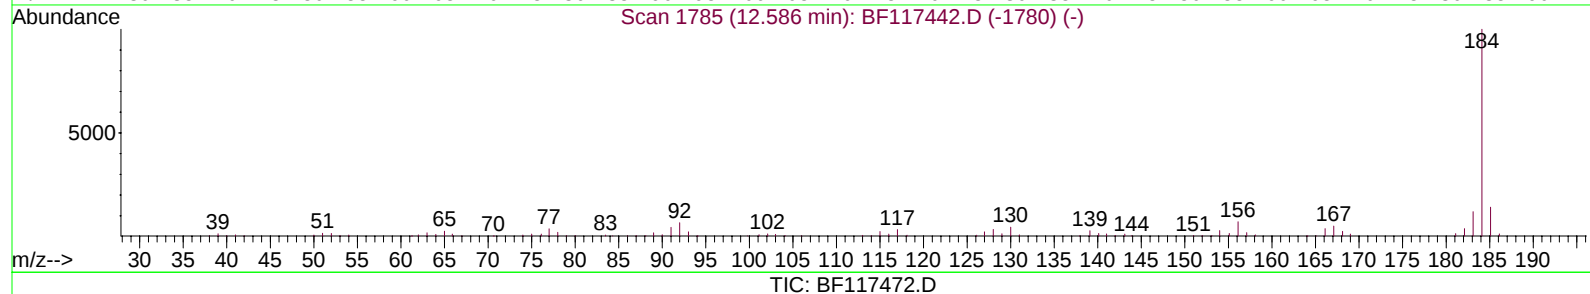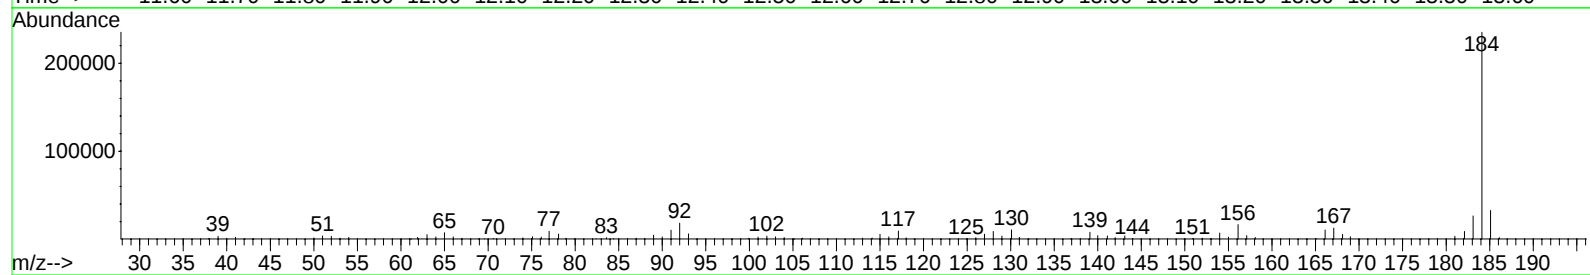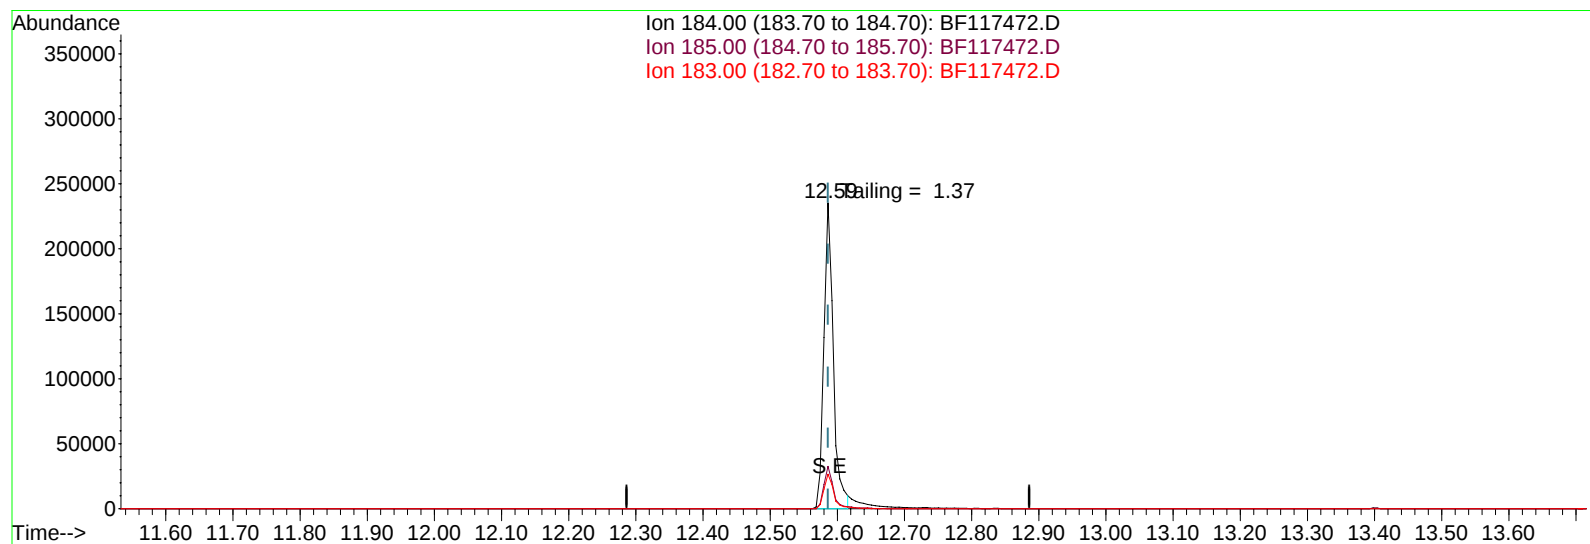

(77) Benzidine

12.586min (+0.000) 0.00ng

response 245190

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.89
183.00	12.00	11.29
0.00	0.00	0.00