

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102219\
 Data File : BF117479.D
 Acq On : 22 Oct 2019 15:51
 Operator : JU
 Sample : K5420-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-5

Quant Time: Oct 22 16:21:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 18:53:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	33005	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	129339	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	66944	20.00	ng	0.00
64) Phenanthrene-d10	11.25	188	109875	20.00	ng	0.00
76) Chrysene-d12	13.89	240	79617	20.00	ng	0.00
87) Perylene-d12	15.33	264	77607	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	219784	99.07	ng	0.00
7) Phenol-d6	6.38	99	299468	100.50	ng	0.00
23) Nitrobenzene-d5	7.29	82	188500	71.95	ng	-0.01
42) 2,4,6-Tribromophenol	10.56	330	54515	94.12	ng	0.00
45) 2-Fluorobiphenyl	9.09	172	335725	70.66	ng	0.00
79) Terphenyl-d14	12.83	244	326089	66.81	ng	0.00
Target Compounds						
10) Phenol	6.39	94	6295	2.070	ng	Qvalue # 83
50) Dimethylphthalate	9.48	163	60536	12.685	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102219\
Data File : BF117479.D
Acq On : 22 Oct 2019 15:51
Operator : JU
Sample : K5420-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-5

Quant Time: Oct 22 16:21:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

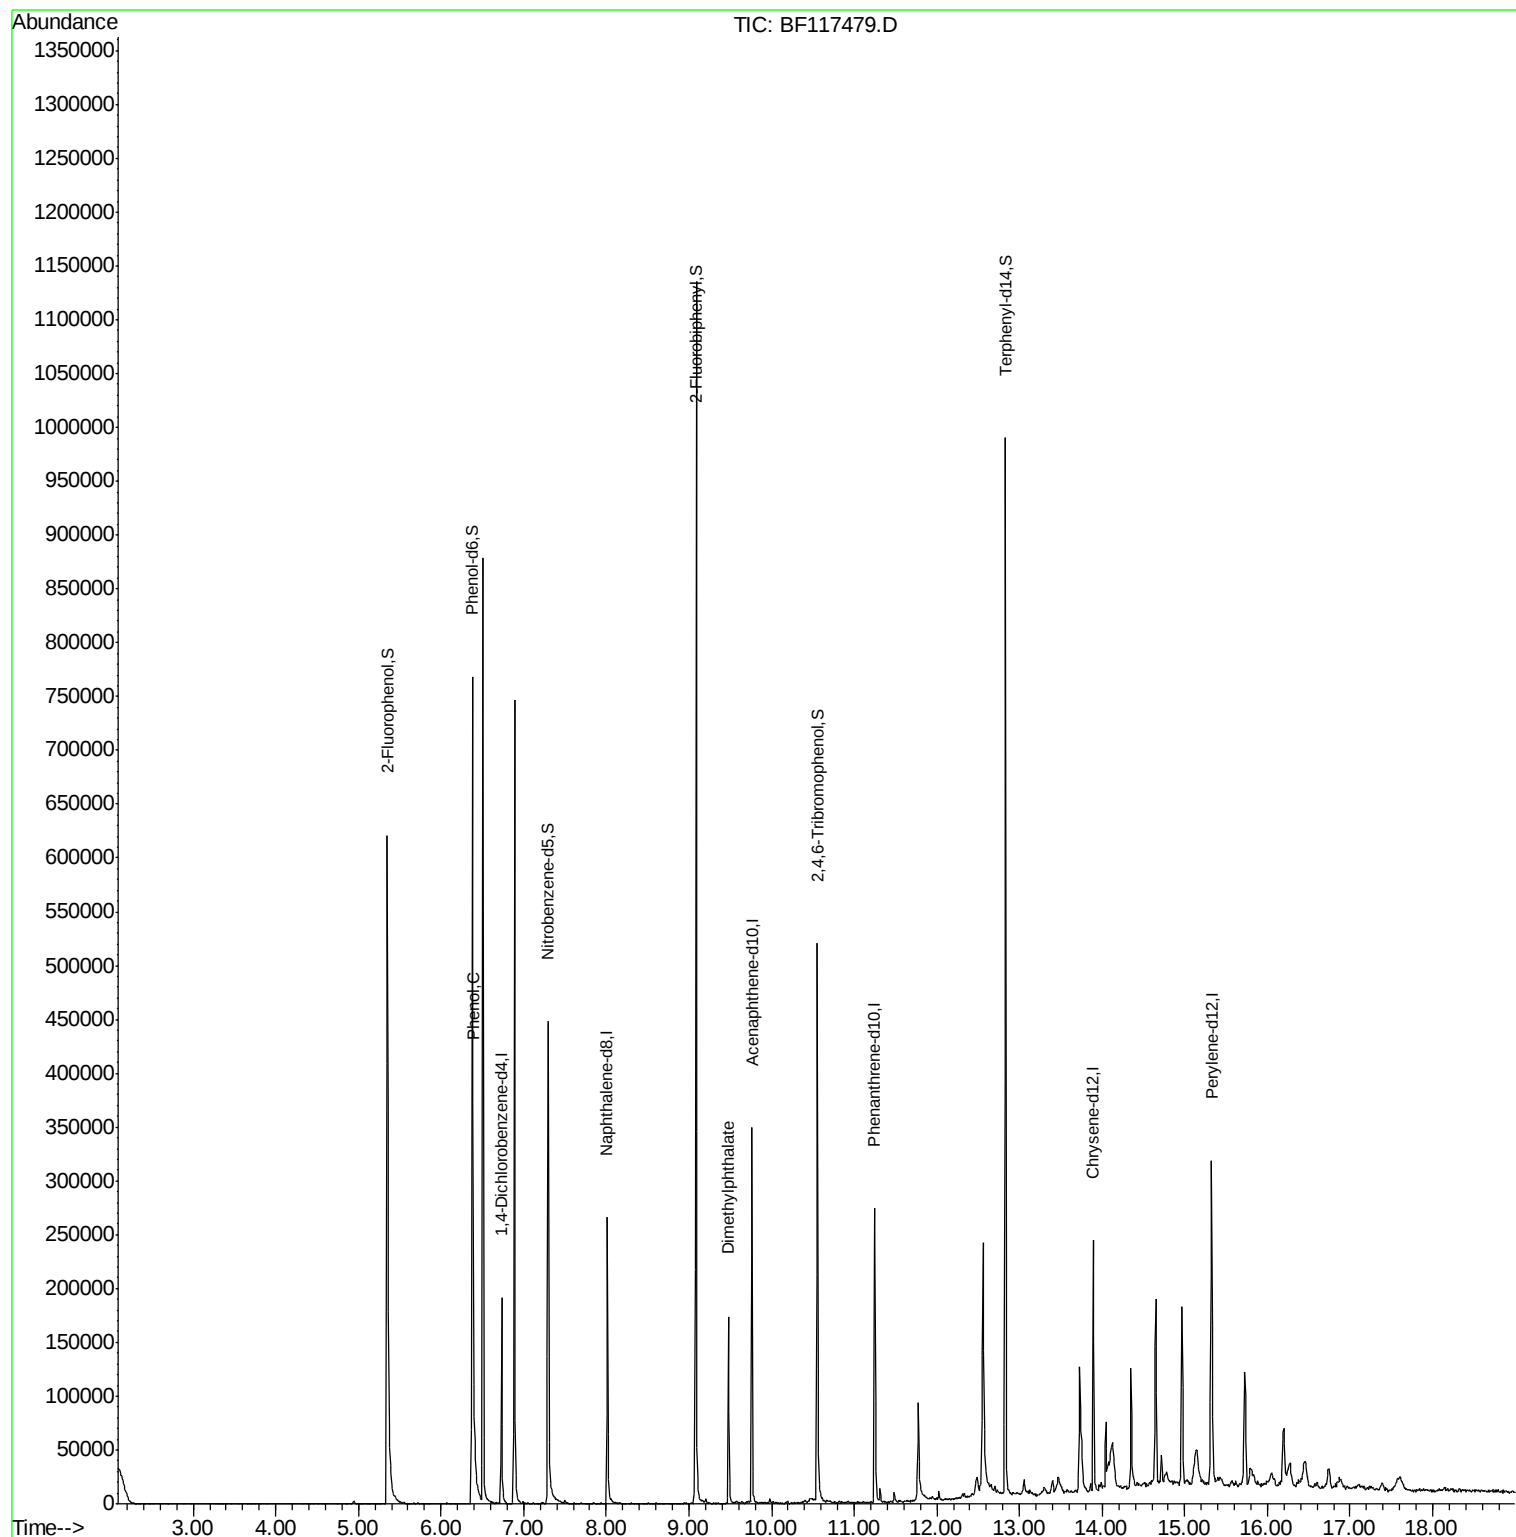

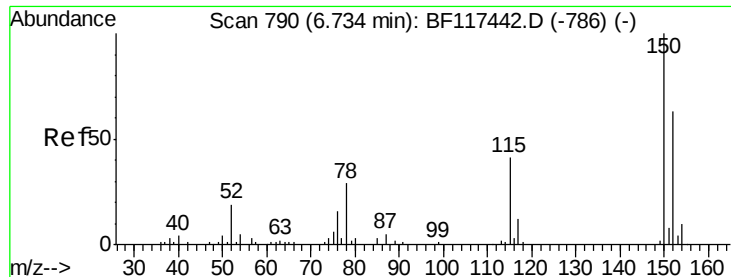


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 790
Delta R.T. -0.00 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51

Instrument :
BNA_F
ClientSampleId :
TP-5

Tot Ion	Ratio	Lower	Upper
152	100		
150	161.1	126.8	190.2
115	59.4	51.6	77.4


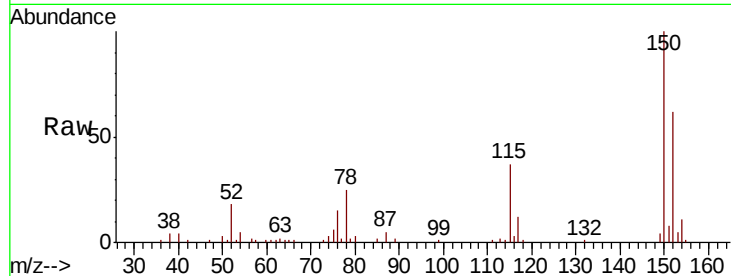


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

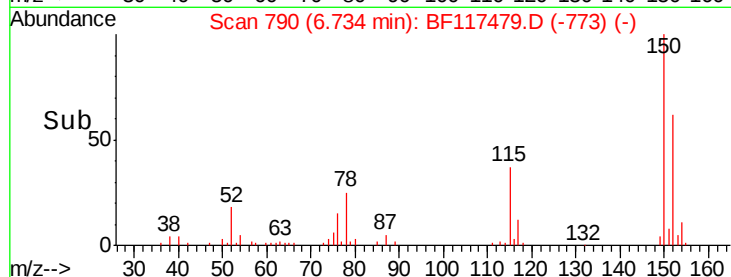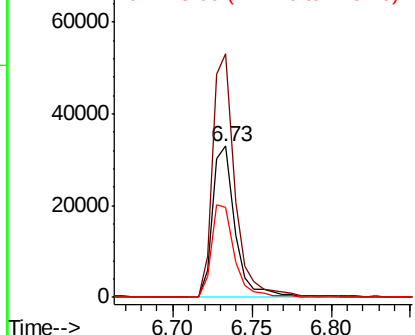

#5

2-Fluorophenol
Concen: 99.068 ng
RT: 5.35 min Scan# 555
Delta R.T. 0.00 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.2	44.1	66.1
63	30.1	23.4	35.2


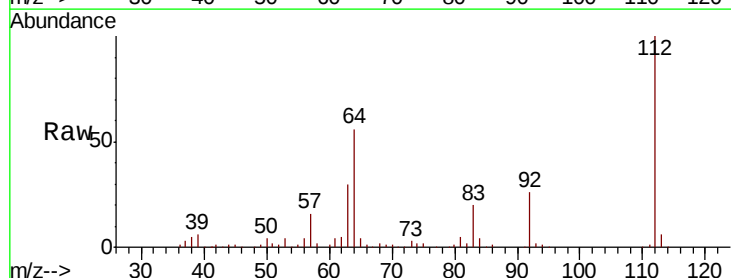



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

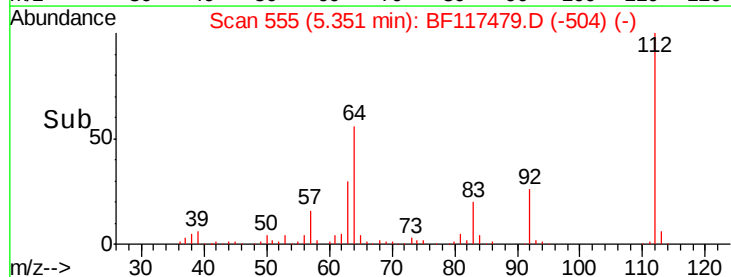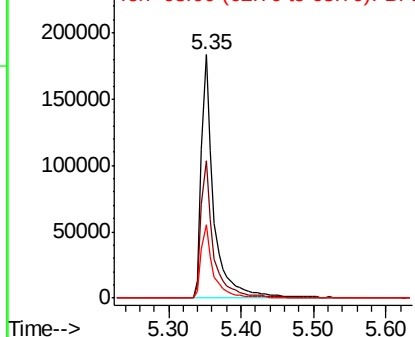

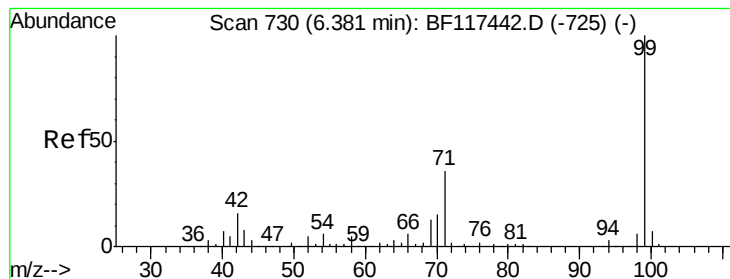

#7

Phenol-d6

Concen: 100.502 ng

RT: 6.38 min Scan# 730

Delta R.T. -0.00 min

Lab File: BF117479.D

Acq: 22 Oct 2019 15:51

Instrument :

BNA_F

ClientSampleId :

TP-5


Tot Ion: 99 Resp: 299468

Ion Ratio Lower Upper




99 100

42 15.1 12.8 19.2

71 37.0 28.6 43.0

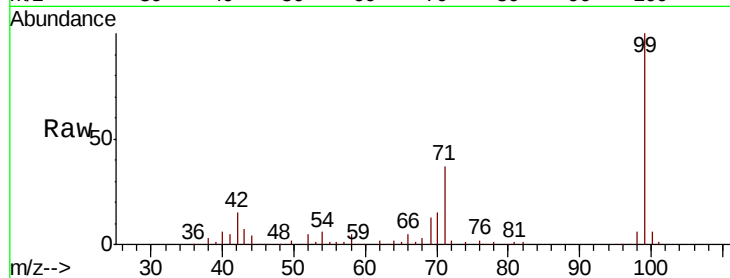

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

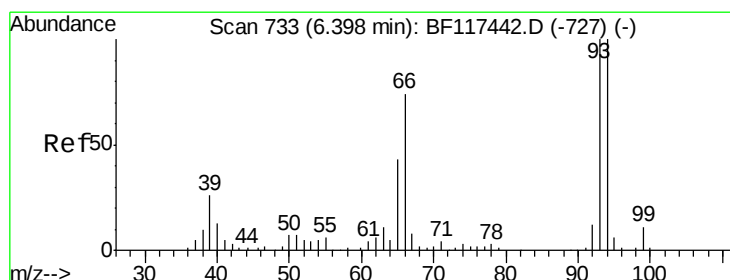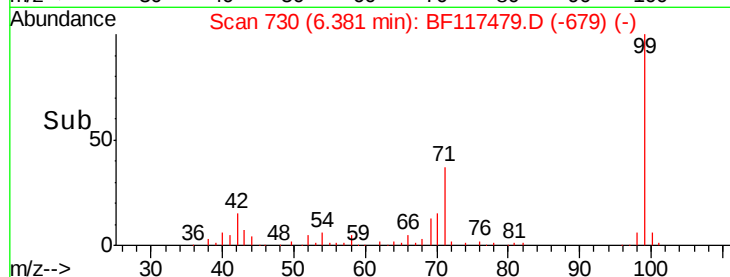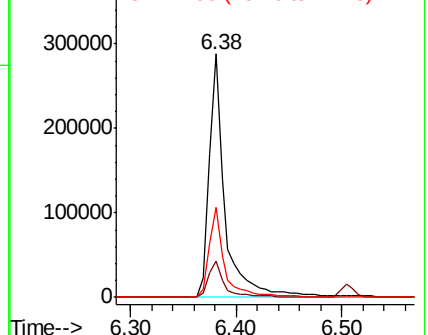

#10

Phenol

Concen: 2.070 ng

RT: 6.39 min Scan# 732

Delta R.T. -0.01 min

Lab File: BF117479.D

Acq: 22 Oct 2019 15:51


Tgt Ion: 94 Resp: 6295

Ion Ratio Lower Upper



94 100

65 44.1 23.4 63.4

66 96.7 54.7 94.7#

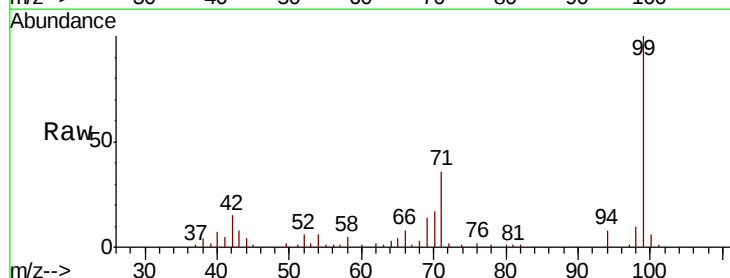

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



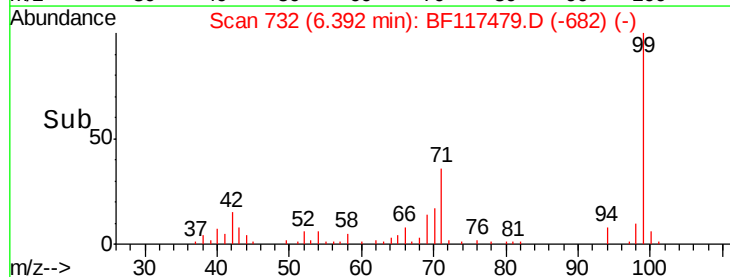
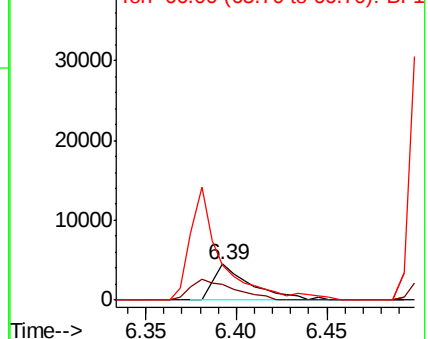




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.01 min Scan# 1007
Delta R.T. -0.01 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51




Instrument :
BNA_F
ClientSampleId :
TP-5


Tot Ion:136	Resp:	129339
Ion	Ratio	Lower Upper
136	100	
137	11.3	8.2 12.4
54	5.5	4.5 6.7
68	5.5	4.3 6.5

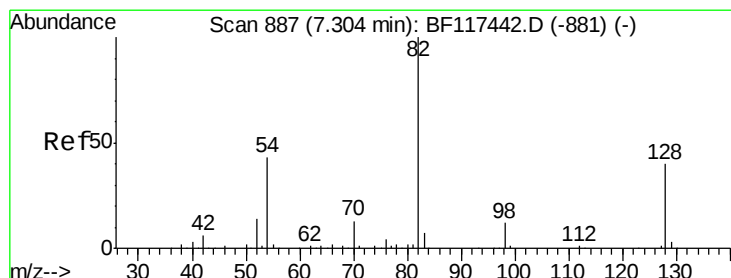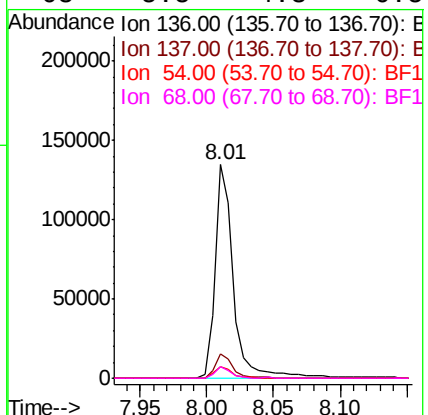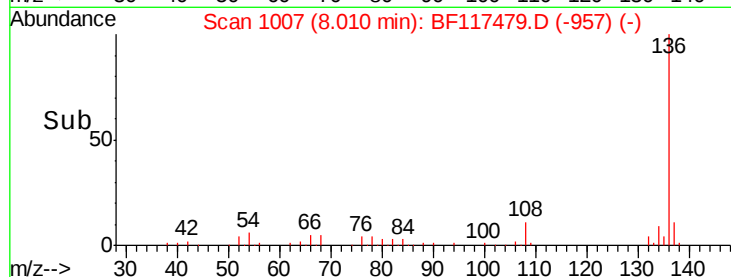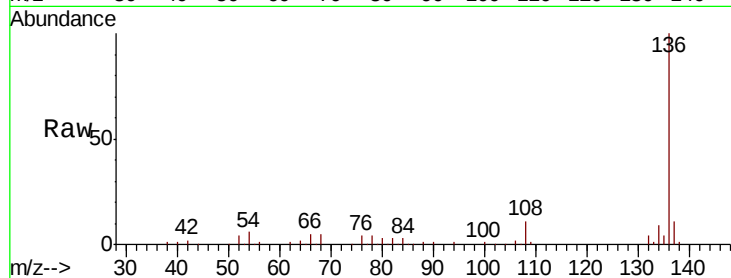

#23
Nitrobenzene-d5
Concen: 71.949 ng
RT: 7.29 min Scan# 885
Delta R.T. -0.01 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51

Tgt Ion: 82	Resp:	188500
Ion	Ratio	Lower Upper
82	100	
128	38.6	32.2 48.2
54	43.6	34.2 51.2

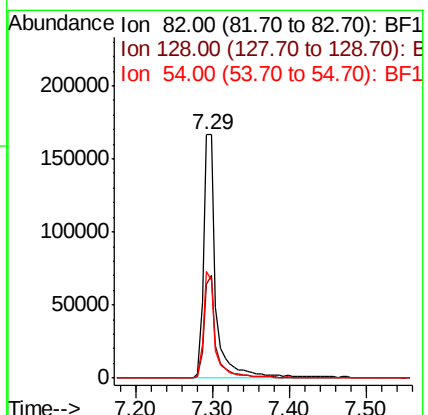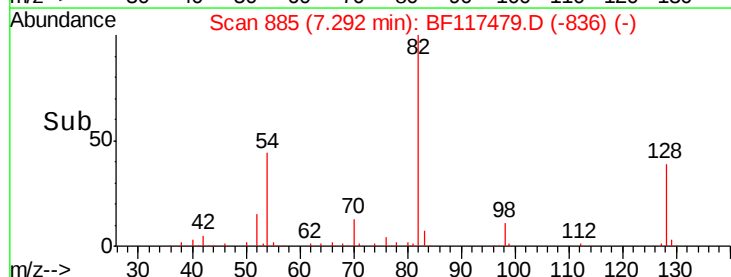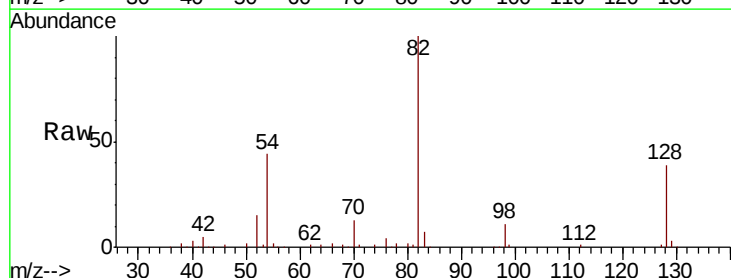


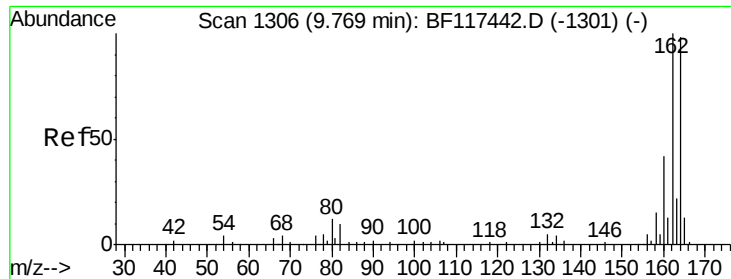




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.76 min Scan# 1305
Delta R.T. -0.01 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51

Instrument :
BNA_F
ClientSampled :
TP-5

Tot Ion:164 Resp: 66944
Ion Ratio Lower Upper
164 100
162 102.1 81.8 122.6
160 41.7 34.4 51.6

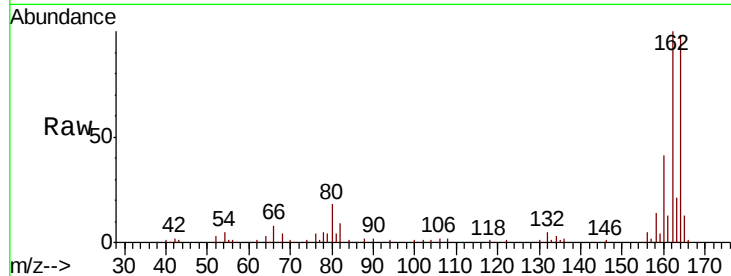


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

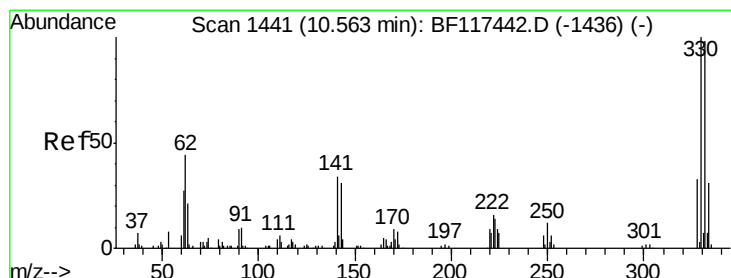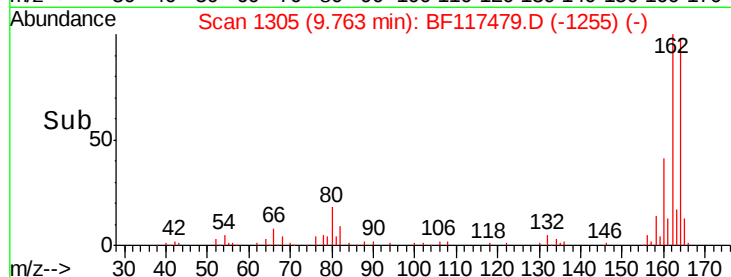
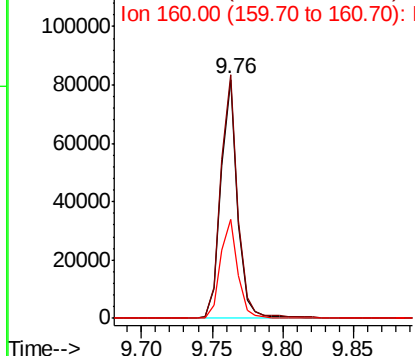


#42
2,4,6-Tribromophenol
Concen: 94.115 ng
RT: 10.56 min Scan# 1440
Delta R.T. -0.01 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51

Tgt Ion:330 Resp: 54515
Ion Ratio Lower Upper
330 100
332 98.1 78.5 117.7
141 46.1 37.0 55.6

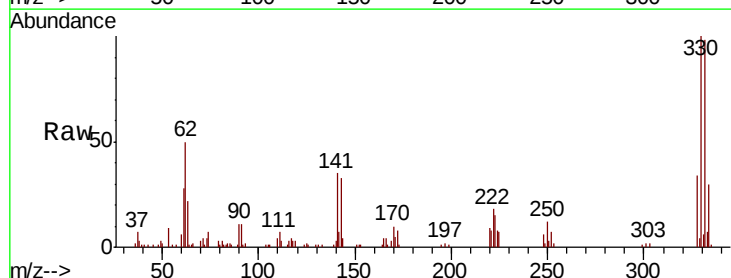

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



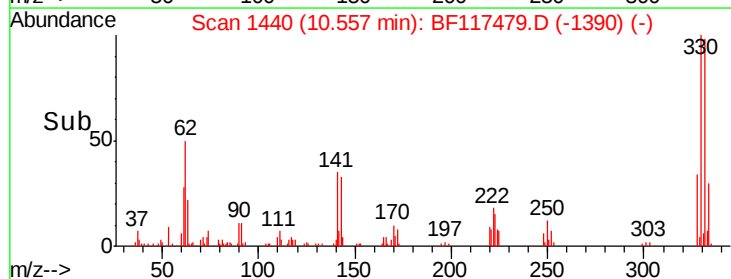
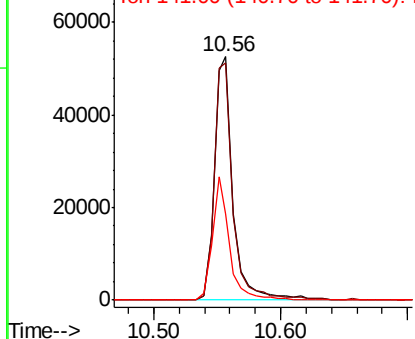




#45
2-Fluorobiphenyl
Concen: 70.661 ng
RT: 9.09 min Scan# 1190
Delta R.T. -0.01 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51




Instrument :
BNA_F
ClientSampled :
TP-5


Tot Ion:172 Resp: 335725
Ion Ratio Lower Upper
172 100
171 35.0 27.5 41.3
170 22.7 18.6 27.8

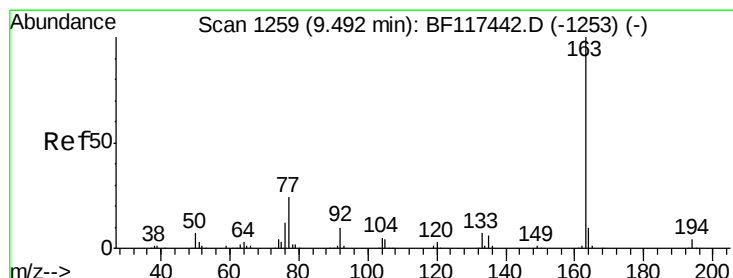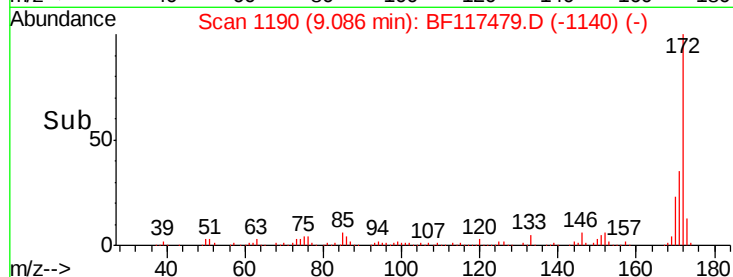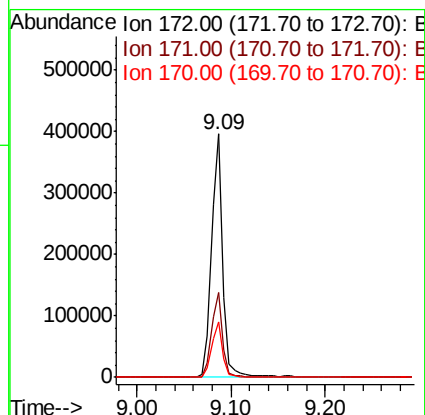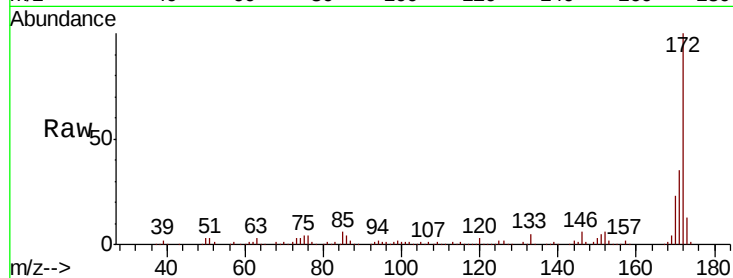

#50
Dimethylphthalate
Concen: 12.685 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.01 min
Lab File: BF117479.D
Acq: 22 Oct 2019 15:51

Tgt Ion:163 Resp: 60536
Ion Ratio Lower Upper
163 100
194 3.8 2.9 4.3
164 10.0 8.2 12.2

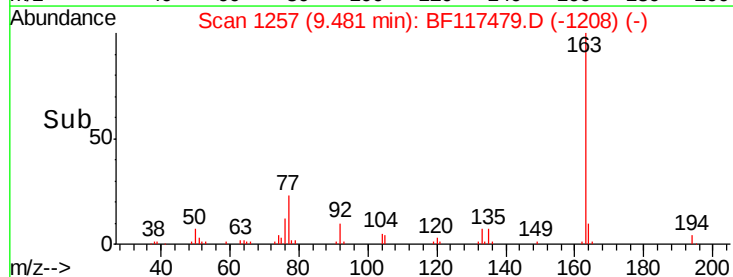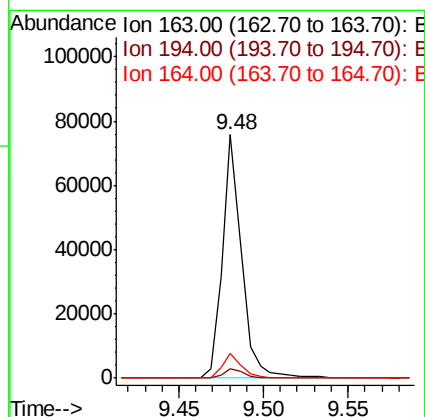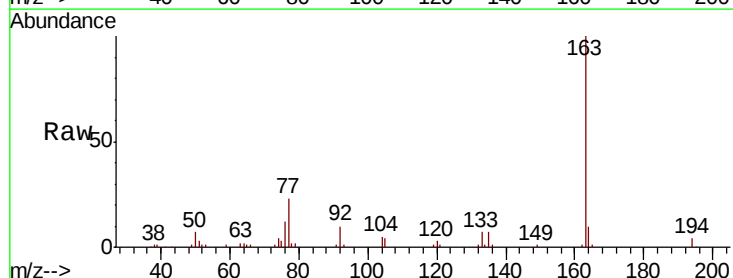

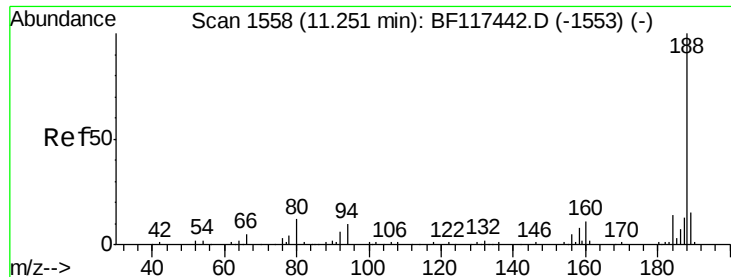

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.25 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF117479.D

Acq: 22 Oct 2019 15:51

Instrument :

BNA_F

ClientSampled :

TP-5


Tot Ion:188 Resp: 109875

Ion Ratio Lower Upper

188 100

94 10.7 8.0 12.0




80 11.9 9.5 14.3

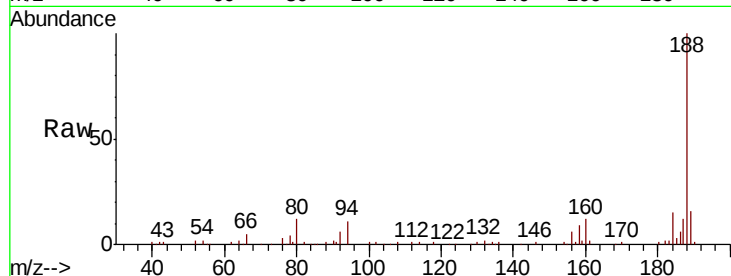

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

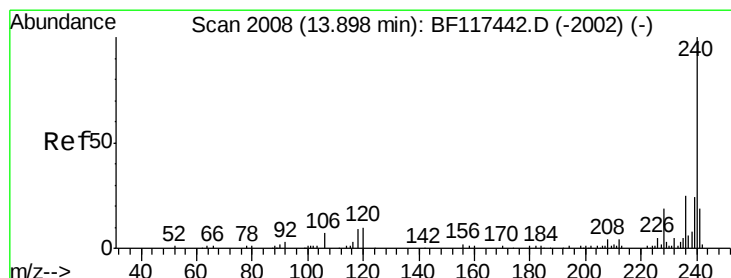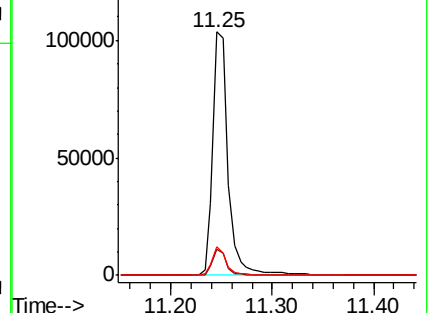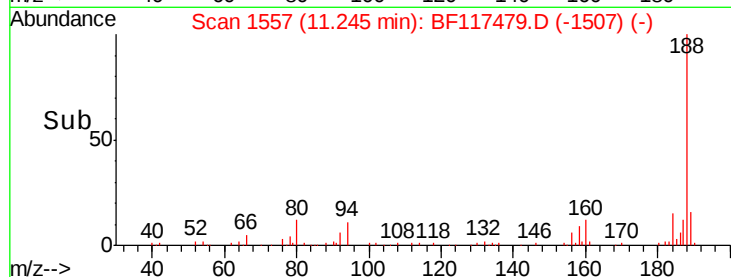

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.89 min Scan# 2007

Delta R.T. -0.01 min

Lab File: BF117479.D

Acq: 22 Oct 2019 15:51


Tgt Ion:240 Resp: 79617

Ion Ratio Lower Upper

240 100

120 12.2 8.4 12.6



236 25.9 20.0 30.0

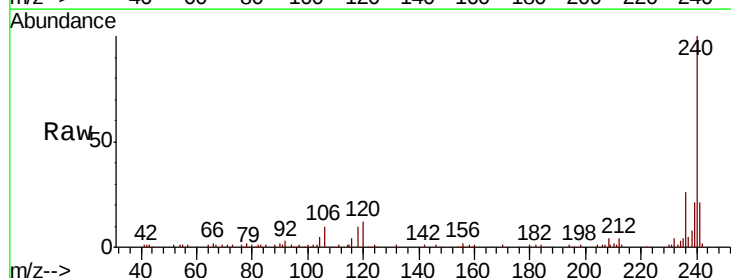


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

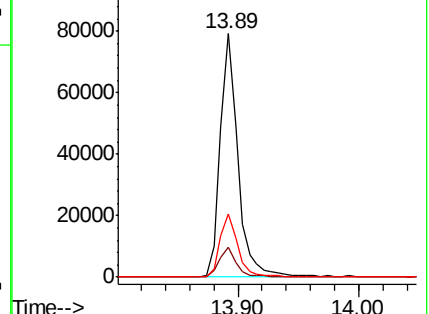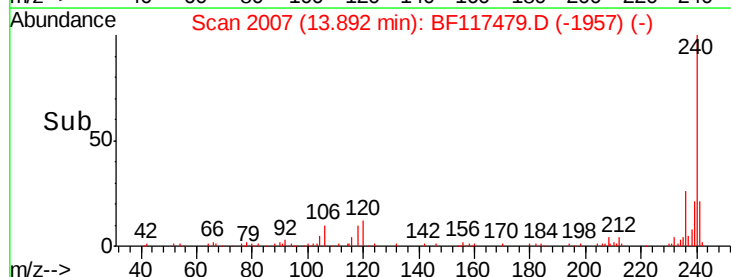

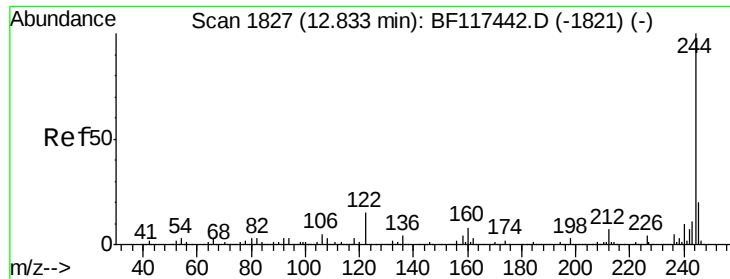

#79

Terphenyl-d14

Concen: 66.806 ng

RT: 12.83 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BF117479.D

Acq: 22 Oct 2019 15:51

Instrument :

BNA_F

ClientSampleId :

TP-5


Tot Ion:244 Resp: 326089

Ion Ratio Lower Upper

244 100

212 6.8 5.8 8.6




122 11.7 11.8 17.8#

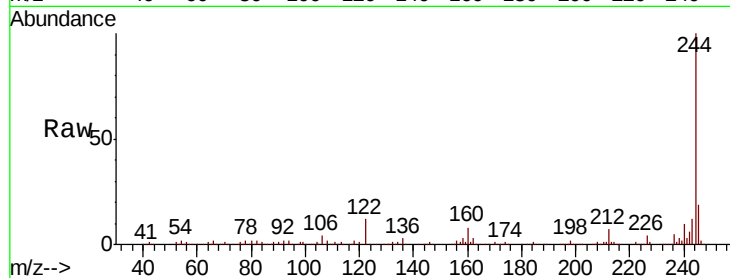

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

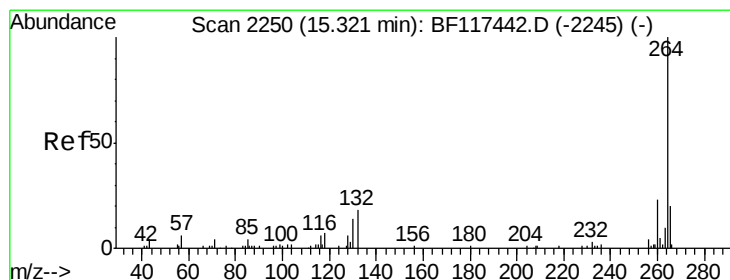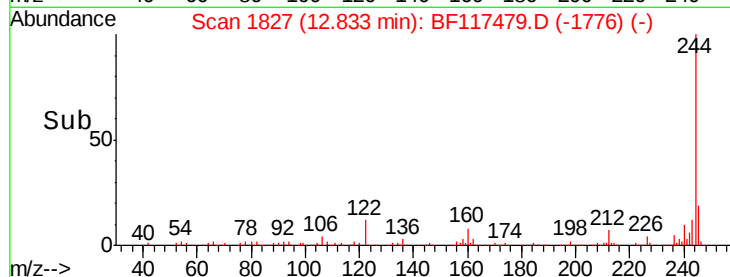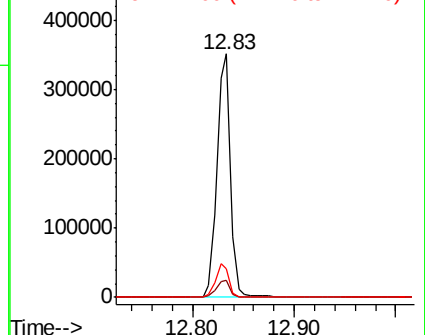

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.33 min Scan# 2251

Delta R.T. 0.01 min

Lab File: BF117479.D

Acq: 22 Oct 2019 15:51


Tgt Ion:264 Resp: 77607

Ion Ratio Lower Upper

264 100

260 24.1 18.4 27.6

265 21.0 16.1 24.1

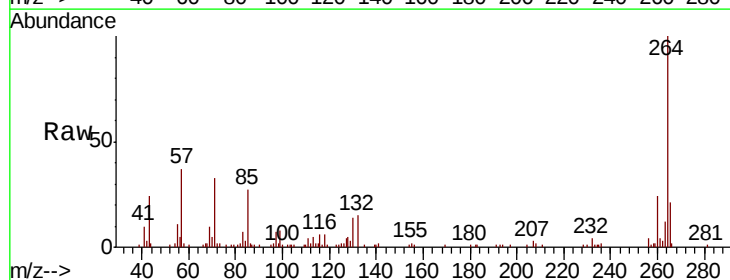

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

