


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102318\
 Data File : BF110070.D
 Acq On : 23 Oct 2018 10:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 23 15:06:18 2018

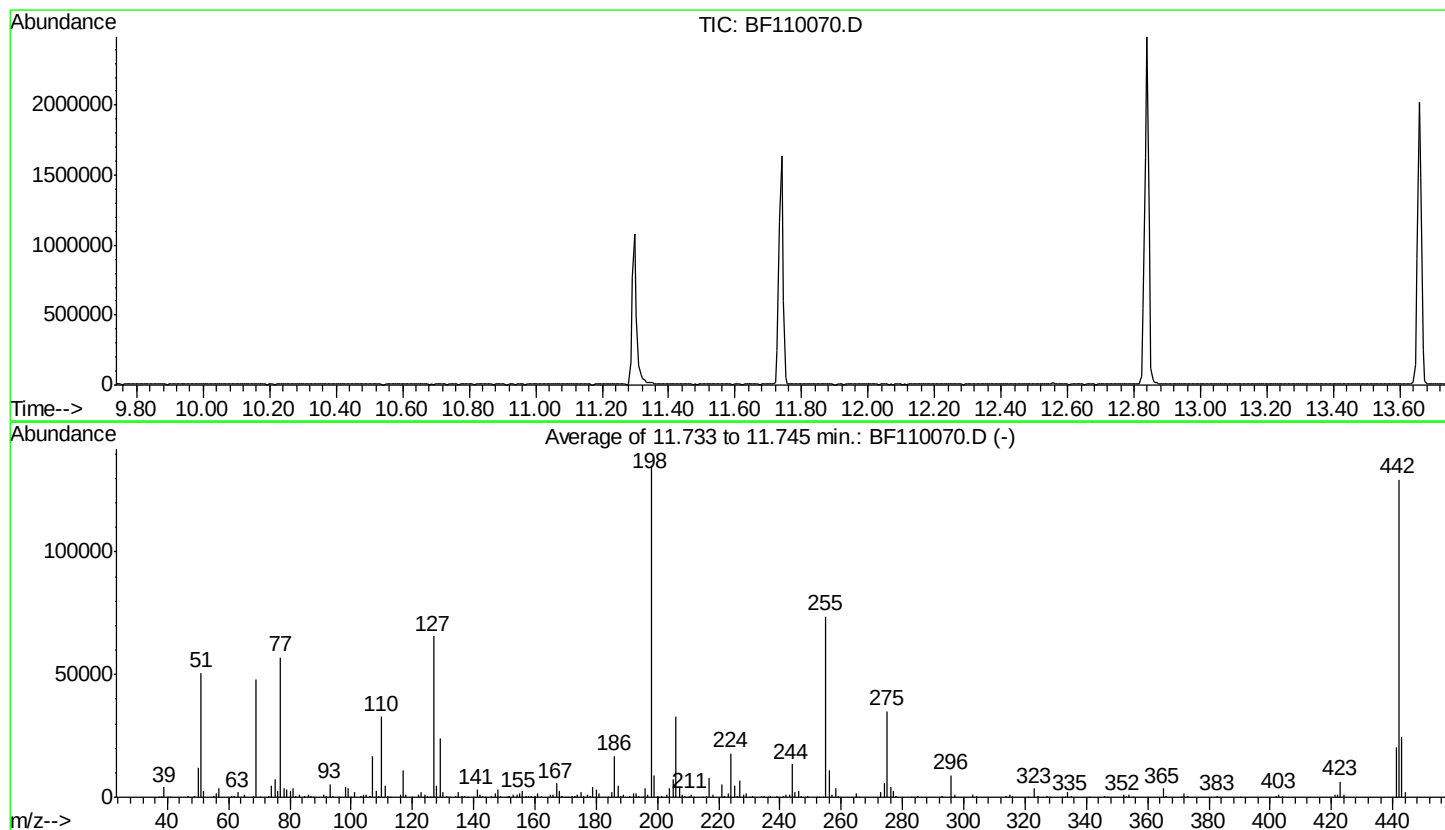

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	50888	PASS
68	69	0.00	2	1.5	707	PASS
69	198	0.00	100	35.6	48104	PASS
70	69	0.00	2	0.3	130	PASS
127	198	10	80	48.5	65600	PASS
197	198	0.00	2	0.6	802	PASS
198	198	100	100	100.0	135181	PASS
199	198	5	9	6.4	8700	PASS
275	198	10	60	25.9	35045	PASS
365	198	1	100	2.6	3580	PASS
441	198	0.01	100	14.9	20141	PASS
442	198	50	100	95.7	129421	PASS
443	442	15	24	18.9	24417	PASS