

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102319\
 Data File : BF117489.D
 Acq On : 23 Oct 2019 18:04
 Operator : JU
 Sample : K5485-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-24B-S

Quant Time: Oct 24 08:45:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 18:53:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	43772	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	177350	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	93573	20.00	ng	0.00
64) Phenanthrene-d10	11.25	188	154487	20.00	ng	0.00
76) Chrysene-d12	13.89	240	113556	20.00	ng	0.00
87) Perylene-d12	15.32	264	95620	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	250796	85.24	ng	0.00
7) Phenol-d6	6.38	99	352697	89.25	ng	0.00
23) Nitrobenzene-d5	7.30	82	211852	58.97	ng	0.00
42) 2,4,6-Tribromophenol	10.56	330	69125	85.38	ng	0.00
45) 2-Fluorobiphenyl	9.09	172	368581	55.50	ng	0.00
79) Terphenyl-d14	12.83	244	372698	53.53	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.48	163	54266	8.135	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102319\
Data File : BF117489.D
Acq On : 23 Oct 2019 18:04
Operator : JU
Sample : K5485-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-24B-S

Quant Time: Oct 24 08:45:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

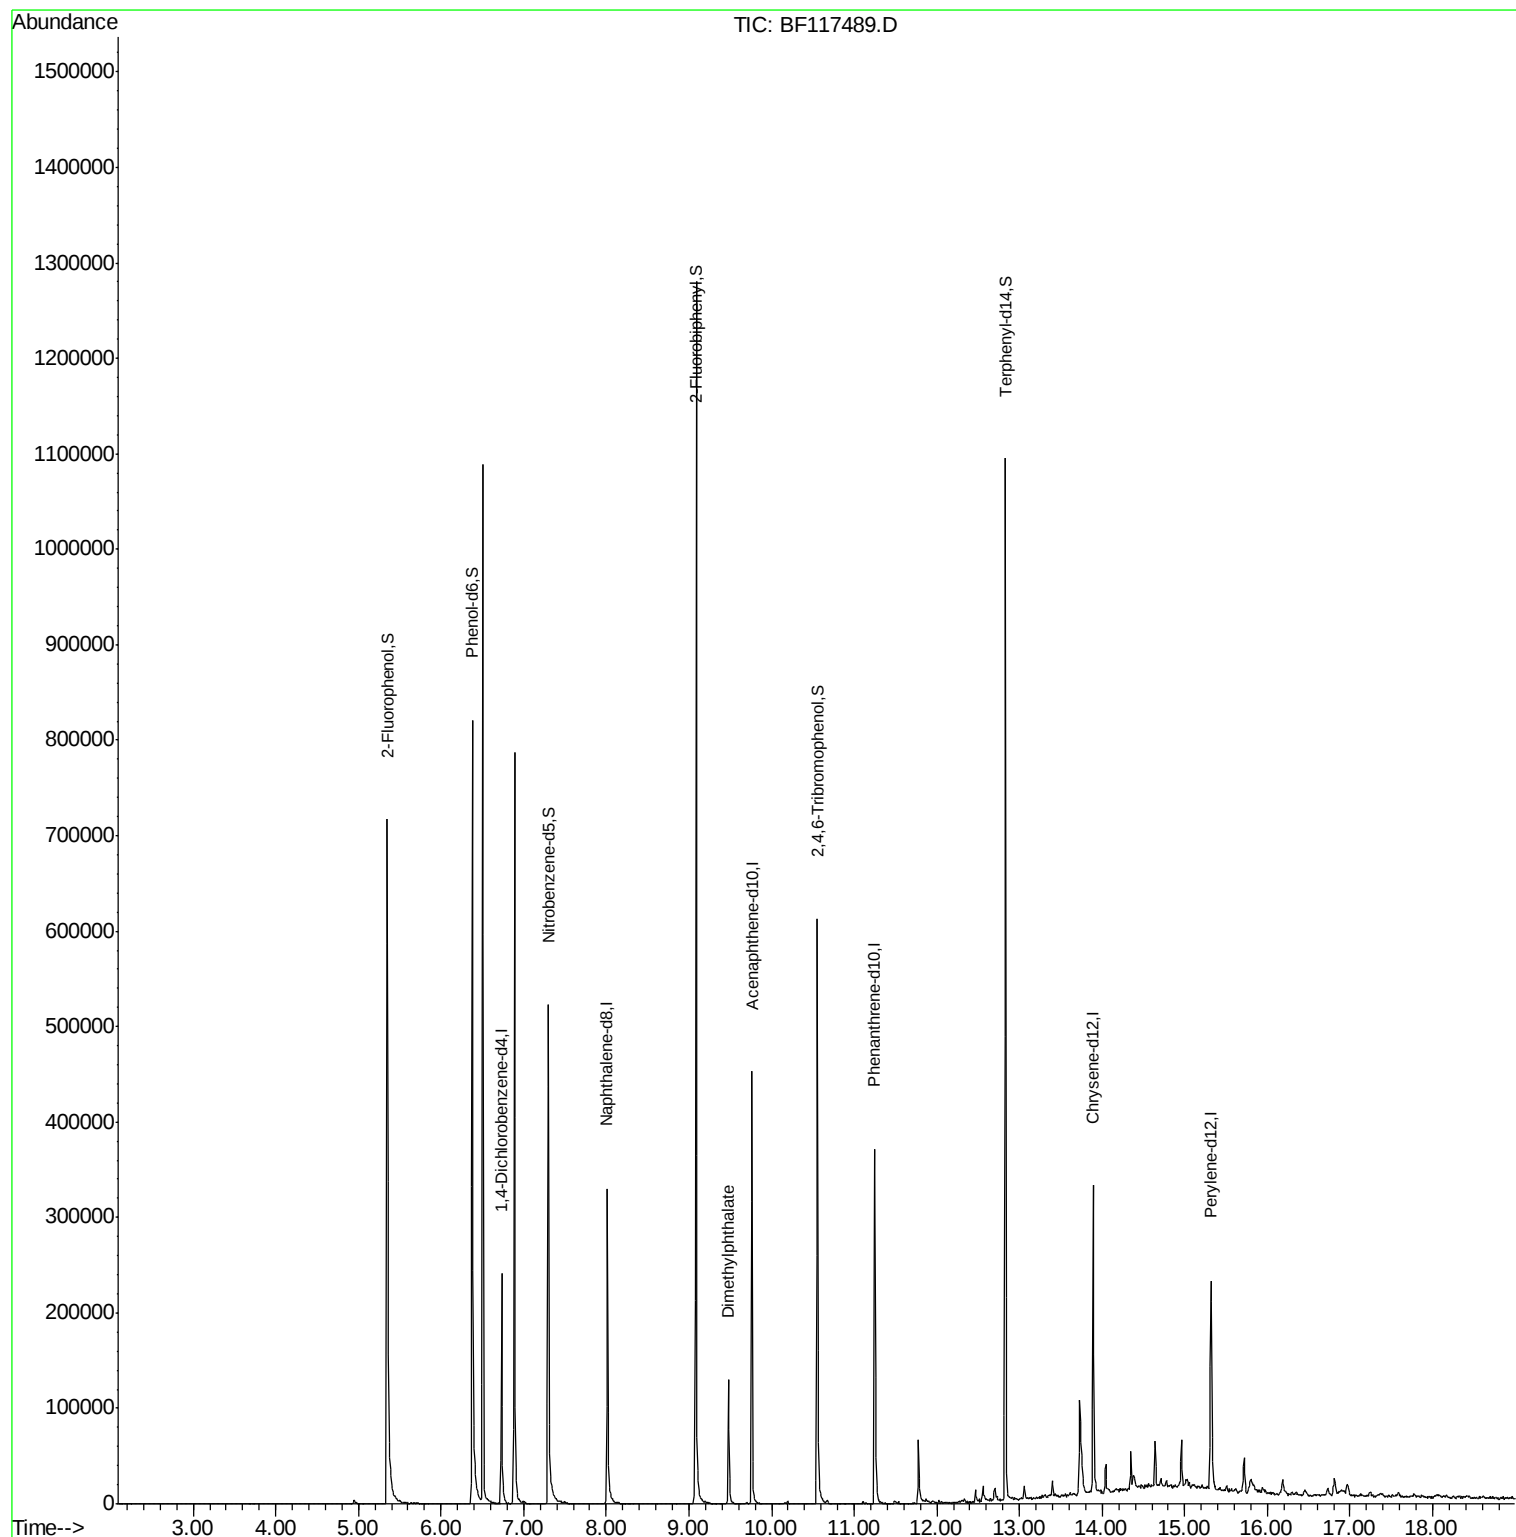

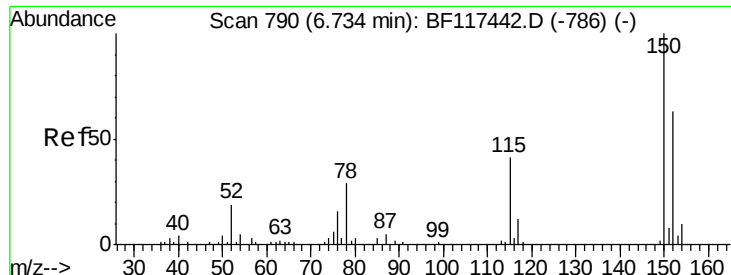


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 790
Delta R.T. -0.00 min
Lab File: BF117489.D
Acq: 23 Oct 2019 18:04

Instrument :
BNA_F
ClientSampleId :
TP-24B-S

Tot Ion:152 Resp: 43772
Ion Ratio Lower Upper
152 100
150 154.1 126.8 190.2
115 60.9 51.6 77.4

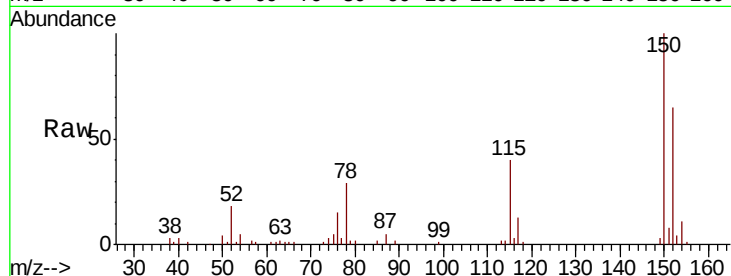


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

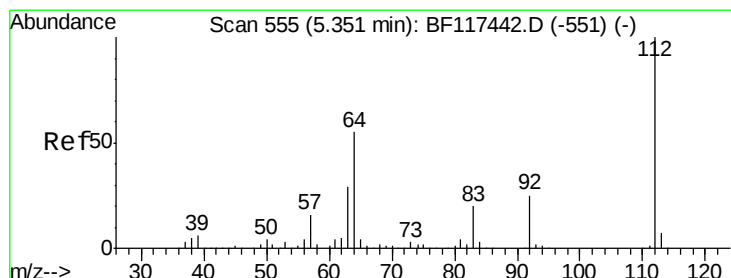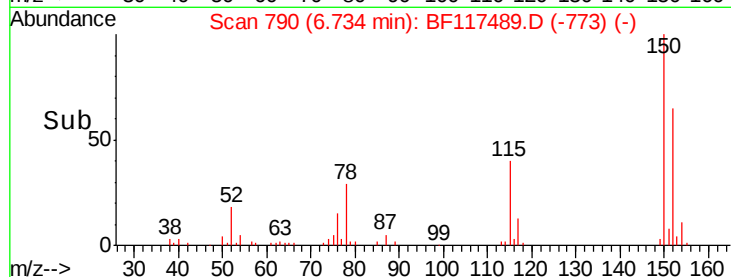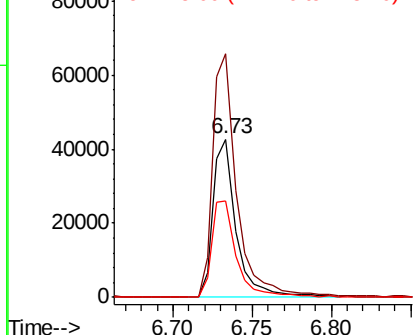



#5


2-Fluorophenol
Concen: 85.239 ng
RT: 5.35 min Scan# 555
Delta R.T. -0.00 min
Lab File: BF117489.D
Acq: 23 Oct 2019 18:04

Tgt Ion:112 Resp: 250796
Ion Ratio Lower Upper
112 100
64 56.6 44.1 66.1
63 29.8 23.4 35.2

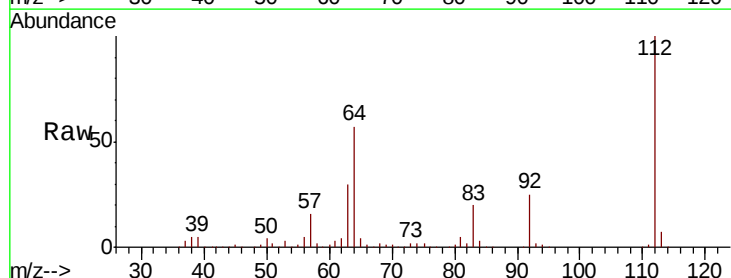

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

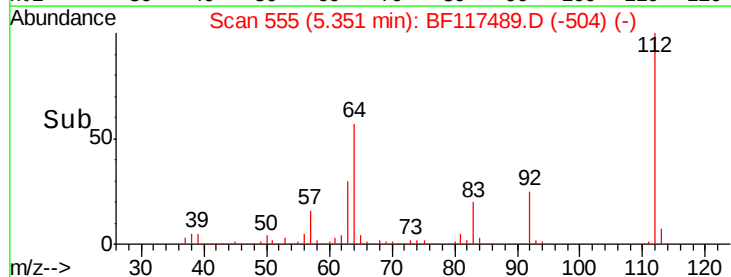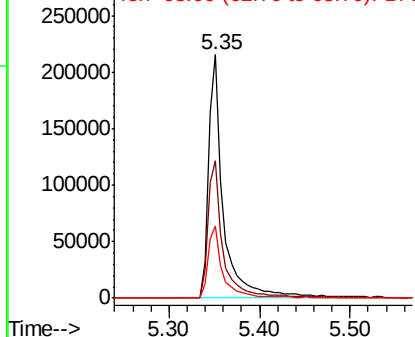

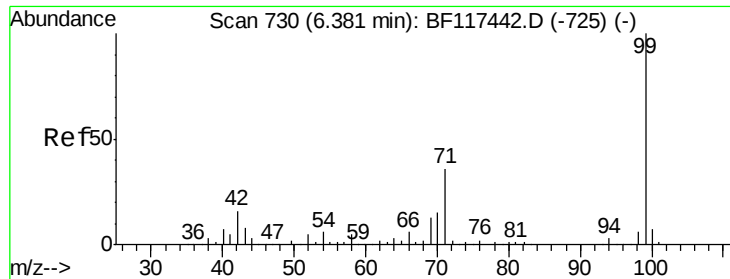

#7

Phenol-d6

Concen: 89.250 ng

RT: 6.38 min Scan# 730

Delta R.T. -0.00 min

Lab File: BF117489.D

Acq: 23 Oct 2019 18:04

Instrument :

BNA_F

ClientSampleId :

TP-24B-S


Tot Ion: 99 Resp: 352697

Ion Ratio Lower Upper




99 100

42 14.6 12.8 19.2

71 36.0 28.6 43.0

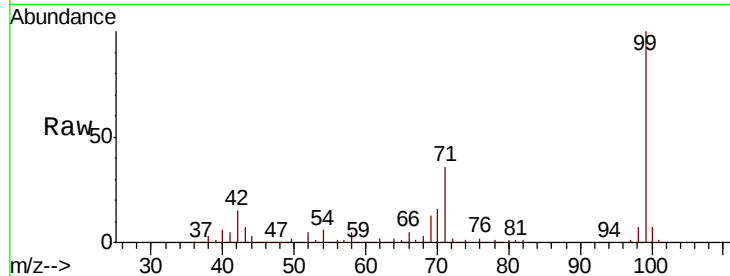

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

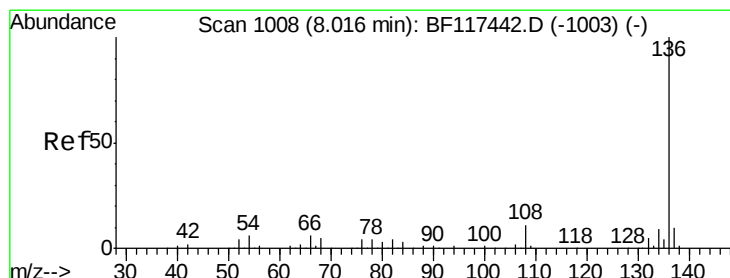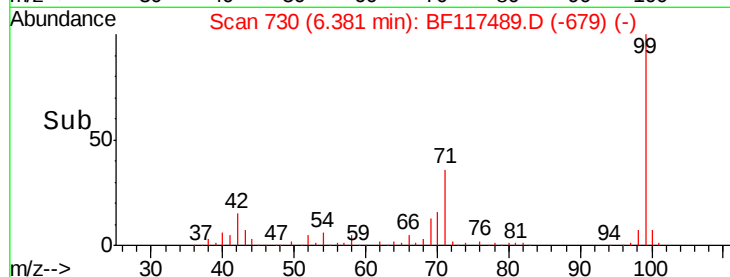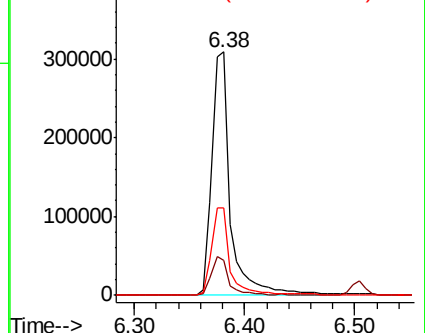

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.01 min

Lab File: BF117489.D

Acq: 23 Oct 2019 18:04

Tgt Ion: 136 Resp: 177350


Ion Ratio Lower Upper

136 100



137 10.7 8.2 12.4


54 6.1 4.5 6.7

68 5.2 4.3 6.5

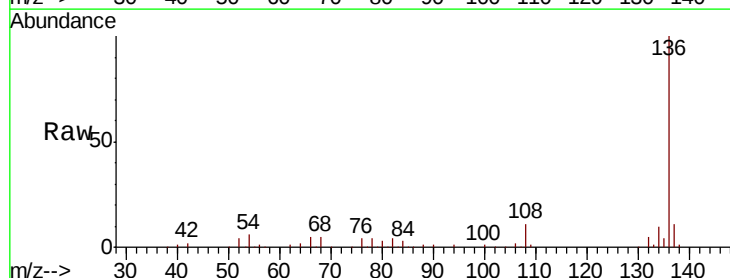

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



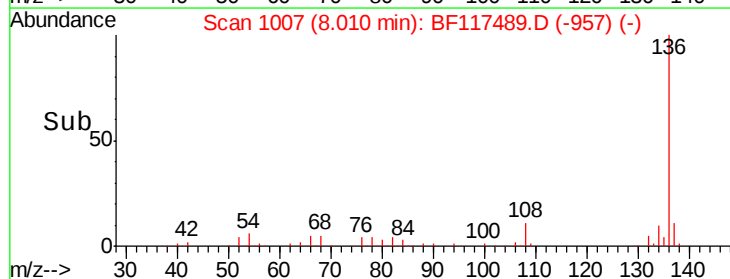
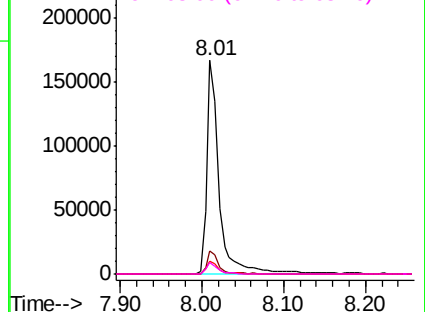


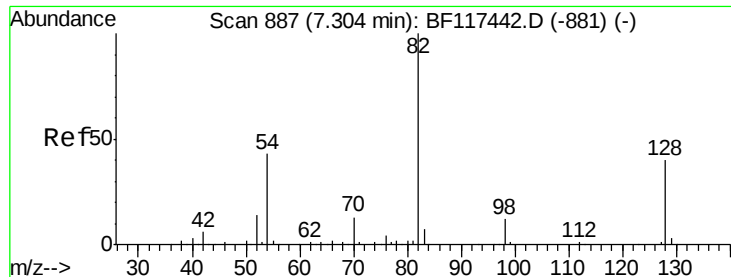

#23
Nitrobenzene-d5
Concen: 58.972 ng
RT: 7.30 min Scan# 886
Delta R.T. -0.01 min
Lab File: BF117489.D
Acq: 23 Oct 2019 18:04




Instrument :
BNA_F
ClientSampleId :
TP-24B-S


Tot Ion: 82 Resp: 211852
Ion Ratio Lower Upper
82 100
128 43.2 32.2 48.2
54 41.2 34.2 51.2

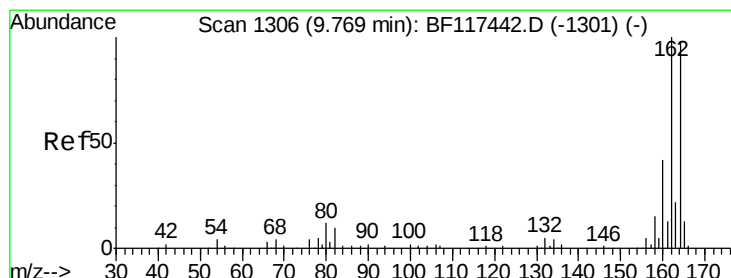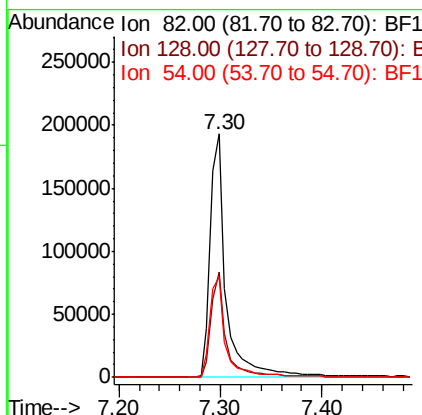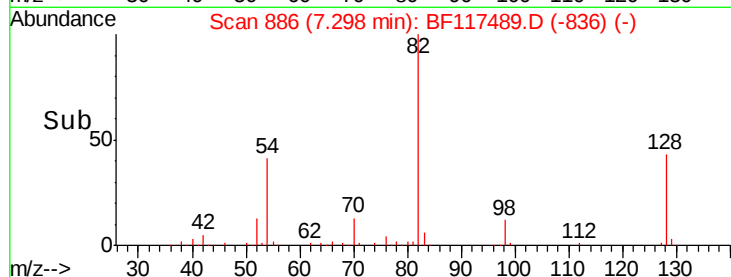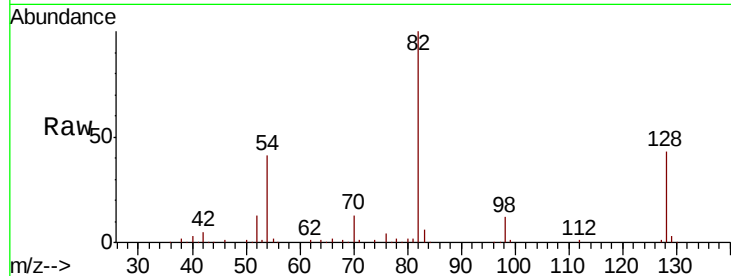

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.76 min Scan# 1305
Delta R.T. -0.01 min
Lab File: BF117489.D
Acq: 23 Oct 2019 18:04

Tgt Ion:164 Resp: 93573
Ion Ratio Lower Upper
164 100
162 98.6 81.8 122.6
160 42.3 34.4 51.6

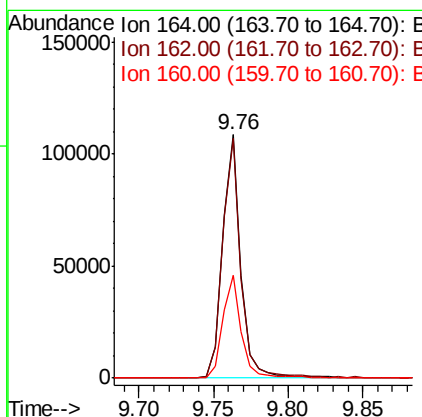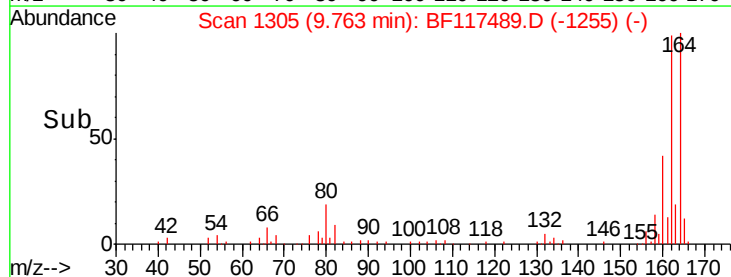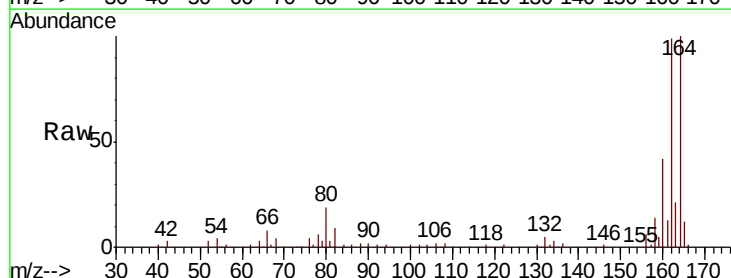


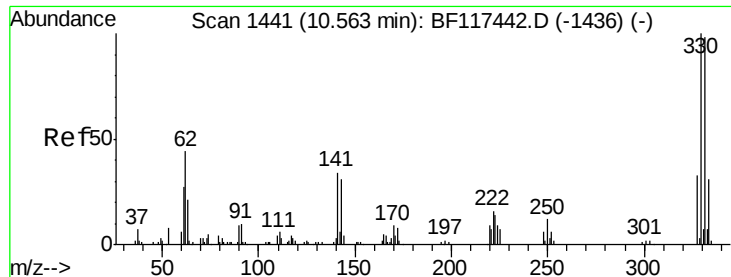




#42
 2,4,6-Tribromophenol
 Concen: 85.377 ng
 RT: 10.56 min Scan# 1440
 Delta R.T. -0.01 min
 Lab File: BF117489.D
 Acq: 23 Oct 2019 18:04

Instrument :
 BNA_F
 ClientSampleId :
 TP-24B-S

Tot Ion:330 Resp: 69125
 Ion Ratio Lower Upper
 330 100
 332 97.1 78.5 117.7
 141 46.6 37.0 55.6

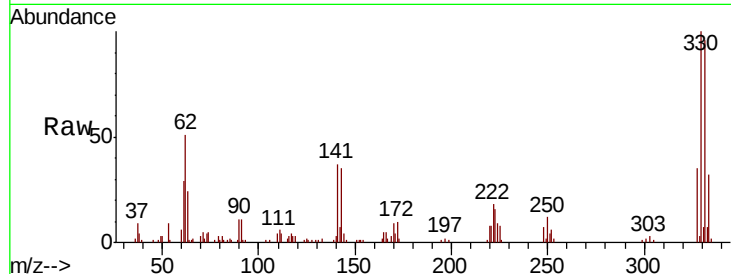


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

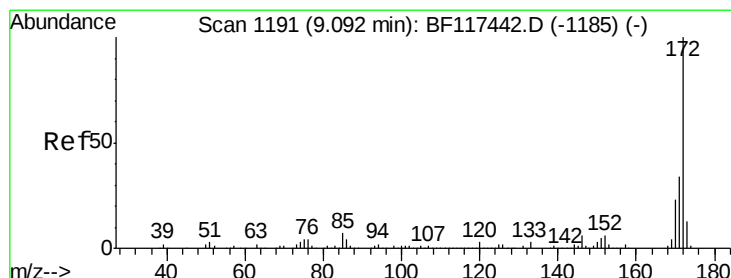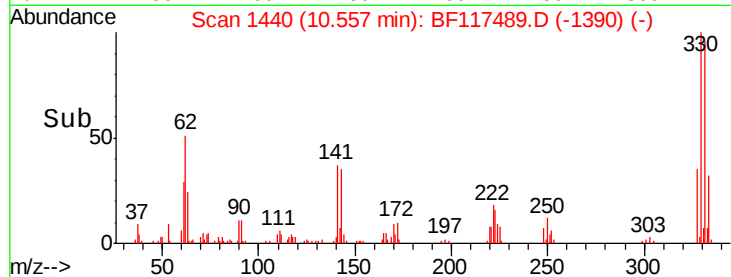
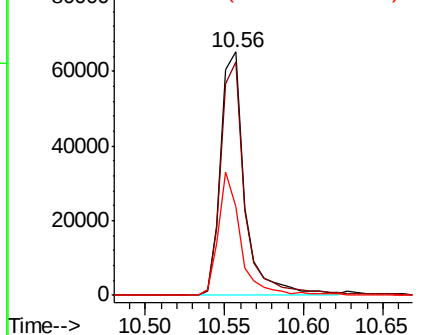



#45
 2-Fluorobiphenyl
 Concen: 55.500 ng
 RT: 9.09 min Scan# 1190
 Delta R.T. -0.01 min
 Lab File: BF117489.D
 Acq: 23 Oct 2019 18:04

Tgt Ion:172 Resp: 368581
 Ion Ratio Lower Upper
 172 100
 171 34.6 27.5 41.3
 170 22.7 18.6 27.8

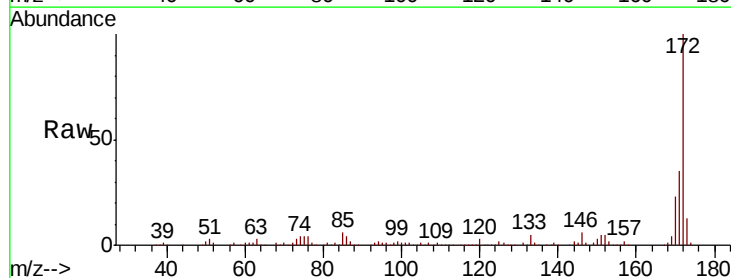

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

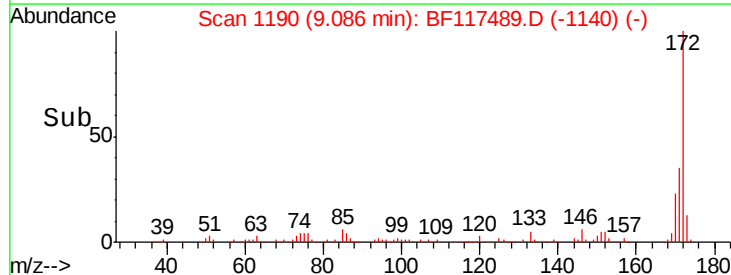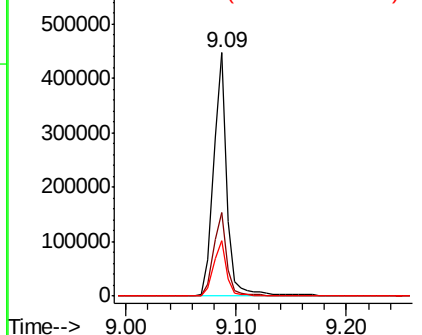


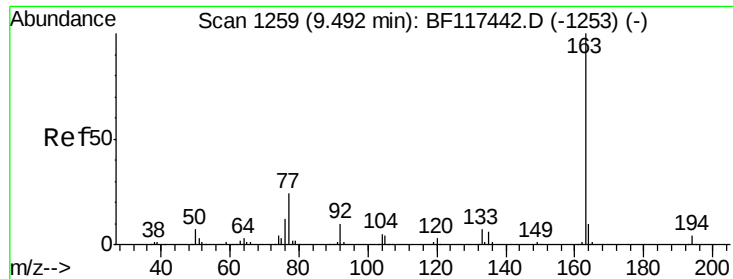




#50
Dimethylphthalate
Concen: 8.135 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.01 min
Lab File: BF117489.D
Acq: 23 Oct 2019 18:04

Instrument :
BNA_F
ClientSampleId :
TP-24B-S

Tot Ion:163 Resp: 54266
Ion Ratio Lower Upper
163 100
194 3.6 2.9 4.3
164 10.8 8.2 12.2

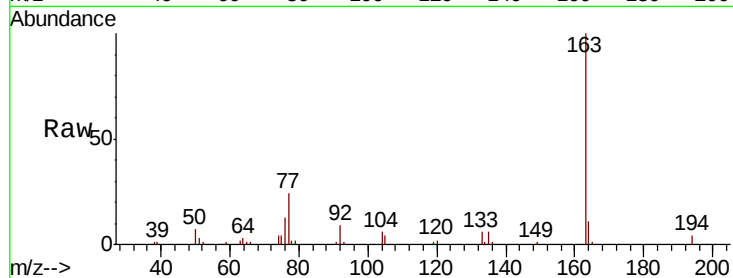


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

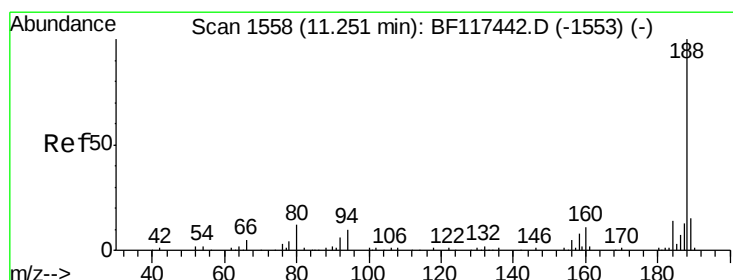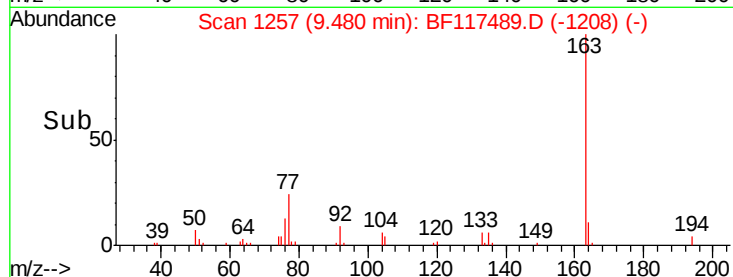
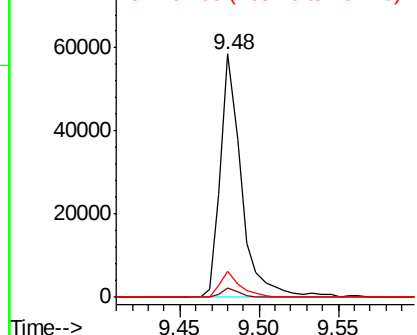



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.25 min Scan# 1557
Delta R.T. -0.01 min
Lab File: BF117489.D
Acq: 23 Oct 2019 18:04

Tgt Ion:188 Resp: 154487
Ion Ratio Lower Upper
188 100
94 10.4 8.0 12.0
80 11.8 9.5 14.3

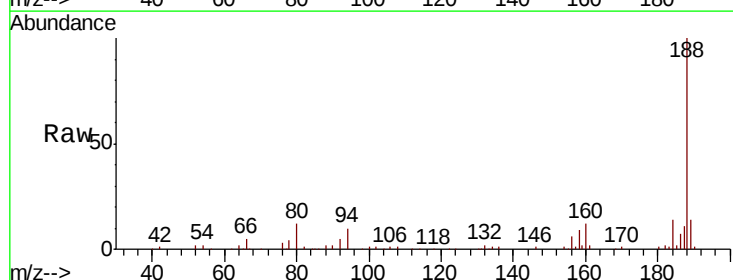

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1



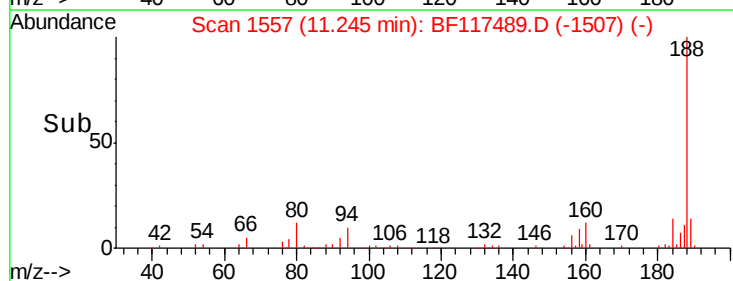
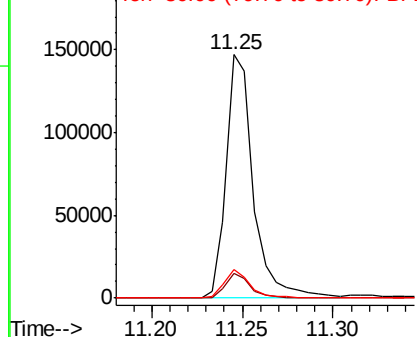


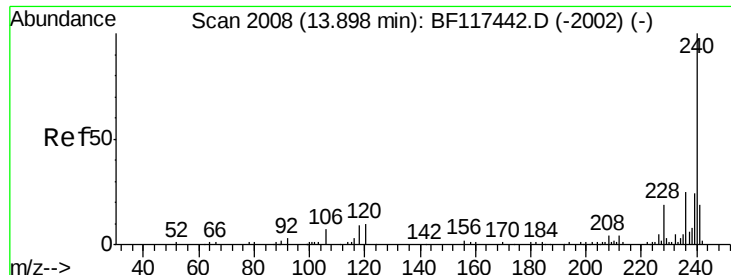

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.89 min Scan# 2007
 Delta R.T. -0.01 min
 Lab File: BF117489.D
 Acq: 23 Oct 2019 18:04




Instrument :
 BNA_F
 ClientSampleId :
 TP-24B-S


Tot Ion	Ratio	Lower	Upper
240	100		
120	10.4	8.4	12.6
236	26.5	20.0	30.0

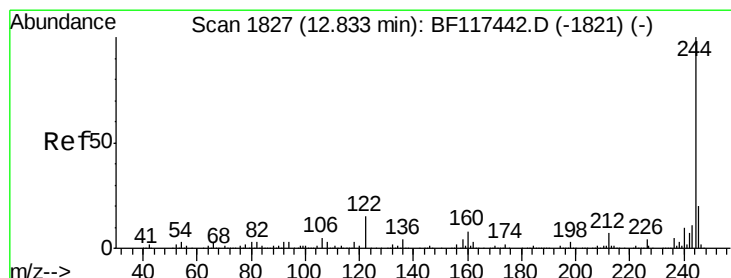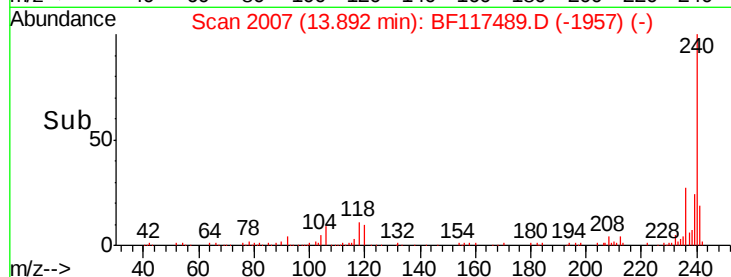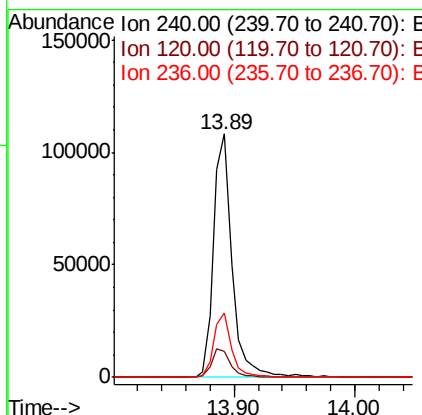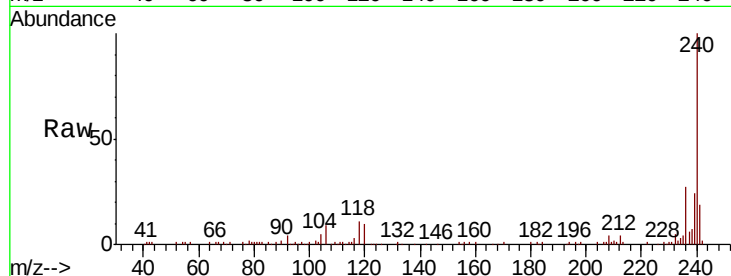

#79
 Terphenyl-d14
 Concen: 53.534 ng
 RT: 12.83 min Scan# 1827
 Delta R.T. -0.00 min
 Lab File: BF117489.D
 Acq: 23 Oct 2019 18:04

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.6	5.8	8.6
122	10.5	11.8	17.8#

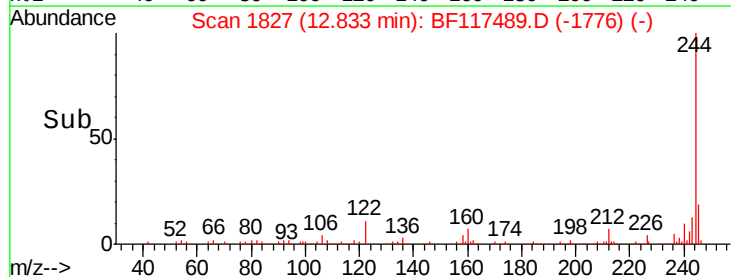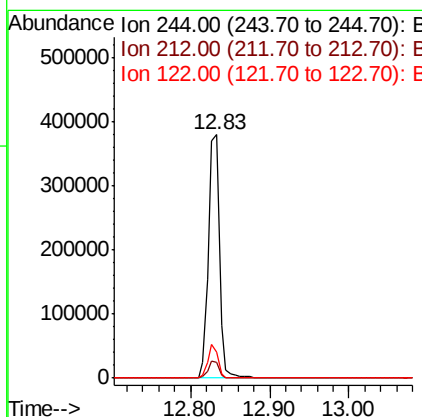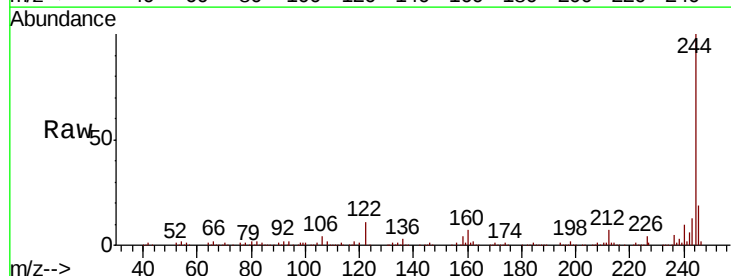

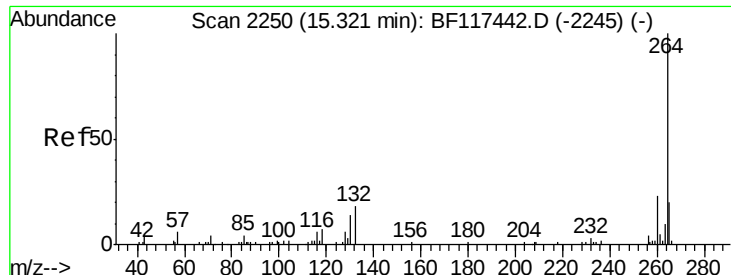

#87
Pervlone-d12
Concen: 20.000 ng
RT: 15.32 min Scan# 2250
Delta R.T. -0.00 min
Lab File: BF117489.D
Acq: 23 Oct 2019 18:04

Instrument :
BNA_F
ClientSampleId :
TP-24B-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.4	27.6
265	21.1	16.1	24.1

