

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102418\
 Data File : BF110136.D
 Acq On : 25 Oct 2018 1:53
 Operator : JU/SJ
 Sample : J5640-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 25 09:04:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 25 02:28:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	124061	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	424965	20.00	ng	0.00
39) Acenaphthene-d10	10.01	164	159118	20.00	ng	0.00
64) Phenanthrene-d10	11.50	188	268330	20.00	ng	0.00
76) Chrysene-d12	14.15	240	237772	20.00	ng	0.00
87) Perylene-d12	15.67	264	157942	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	299356	39.29	ng	0.00
7) Phenol-d6	6.58	99	226581	23.25	ng	0.00
23) Nitrobenzene-d5	7.53	82	708429	98.88	ng	0.00
42) 2,4,6-Tribromophenol	10.80	330	123103	78.10	ng	0.00
45) 2-Fluorobiphenyl	9.33	172	1175539	116.01	ng	0.00
79) Terphenyl-d14	13.09	244	995238	87.05	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.53	70	93818	15.007	ng	# 78
25) Isophorone	7.53	82	708423	58.005	ng	# 67
51) 2,6-Dinitrotoluene	10.01	165	20417	8.070	ng	# 23
57) 2,4-Dinitrotoluene	10.01	165	20417	6.353	ng	# 19
67) 4-Bromophenyl-phenylether	10.80	248	8156	2.802	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102418\
Data File : BF110136.D
Acq On : 25 Oct 2018 1:53
Operator : JU/SJ
Sample : J5640-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 25 09:04:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 25 02:28:50 2018
Response via : Initial Calibration

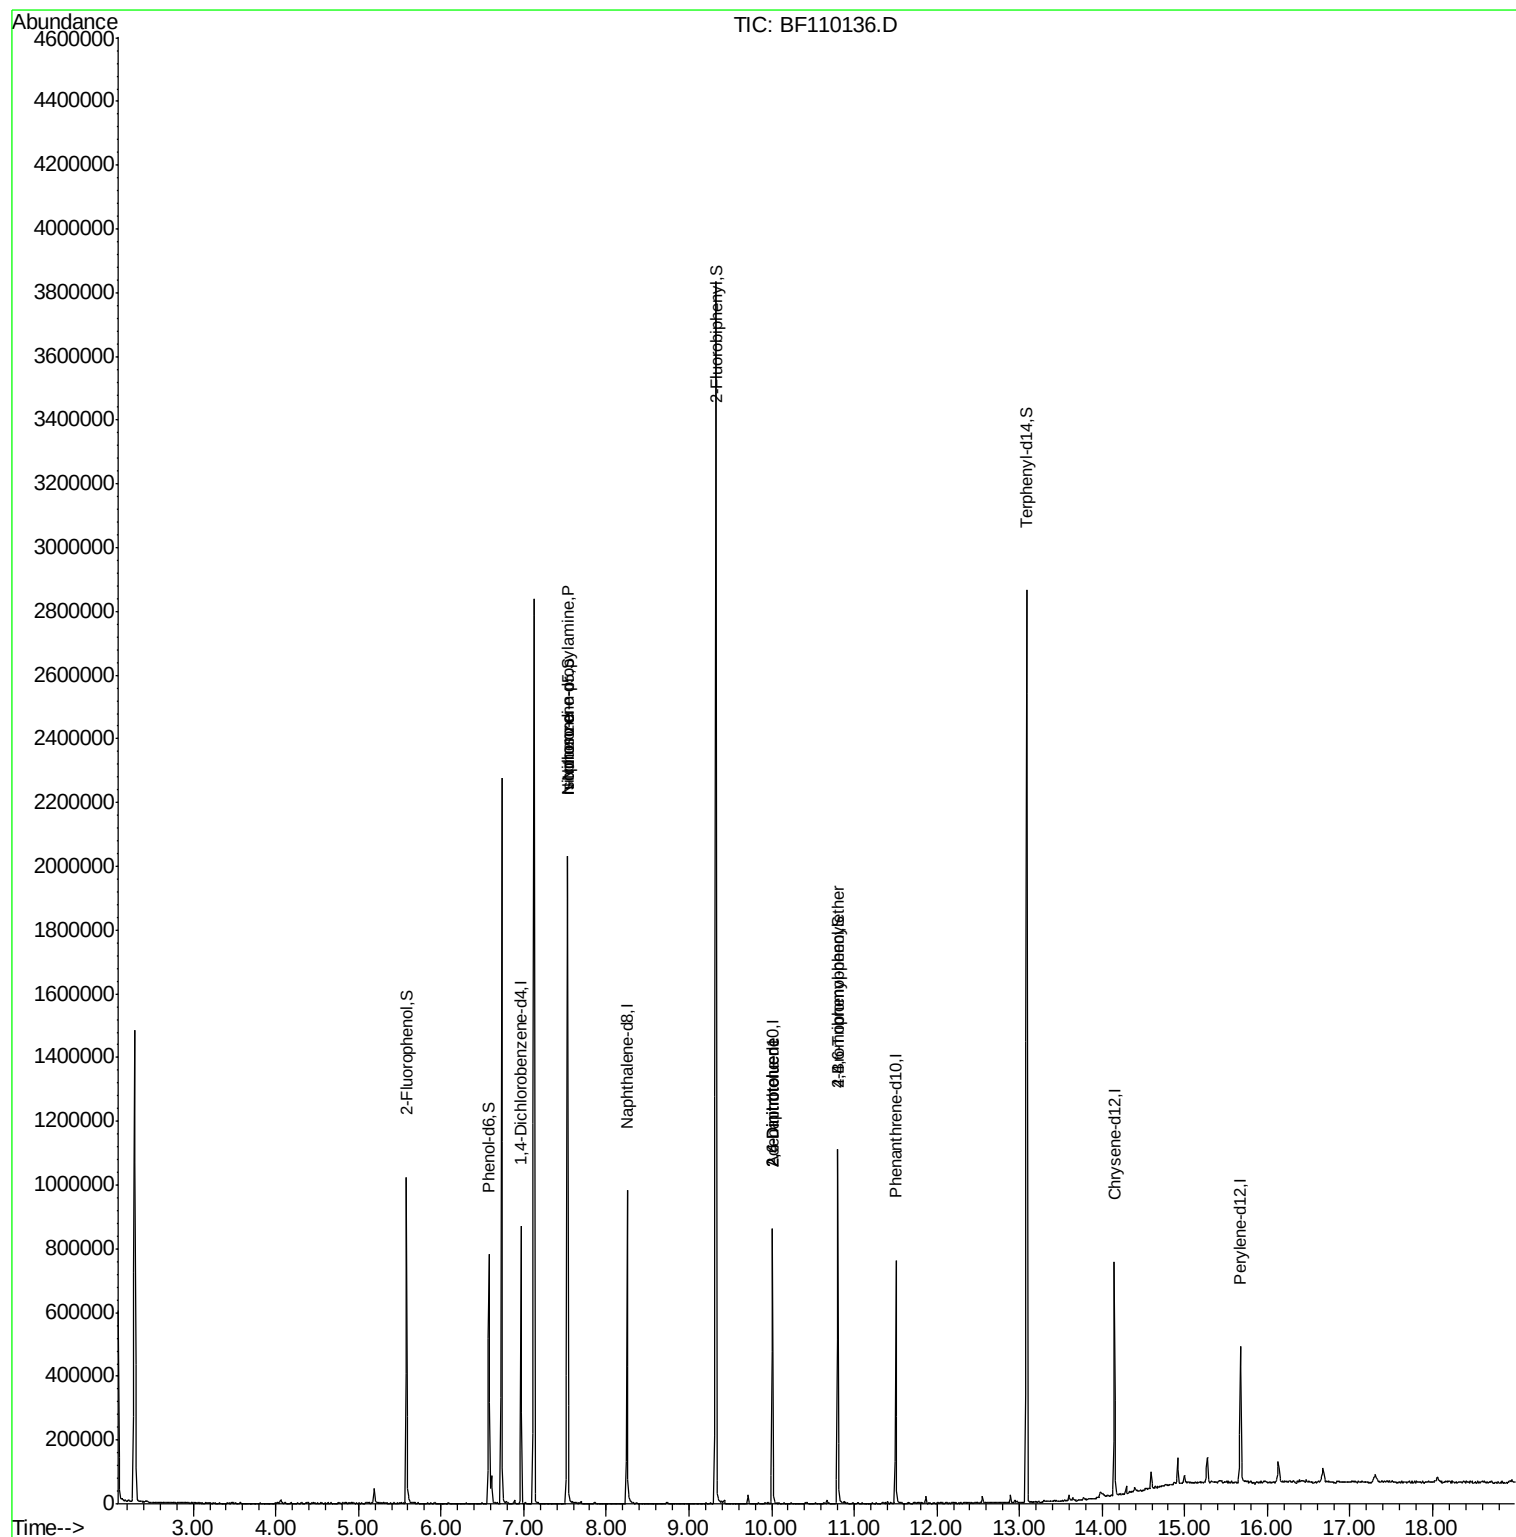

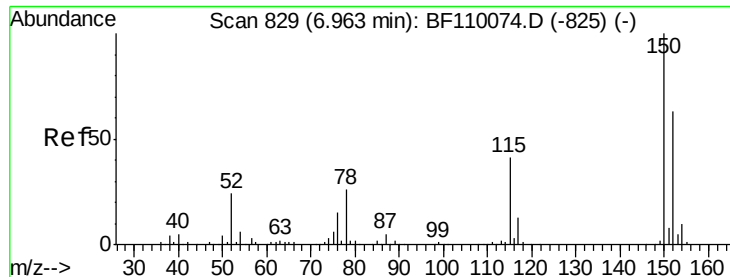


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 830
Delta R.T. 0.01 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.5	122.7	184.1
115	60.3	49.1	73.7



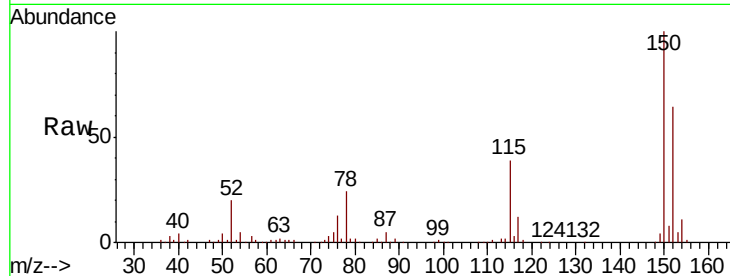


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

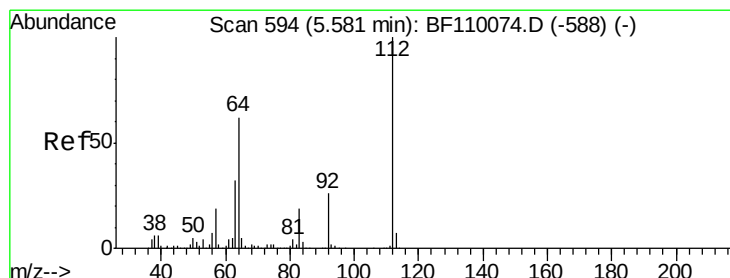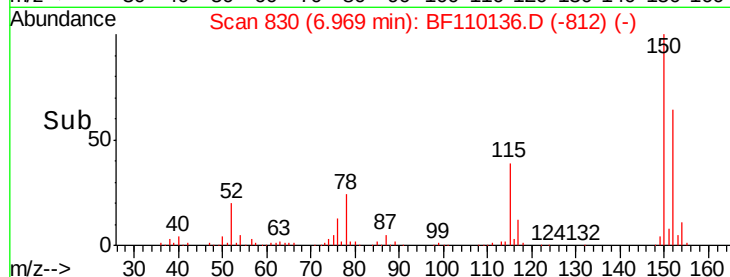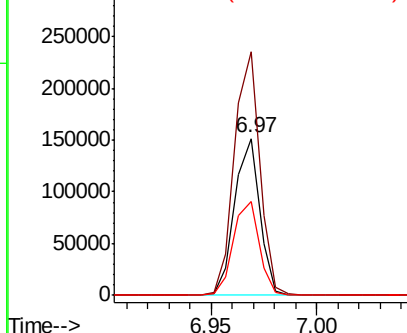

#5

2-Fluorophenol
Concen: 39.294 ng
RT: 5.59 min Scan# 595
Delta R.T. 0.01 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.6	44.1	66.1
63	28.9	23.7	35.5


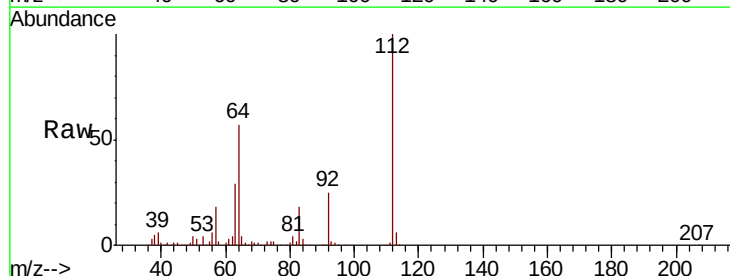



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

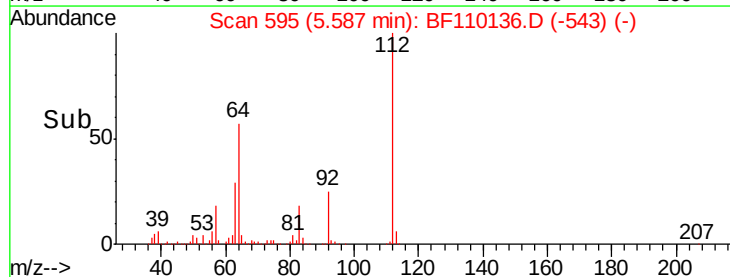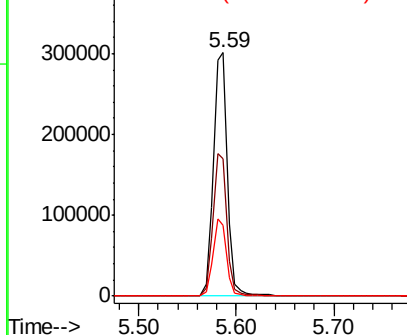

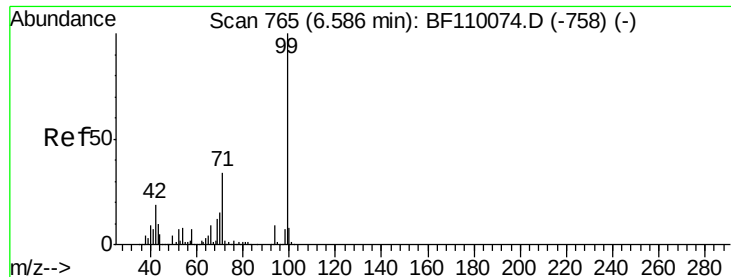

#7

Phenol-d6

Concen: 23.252 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.01 min

Lab File: BF110136.D

Acq: 25 Oct 2018 1:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 226581

Ion Ratio Lower Upper

99 100

42 17.9 15.8 23.6




71 33.3 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

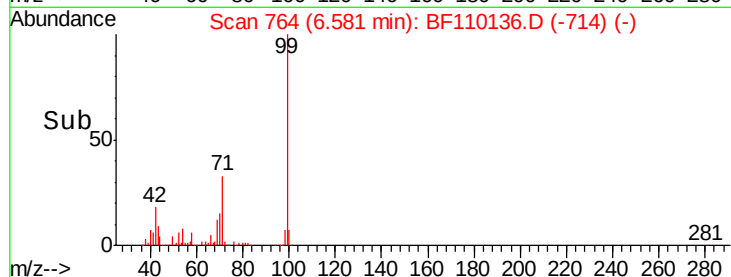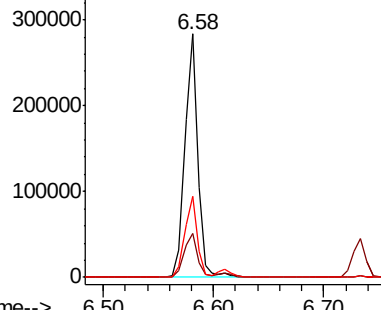

#19

n-Nitroso-di-n-propylamine

Concen: 15.007 ng

RT: 7.53 min Scan# 926

Delta R.T. 0.16 min

Lab File: BF110136.D

Acq: 25 Oct 2018 1:53

Tgt Ion: 70 Resp: 93818


Ion Ratio Lower Upper

70 100

42 47.4 47.4 71.2#

101 0.0 7.3 10.9#

130 2.0 16.2 24.2#






Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

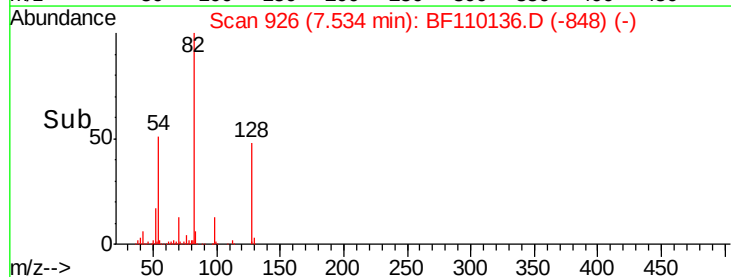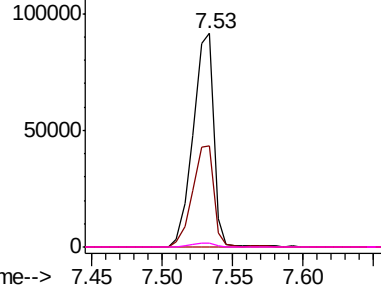


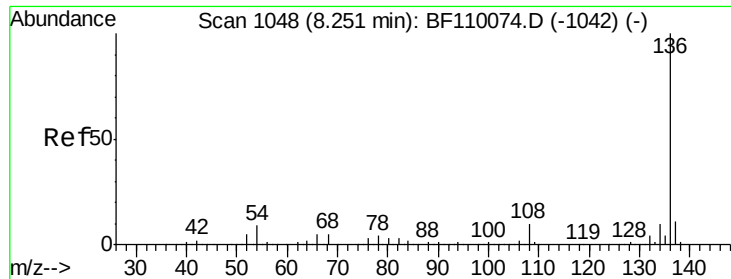




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.25 min Scan# 1048
Delta R.T. 0.00 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	424965
Ion Ratio	Lower	Upper
136	100	
137	10.5	8.8 13.2
54	8.1	5.4 8.2
68	5.4	4.2 6.2




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

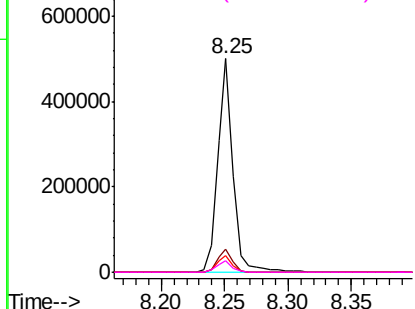
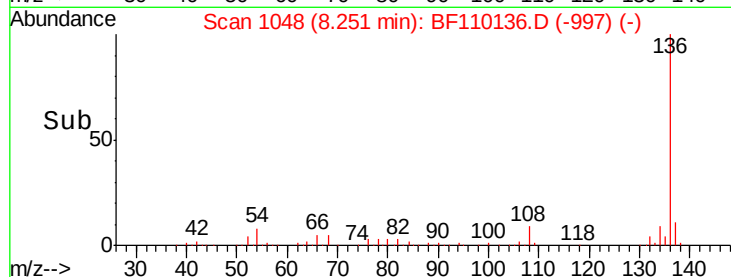



#23
Nitrobenzene-d5
Concen: 98.877 ng
RT: 7.53 min Scan# 926
Delta R.T. 0.00 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53

Tgt Ion: 82	Resp:	708429
Ion Ratio	Lower	Upper
82	100	
128	47.7	34.2 51.2
54	50.9	38.6 58.0



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

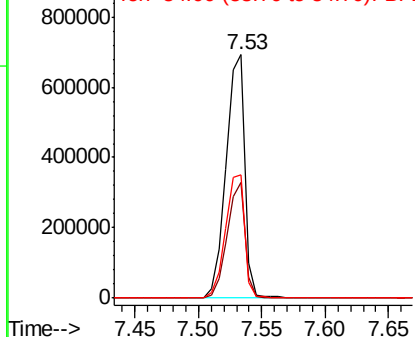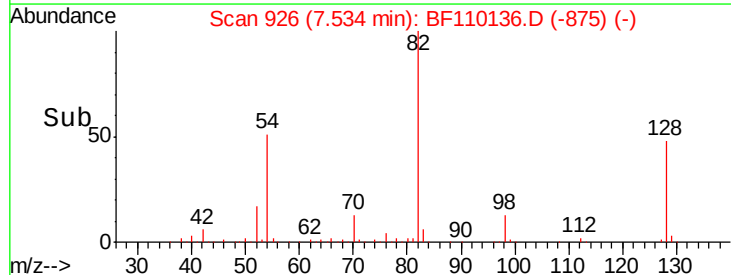

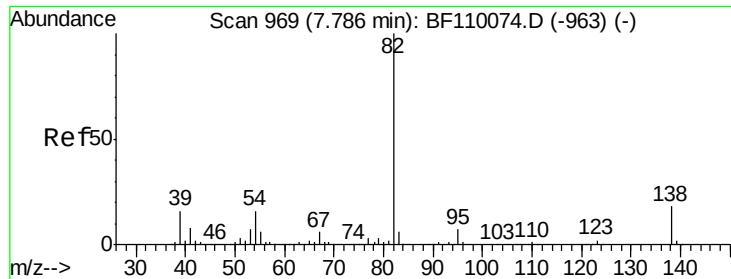

#25

Isophorone

Concen: 58.005 ng

RT: 7.53 min Scan# 926

Delta R.T. -0.25 min

Lab File: BF110136.D

Acq: 25 Oct 2018 1:53

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 708423

Ion Ratio Lower Upper

82 100

95 0.0 5.7 8.5#




138 0.0 13.2 19.8#

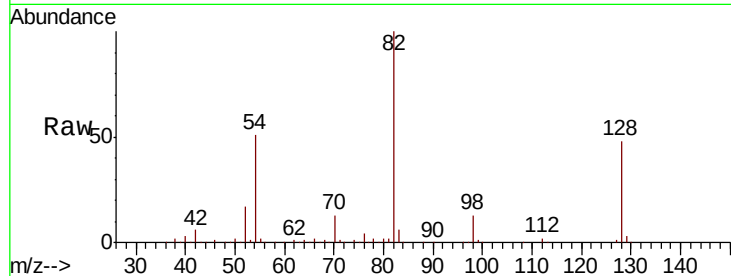

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

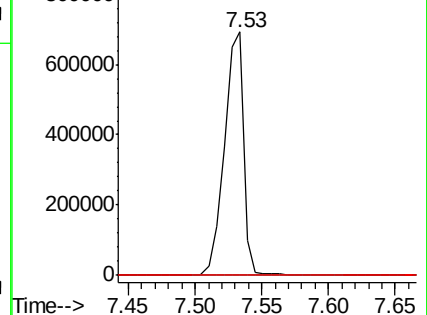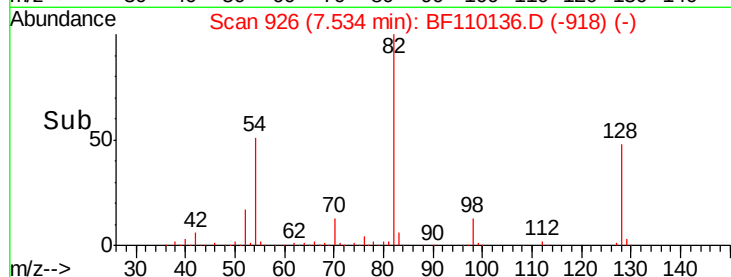

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1347

Delta R.T. 0.00 min

Lab File: BF110136.D

Acq: 25 Oct 2018 1:53


Tgt Ion: 164 Resp: 159118

Ion Ratio Lower Upper

164 100

162 104.3 83.0 124.6



160 46.3 37.0 55.6




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



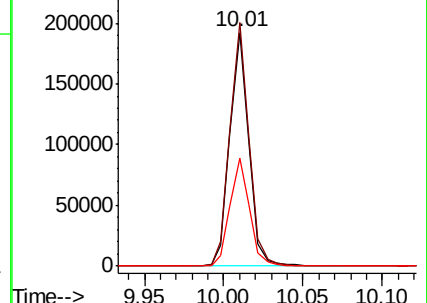
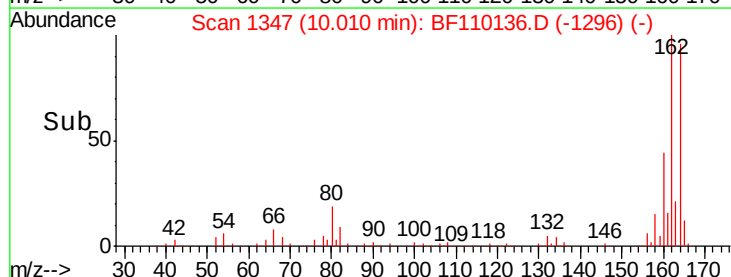


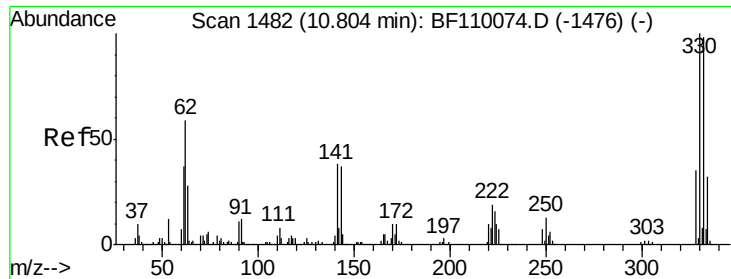

#42
 2,4,6-Tribromophenol
 Concen: 78.103 ng
 RT: 10.80 min Scan# 1481
 Delta R.T. -0.01 min
 Lab File: BF110136.D
 Acq: 25 Oct 2018 1:53




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	77.1	115.7
141	35.7	27.0	40.4

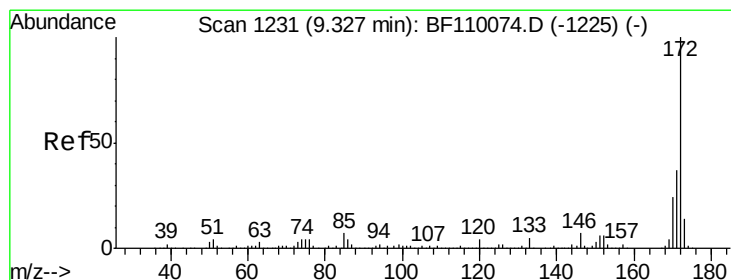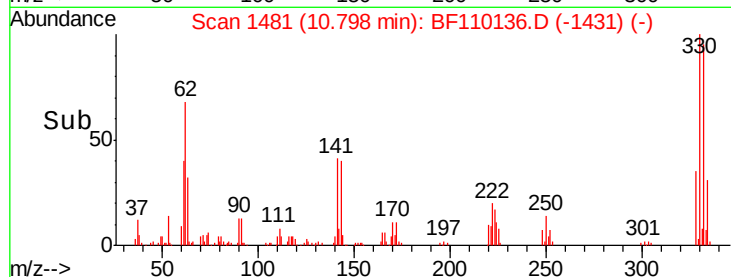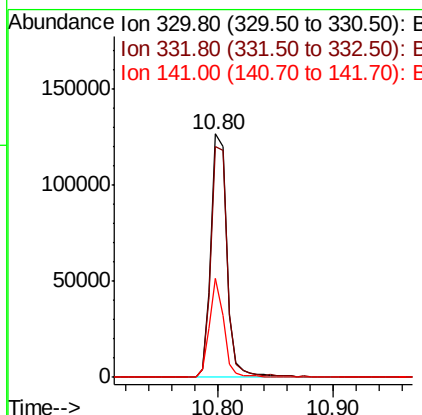

#45
 2-Fluorobiphenyl
 Concen: 116.008 ng
 RT: 9.33 min Scan# 1231
 Delta R.T. 0.00 min
 Lab File: BF110136.D
 Acq: 25 Oct 2018 1:53

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	28.6	43.0
170	23.6	19.7	29.5

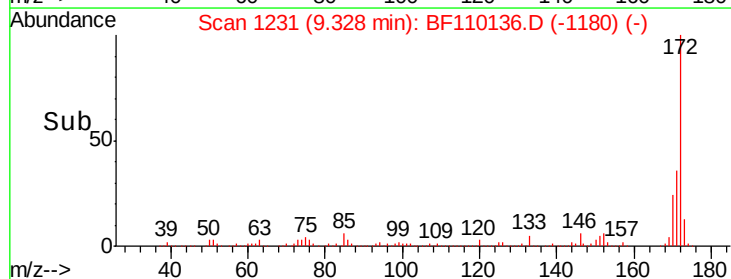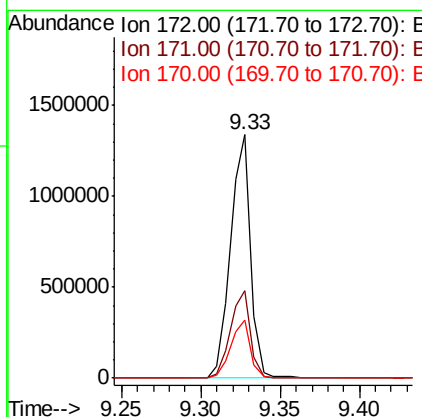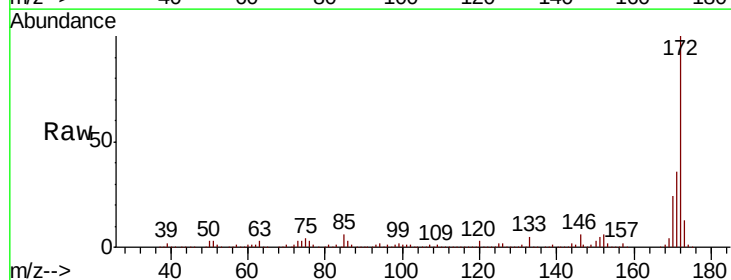

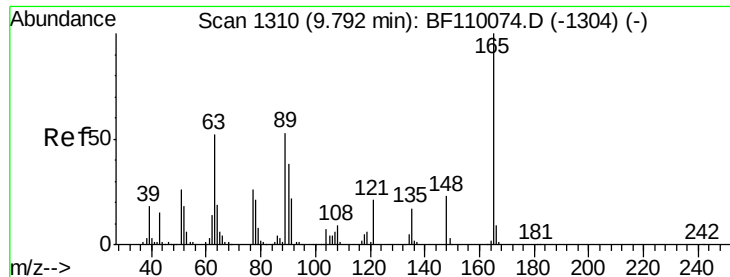

#51

2,6-Dinitrotoluene

Concen: 8.070 ng

RT: 10.01 min Scan# 1347

Delta R.T. 0.22 min

Lab File: BF110136.D

Acq: 25 Oct 2018 1:53

Instrument :

BNA_F

ClientSampleId :



Tot Ion:165 Resp: 20417

Ion Ratio Lower Upper

165 100

63 1.6 48.9 73.3#



89 1.4 46.6 69.8#

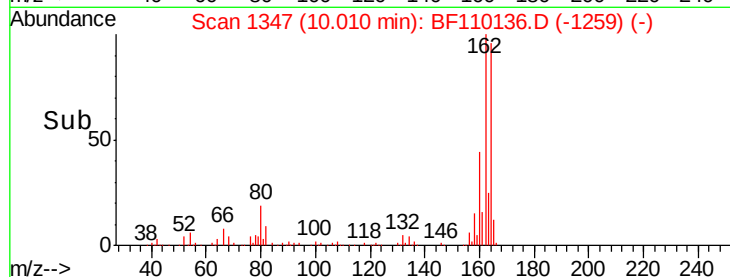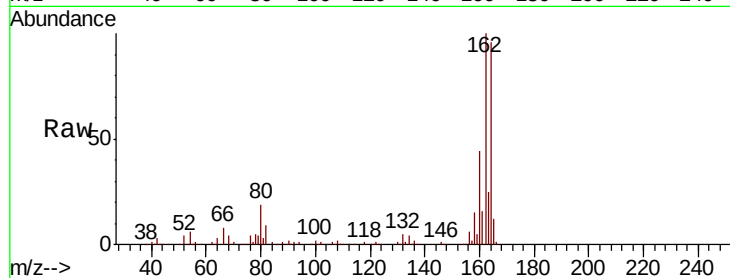

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

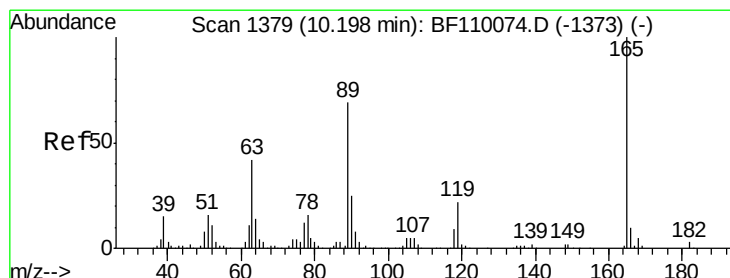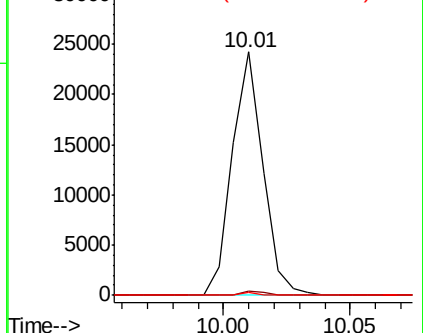

#57

2,4-Dinitrotoluene

Concen: 6.353 ng

RT: 10.01 min Scan# 1347

Delta R.T. -0.18 min

Lab File: BF110136.D

Acq: 25 Oct 2018 1:53

Tgt Ion:165 Resp: 20417



Ion Ratio Lower Upper

165 100

63 1.6 44.8 67.2#

89 1.4 62.2 93.4#

182 0.0 2.1 3.1#

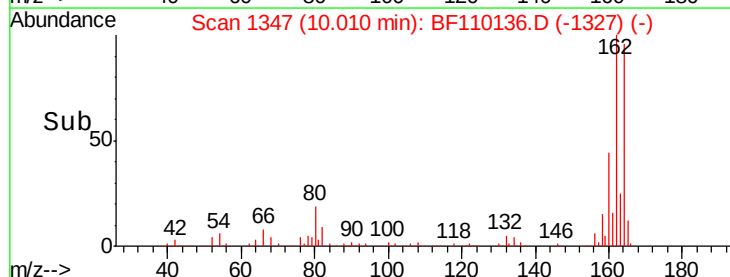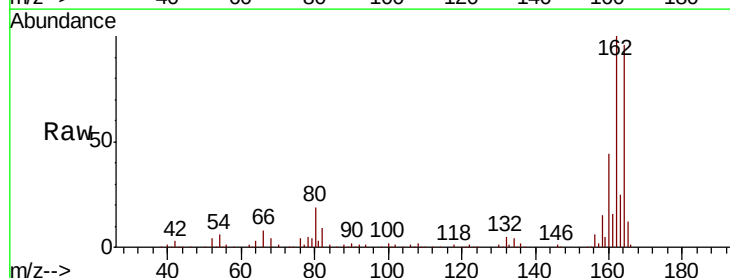



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E




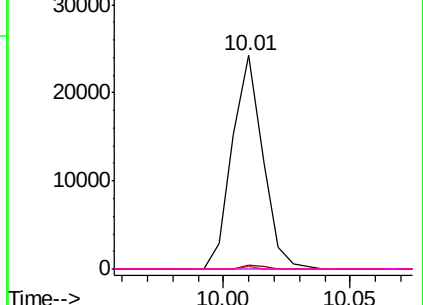


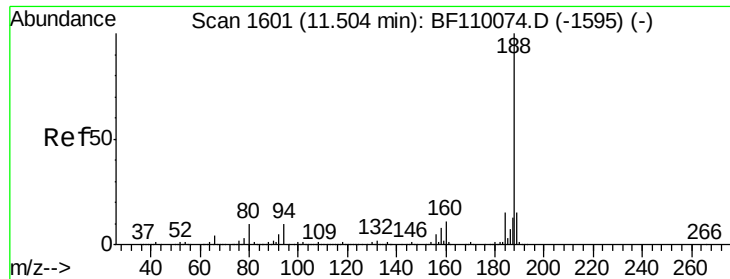

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1601
Delta R.T. 0.01 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 268330
Ion Ratio Lower Upper
188 100
94 8.6 7.2 10.8
80 9.0 7.9 11.9

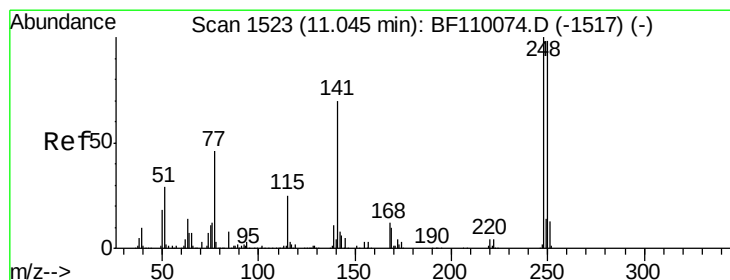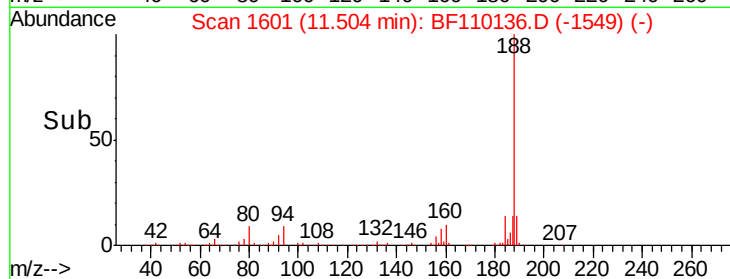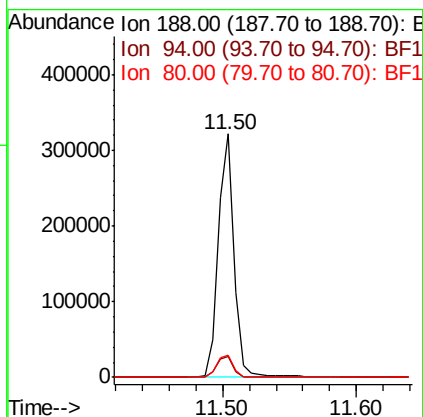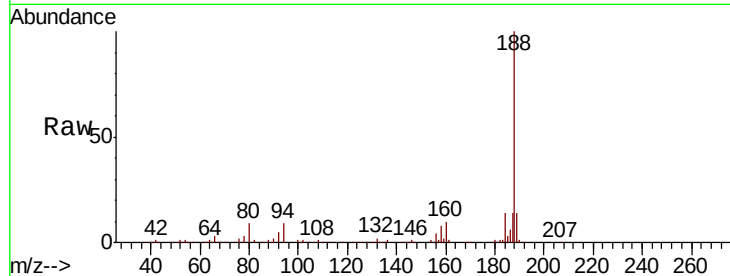

#67
4-Bromophenyl-phenylether
Concen: 2.802 ng
RT: 10.80 min Scan# 1481
Delta R.T. -0.24 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53

Tgt Ion:248 Resp: 8156
Ion Ratio Lower Upper
248 100
250 194.2 79.4 119.2#
141 570.6 55.9 83.9#


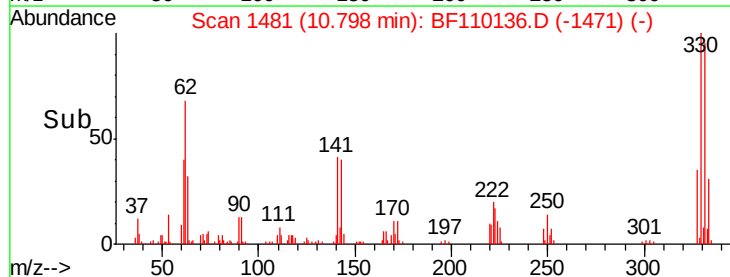
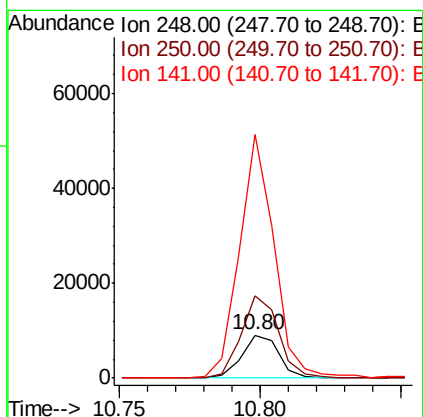
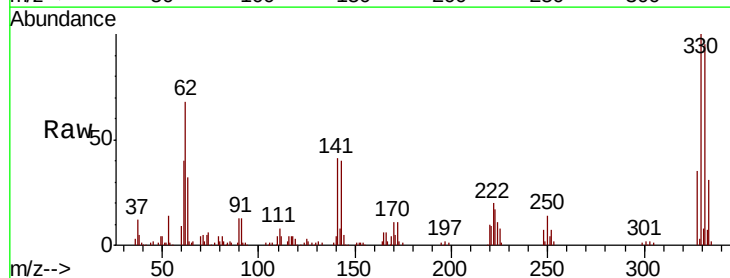


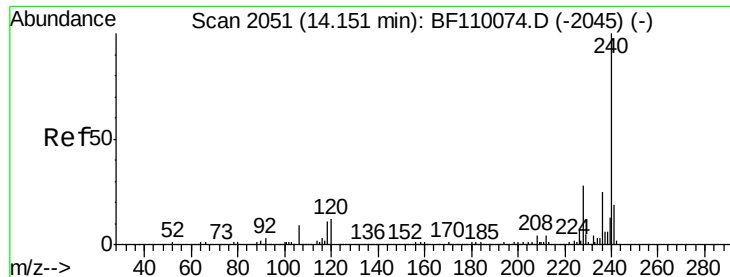

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.15 min Scan# 2051
Delta R.T. 0.00 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53




Instrument :
BNA_F
ClientSampleId :


Tot Ion:240 Resp: 237772
Ion Ratio Lower Upper
240 100
120 11.2 8.3 12.5
236 26.4 21.2 31.8

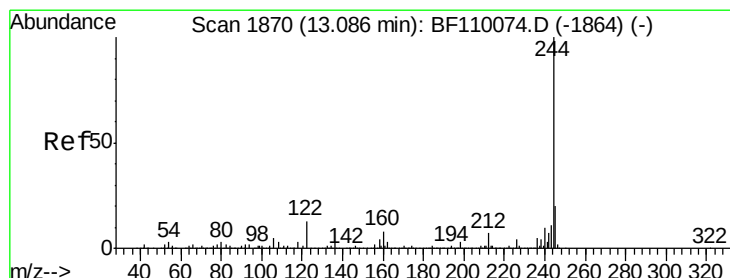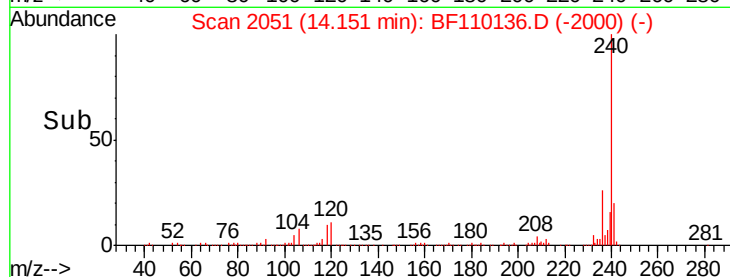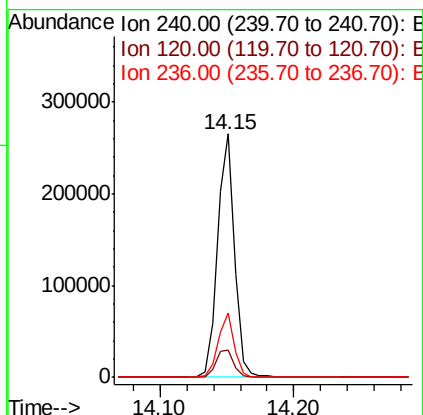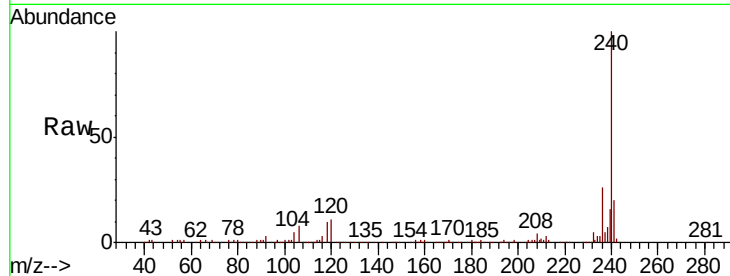

#79
Terphenyl-d14
Concen: 87.050 ng
RT: 13.09 min Scan# 1870
Delta R.T. 0.00 min
Lab File: BF110136.D
Acq: 25 Oct 2018 1:53

Tgt Ion:244 Resp: 995238
Ion Ratio Lower Upper
244 100
212 6.8 5.8 8.8
122 13.3 8.7 13.1#

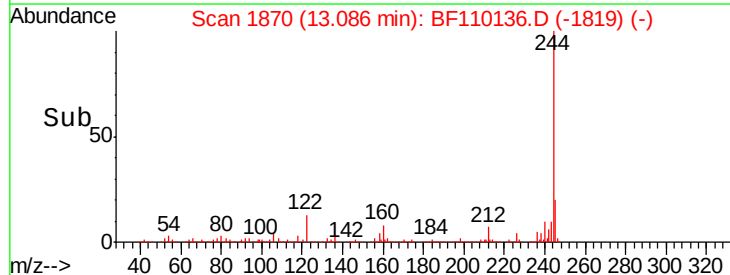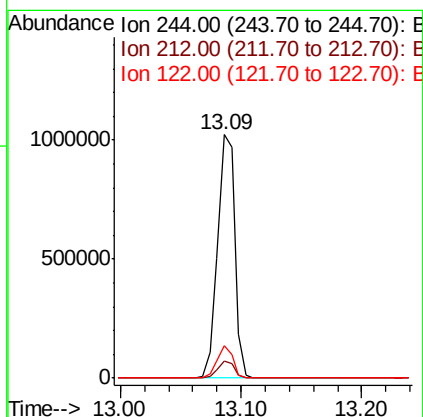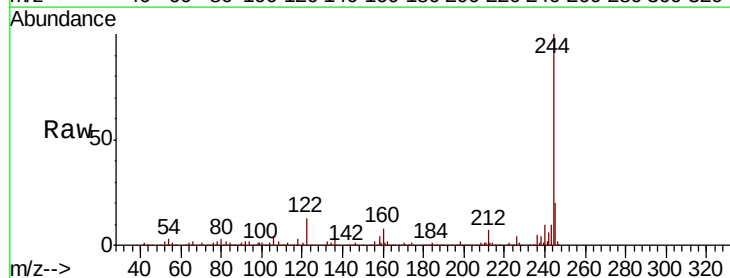


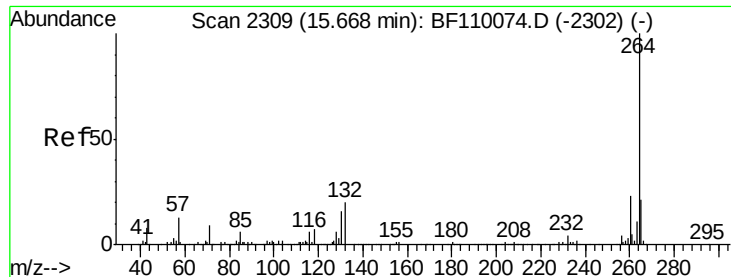

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.67 min Scan# 2310
 Delta R.T. 0.01 min
 Lab File: BF110136.D
 Acq: 25 Oct 2018 1:53

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.7	28.1
265	23.4	16.7	25.1



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

