


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102418\
Data File : BF110129.D
Acq On : 24 Oct 2018 22:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 23 15:06:18 2018

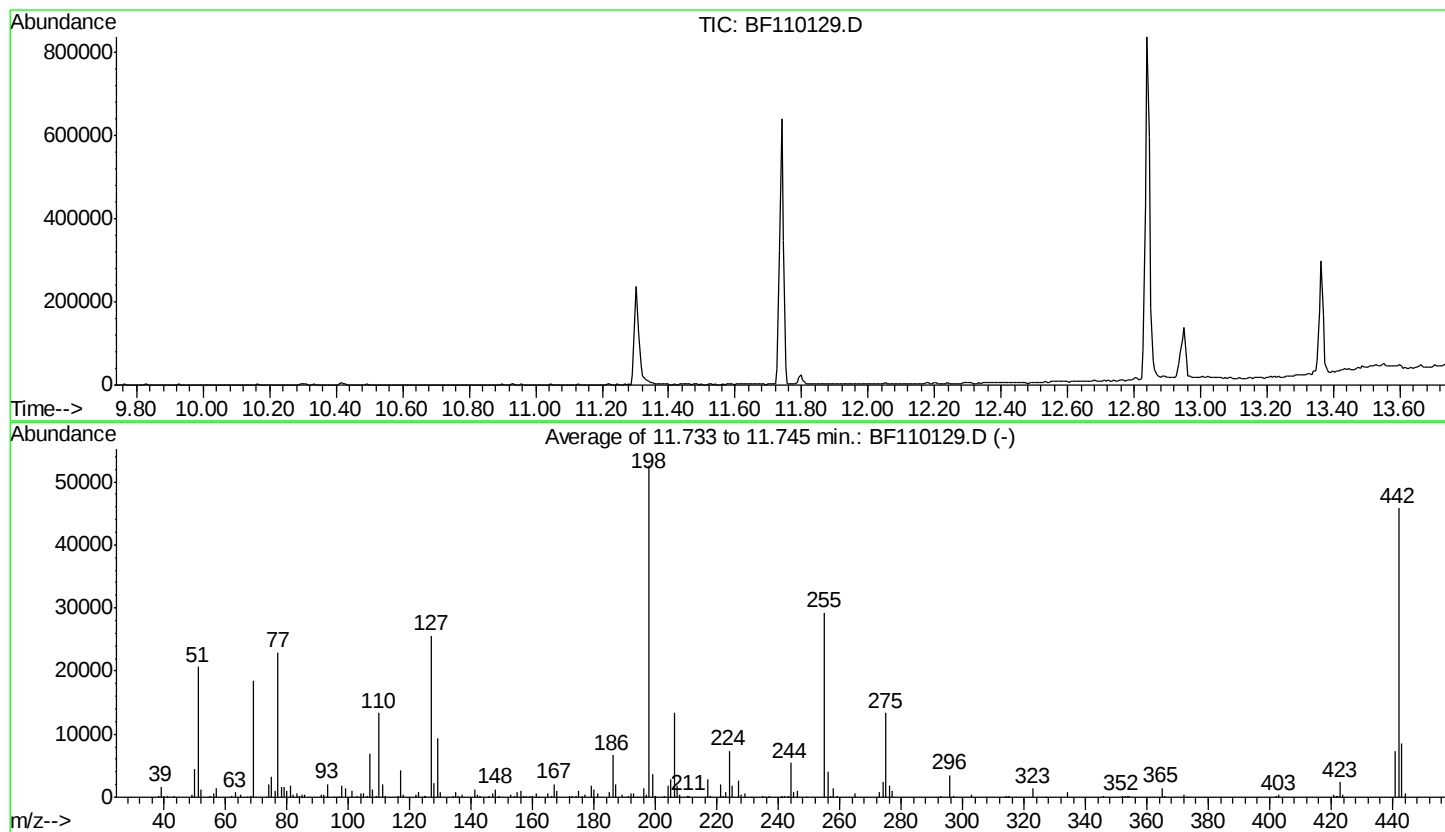

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	20645	PASS
68	69	0.00	2	1.2	225	PASS
69	198	0.00	100	35.3	18561	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	25573	PASS
197	198	0.00	2	0.6	338	PASS
198	198	100	100	100.0	52552	PASS
199	198	5	9	6.9	3637	PASS
275	198	10	60	25.3	13307	PASS
365	198	1	100	2.8	1469	PASS
441	198	0.01	100	13.8	7233	PASS
442	198	50	100	87.2	45800	PASS
443	442	15	24	18.7	8578	PASS