
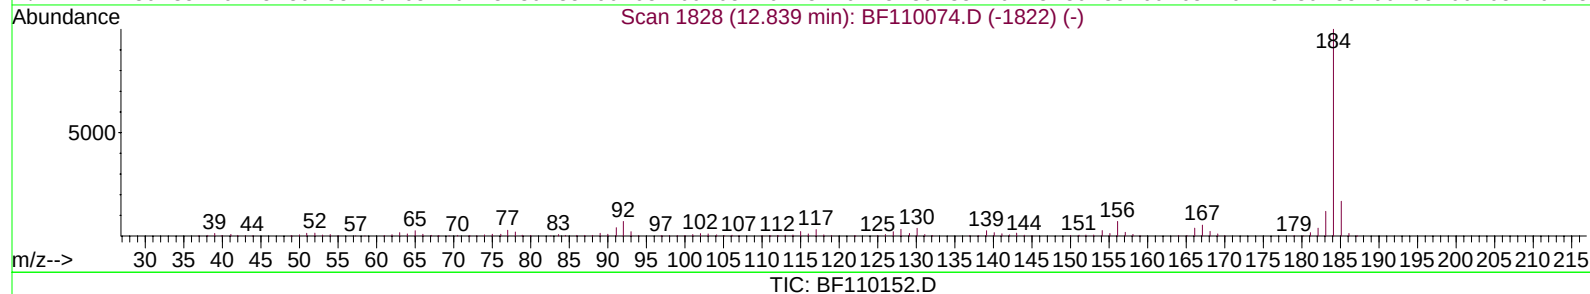
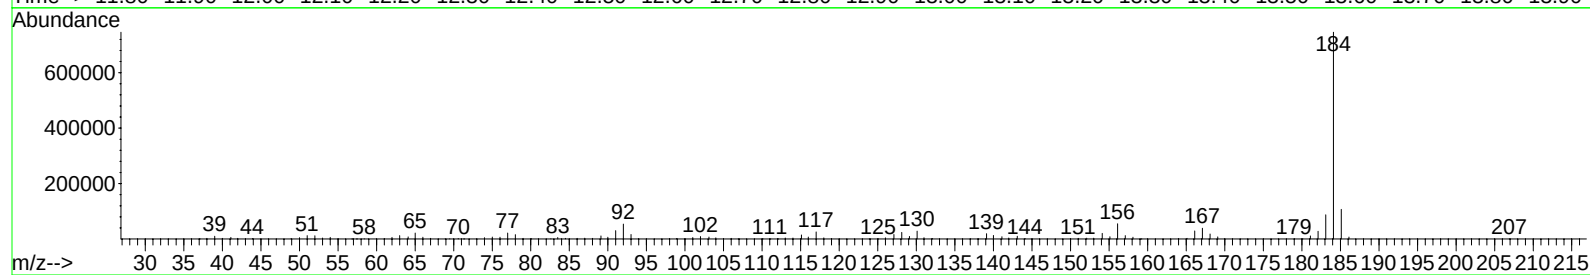


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102518\
 Data File : BF110152.D
 Acq On : 25 Oct 2018 10:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 10:00:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 23 15:06:18 2018
 Response via : Initial Calibration

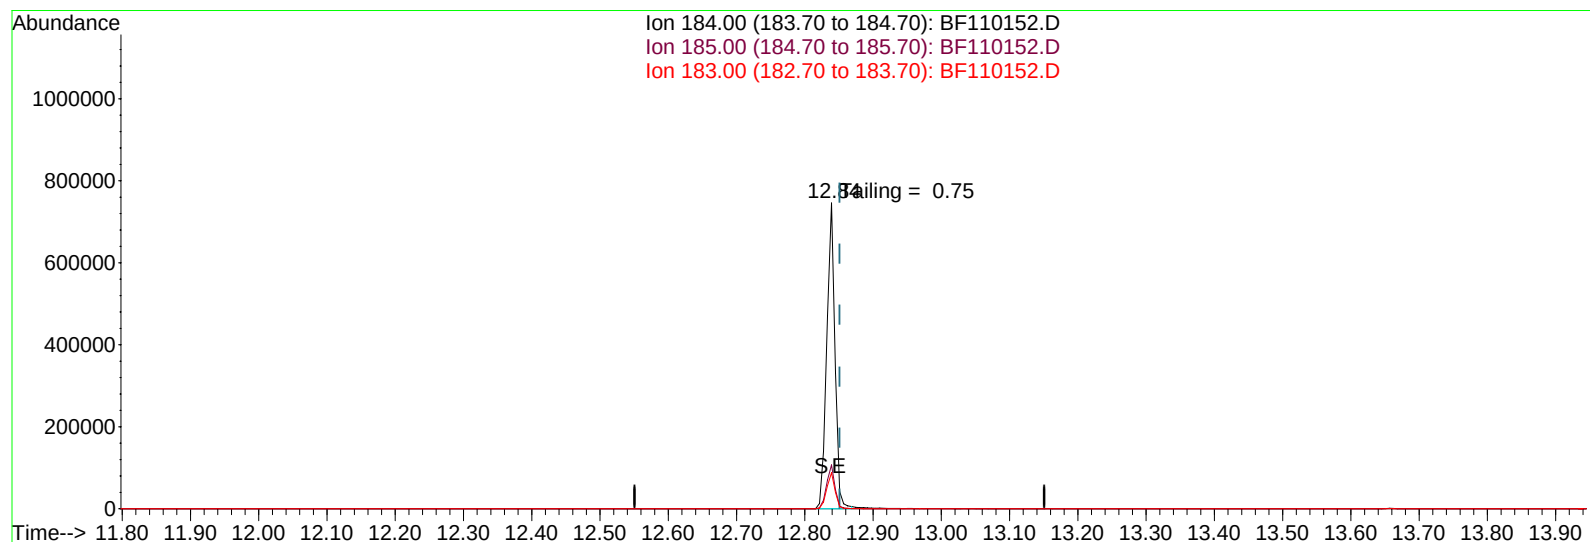

(77) Benzidine




12.839min (-0.012) 0.00ng

response 630617

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.36
183.00	11.80	11.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102518\
 Data File : BF110152.D
 Acq On : 25 Oct 2018 10:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 10:00:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 23 15:06:18 2018
 Response via : Initial Calibration

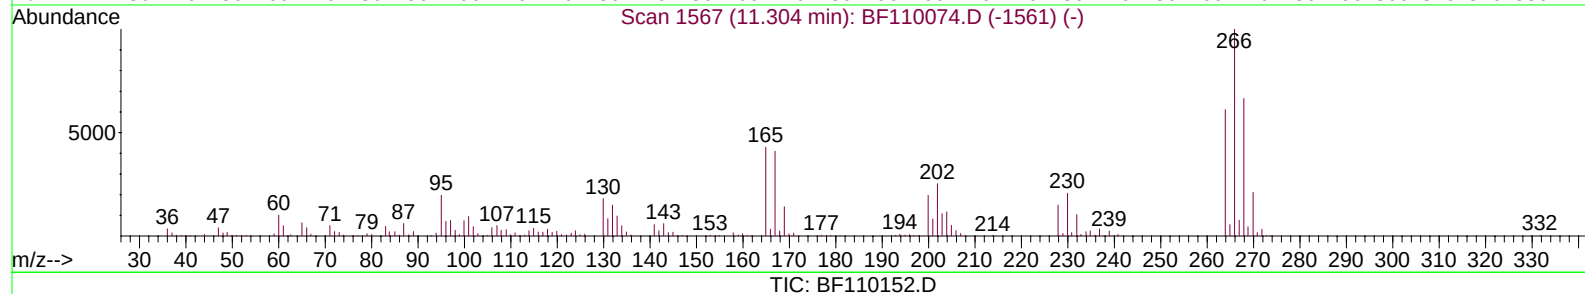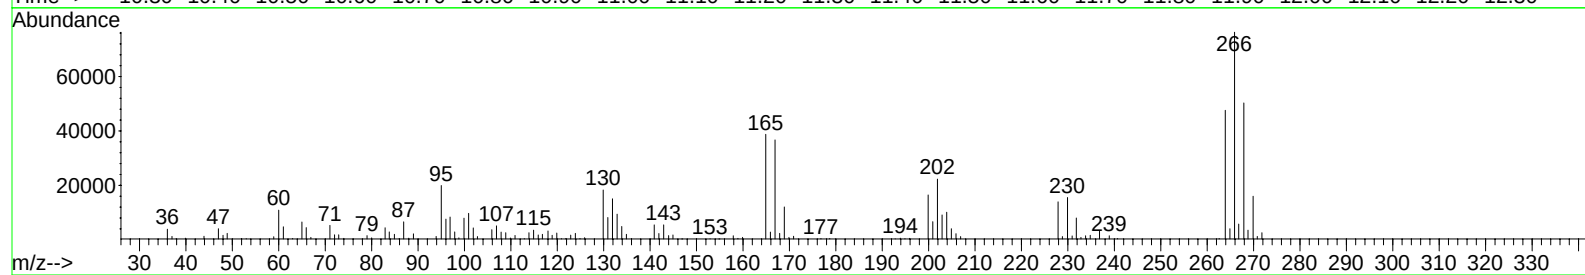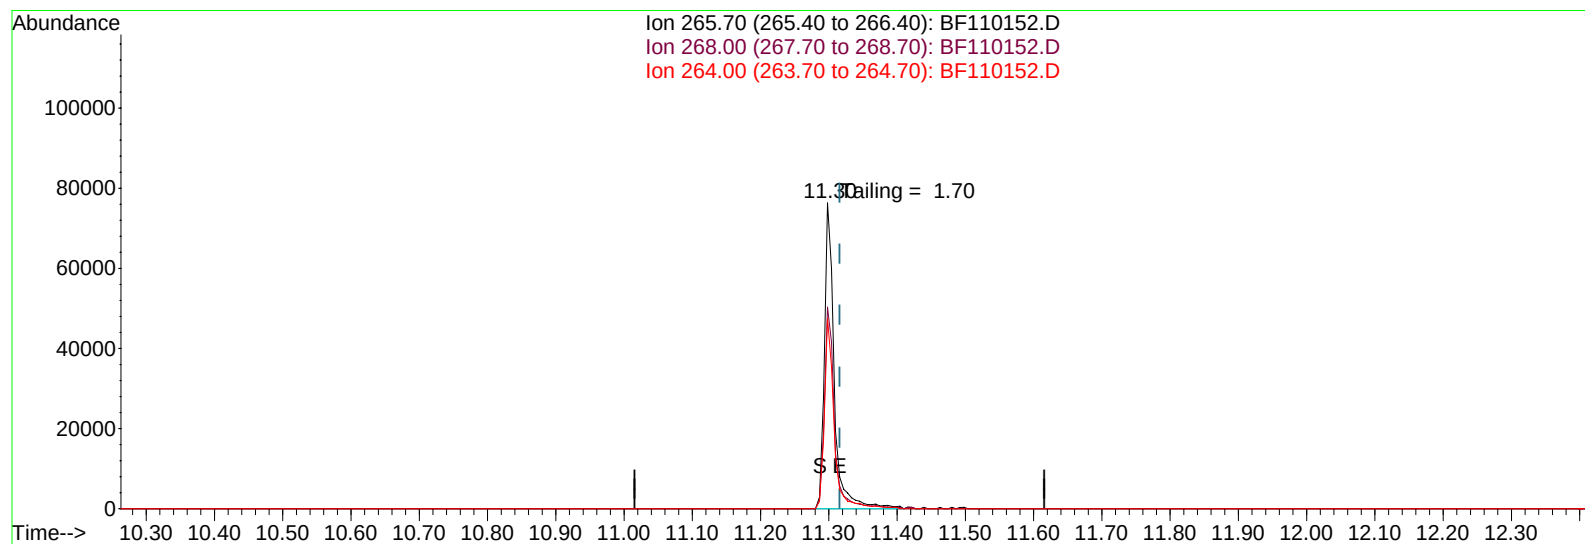

(70) Pentachlorophenol (C)

11.298min (-0.018) 35099.79ng

response 77027

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	65.96
264.00	63.20	62.34
0.00	0.00	0.00