
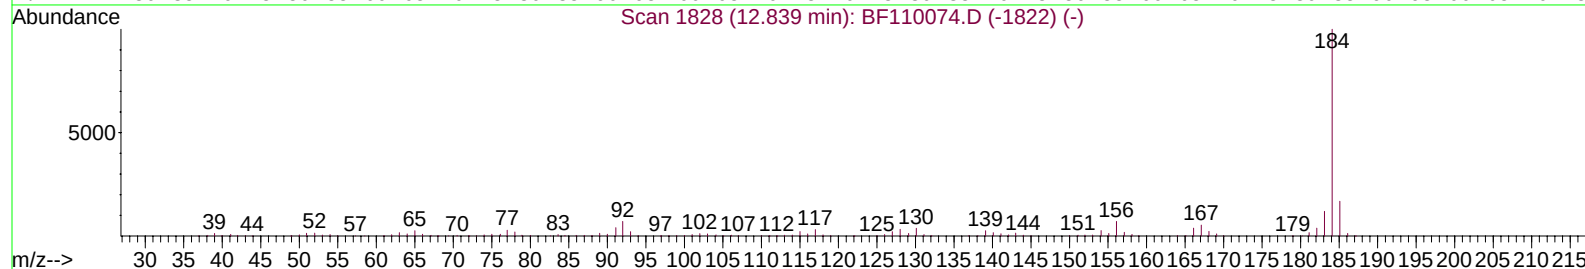
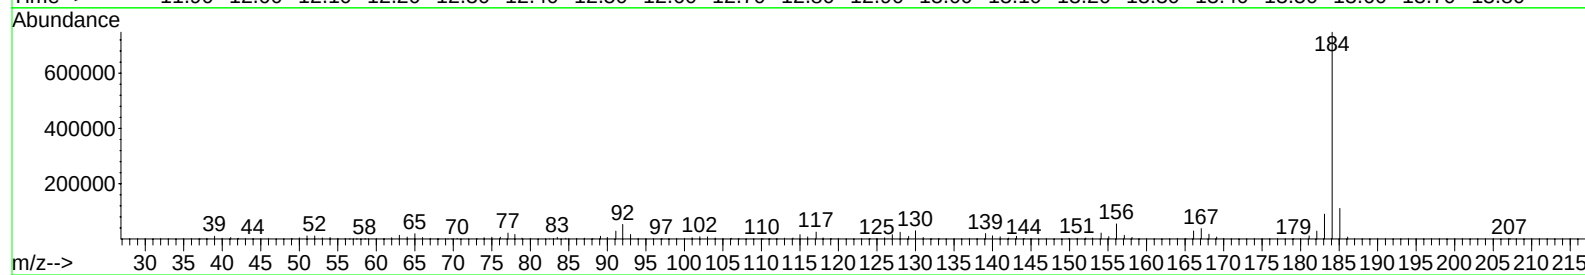


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102518\  
Data File   : BF110162.D  
Acq On      : 25 Oct 2018  16:00  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Oct 26 10:02:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 15:06:18 2018
Response via : Initial Calibration

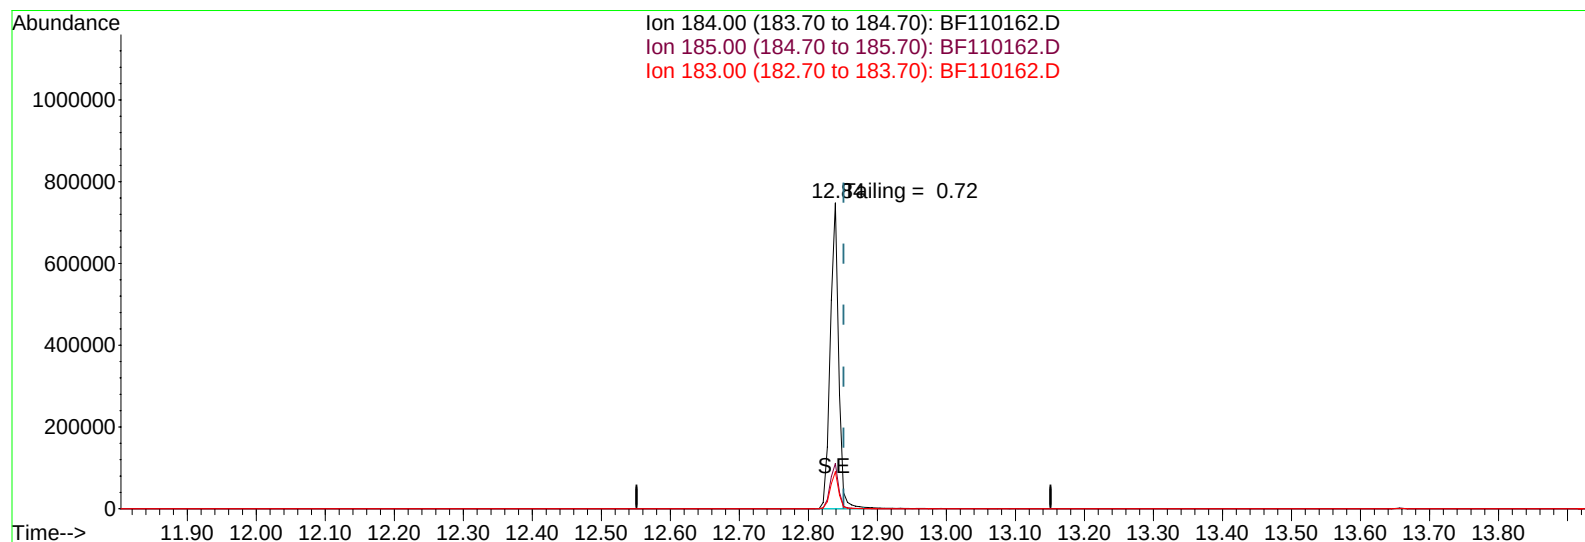

TIC: BF110162.D

(77) Benzidine




12.839min (-0.012) 0.00ng

response 634135

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.82
183.00	11.80	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102518\
Data File : BF110162.D
Acq On : 25 Oct 2018 16:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 10:02:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 15:06:18 2018
Response via : Initial Calibration

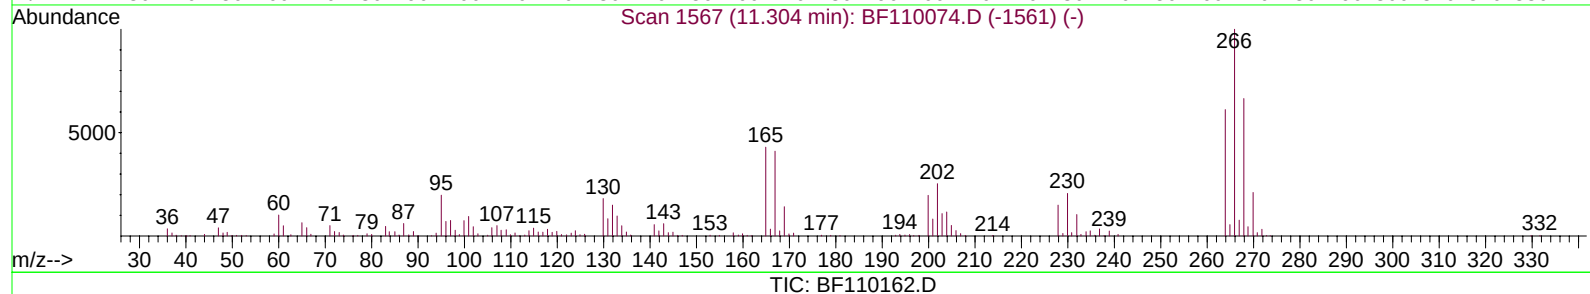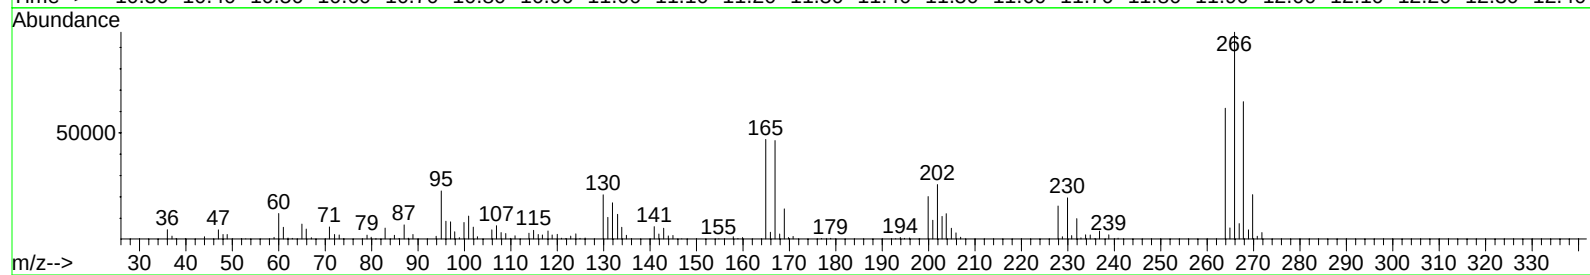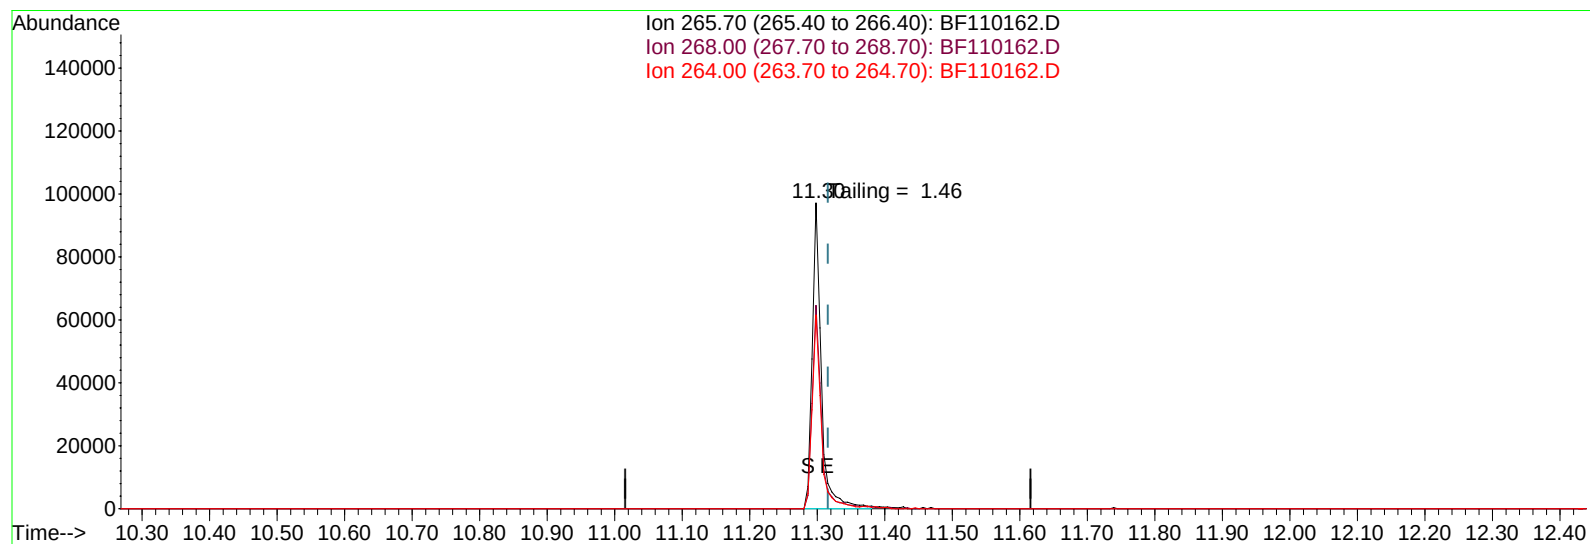

(70) Pentachlorophenol (C)

11.298min (-0.018) 40177.83ng

response 92485

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	66.50
264.00	63.20	63.39
0.00	0.00	0.00