
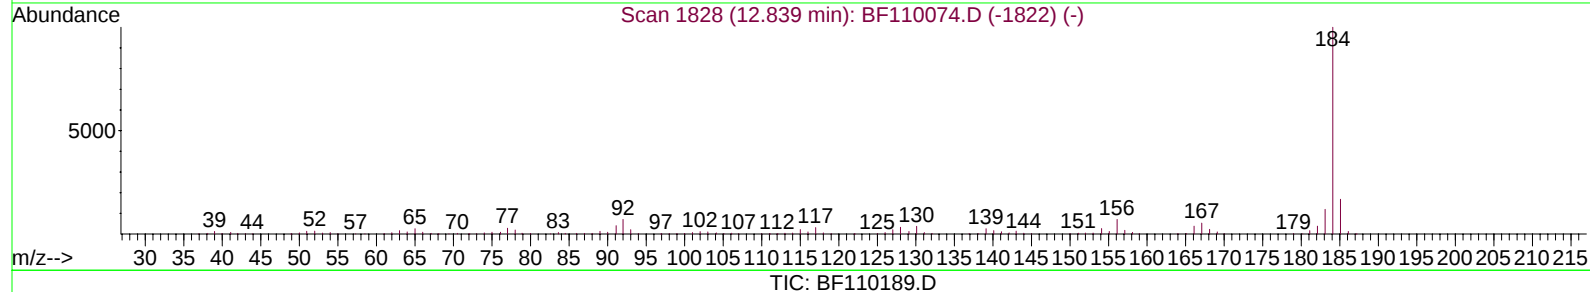
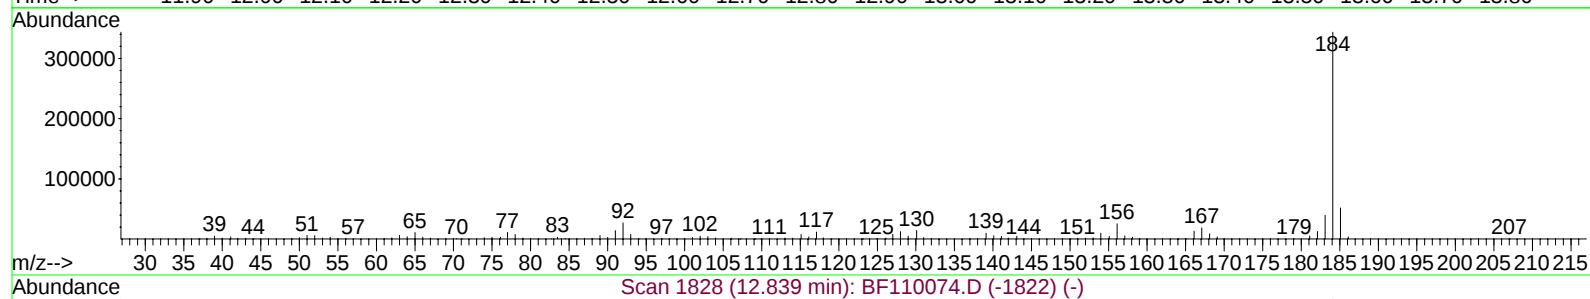


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102518\
Data File : BF110189.D
Acq On : 26 Oct 2018 4:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 10:03:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 15:06:18 2018
Response via : Initial Calibration

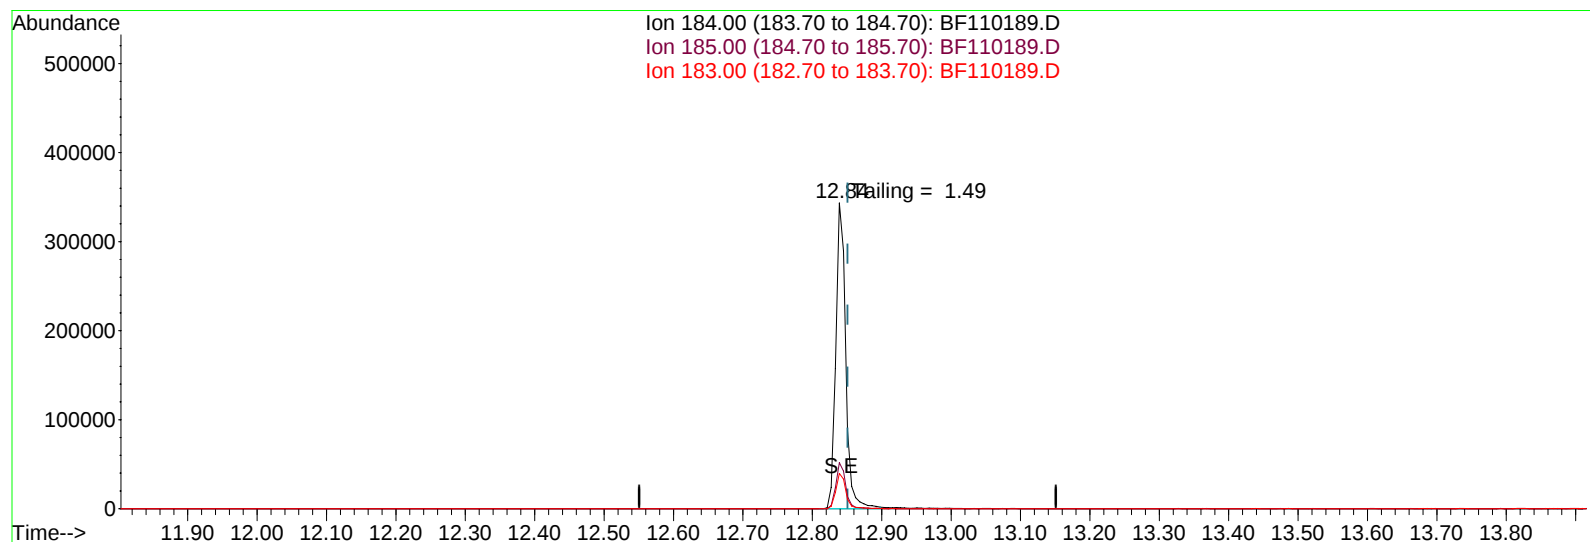

(77) Benzidine




12.839min (-0.012) -20.00ng

response 342080

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.10
183.00	11.80	11.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102518\
 Data File : BF110189.D
 Acq On : 26 Oct 2018 4:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 10:03:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 23 15:06:18 2018
 Response via : Initial Calibration

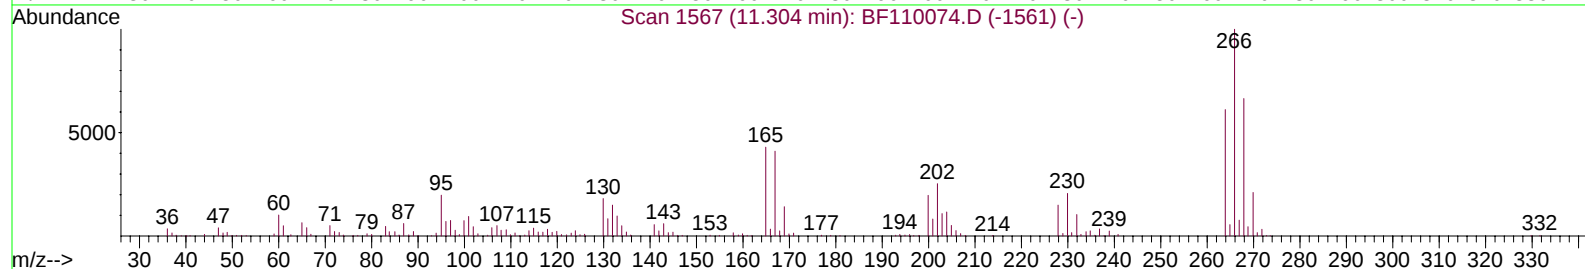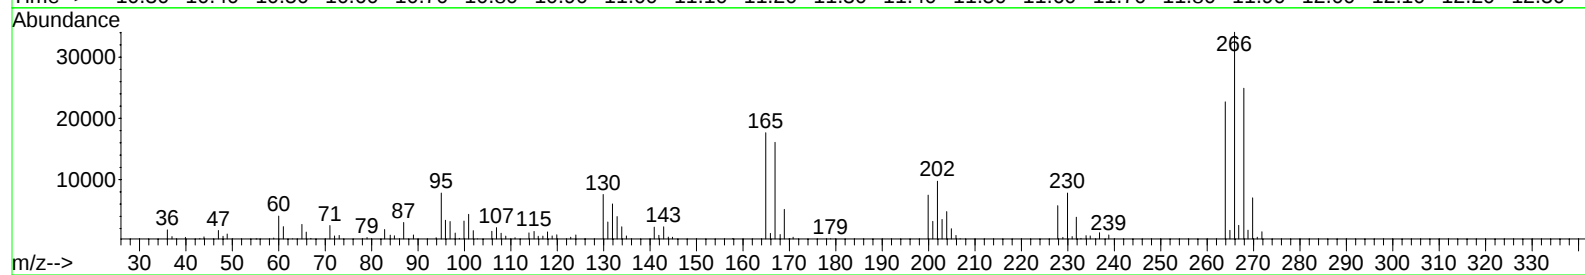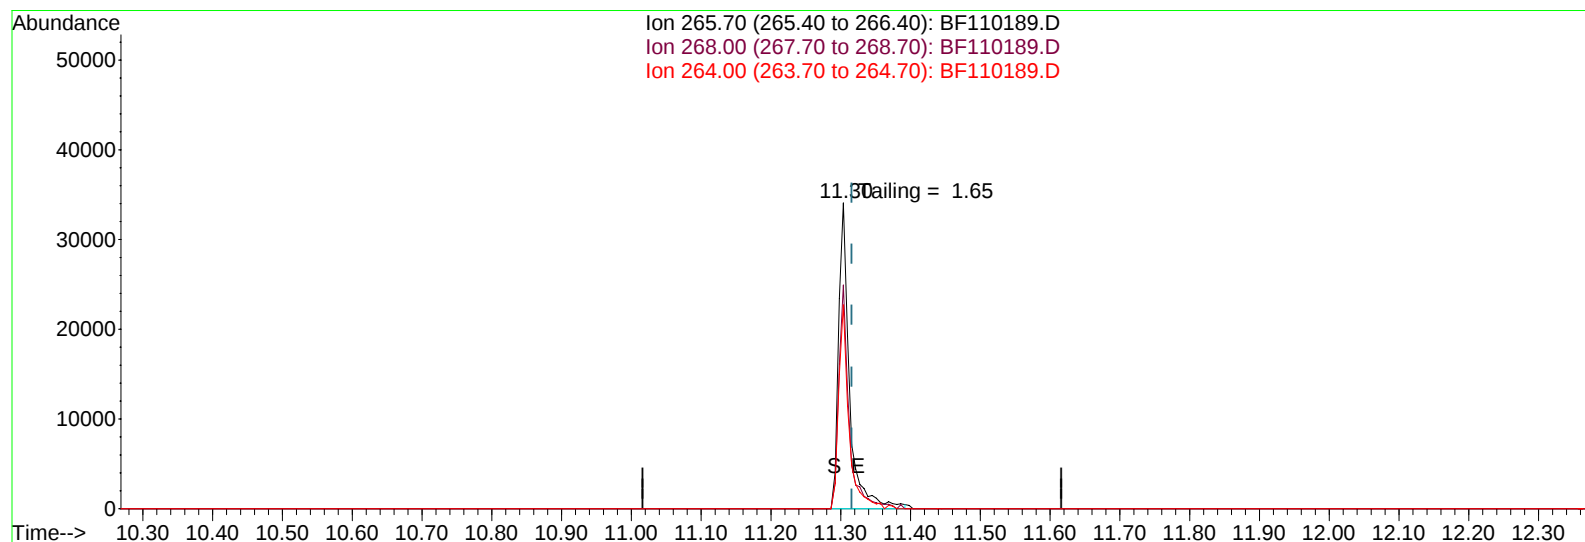

(70) Pentachlorophenol (C)

11.304min (-0.012) 0.00ng

response 36223

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	73.14
264.00	63.20	66.66
0.00	0.00	0.00