


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102518\
Data File : BF110152.D
Acq On : 25 Oct 2018 10:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 23 15:06:18 2018

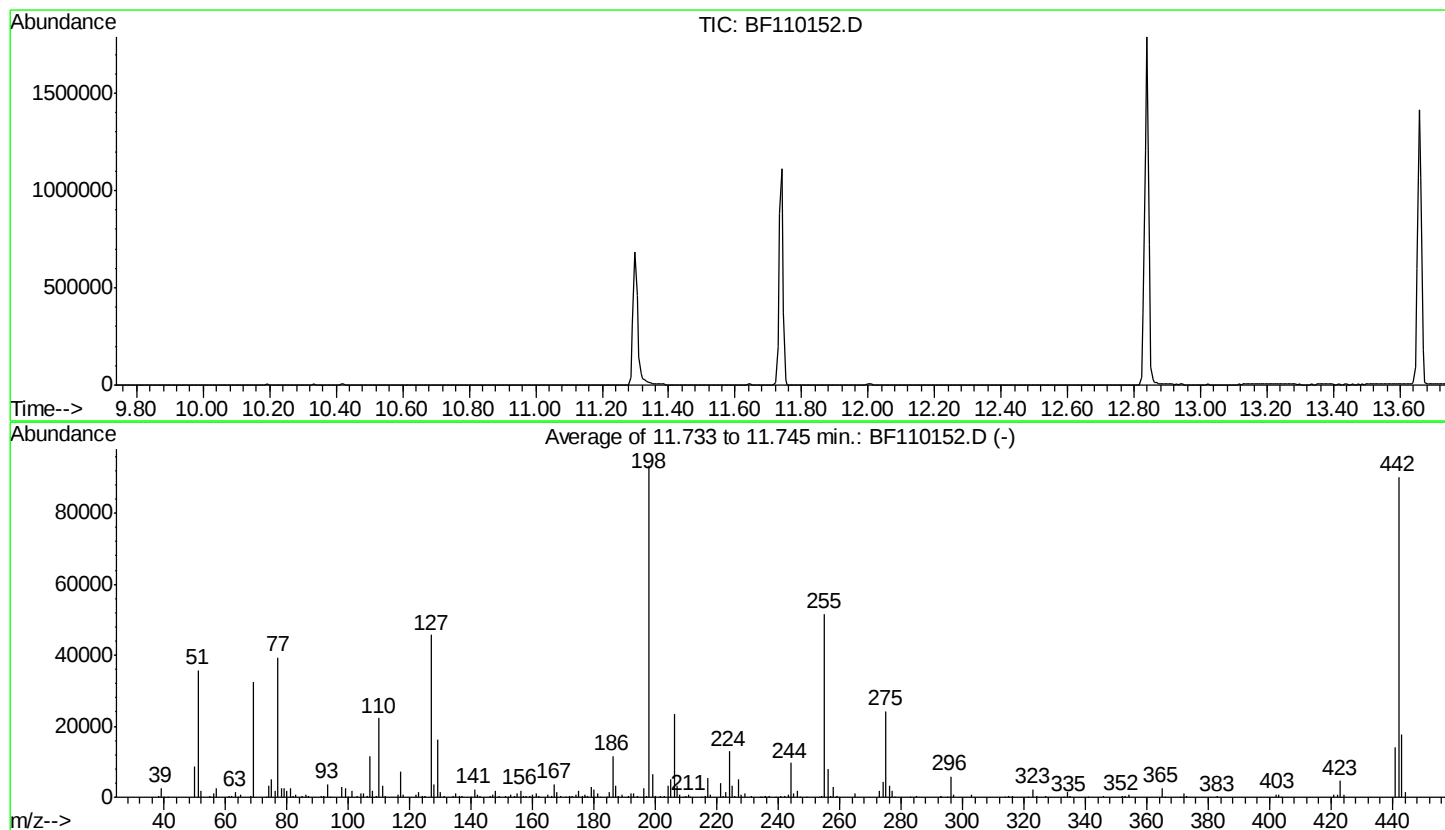

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	35754	PASS
68	69	0.00	2	1.4	443	PASS
69	198	0.00	100	34.7	32380	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	45785	PASS
197	198	0.00	2	0.3	316	PASS
198	198	100	100	100.0	93394	PASS
199	198	5	9	6.9	6471	PASS
275	198	10	60	25.9	24210	PASS
365	198	1	100	2.9	2665	PASS
441	198	0.01	100	14.9	13957	PASS
442	198	50	100	96.6	90240	PASS
443	442	15	24	19.4	17507	PASS