


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102518\
Data File : BF110189.D
Acq On : 26 Oct 2018 4:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 23 15:06:18 2018

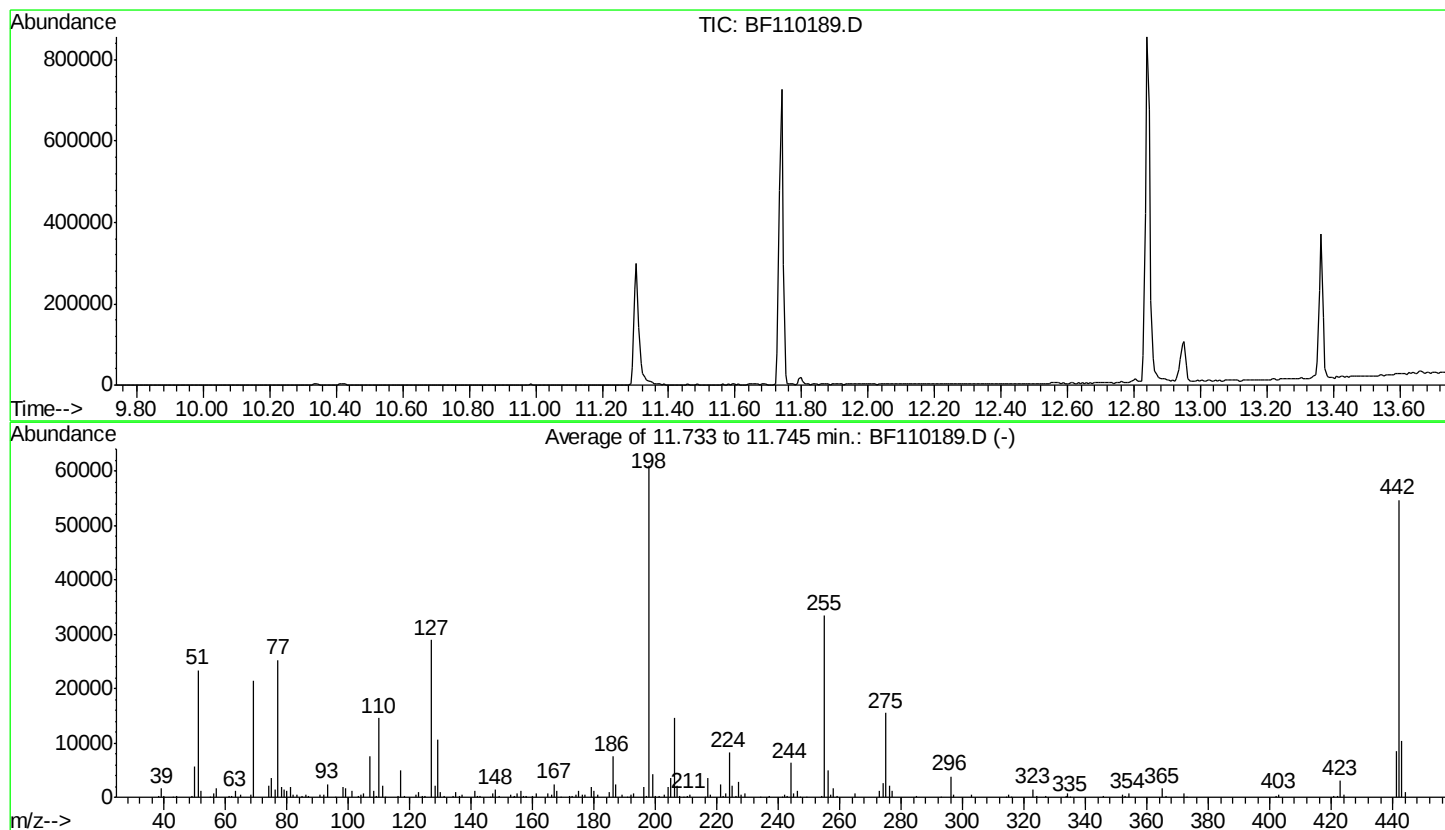

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	23348	PASS
68	69	0.00	2	1.7	370	PASS
69	198	0.00	100	35.0	21348	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	28888	PASS
197	198	0.00	2	0.6	347	PASS
198	198	100	100	100.0	60973	PASS
199	198	5	9	7.0	4273	PASS
275	198	10	60	25.4	15504	PASS
365	198	1	100	2.6	1578	PASS
441	198	0.01	100	14.0	8525	PASS
442	198	50	100	89.6	54629	PASS
443	442	15	24	19.2	10471	PASS