
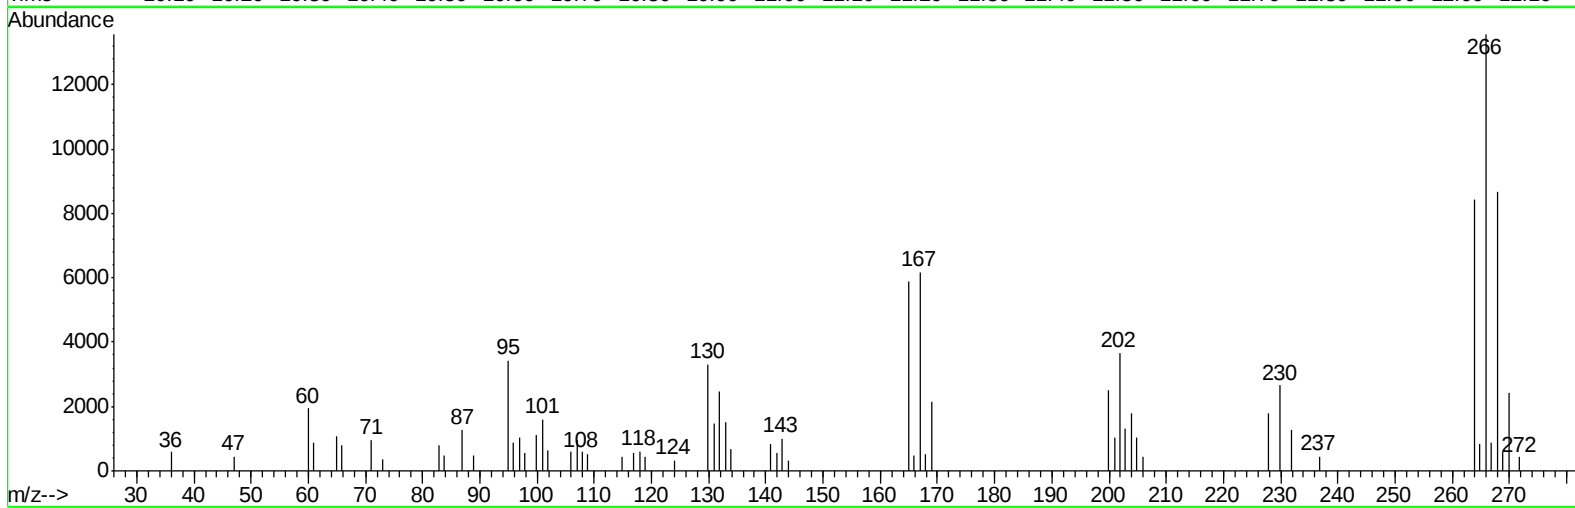


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102519\
Data File : BF117532.D
Acq On : 25 Oct 2019 12:28
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 07:14:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

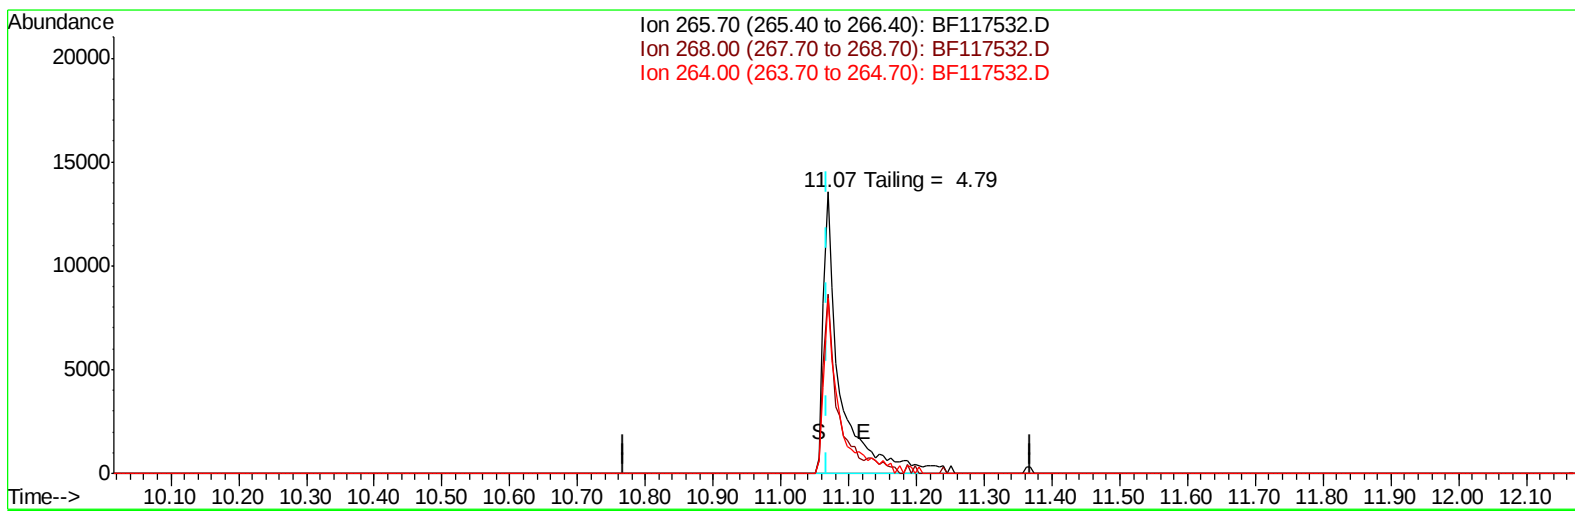

TIC: BF117532.D

(70) Pentachlorophenol (C)



11.069min (-0.000) 0.00ng

response 21378

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	63.84
264.00	64.30	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102519\
Data File : BF117532.D
Acq On : 25 Oct 2019 12:28
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 07:14:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

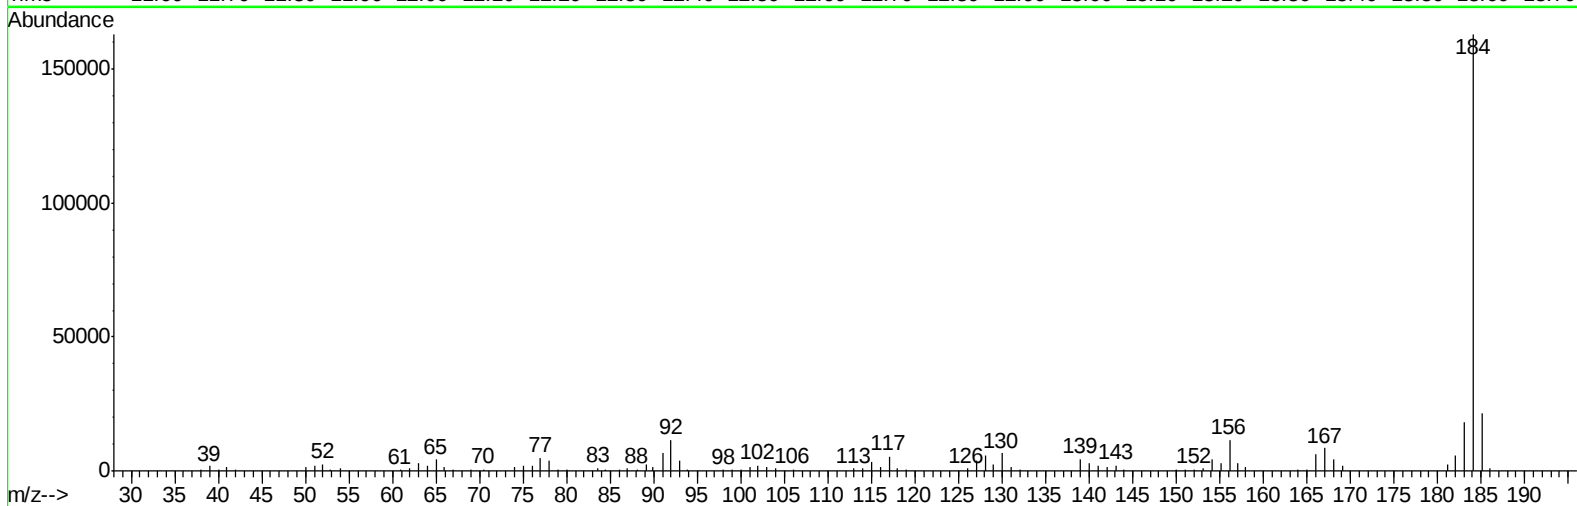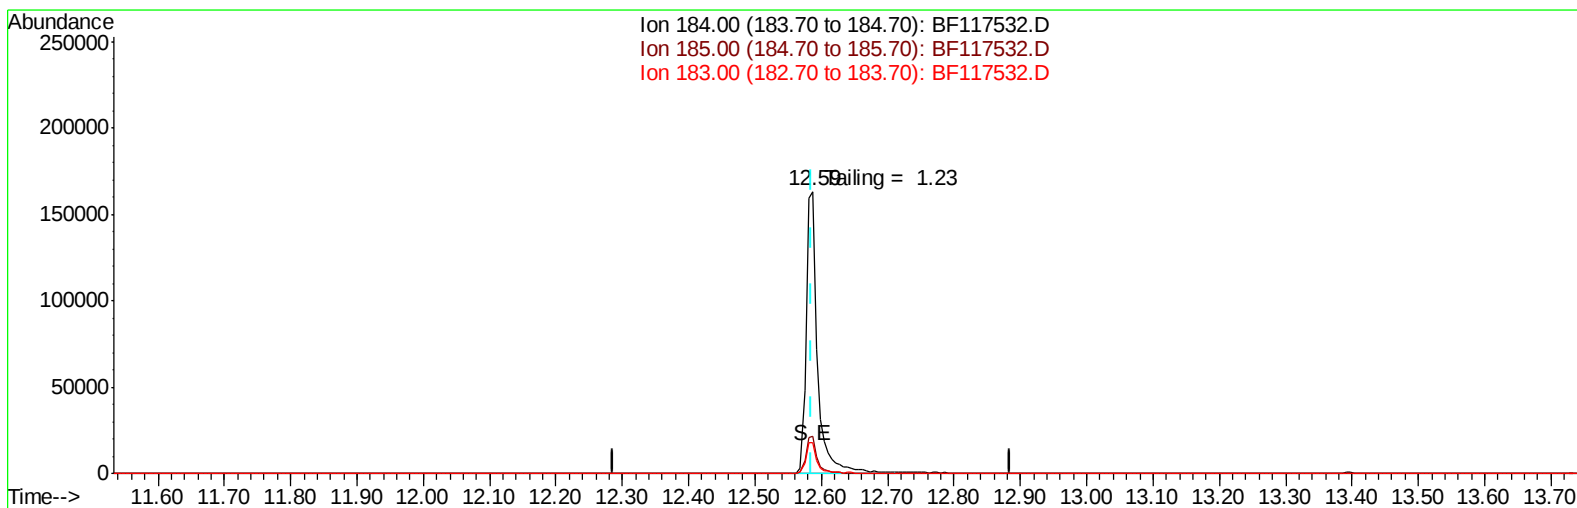

TIC: BF117532.D

(77) Benzidine

12.586min (+0.000) -20.00ng

response 195668

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.33
183.00	12.00	11.09
0.00	0.00	0.00