

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
 Data File : BF117549.D
 Acq On : 25 Oct 2019 21:07
 Operator : JU
 Sample : K5500-05 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 801-50-(0-1.1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	555	558	571	rBV	49818	89353	37.44%	4.193%
2	6.398	730	733	749	rBV2	65764	116371	48.77%	5.461%
3	6.516	749	753	760	rBV	98436	120558	50.52%	5.657%
4	6.733	787	790	801	rBV	192265	186302	78.07%	8.742%
5	6.886	813	816	824	rBV	93621	92132	38.61%	4.323%
6	7.304	884	887	908	rBV	28114	55216	23.14%	2.591%
7	8.016	1004	1008	1024	rBV	235960	236671	99.18%	11.106%
8	9.033	1178	1181	1184	rBB	6376	5474	2.29%	0.257%
9	9.086	1187	1190	1200	rVV	129737	126438	52.98%	5.933%
10	9.157	1200	1202	1209	rVB4	6429	9746	4.08%	0.457%
11	9.486	1253	1258	1261	rBV2	15071	19254	8.07%	0.904%
12	9.533	1263	1266	1271	rVB3	2353	3207	1.34%	0.150%
13	9.580	1271	1274	1279	rVB	1945	3169	1.33%	0.149%
14	9.627	1279	1282	1286	rBV2	3299	4602	1.93%	0.216%
15	9.669	1286	1289	1291	rVB	5926	4362	1.83%	0.205%
16	9.763	1302	1305	1311	rBV	267567	238631	100.00%	11.198%
17	10.410	1414	1415	1420	rVB	3345	3947	1.65%	0.185%
18	10.563	1438	1441	1447	rBV	48618	49437	20.72%	2.320%
19	10.680	1454	1461	1464	rBV3	8037	9839	4.12%	0.462%
20	10.986	1510	1513	1516	rBV2	2378	3706	1.55%	0.174%
21	11.145	1537	1540	1543	rVB3	4390	4871	2.04%	0.229%
22	11.251	1555	1558	1565	rBV2	226119	218024	91.36%	10.231%
23	11.498	1594	1600	1602	rBV5	3435	5659	2.37%	0.266%
24	11.780	1646	1648	1652	rBV3	3792	3231	1.35%	0.152%
25	12.327	1736	1741	1745	rBV7	4034	7256	3.04%	0.340%
26	12.833	1823	1827	1831	rBV	143300	120140	50.35%	5.638%
27	13.010	1855	1857	1860	rBV4	4773	3967	1.66%	0.186%
28	13.268	1899	1901	1908	rVB8	7709	10644	4.46%	0.499%
29	13.898	2005	2008	2014	rBV	216793	213297	89.38%	10.009%
30	15.339	2250	2253	2262	rVB	118843	165492	69.35%	7.766%


Sum of corrected areas: 2130996

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
Data File : BF117549.D
Acq On : 25 Oct 2019 21:07
Operator : JU
Sample : K5500-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
801-50-(0-1.1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

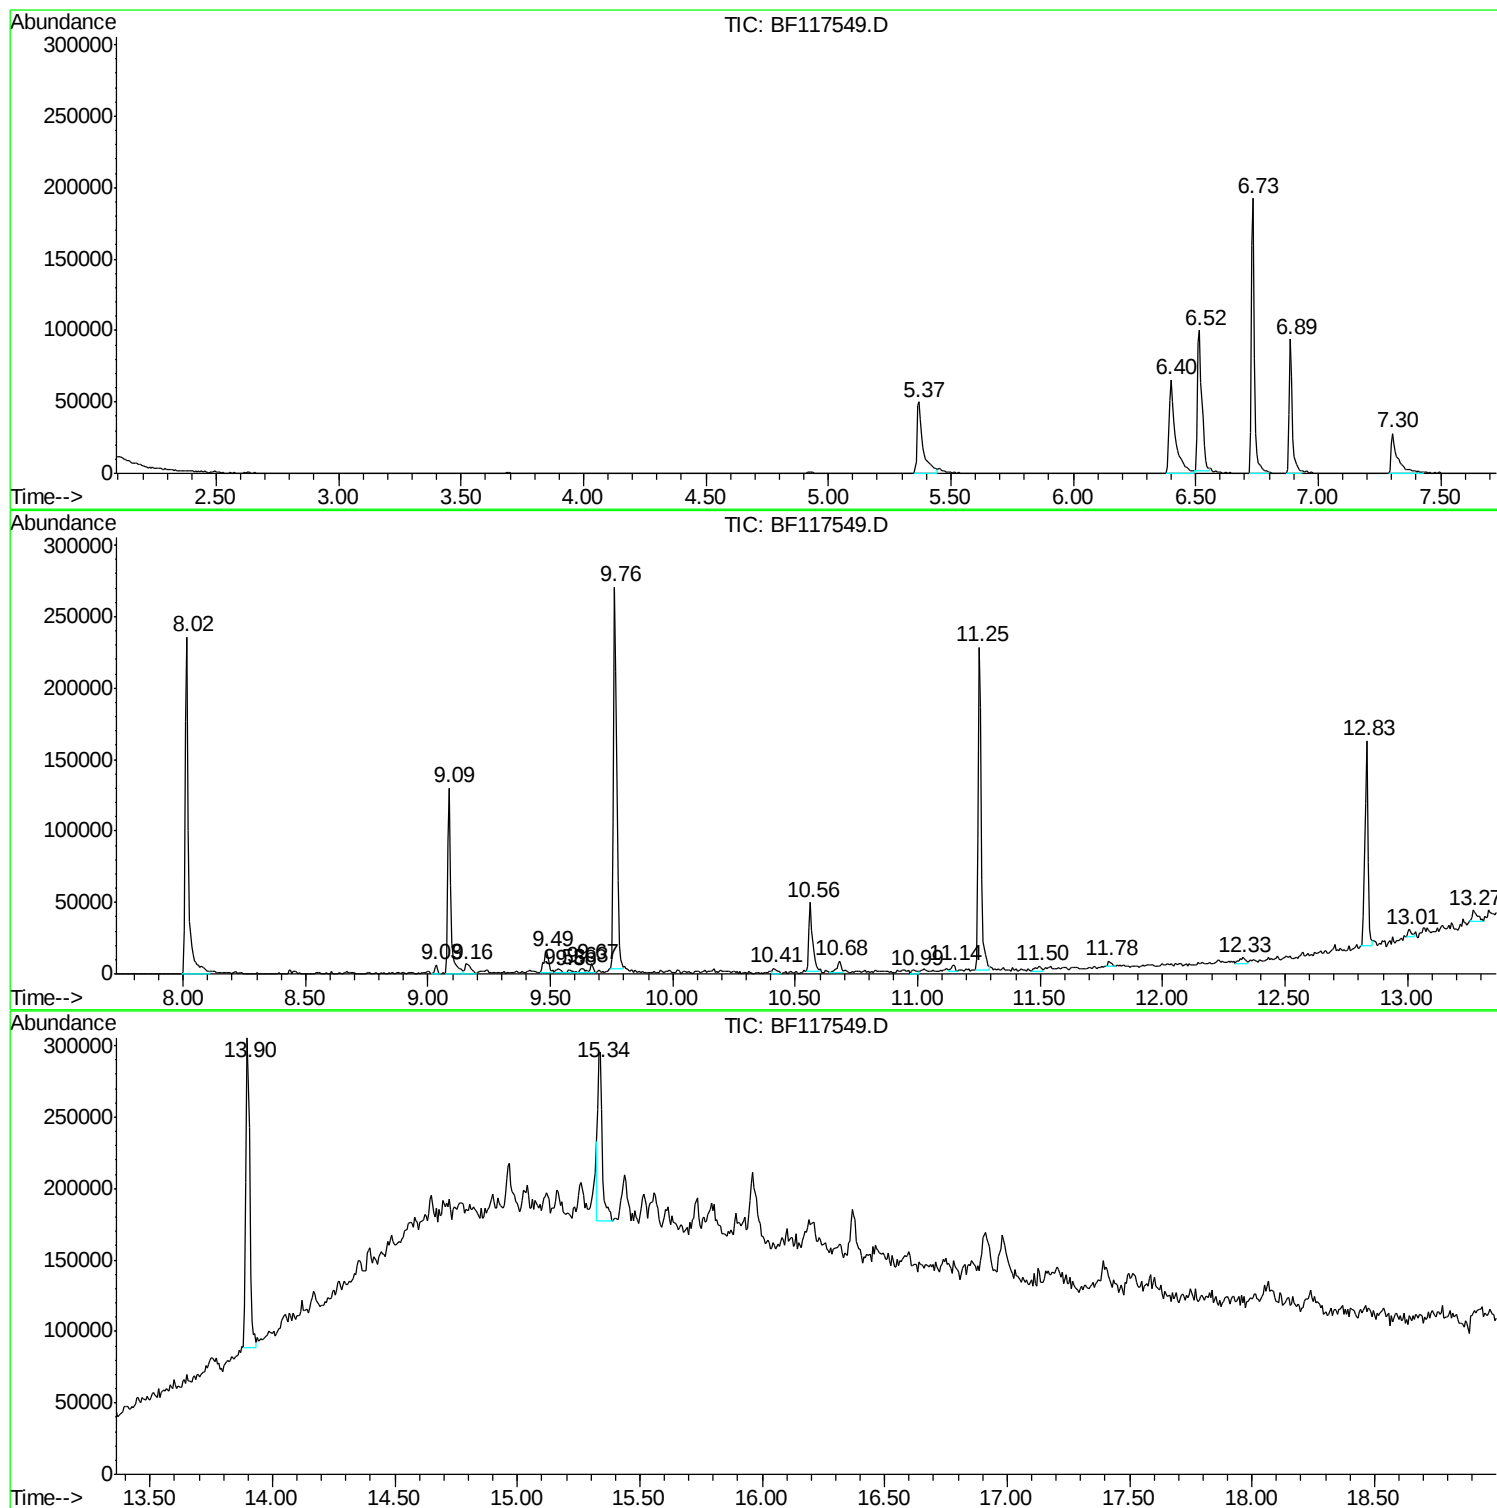

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
Data File : BF117549.D
Acq On : 25 Oct 2019 21:07
Operator : JU
Sample : K5500-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
801-50-(0-1.1)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	12.94 ng	120558	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
4		1-Isoquinolinemethanol, .alpha.-...	191	C12H17NO	114608-92-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

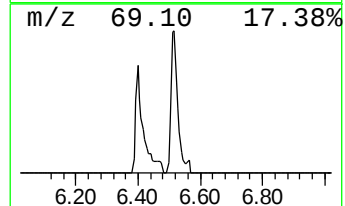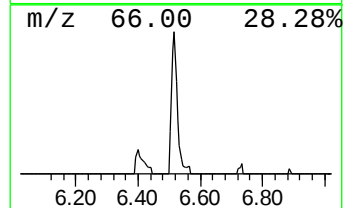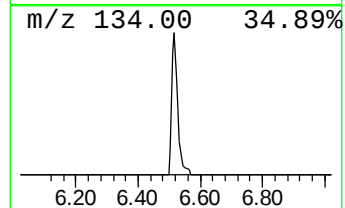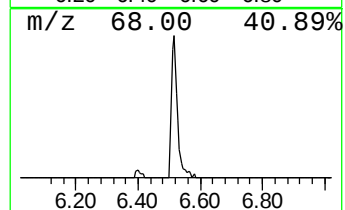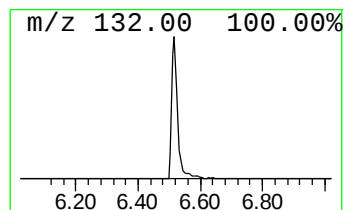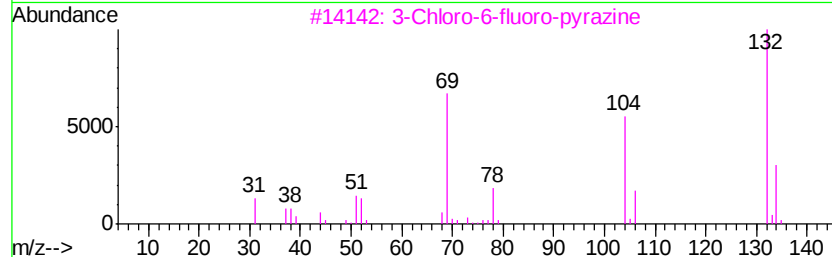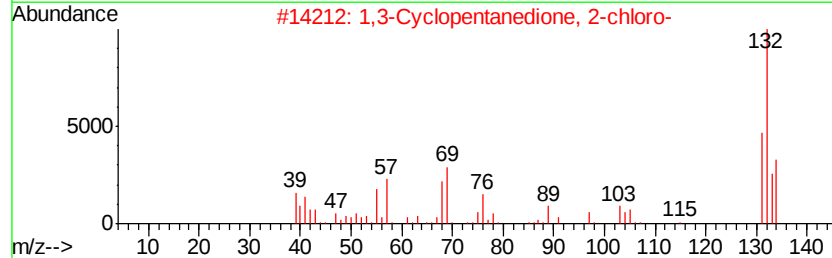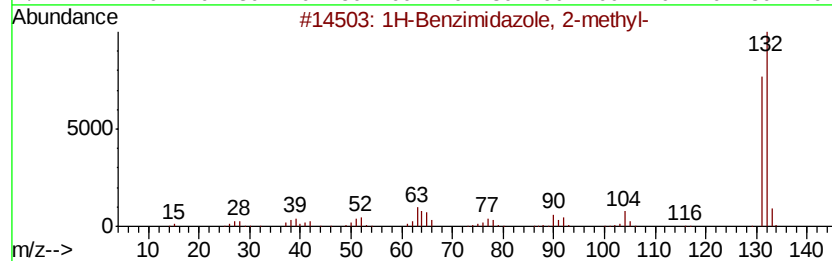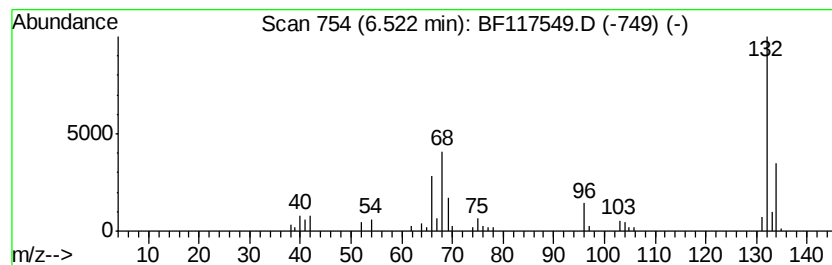

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102519\
Data File : BF117549.D
Acq On : 25 Oct 2019 21:07
Operator : JU
Sample : K5500-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
801-50-(0-1.1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.52	6.52	12.9	ng	120558	1	6.73	186302	20.0