

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
 Data File : BF117551.D
 Acq On : 25 Oct 2019 22:00
 Operator : JU
 Sample : K5501-19 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 182-66-(0-2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	555	558	569	rBV	57767	93340	36.29%	4.208%
2	6.398	730	733	748	rBV	72403	122374	47.58%	5.517%
3	6.516	750	753	766	rVB	110410	131676	51.19%	5.937%
4	6.734	786	790	802	rBV	207445	200864	78.09%	9.056%
5	6.886	813	816	822	rBV	95466	94103	36.59%	4.243%
6	7.304	884	887	897	rBV	30844	52460	20.40%	2.365%
7	8.016	1004	1008	1016	rBV	259338	244894	95.21%	11.041%
8	8.639	1111	1114	1121	rBB2	3997	6448	2.51%	0.291%
9	8.839	1145	1148	1154	rBV2	3208	5433	2.11%	0.245%
10	9.086	1187	1190	1198	rBV	152956	128126	49.81%	5.777%
11	9.480	1252	1257	1262	rBV	16714	17319	6.73%	0.781%
12	9.769	1302	1306	1320	rVB	270668	257206	100.00%	11.596%
13	10.192	1375	1378	1382	rVB3	2645	3272	1.27%	0.148%
14	10.492	1425	1429	1431	rBV	3132	3044	1.18%	0.137%
15	10.563	1438	1441	1447	rBV	55854	53419	20.77%	2.408%
16	10.633	1449	1453	1456	rVV2	3182	2908	1.13%	0.131%
17	10.669	1456	1459	1461	rBV	2963	2880	1.12%	0.130%
18	10.692	1461	1463	1466	rVB2	2510	2910	1.13%	0.131%
19	10.739	1469	1471	1472	rBV	3688	3158	1.23%	0.142%
20	10.769	1472	1476	1480	rVB4	2791	5040	1.96%	0.227%
21	10.921	1498	1502	1505	rBV4	4946	6073	2.36%	0.274%
22	10.957	1505	1508	1511	rVB	4186	4827	1.88%	0.218%
23	10.992	1511	1514	1517	rBV3	3305	4002	1.56%	0.180%
24	11.116	1532	1535	1536	rBV3	2990	3162	1.23%	0.143%
25	11.204	1547	1550	1555	rBV5	3718	4858	1.89%	0.219%
26	11.257	1555	1559	1566	rBV	230803	237609	92.38%	10.713%
27	11.786	1645	1649	1651	rBV3	12294	15172	5.90%	0.684%
28	12.051	1692	1694	1696	rBV2	2917	3532	1.37%	0.159%
29	12.474	1763	1766	1768	rBV	16288	16958	6.59%	0.765%
30	12.704	1802	1805	1807	rBV	12218	14793	5.75%	0.667%
31	12.833	1824	1827	1832	rBV	143146	121707	47.32%	5.487%
32	12.915	1839	1841	1842	rBV2	7915	3771	1.47%	0.170%
33	13.898	2005	2008	2015	rBV	191915	229901	89.38%	10.365%
34	15.339	2250	2253	2257	rVB	98667	120735	46.94%	5.443%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102519\
Data File : BF117551.D
Acq On : 25 Oct 2019 22:00
Operator : JU
Sample : K5501-19 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
182-66-(0-2)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 2217974

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
Data File : BF117551.D
Acq On : 25 Oct 2019 22:00
Operator : JU
Sample : K5501-19 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
182-66-(0-2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

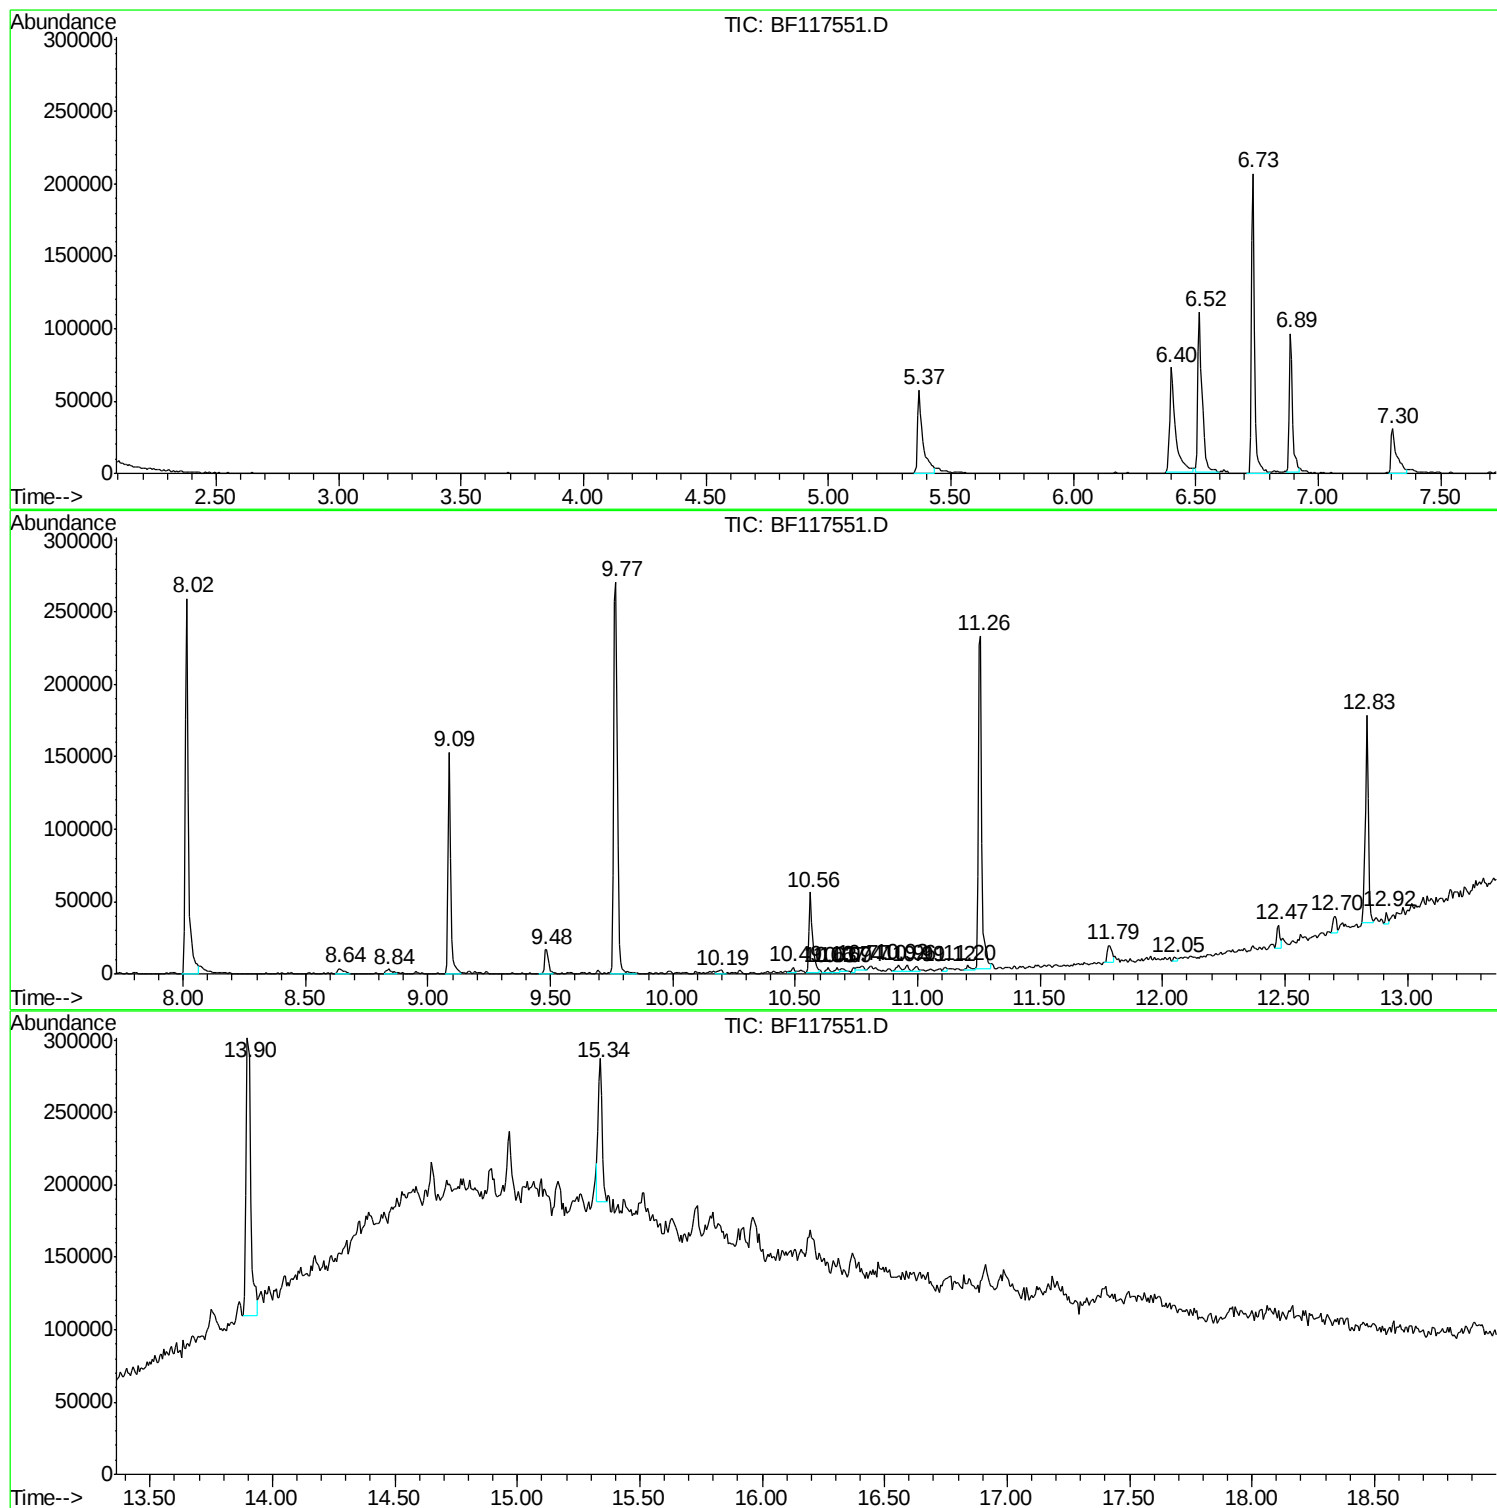

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
Data File : BF117551.D
Acq On : 25 Oct 2019 22:00
Operator : JU
Sample : K5501-19 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
182-66-(0-2)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	13.11 ng	131676	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		Amphetaminil	250	C17H18N2	017590-01-1	10
5		5-Aminoindole	132	C8H8N2	005192-03-0	10

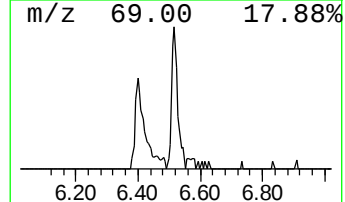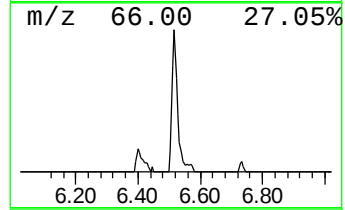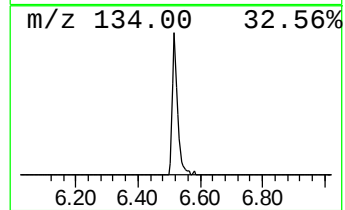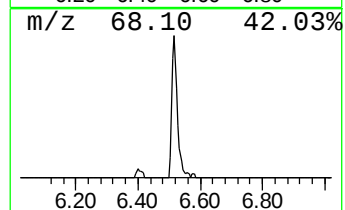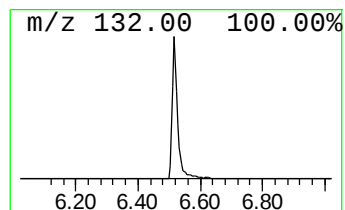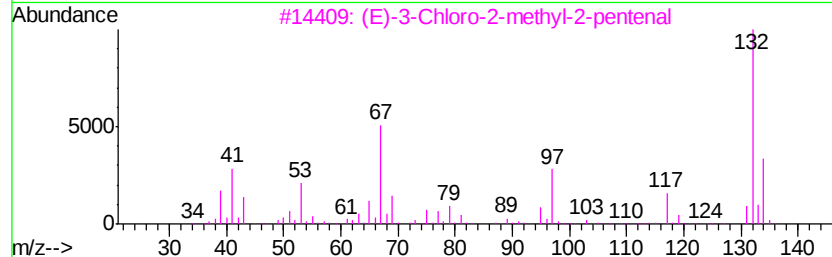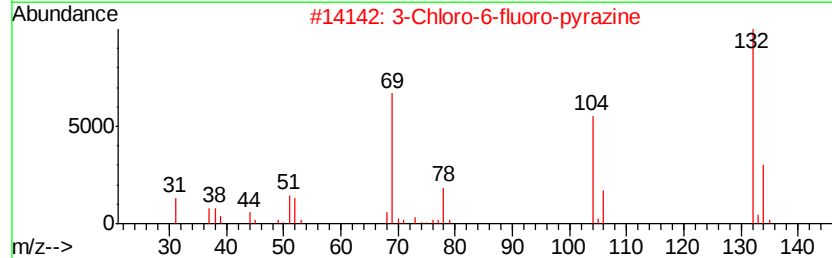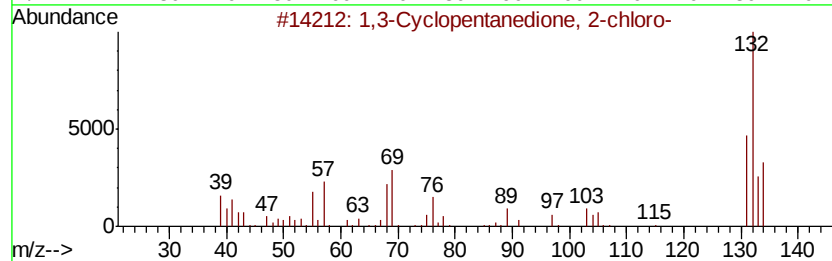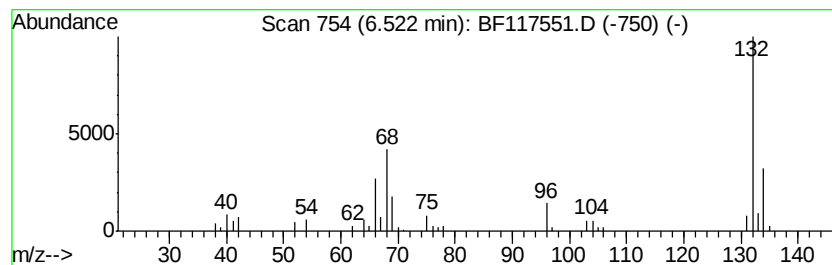

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102519\
Data File : BF117551.D
Acq On : 25 Oct 2019 22:00
Operator : JU
Sample : K5501-19 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
182-66-(0-2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.52	6.52	13.1	ng	131676	1	6.73	200864	20.0