

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
 Data File : BF117552.D
 Acq On : 25 Oct 2019 22:27
 Operator : JU
 Sample : K5502-03 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 181-50-(0-2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	555	558	568	rBV	59508	99063	37.55%	4.516%
2	6.398	729	733	750	rBV	78992	138817	52.62%	6.328%
3	6.516	750	753	762	rVB	111537	138703	52.57%	6.323%
4	6.734	787	790	800	rBV	207258	197171	74.73%	8.989%
5	6.887	813	816	829	rBV	100217	99197	37.60%	4.522%
6	7.304	884	887	901	rBV	33499	55902	21.19%	2.548%
7	8.016	1005	1008	1019	rBV	253684	248320	94.12%	11.320%
8	9.086	1187	1190	1202	rBV	135501	118976	45.10%	5.424%
9	9.486	1255	1258	1264	rBB	18481	16505	6.26%	0.752%
10	9.769	1302	1306	1315	rBV	265798	263830	100.00%	12.027%
11	10.563	1438	1441	1449	rBB	53588	50502	19.14%	2.302%
12	10.669	1454	1459	1465	rBB3	2107	3448	1.31%	0.157%
13	11.251	1555	1558	1568	rBV	222305	238465	90.39%	10.871%
14	11.780	1645	1648	1655	rBV5	5690	7827	2.97%	0.357%
15	11.945	1673	1676	1678	rBV3	2068	3157	1.20%	0.144%
16	12.369	1745	1748	1750	rBV2	3143	3367	1.28%	0.153%
17	12.439	1758	1760	1764	rBV4	2480	3510	1.33%	0.160%
18	12.474	1764	1766	1770	rVV	5859	6617	2.51%	0.302%
19	12.698	1802	1804	1808	rVB2	6827	7734	2.93%	0.353%
20	12.733	1808	1810	1813	rBV4	3371	4212	1.60%	0.192%
21	12.833	1824	1827	1832	rBV	115913	100121	37.95%	4.564%
22	13.063	1864	1866	1869	rVB3	6128	4454	1.69%	0.203%
23	13.092	1869	1871	1873	rBV3	3647	3415	1.29%	0.156%
24	13.139	1877	1879	1880	rBV2	4345	2838	1.08%	0.129%
25	13.198	1887	1889	1890	rBV	3772	3029	1.15%	0.138%
26	13.386	1917	1921	1922	rBV4	5676	4920	1.86%	0.224%
27	13.898	2005	2008	2013	rBV	189965	206874	78.41%	9.431%
28	15.339	2249	2253	2259	rVB	117232	162593	61.63%	7.412%


Sum of corrected areas: 2193567

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
Data File : BF117552.D
Acq On : 25 Oct 2019 22:27
Operator : JU
Sample : K5502-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
181-50-(0-2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

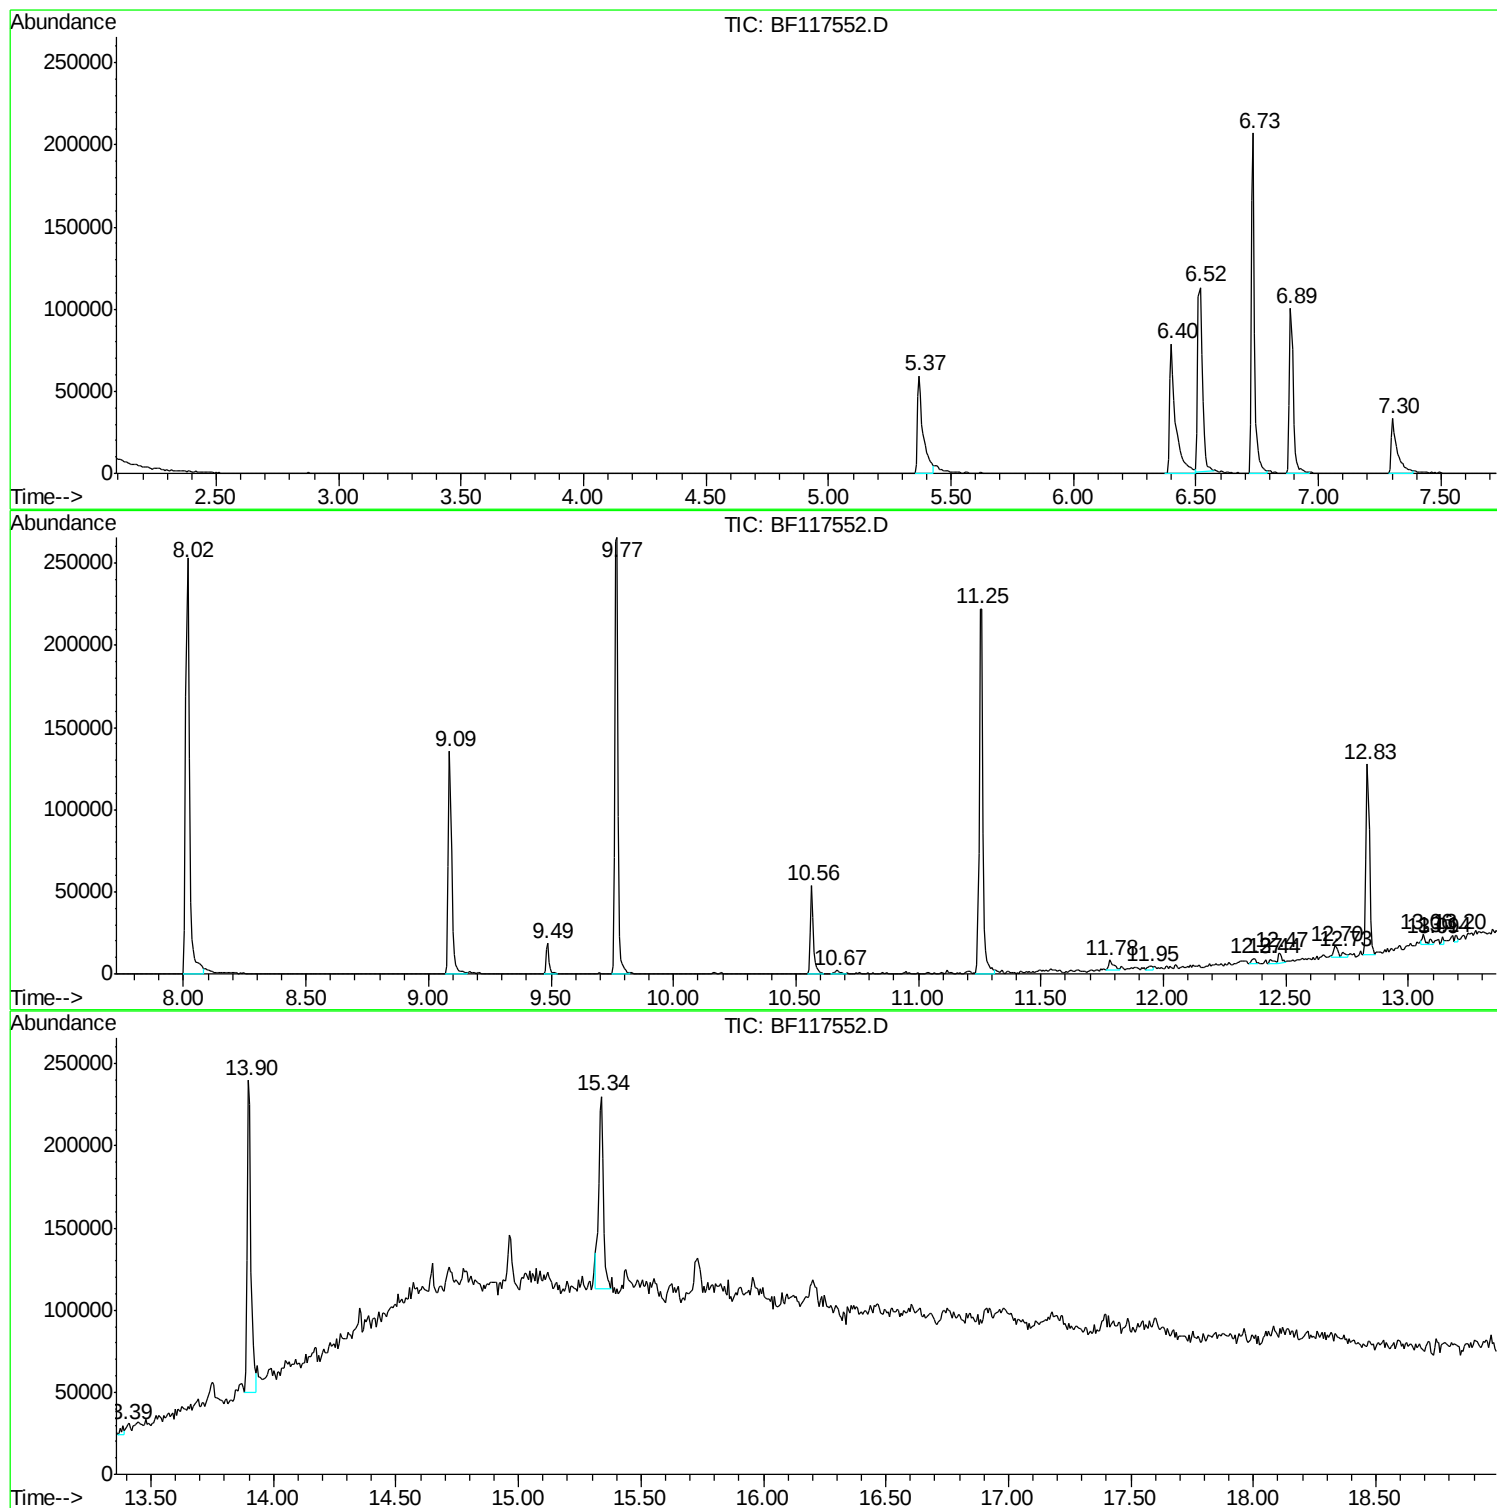

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102519\
Data File : BF117552.D
Acq On : 25 Oct 2019 22:27
Operator : JU
Sample : K5502-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
181-50-(0-2)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	14.07 ng	138703	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
2		Amphetaminil	250	C17H18N2	017590-01-1	10
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

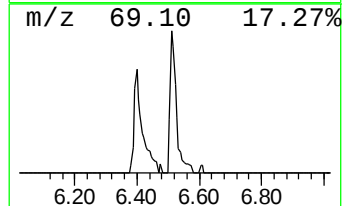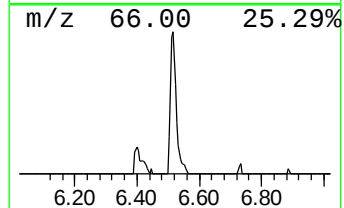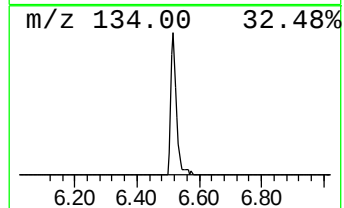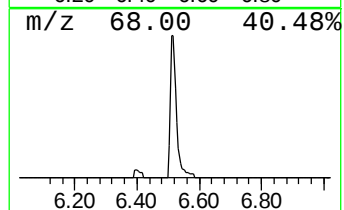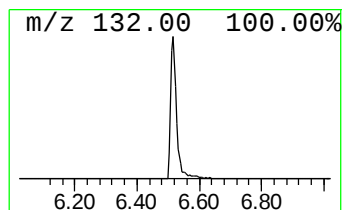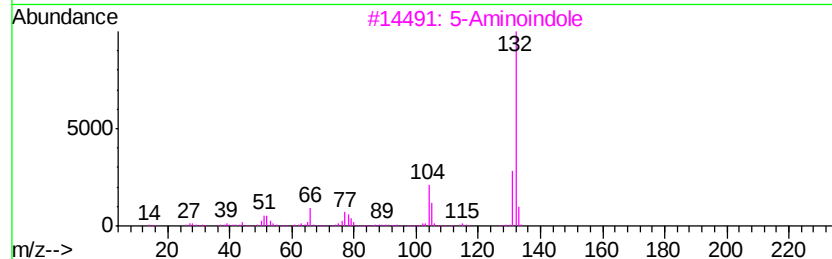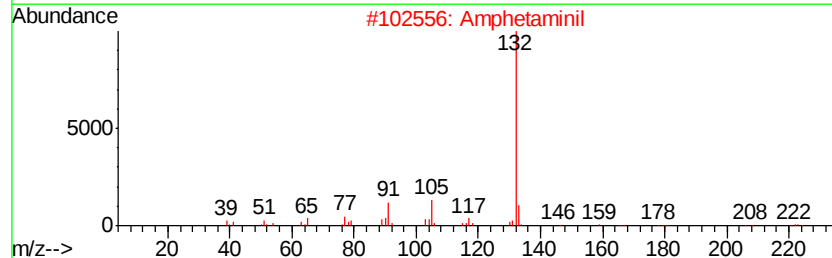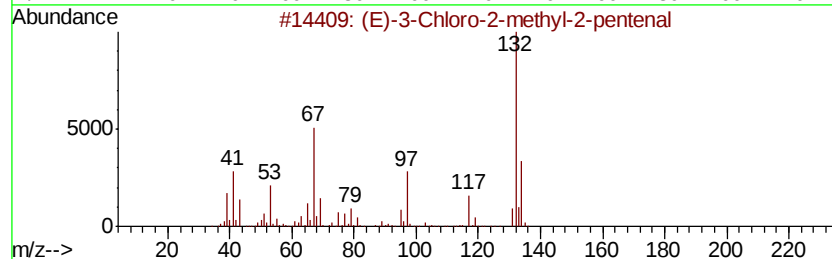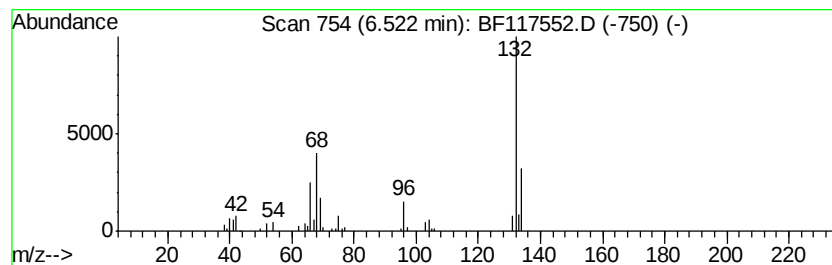

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102519\
Data File : BF117552.D
Acq On : 25 Oct 2019 22:27
Operator : JU
Sample : K5502-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
181-50-(0-2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.52	6.52	14.1	ng	138703	1	6.73	197171	20.0