


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102519\
 Data File : BF117532.D
 Acq On : 25 Oct 2019 12:28
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

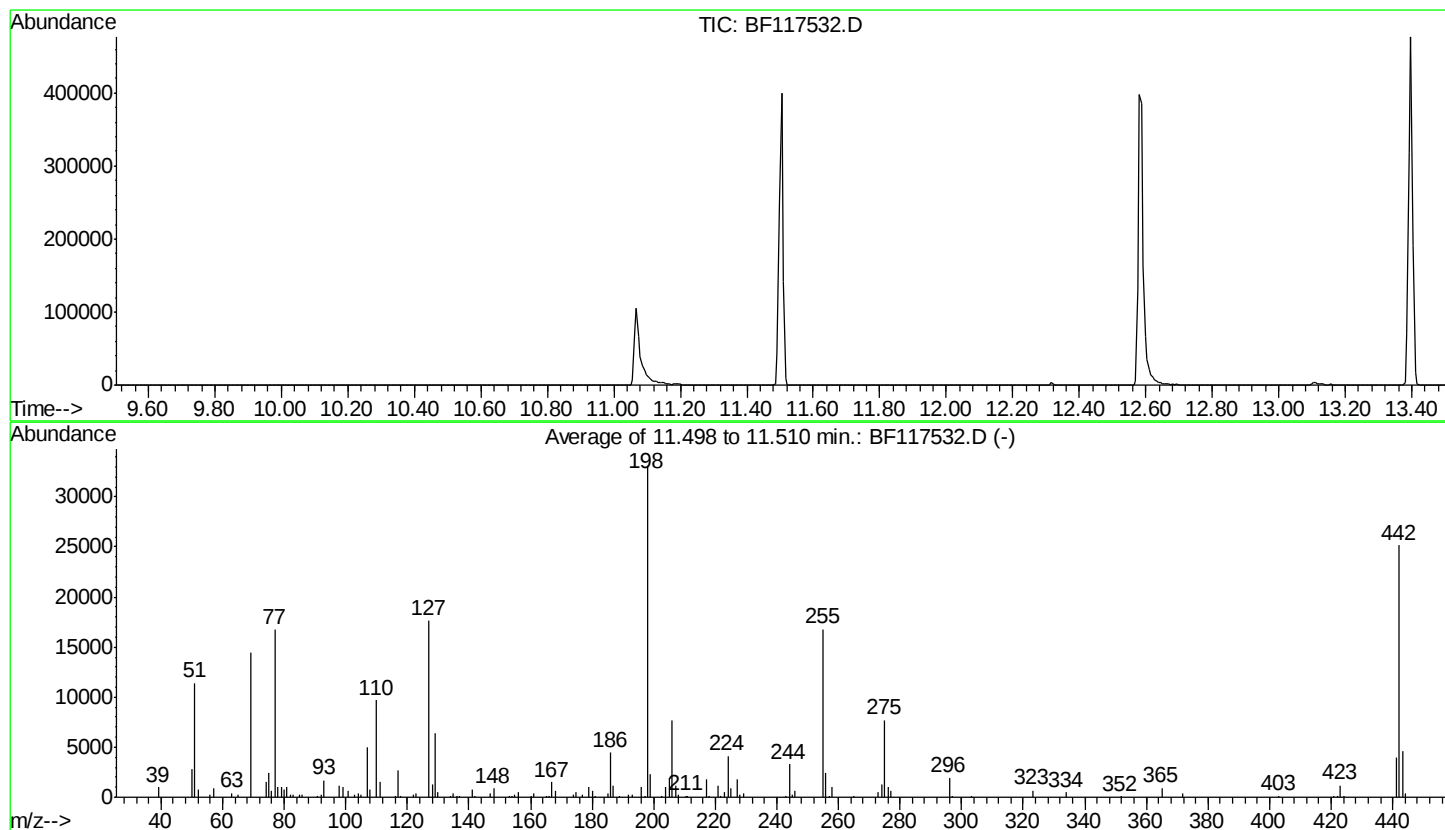

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	11423	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.6	14444	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	17609	PASS
197	198	0.00	2	0.4	148	PASS
198	198	100	100	100.0	33114	PASS
199	198	5	9	6.8	2260	PASS
275	198	10	60	23.2	7694	PASS
365	198	1	100	2.9	963	PASS
441	198	0.01	100	11.8	3923	PASS
442	198	50	100	75.9	25137	PASS
443	442	15	24	18.3	4609	PASS