
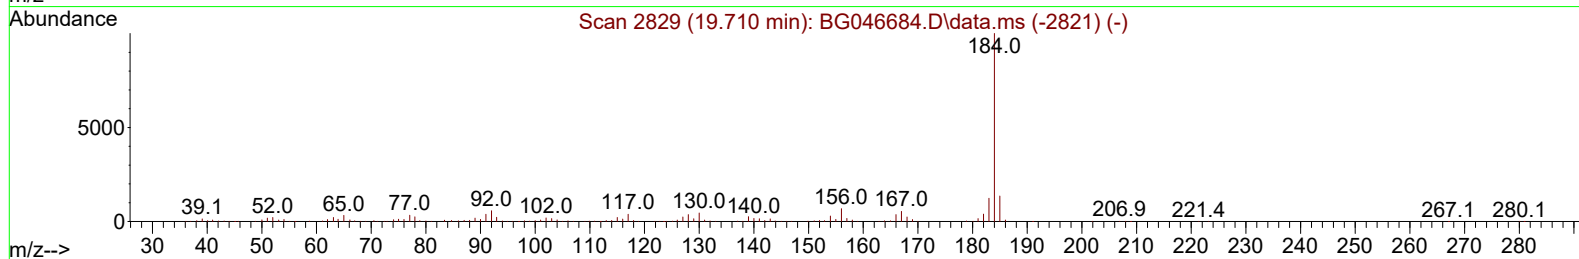
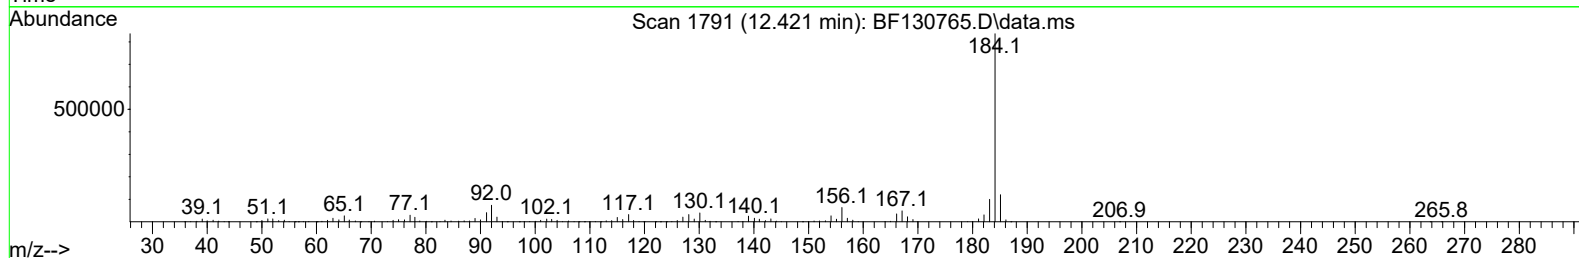


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102522\
 Data File : BF130765.D
 Acq On : 25 Oct 2022 10:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 15:09:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 21 06:12:36 2022
 Response via : Initial Calibration

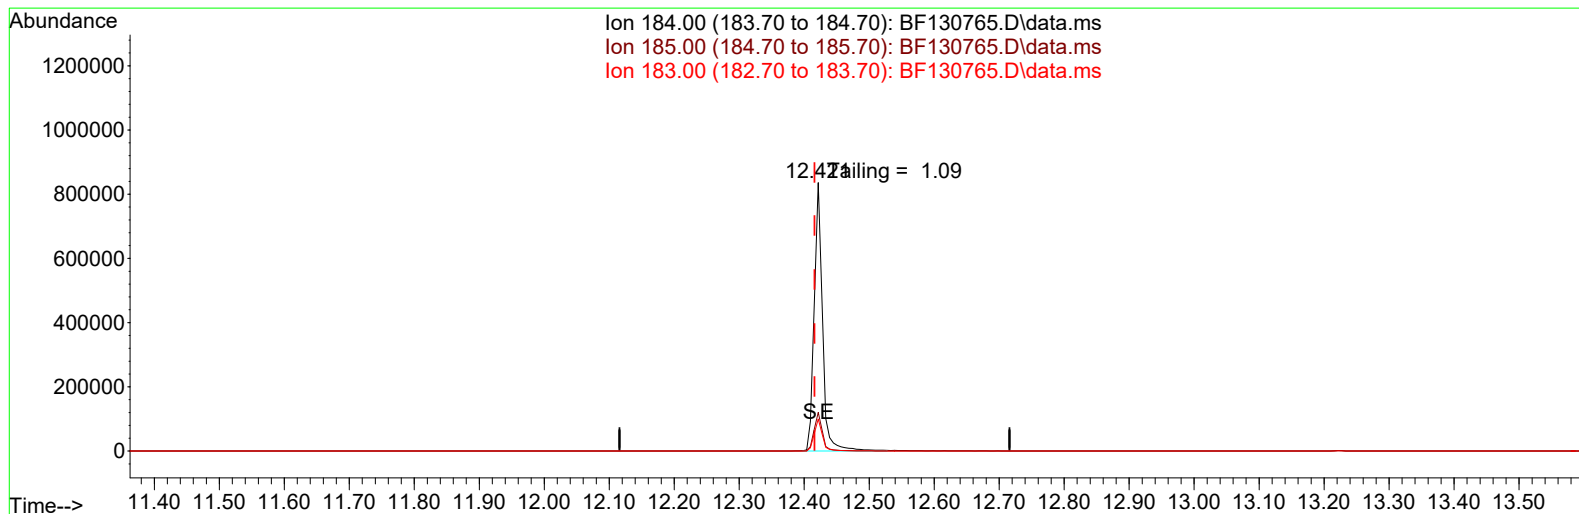

TIC: BF130765.D\data.ms

(77) Benzidine




12.421min (+ 0.005) 0.00 ng

response 759841

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.40
183.00	11.60	11.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102522\
Data File : BF130765.D
Acq On : 25 Oct 2022 10:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 15:09:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 06:12:36 2022
Response via : Initial Calibration

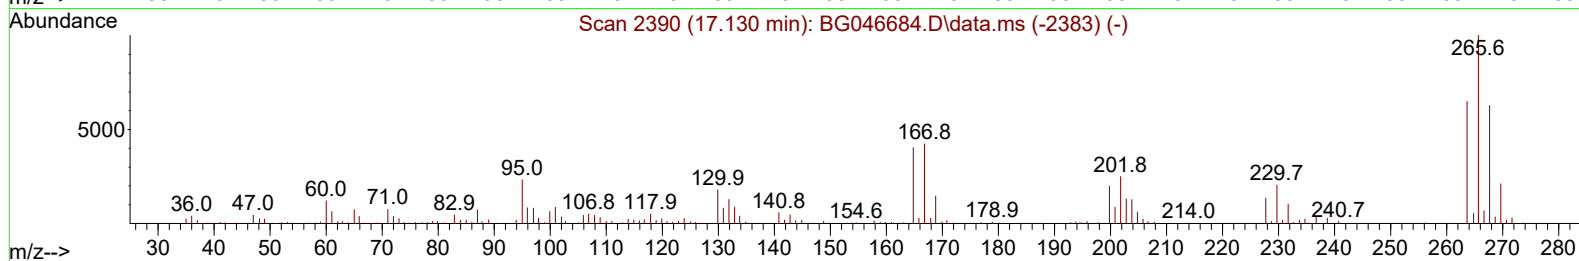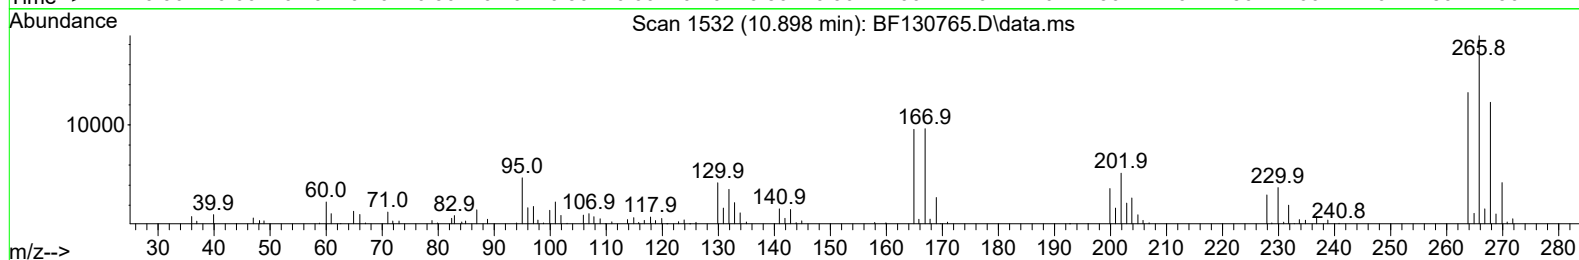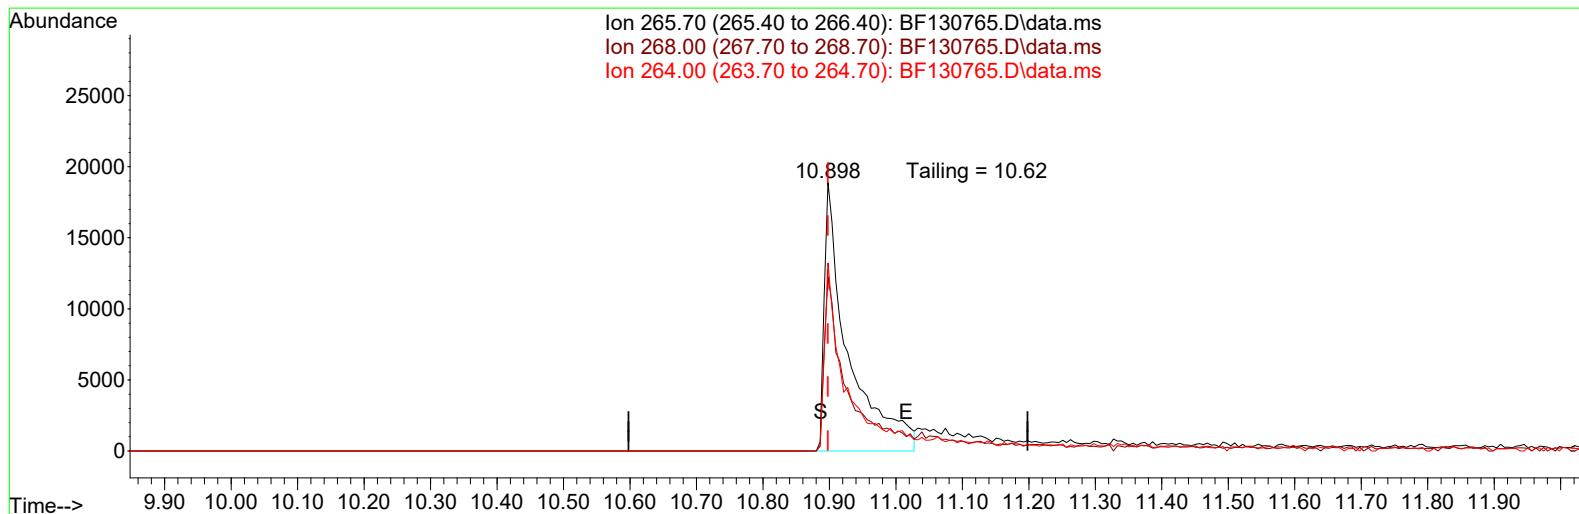

TIC: BF130765.D\data.ms

(70) Pentachlorophenol (C)**10.898min (-0.000) 2044.80 ng****response 46896**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.86
264.00	67.00	70.04
0.00	0.00	0.00