


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102522\
 Data File : BF130765.D
 Acq On : 25 Oct 2022 10:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 21 06:12:36 2022

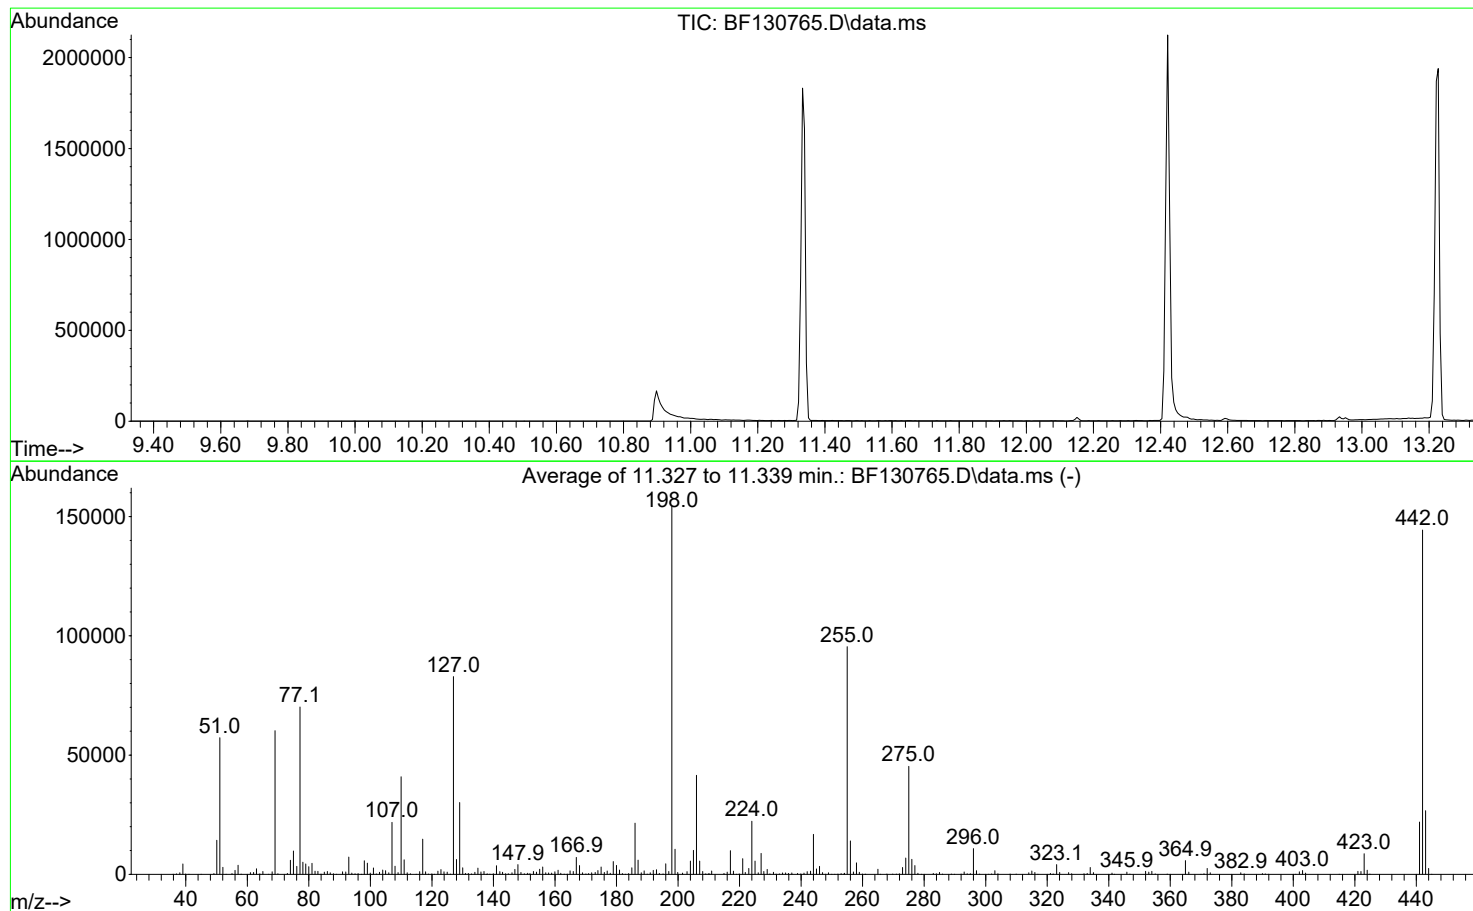




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	57283	PASS
68	69	0.00	2	1.8	1110	PASS
69	198	0.00	100	39.1	60264	PASS
70	69	0.00	2	0.5	295	PASS
127	198	10	80	53.8	82904	PASS
197	198	0.00	2	0.8	1239	PASS
198	198	100	100	100.0	154203	PASS
199	198	5	9	6.8	10546	PASS
275	198	10	60	29.4	45304	PASS
365	198	1	100	3.7	5758	PASS
441	198	0.01	100	14.2	21934	PASS
442	442	50	100	100.0	144320	PASS
443	442	15	24	18.5	26718	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102522\
 Data File : BF130765.D
 Acq On : 25 Oct 2022 10:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 25 15:09:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 21 06:12:36 2022
 Response via : Initial Calibration

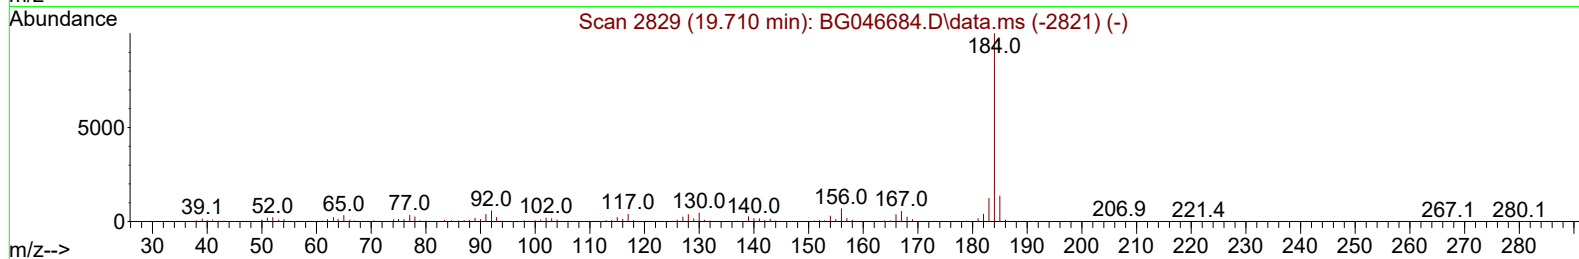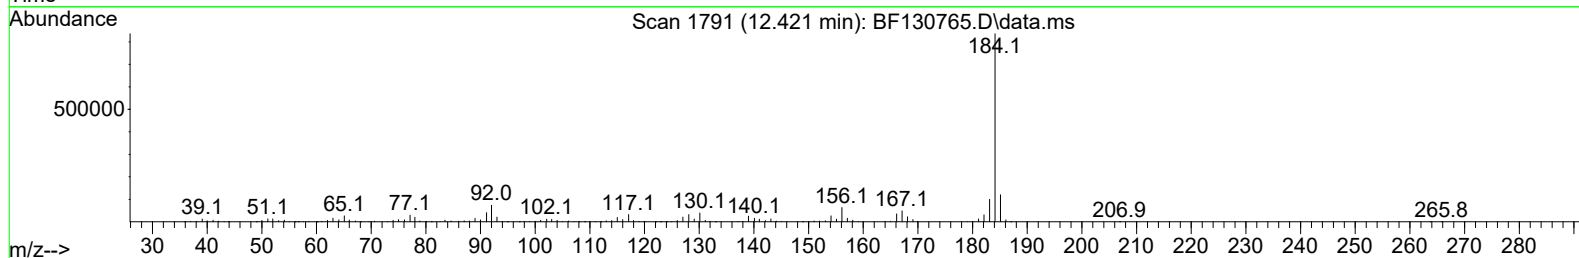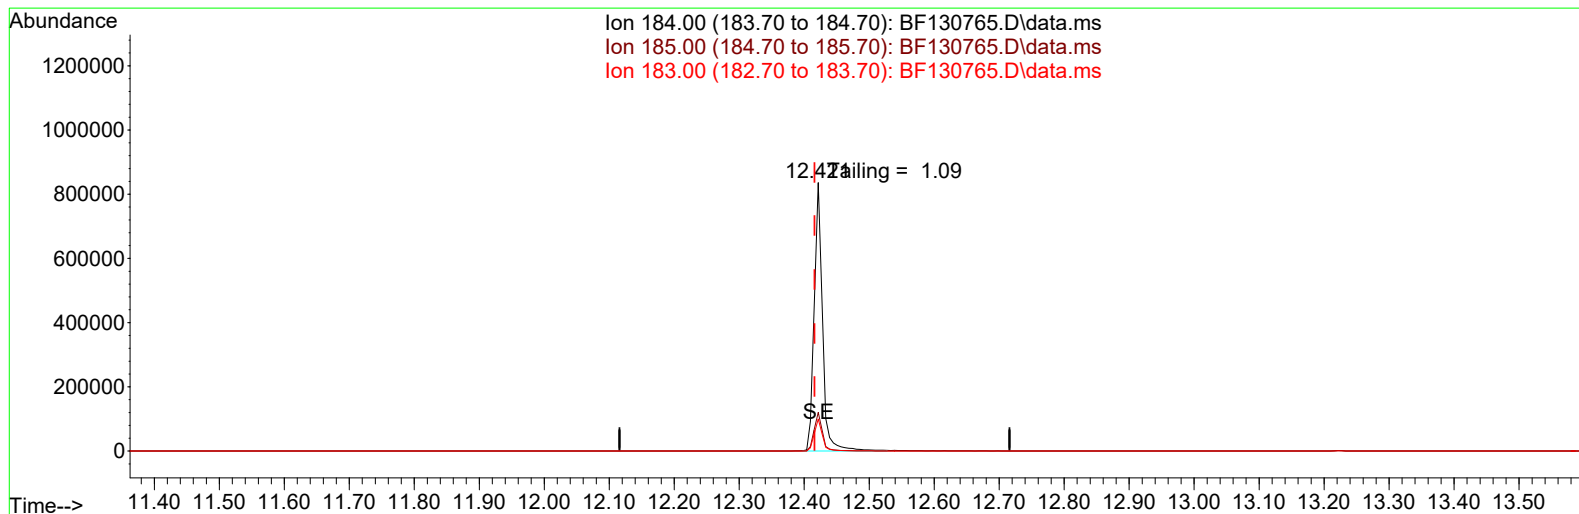

TIC: BF130765.D\data.ms

(77) Benzidine

12.421min (+ 0.005) 0.00 ng




response 759841

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.40
183.00	11.60	11.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102522\
Data File : BF130765.D
Acq On : 25 Oct 2022 10:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 15:09:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 06:12:36 2022
Response via : Initial Calibration

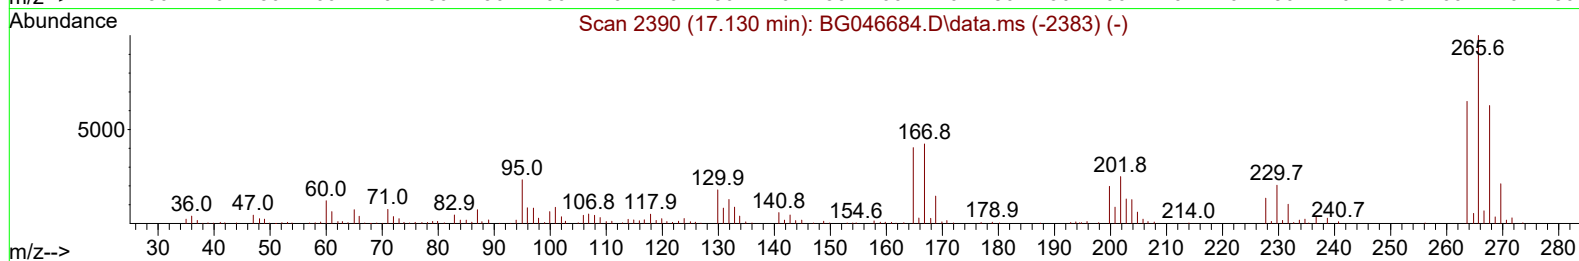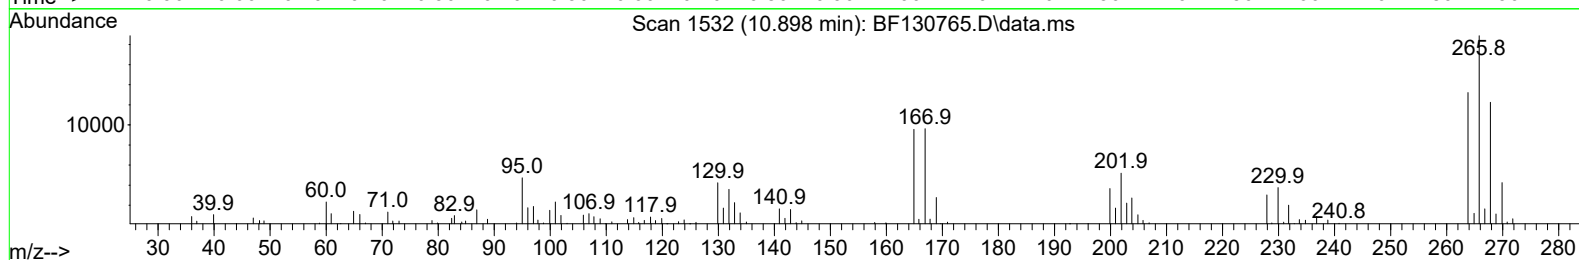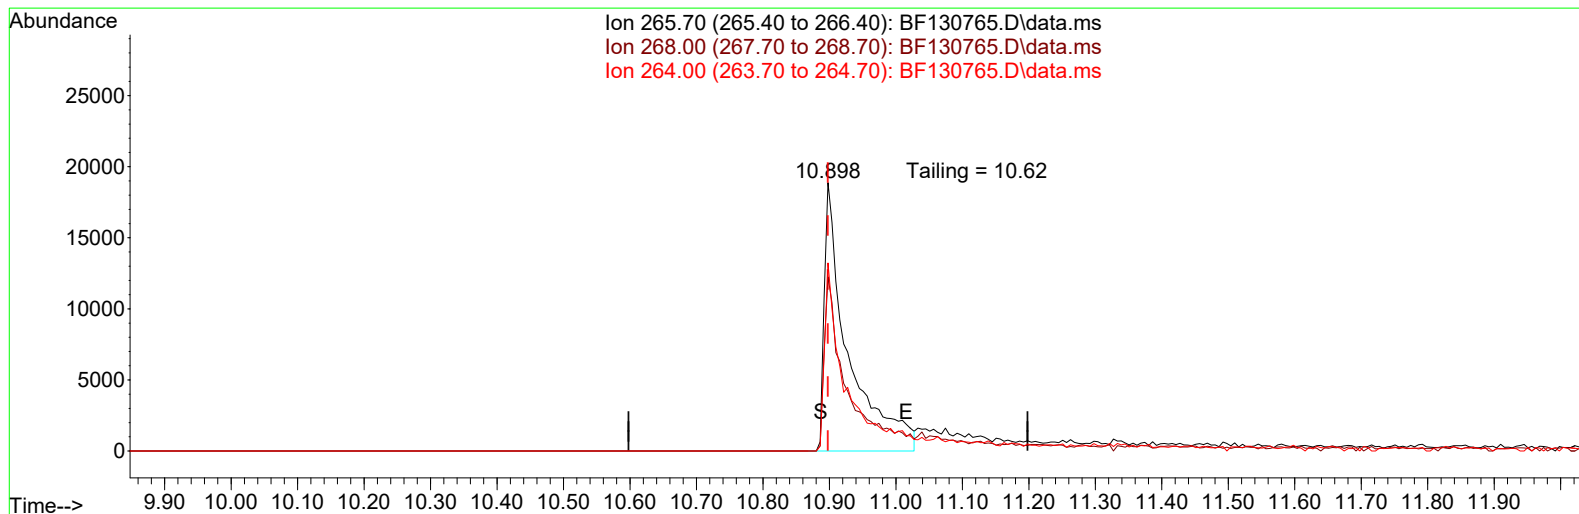

TIC: BF130765.D\data.ms

(70) Pentachlorophenol (C)

10.898min (-0.000) 2044.80 ng

response 46896

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.86
264.00	67.00	70.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2022	BNA_F	<u>BF130765.D</u>
Compound Name	Response	Retention Time
DDT	351414	13.227
DDD	5930	12.933
DDE	3878	11.339
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9808	361222	2.72

Instrument :
BNA_F
ClientSampleId :
DFTPP