
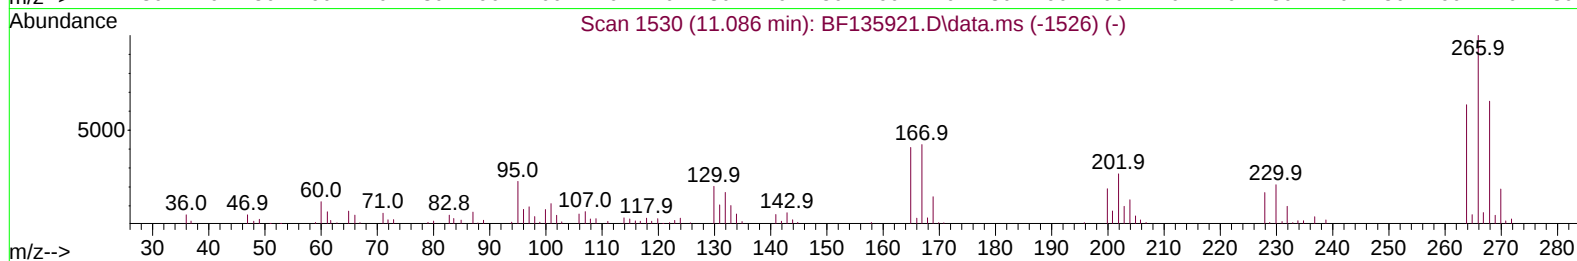
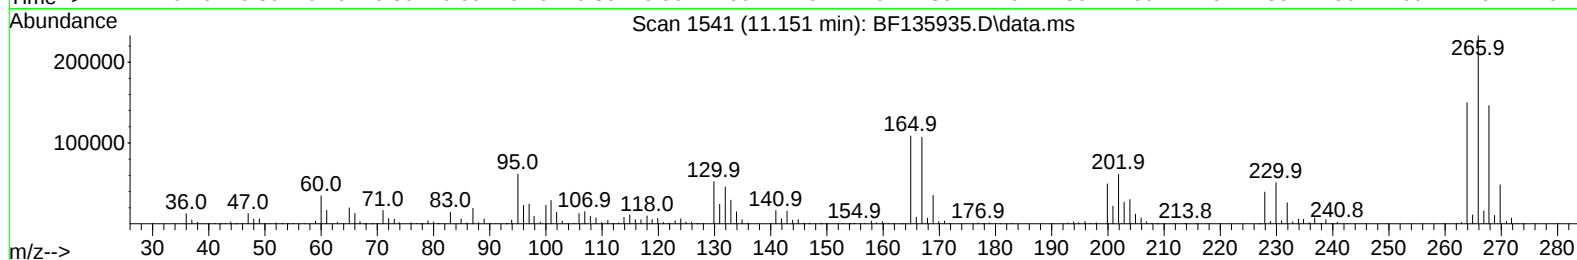


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102523\
Data File : BF135935.D
Acq On : 25 Oct 2023 11:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 12:32:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 12:04:11 2023
Response via : Initial Calibration

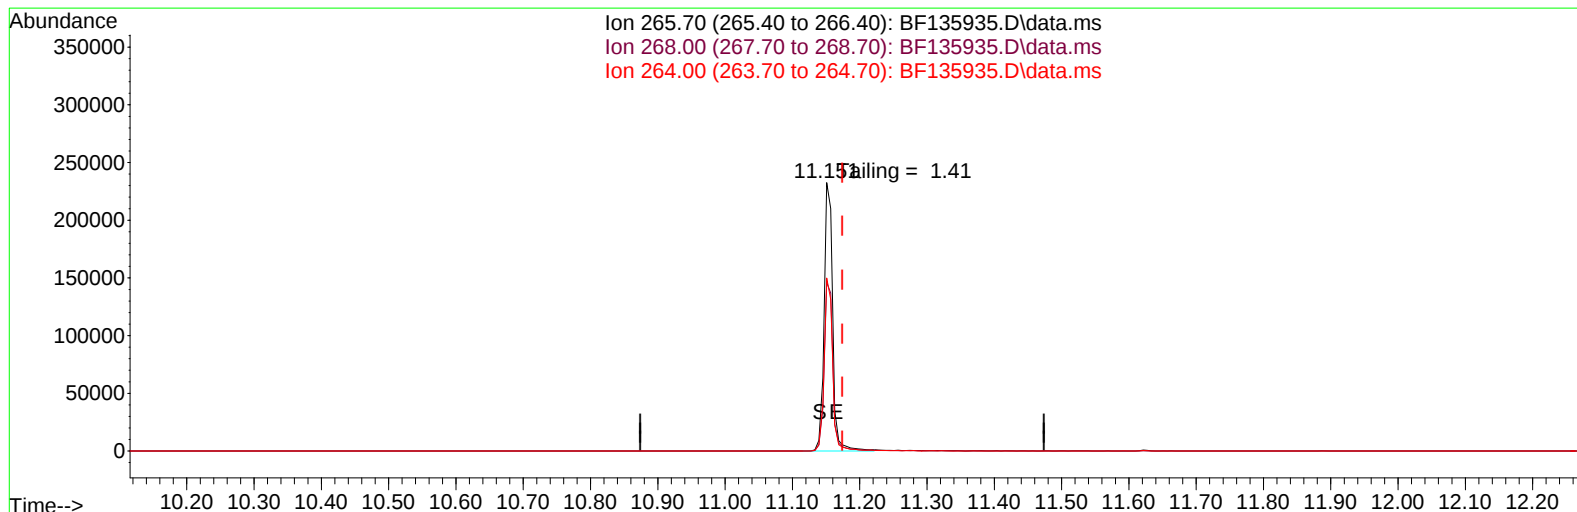

TIC: BF135935.D\data.ms




(70) Pentachlorophenol (C)

11.151min (-0.023) 293202.77 ng

response 207099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.82
264.00	63.40	64.47
0.00	0.00	0.00

Quant Time: Oct 25 12:32:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 12:04:11 2023
Response via : Initial Calibration

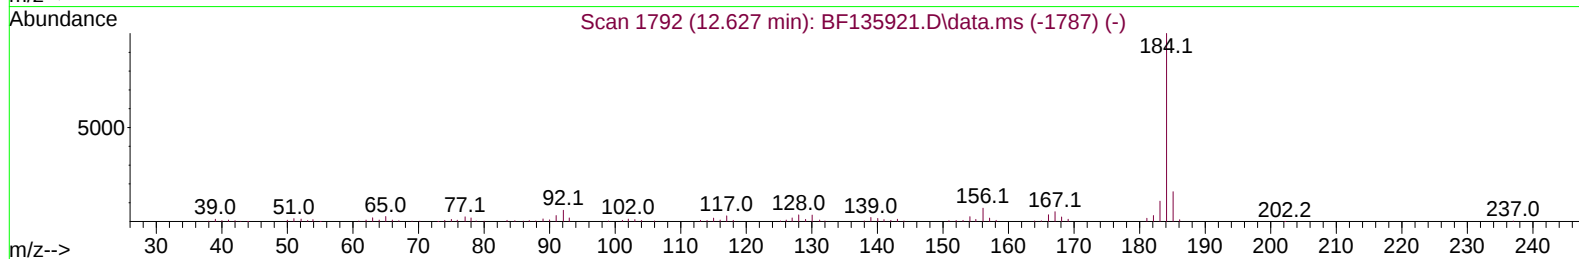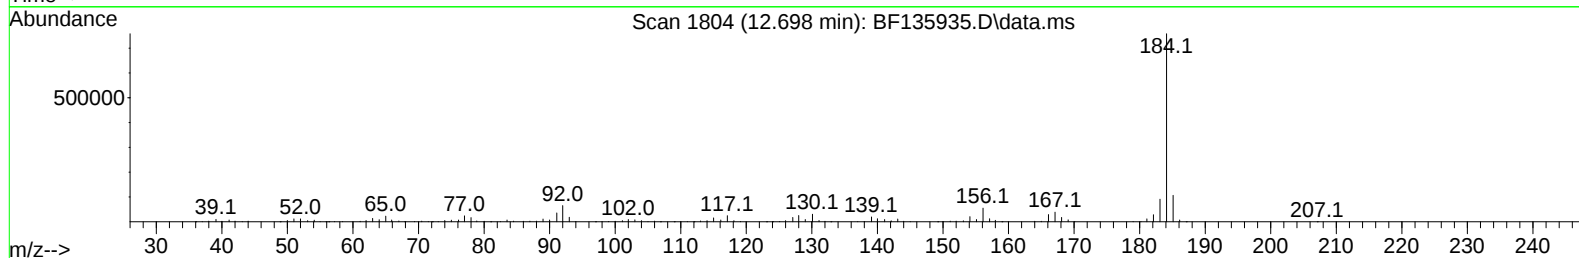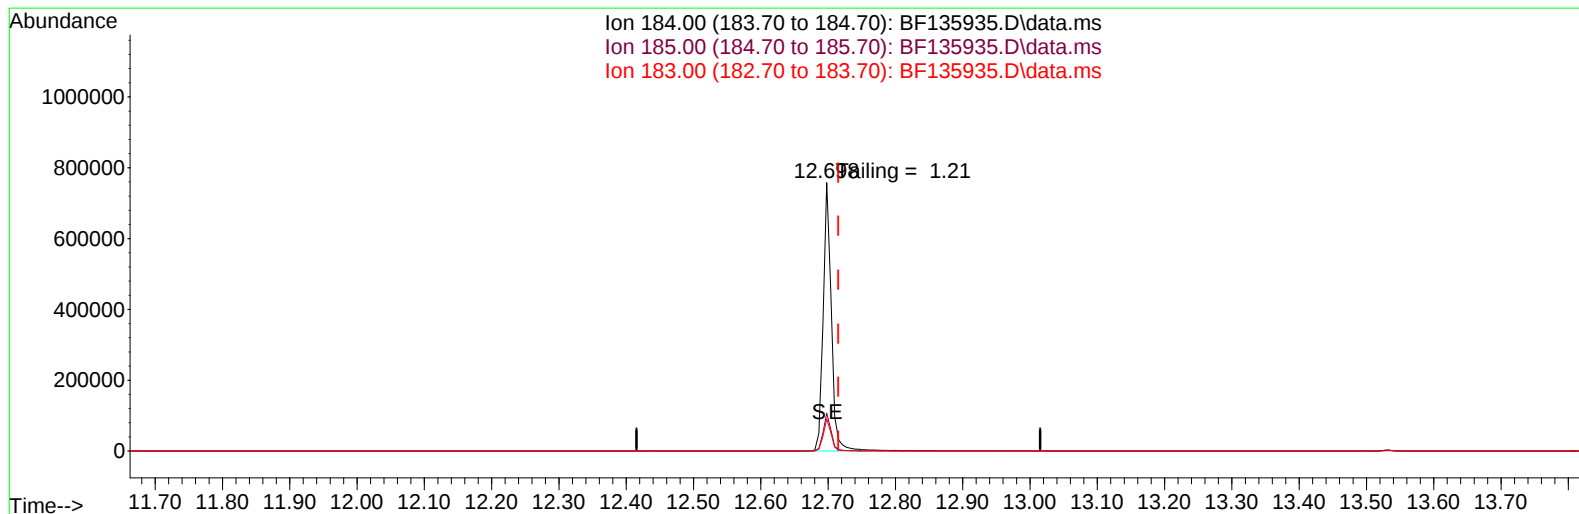

TIC: BF135935.D\data.ms

(77) Benzidine

12.698min (-0.017) 174752.47 ng

response 643784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.06
183.00	10.90	11.99
0.00	0.00	0.00