


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102523\
Data File : BF135935.D
Acq On : 25 Oct 2023 11:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 26 03:58:01 2023

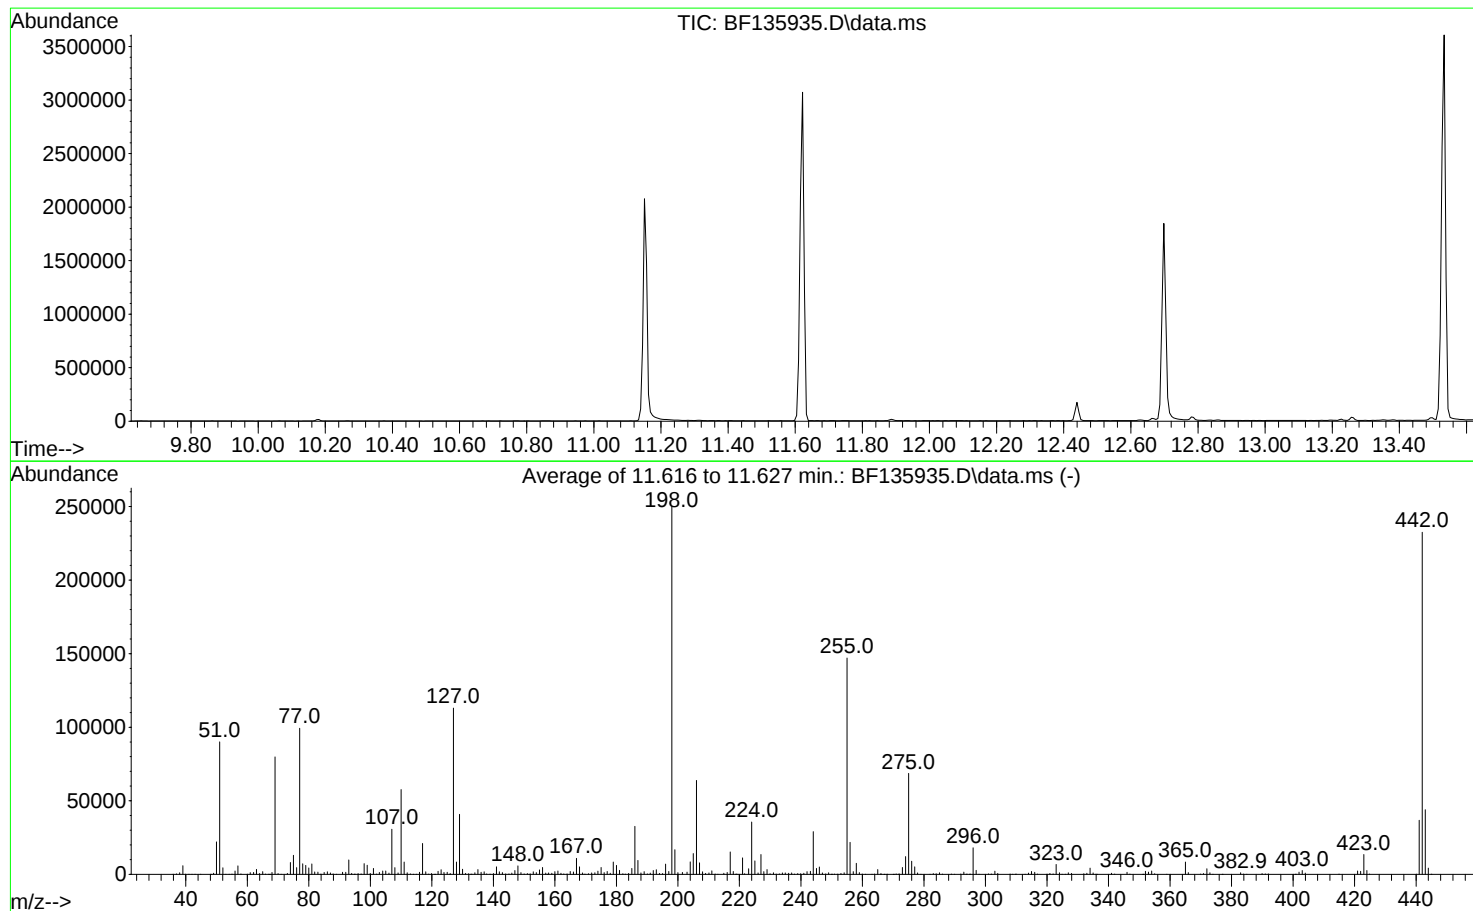


AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	90037	PASS
68	69	0.00	2	1.7	1330	PASS
69	198	0.00	100	31.9	79835	PASS
70	69	0.00	2	0.7	522	PASS
127	198	10	80	45.2	113000	PASS
197	198	0.00	2	0.8	1931	PASS
198	198	100	100	100.0	250048	PASS
199	198	5	9	6.7	16733	PASS
275	198	10	60	27.4	68605	PASS
365	198	1	100	3.4	8388	PASS
441	198	0.01	100	14.7	36744	PASS
442	442	50	100	100.0	232576	PASS
443	442	15	24	18.9	43917	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102523\
Data File : BF135935.D
Acq On : 25 Oct 2023 11:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 12:32:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 12:04:11 2023
Response via : Initial Calibration

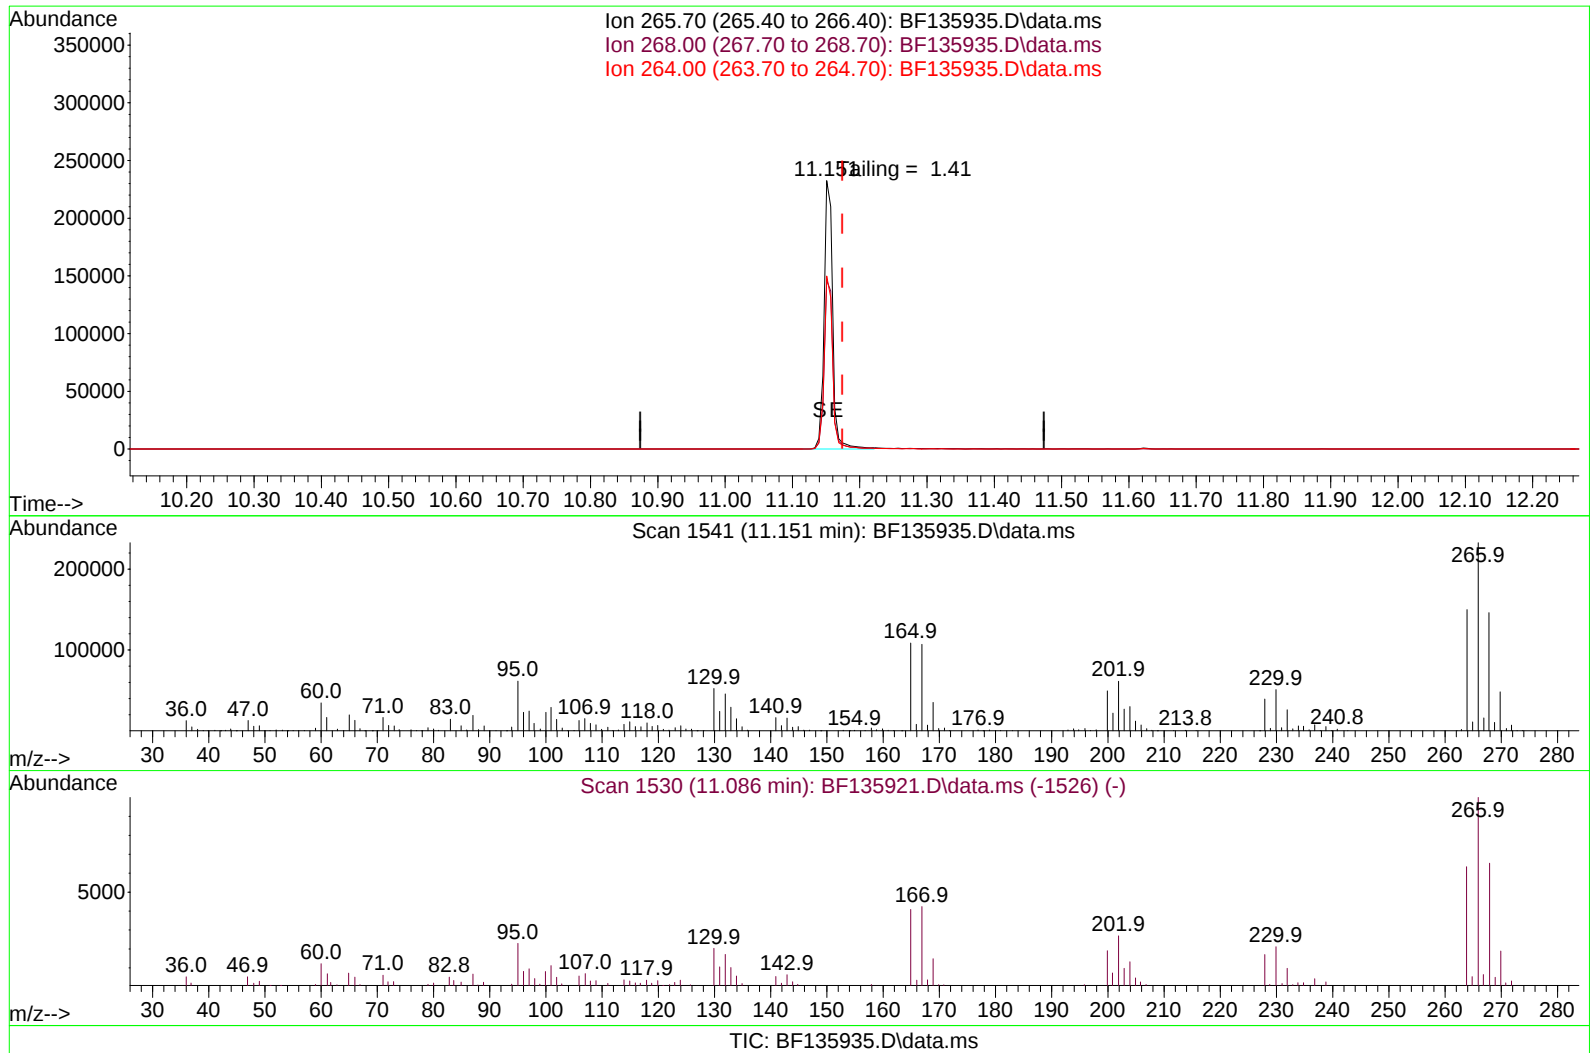

(70) Pentachlorophenol (C)

11.151min (-0.023) 293202.77 ng




response 207099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.82
264.00	63.40	64.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102523\
Data File : BF135935.D
Acq On : 25 Oct 2023 11:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 12:32:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 12:04:11 2023
Response via : Initial Calibration

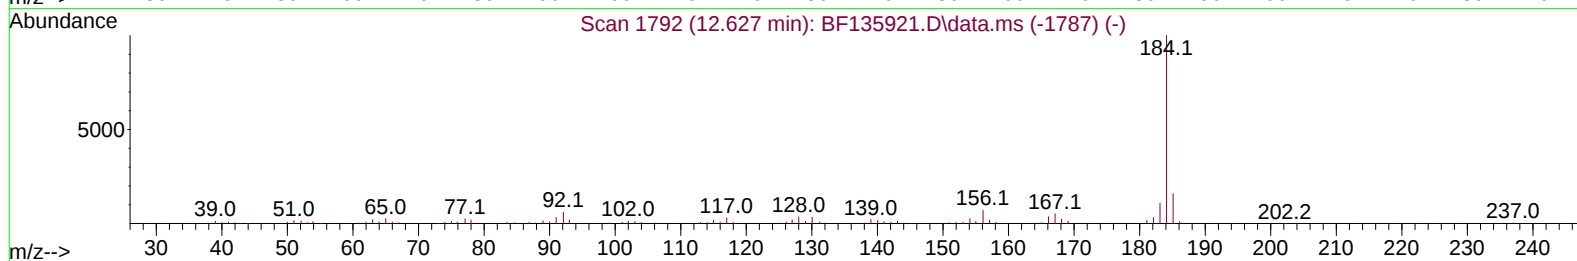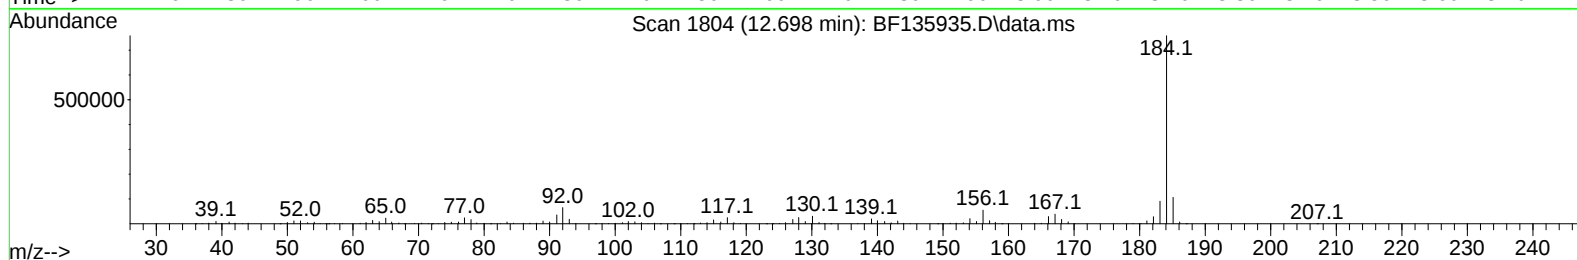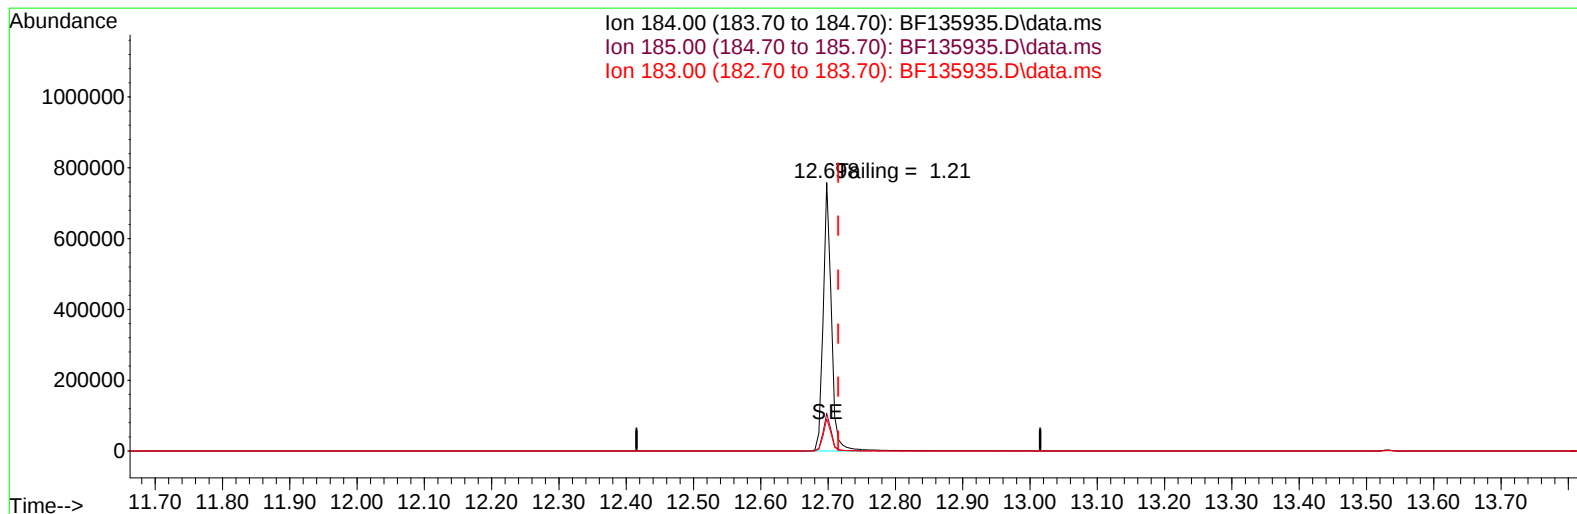

TIC: BF135935.D\data.ms

(77) Benzidine

12.698min (-0.017) 174752.47 ng

response 643784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.06
183.00	10.90	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/25/2023	BNA_F	<u>BF135935.D</u>
Compound Name	Response	Retention Time
DDT	524527	13.533
DDD	5142	13.257
DDE	0	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5142	529669	0.97

Instrument :
BNA_F
ClientSampleId :
DFTPP