

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102618\
 Data File : BF110225.D
 Acq On : 26 Oct 2018 22:19
 Operator : JU/SJ
 Sample : J5205-05 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 26 23:42:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 23 15:06:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	135394	20.00	ng	-0.01
21) Naphthalene-d8	8.25	136	520506	20.00	ng	-0.02
39) Acenaphthene-d10	10.01	164	201748	20.00	ng	-0.02
64) Phenanthrene-d10	11.50	188	313435	20.00	ng	-0.01
76) Chrysene-d12	14.15	240	227629	20.00	ng	-0.01
87) Perylene-d12	15.68	264	157327	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.58	112	257445	30.96	ng	-0.02
7) Phenol-d6	6.58	99	337735	31.76	ng	-0.02
23) Nitrobenzene-d5	7.53	82	185656	21.16	ng	-0.02
42) 2,4,6-Tribromophenol	10.80	330	50910	25.47	ng	-0.01
45) 2-Fluorobiphenyl	9.32	172	359793	28.00	ng	-0.02
79) Terphenyl-d14	13.09	244	271835	24.84	ng	-0.01
Target Compounds						
9) Benzaldehyde	6.58	77	610	Below Cal		Qvalue # 1
19) n-Nitroso-di-n-propylamine	7.53	70	24470	3.587 ng	#	81
25) Isophorone	7.53	82	185654	12.411 ng	#	67
51) 2,6-Dinitrotoluene	10.01	165	25456	7.935 ng	#	23
54) 2,4-Dinitrophenol	10.04	184	128	5.269 ng	#	1
57) 2,4-Dinitrotoluene	10.01	165	25456	6.247 ng	#	19
71) Phenanthrene	11.53	178	36740	2.240 ng		97
75) Fluoranthene	12.72	202	68317	4.104 ng		98
78) Pyrene	12.96	202	56932	3.489 ng		97
81) Benzo(a)anthracene	14.14	228	27985	2.073 ng		96
88) Benzo(b)fluoranthene	15.22	252	34900	3.841 ng	#	87
89) Benzo(k)fluoranthene	15.22	252	34900	3.908 ng	#	87
90) Benzo(a)pyrene	15.61	252	17608	2.106 ng	#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102618\
Data File : BF110225.D
Acq On : 26 Oct 2018 22:19
Operator : JU/SJ
Sample : J5205-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 26 23:42:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 23 15:06:18 2018
Response via : Initial Calibration




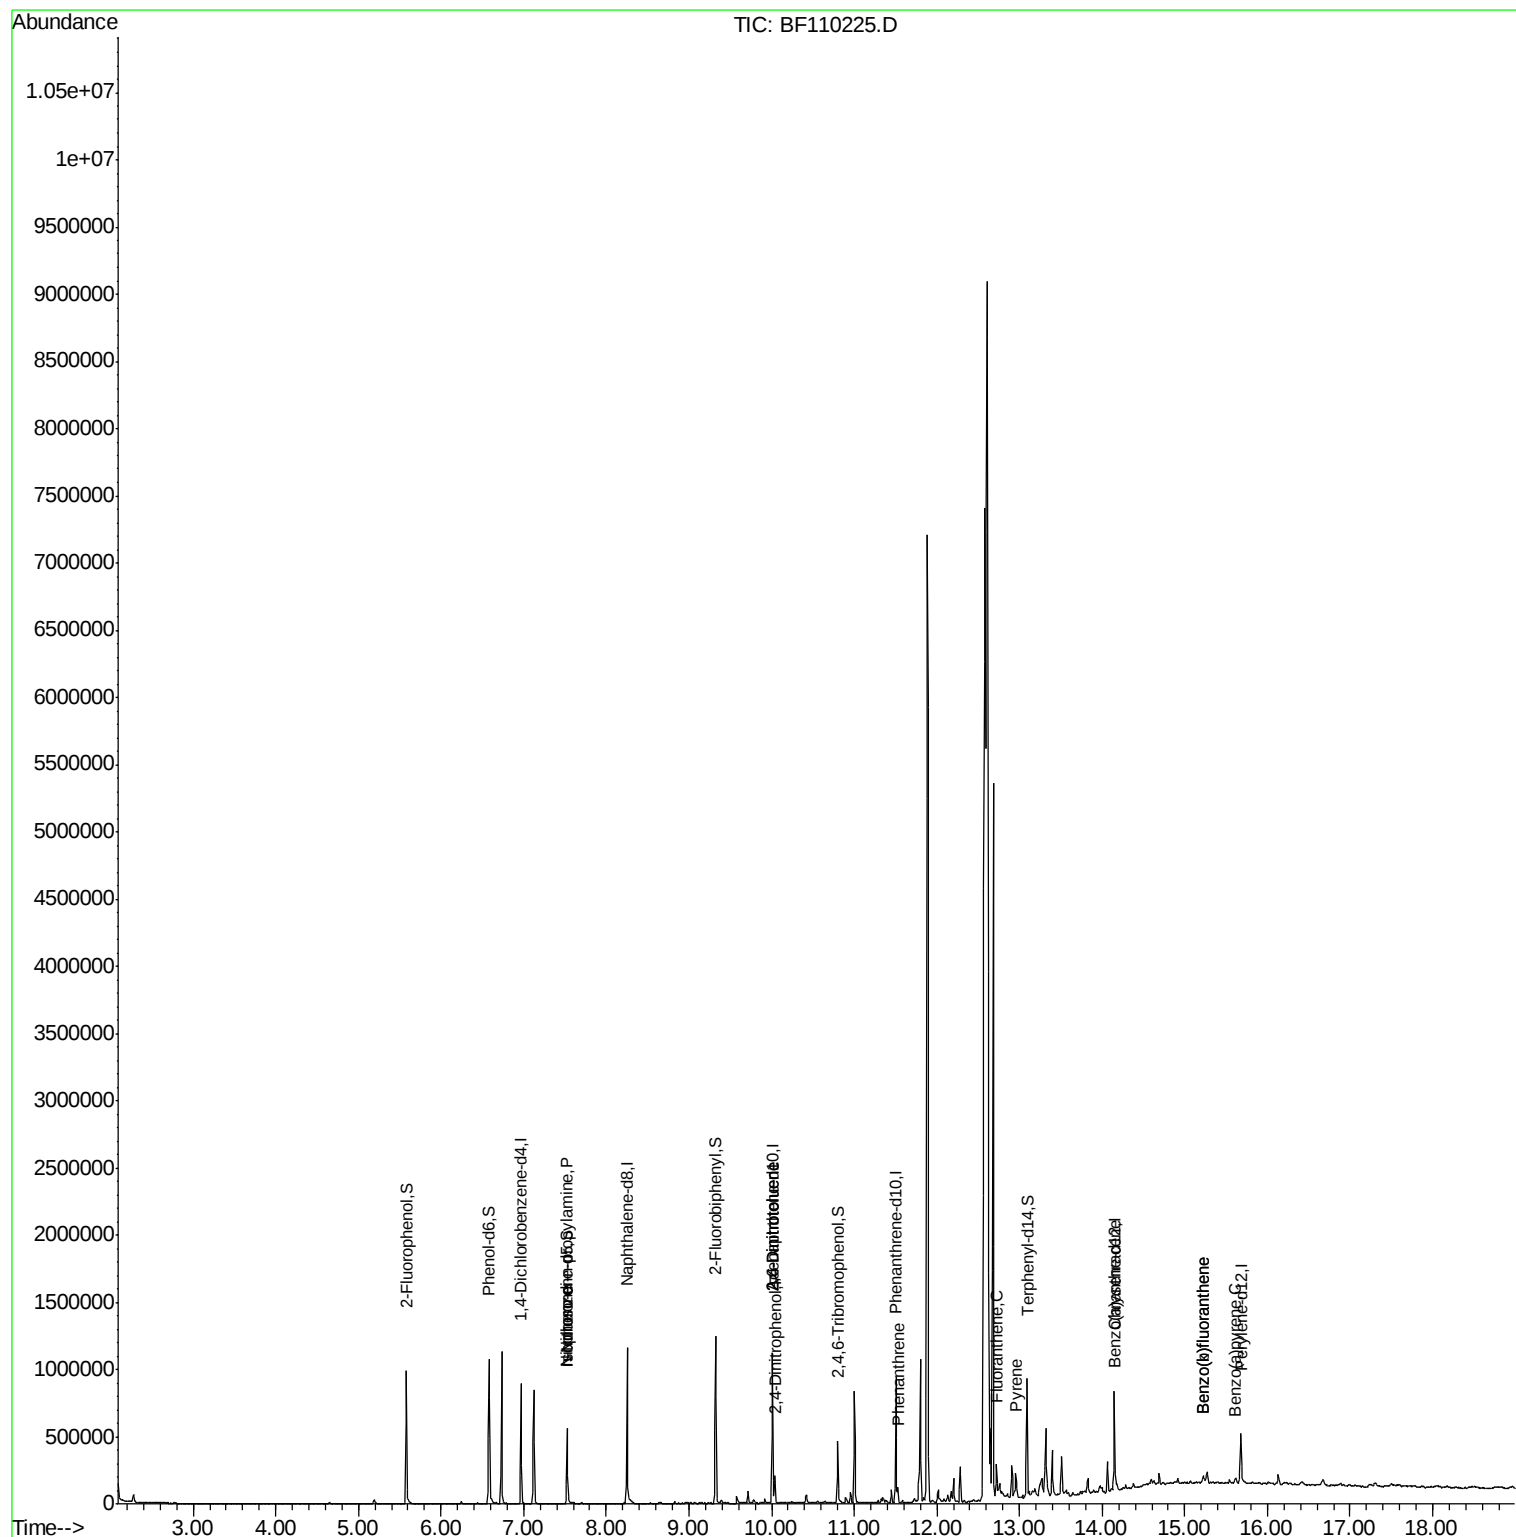




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.97 min Scan# 830
 Delta R.T. -0.01 min
 Lab File: BF110225.D
 Acq: 26 Oct 2018 22:19




Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 135394
 Ion Ratio Lower Upper
 152 100
 150 154.9 122.7 184.1
 115 59.4 49.1 73.7

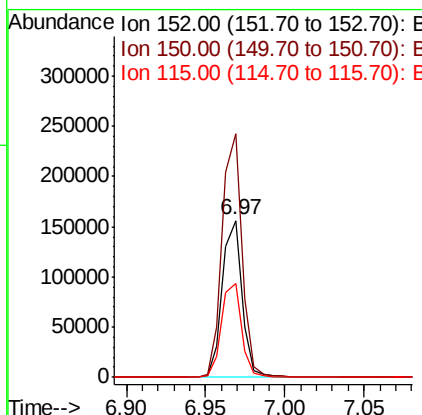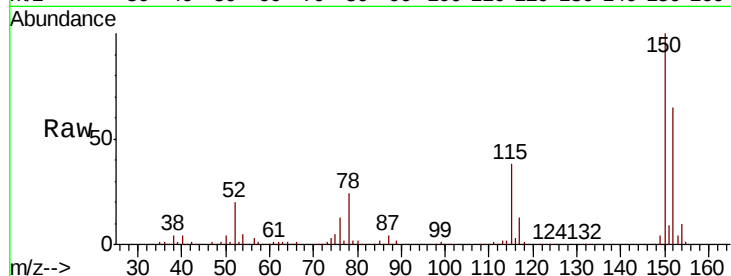

#5
 2-Fluorophenol
 Concen: 30.964 ng
 RT: 5.58 min Scan# 594
 Delta R.T. -0.02 min
 Lab File: BF110225.D
 Acq: 26 Oct 2018 22:19

Tgt Ion:112 Resp: 257445
 Ion Ratio Lower Upper
 112 100
 64 58.0 44.1 66.1
 63 31.3 23.7 35.5

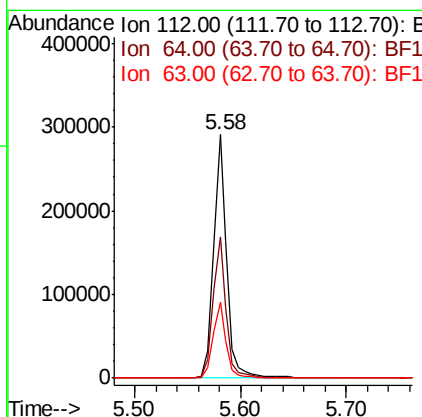



#7

Phenol-d6

Concen: 31.758 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.02 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 337735

Ion Ratio Lower Upper




99 100

42 19.2 15.8 23.6

71 35.1 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

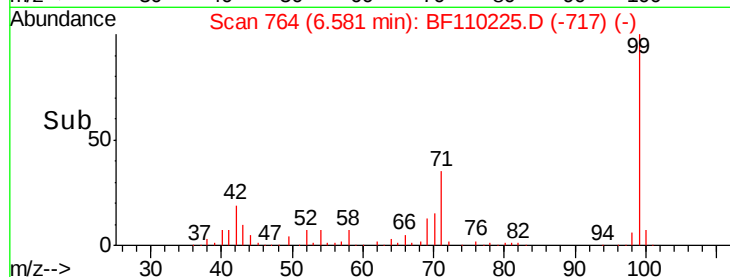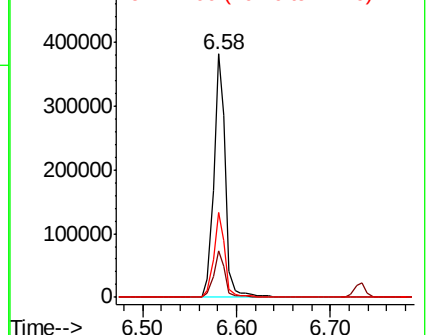

#19

n-Nitroso-di-n-propylamine

Concen: 3.587 ng

RT: 7.53 min Scan# 925

Delta R.T. 0.14 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19

Tgt Ion: 70 Resp: 24470


Ion Ratio Lower Upper

70 100



42 50.7 47.4 71.2

101 0.0 7.3 10.9#

130 2.1 16.2 24.2#



Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1

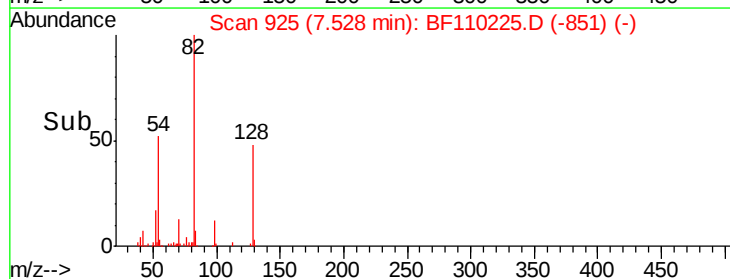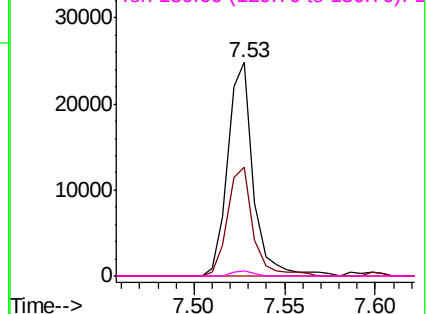



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1048

Delta R.T. -0.02 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 520506


Ion Ratio Lower Upper

136 100

137 11.3 8.8 13.2

54 7.9 5.4 8.2

68 5.4 4.2 6.2



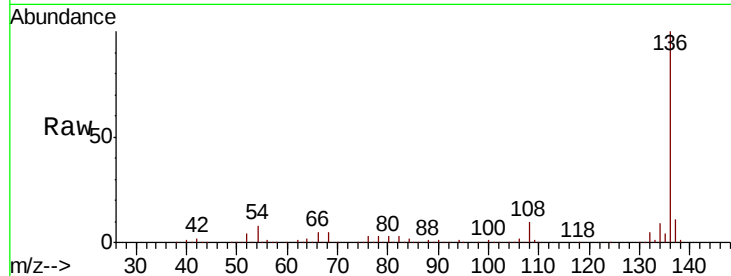


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

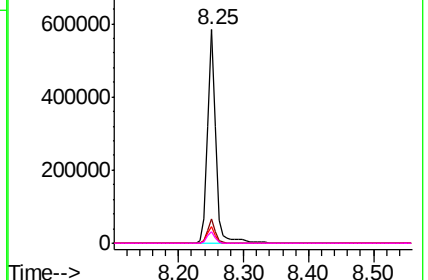

#23

Nitrobenzene-d5

Concen: 21.156 ng

RT: 7.53 min Scan# 925

Delta R.T. -0.02 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19


Tgt Ion: 82 Resp: 185656

Ion Ratio Lower Upper

82 100

128 48.2 34.2 51.2



54 52.3 38.6 58.0




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

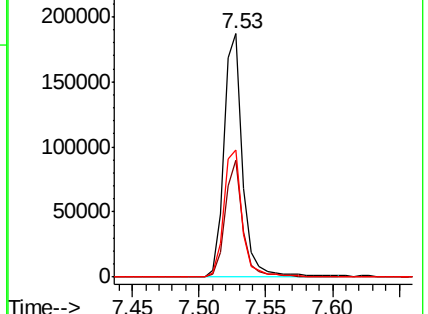

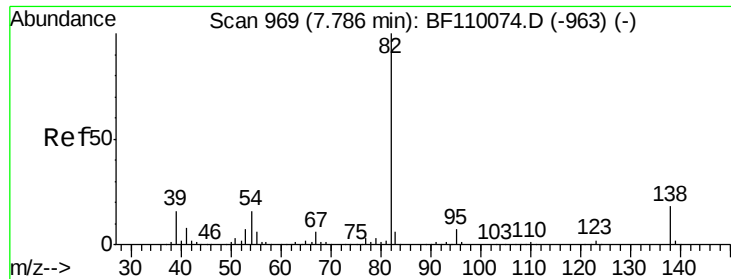

#25

Isophorone

Concen: 12.411 ng

RT: 7.53 min Scan# 925

Delta R.T. -0.28 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 185654

Ion Ratio Lower Upper

82 100

95 0.0 5.7 8.5#




138 0.0 13.2 19.8#

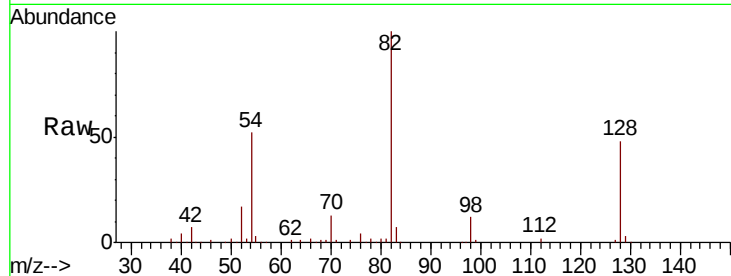

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

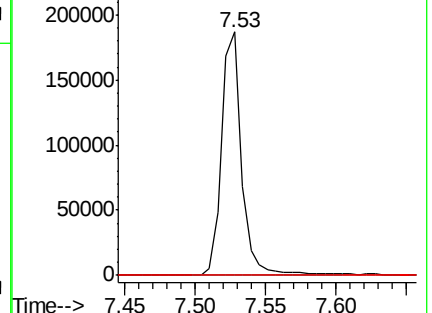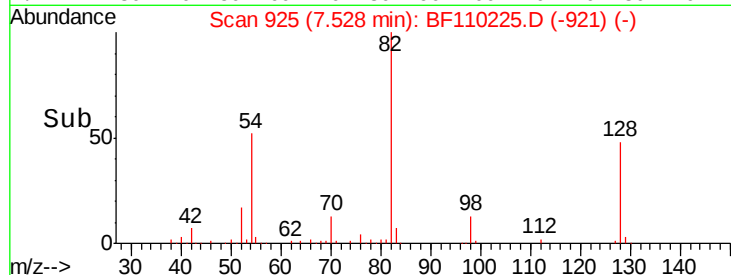

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1347

Delta R.T. -0.02 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19


Tgt Ion:164 Resp: 201748

Ion Ratio Lower Upper

164 100

162 102.4 83.0 124.6



160 45.9 37.0 55.6




Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

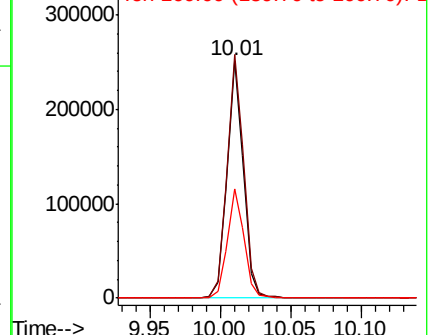


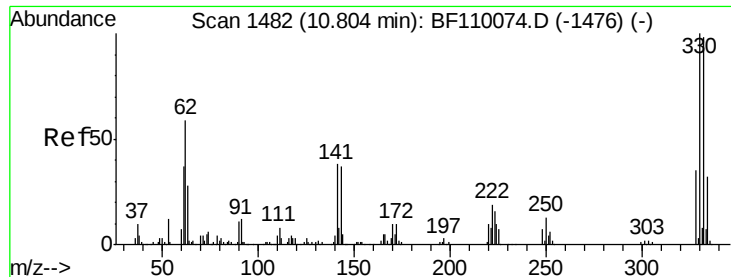

#42
 2,4,6-Tribromophenol
 Concen: 25.475 ng
 RT: 10.80 min Scan# 1482
 Delta R.T. -0.01 min
 Lab File: BF110225.D
 Acq: 26 Oct 2018 22:19

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	101.5	77.1	115.7
141	37.7	27.0	40.4



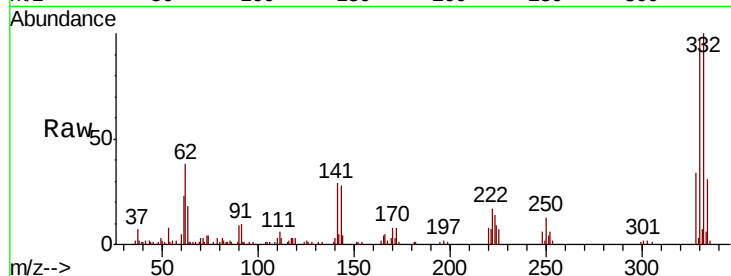


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

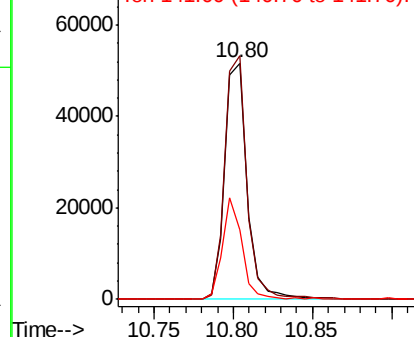

#45
 2-Fluorobiphenyl
 Concen: 28.004 ng
 RT: 9.32 min Scan# 1230
 Delta R.T. -0.02 min
 Lab File: BF110225.D
 Acq: 26 Oct 2018 22:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.3	28.6	43.0
170	22.9	19.7	29.5





Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

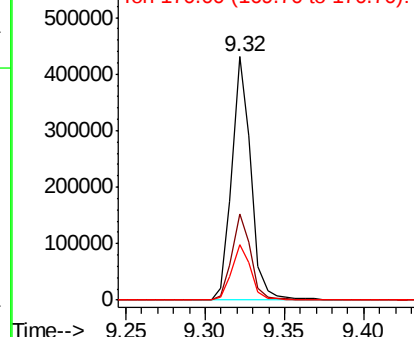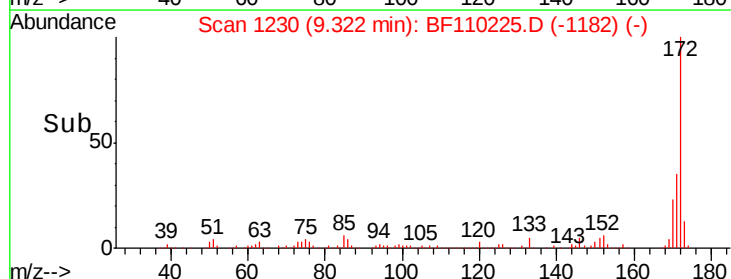







#51
 2,6-Dinitrotoluene
 Concen: 7.935 ng
 RT: 10.01 min Scan# 1347
 Delta R.T. 0.21 min
 Lab File: BF110225.D
 Acq: 26 Oct 2018 22:19

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.6	48.9	73.3#
89	1.2	46.6	69.8#

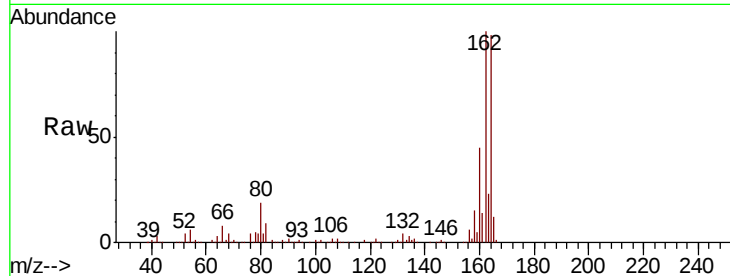


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

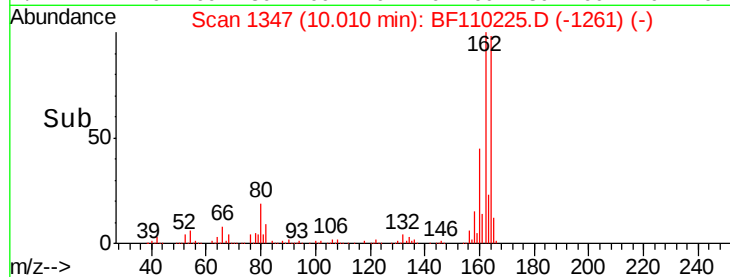
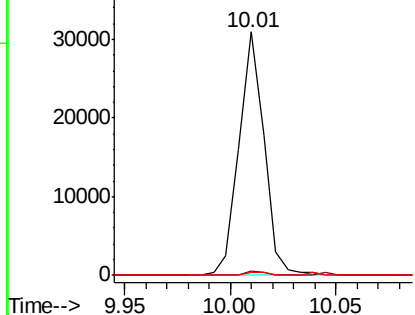


#54
 2,4-Dinitrophenol
 Concen: 5.269 ng
 RT: 10.04 min Scan# 1352
 Delta R.T. -0.04 min
 Lab File: BF110225.D
 Acq: 26 Oct 2018 22:19

Tgt Ion	Ratio	Lower	Upper
184	100		
63	0.0	55.8	83.6#
154	726.8	63.2	94.8#



Abundance Ion 184.00 (183.70 to 184.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 154.00 (153.70 to 154.70): E


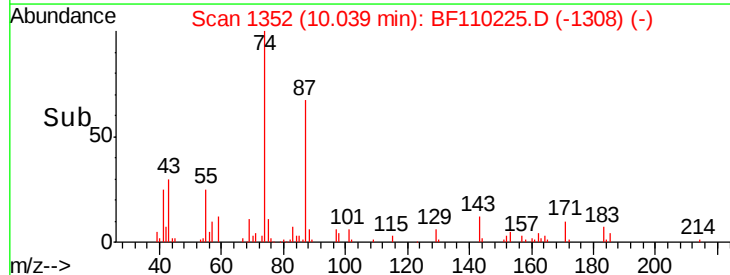
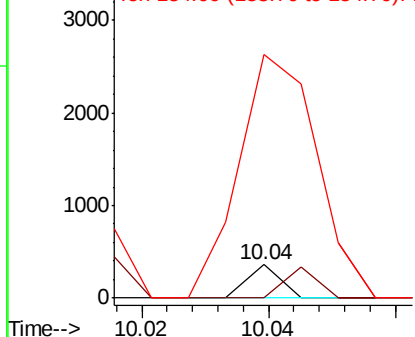




#57
2,4-Dinitrotoluene
Concen: 6.247 ng
RT: 10.01 min Scan# 1347
Delta R.T. -0.20 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.6	44.8	67.2#
89	1.2	62.2	93.4#
182	0.0	2.1	3.1#

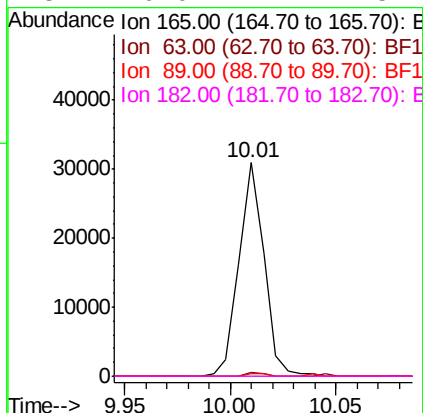

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1601
Delta R.T. -0.01 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.4	7.2	10.8
80	9.6	7.9	11.9

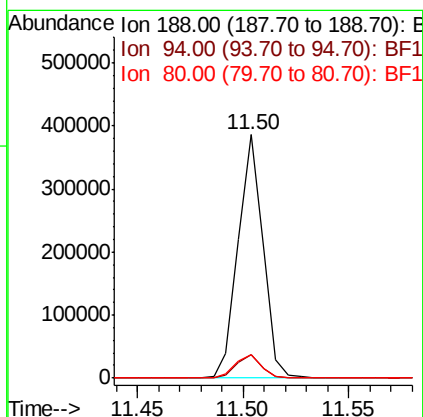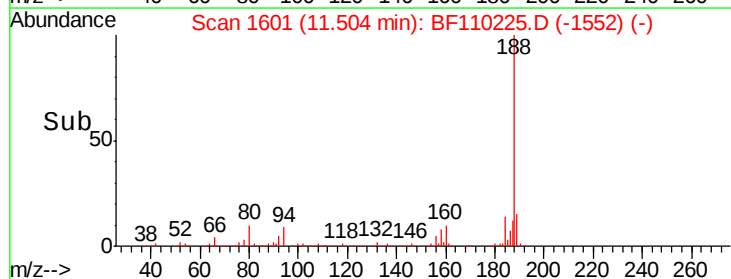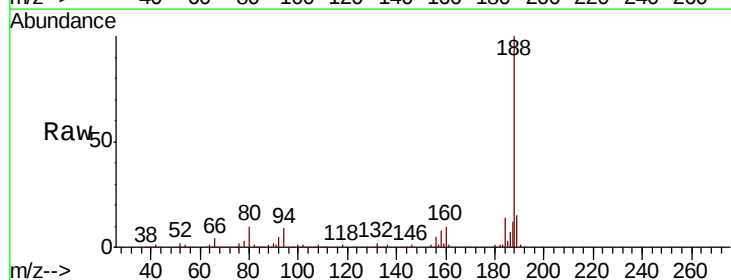

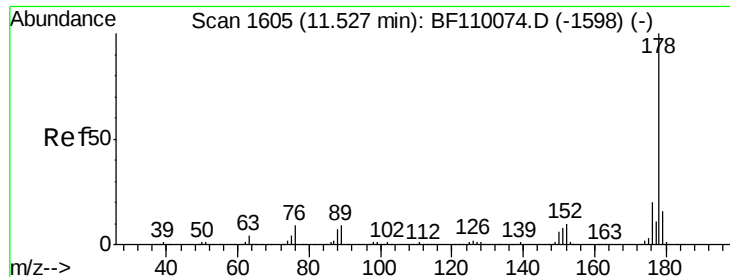

#71

Phenanthrene

Concen: 2.240 ng

RT: 11.53 min Scan# 1605

Delta R.T. -0.02 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19


Instrument :

BNA_F

ClientSampleId :

Tot Ion:178 Resp: 36740

Ion	Ratio	Lower	Upper
178	100		
176	18.0	15.5	23.3
179	14.5	12.5	18.7



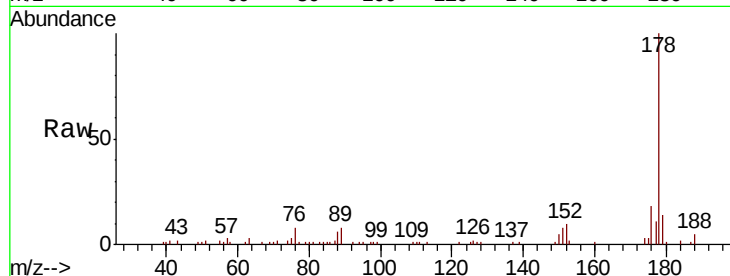


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

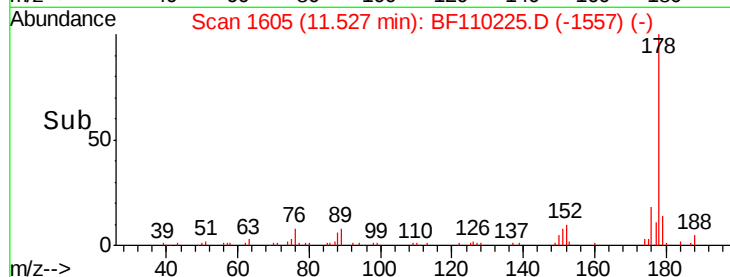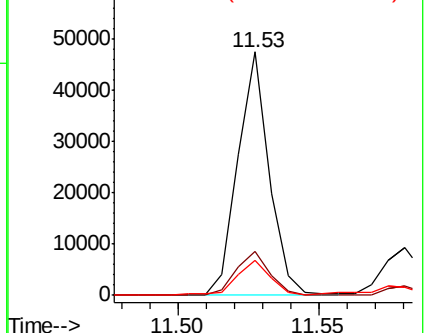

#75

Fluoranthene

Concen: 4.104 ng

RT: 12.72 min Scan# 1808


Delta R.T. -0.01 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19

Tgt Ion:202 Resp: 68317

Ion	Ratio	Lower	Upper
202	100		
101	12.4	0.0	31.4
203	18.2	0.0	37.7






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



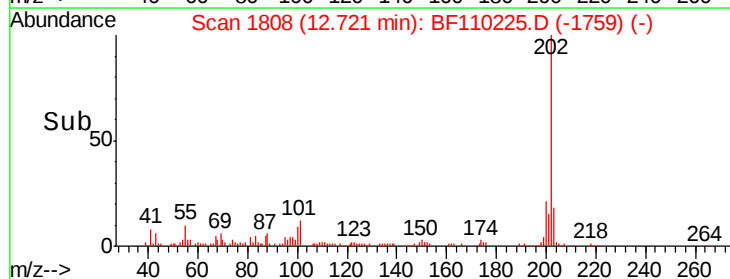
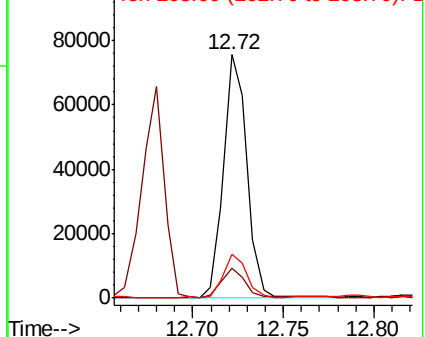


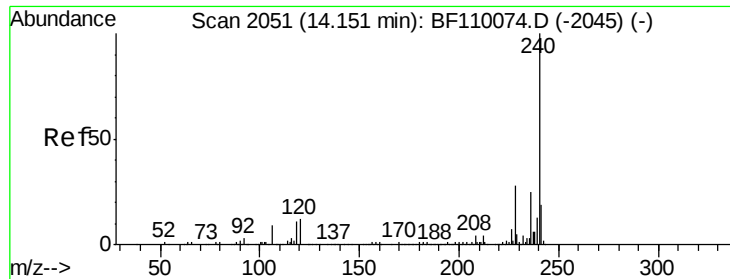

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.15 min Scan# 2051
Delta R.T. -0.01 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
240	100		
120	12.1	8.3	12.5
236	25.4	21.2	31.8

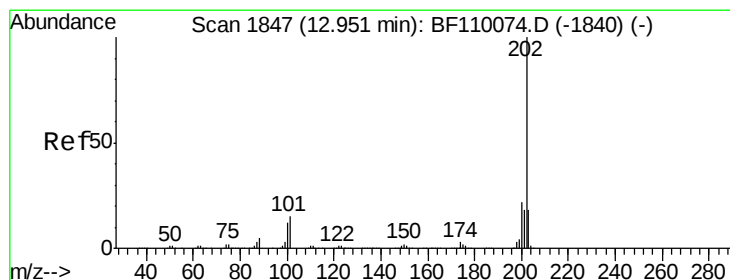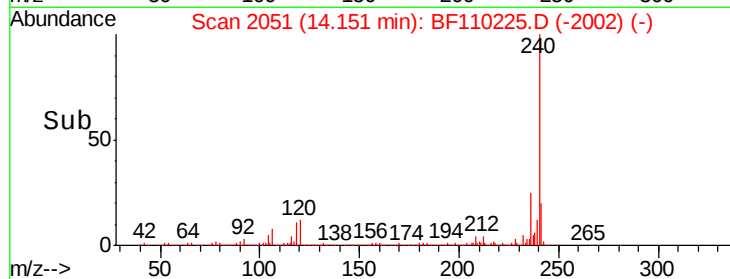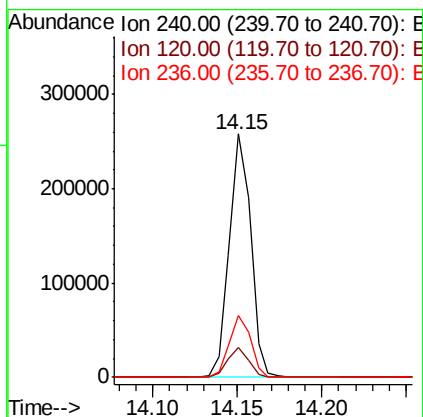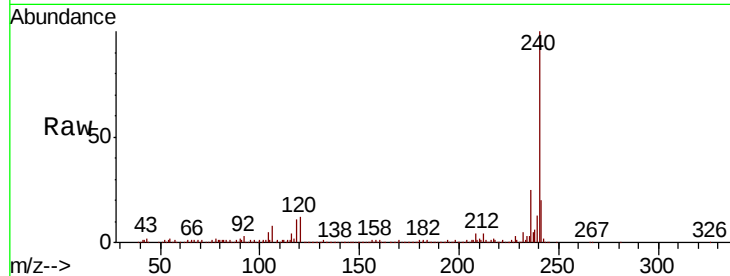

#78
Pyrene
Concen: 3.489 ng
RT: 12.96 min Scan# 1848
Delta R.T. -0.01 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19

Tgt Ion	Ratio	Lower	Upper
202	100		
200	19.8	17.8	26.6
203	17.9	14.2	21.4

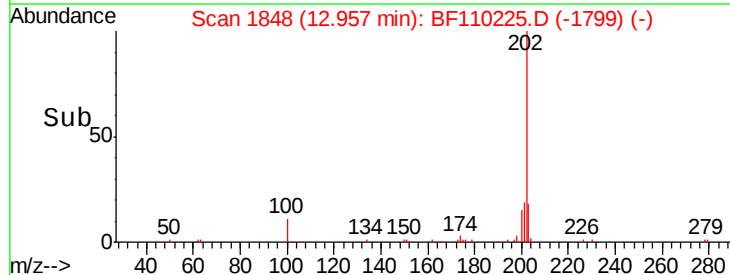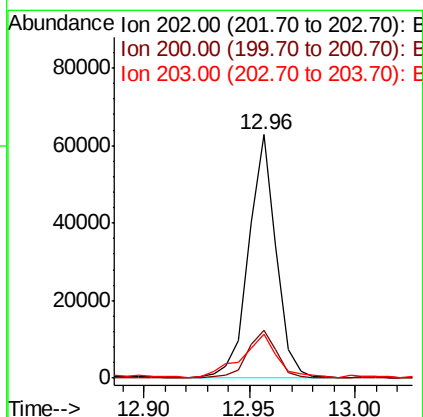

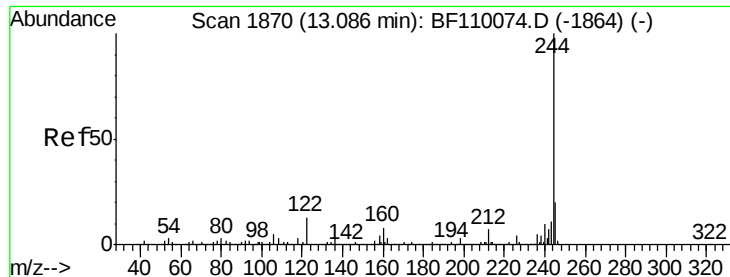

#79

Terphenyl-d14

Concen: 24.836 ng

RT: 13.09 min Scan# 1871

Delta R.T. -0.01 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19

Instrument :

BNA_F

ClientSampled :


Tot Ion:244 Resp: 271835

Ion Ratio Lower Upper




244 100

212 6.2 5.8 8.8

122 10.4 8.7 13.1



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

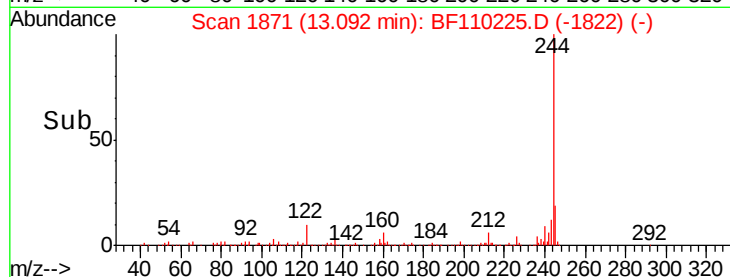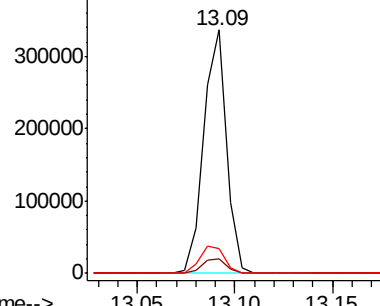

#81

Benzo(a)anthracene

Concen: 2.073 ng

RT: 14.14 min Scan# 2049

Delta R.T. -0.01 min

Lab File: BF110225.D

Acq: 26 Oct 2018 22:19


Tgt Ion:228 Resp: 27985

Ion Ratio Lower Upper



228 100


226 29.3 22.1 33.1

229 21.3 15.6 23.4



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

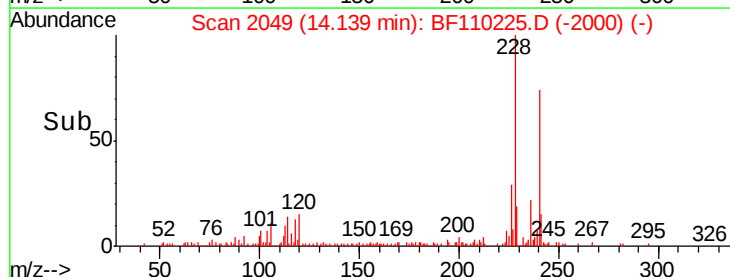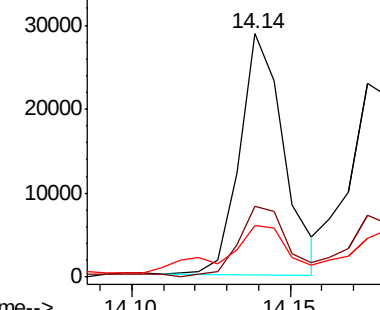




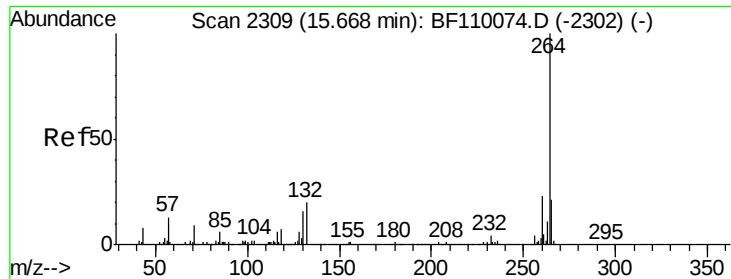


#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.68 min Scan# 2311
Delta R.T. -0.01 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19

Instrument :
BNA_F
ClientSampleId :

Tot Ion:264 Resp: 157327




Ion	Ratio	Lower	Upper
264	100		
260	22.6	18.7	28.1
265	21.0	16.7	25.1

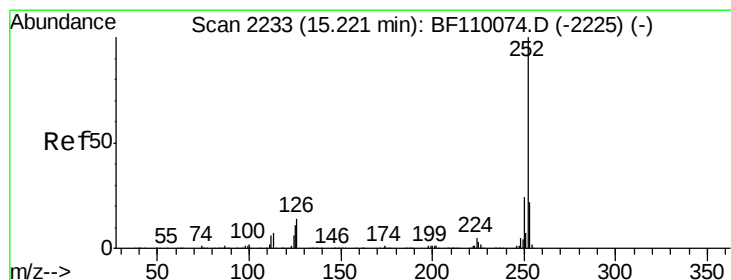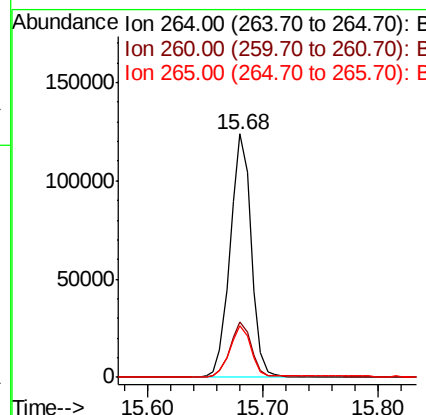


#88
Benzo(b)fluoranthene
Concen: 3.841 ng
RT: 15.22 min Scan# 2233
Delta R.T. -0.01 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19

Tgt Ion:252 Resp: 34900

Ion	Ratio	Lower	Upper
252	100		
253	25.4	17.2	25.8
125	18.3	8.2	12.4#


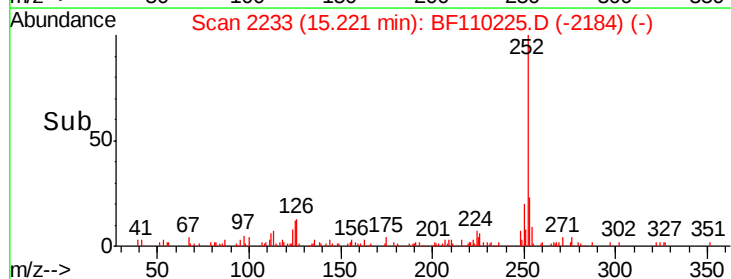
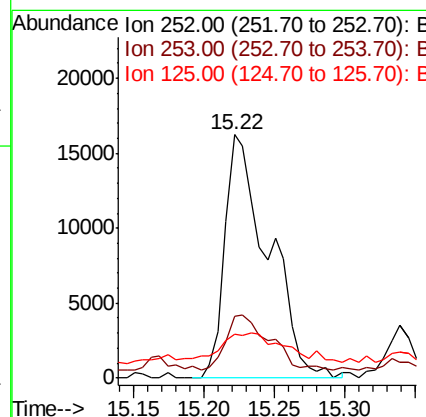
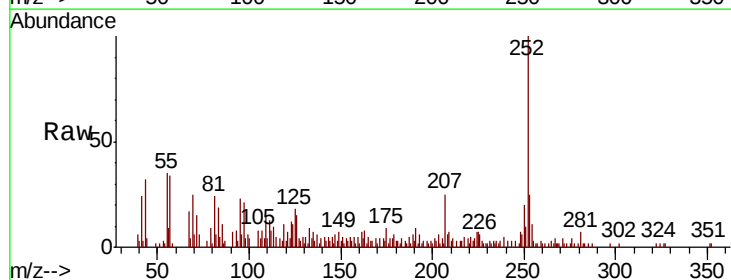


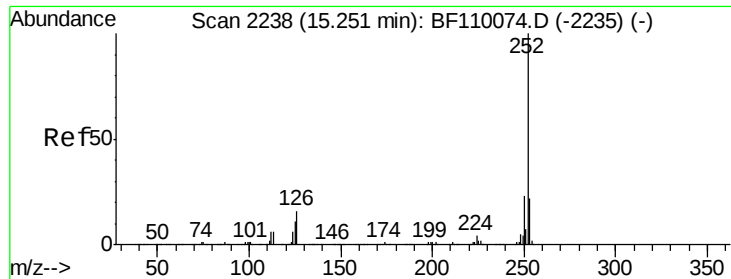

#89
Benzo(k)fluoranthene
Concen: 3.908 ng
RT: 15.22 min Scan# 2233
Delta R.T. -0.05 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	25.4	17.2	25.8
125	18.3	7.4	11.0

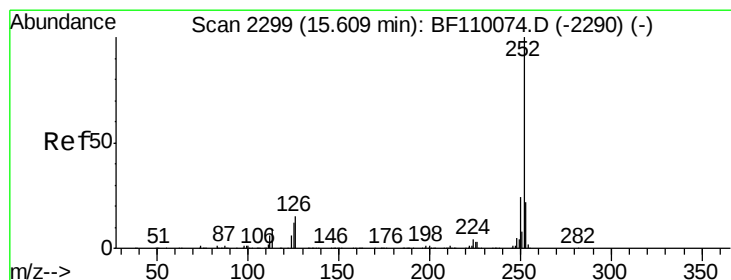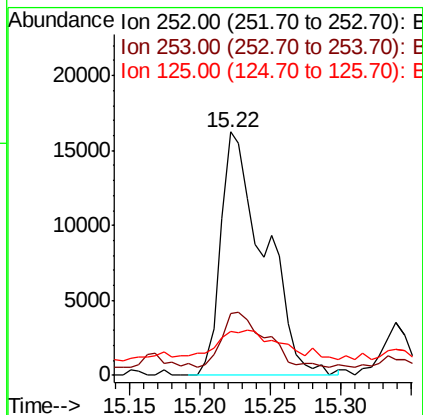

#90
Benzo(a)pyrene
Concen: 2.106 ng
RT: 15.61 min Scan# 2299
Delta R.T. -0.02 min
Lab File: BF110225.D
Acq: 26 Oct 2018 22:19

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.0	18.2	27.4
125	23.0	9.0	13.6

