

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102618\
 Data File : BF110224.D
 Acq On : 26 Oct 2018 21:52
 Operator : JU/SJ
 Sample : J5204-15 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-01-102518-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.275	27	32	38	rVB	47700	61590	6.20%	0.580%
2	5.187	525	527	532	rBV	23640	26648	2.68%	0.251%
3	5.581	590	594	606	rBV	797553	740355	74.58%	6.970%
4	6.581	760	764	776	rBV	904965	836694	84.28%	7.877%
5	6.734	786	790	793	rBV	946173	797363	80.32%	7.507%
6	6.969	826	830	836	rBV	878221	758382	76.39%	7.140%
7	7.122	852	856	867	rBV	731148	594715	59.91%	5.599%
8	7.528	921	925	936	rBV	460627	441576	44.48%	4.157%
9	8.251	1044	1048	1063	rBV	1119846	992750	100.00%	9.347%
10	9.322	1227	1230	1241	rBV	1029506	860606	86.69%	8.102%
11	9.716	1294	1297	1305	rBV	50420	47486	4.78%	0.447%
12	10.010	1343	1347	1361	rBV2	1023444	942049	94.89%	8.869%
13	10.416	1414	1416	1420	rBV	19523	15190	1.53%	0.143%
14	10.798	1478	1481	1490	rBV	373115	365278	36.79%	3.439%
15	11.504	1597	1601	1604	rBV	944138	804045	80.99%	7.570%
16	11.527	1604	1605	1609	rVB	64934	37902	3.82%	0.357%
17	12.004	1683	1686	1689	rBV2	13912	14811	1.49%	0.139%
18	12.033	1689	1691	1697	rVB	13940	13844	1.39%	0.130%
19	12.116	1702	1705	1708	rBV2	16553	20588	2.07%	0.194%
20	12.557	1777	1780	1784	rBV4	12714	19766	1.99%	0.186%
21	12.586	1784	1785	1792	rVB6	8563	13800	1.39%	0.130%
22	12.721	1804	1808	1812	rBV	105796	98017	9.87%	0.923%
23	12.951	1841	1847	1853	rBV	101254	113172	11.40%	1.065%
24	13.086	1866	1870	1873	rBV	828990	687590	69.26%	6.474%
25	13.274	1900	1902	1904	rBV	18278	15079	1.52%	0.142%
26	13.386	1916	1921	1923	rBV2	19484	27118	2.73%	0.255%
27	13.974	2018	2021	2024	rBV4	21973	30766	3.10%	0.290%
28	14.151	2046	2051	2054	rBV	747967	727732	73.30%	6.851%
29	15.680	2306	2311	2317	rBV2	367540	516675	52.04%	4.864%


Sum of corrected areas: 10621587

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102618\
Data File : BF110224.D
Acq On : 26 Oct 2018 21:52
Operator : JU/SJ
Sample : J5204-15 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-01-102518-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

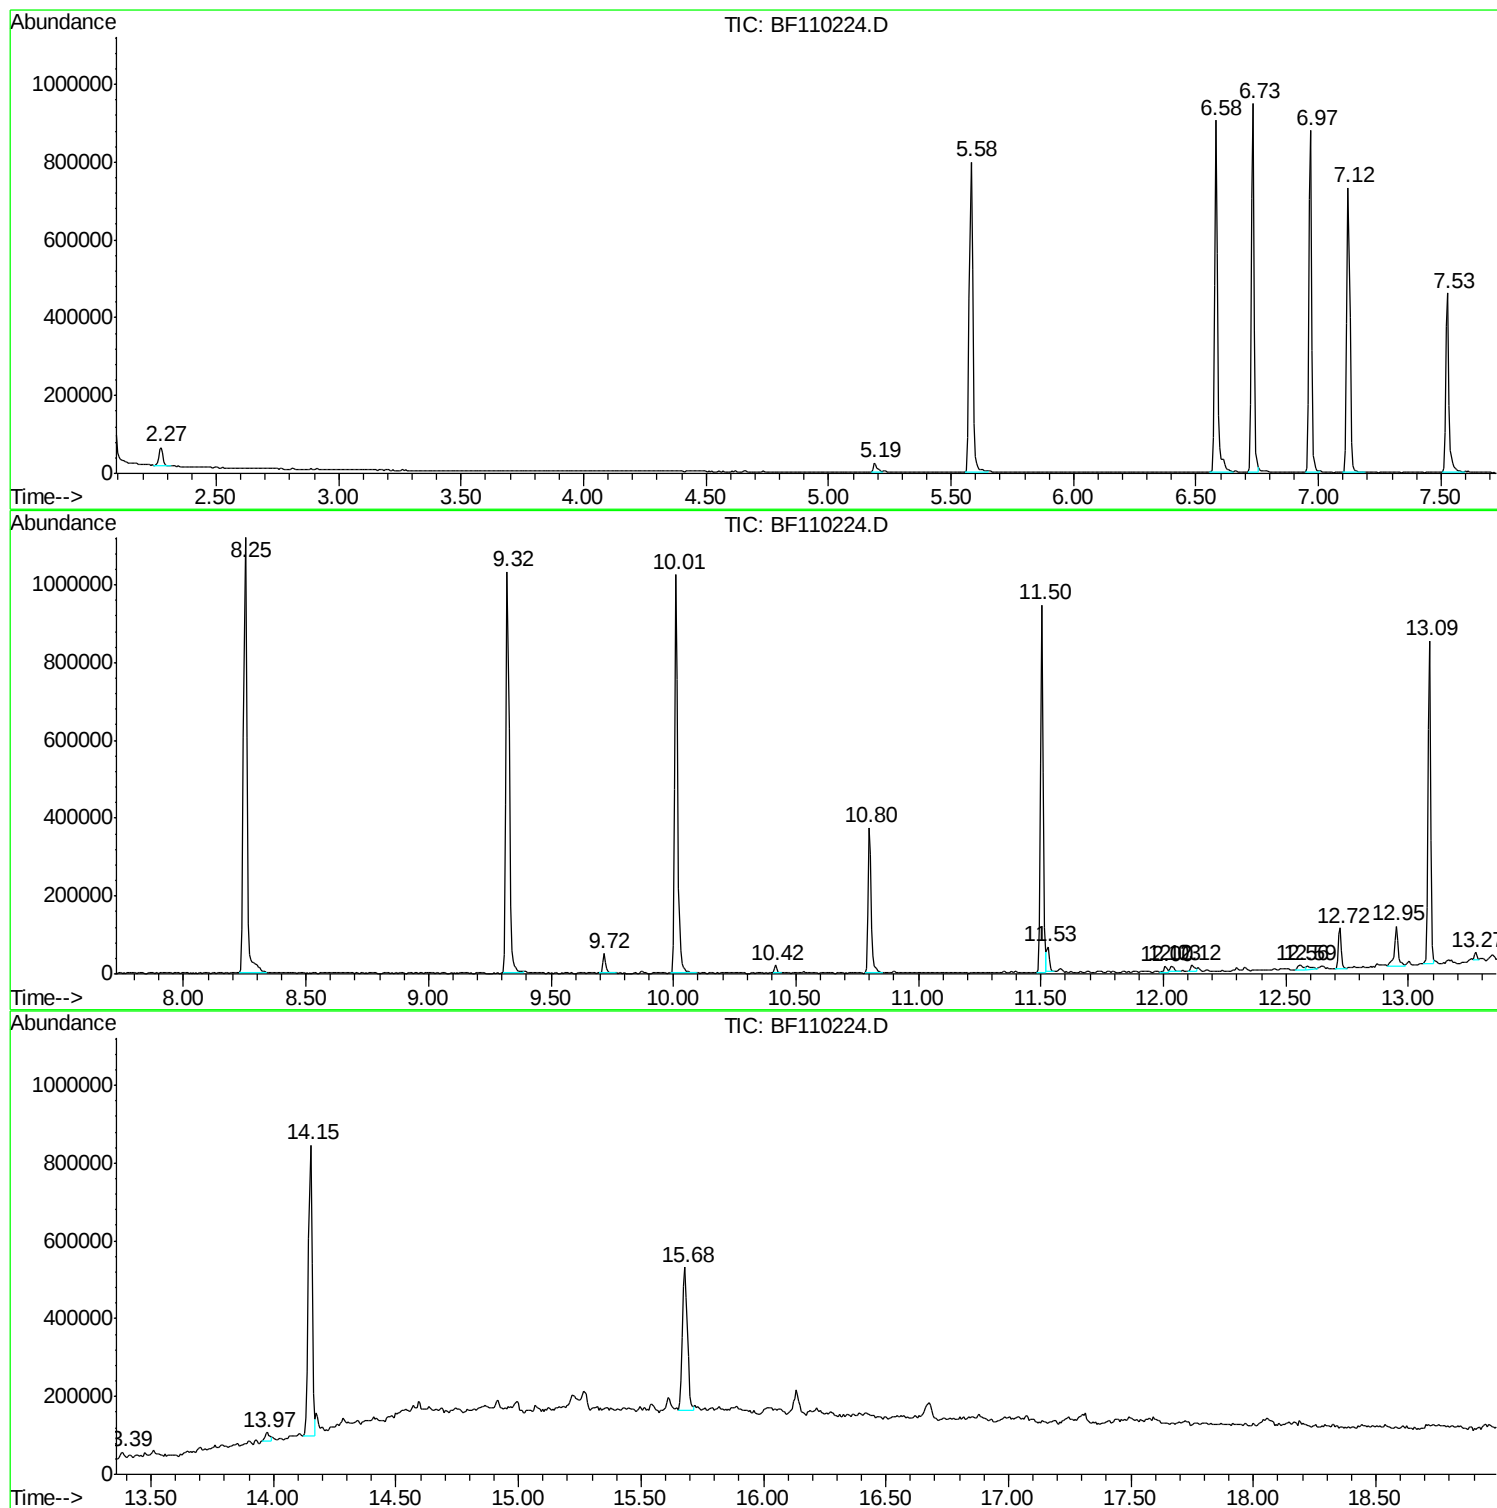

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102618\
Data File : BF110224.D
Acq On : 26 Oct 2018 21:52
Operator : JU/SJ
Sample : J5204-15 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-01-102518-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.73 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.73	21.03 ng	797363	1,4-Dichlorobenzene-d4	6.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

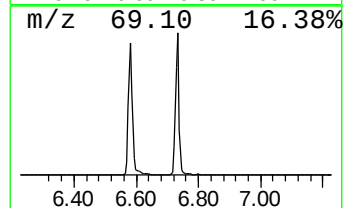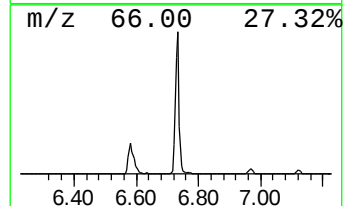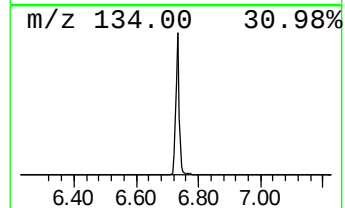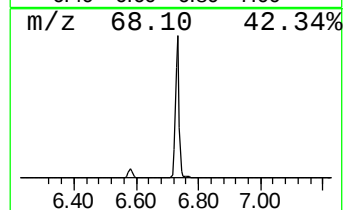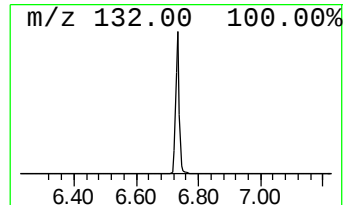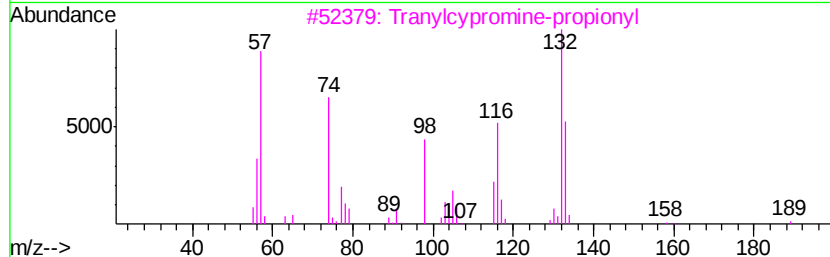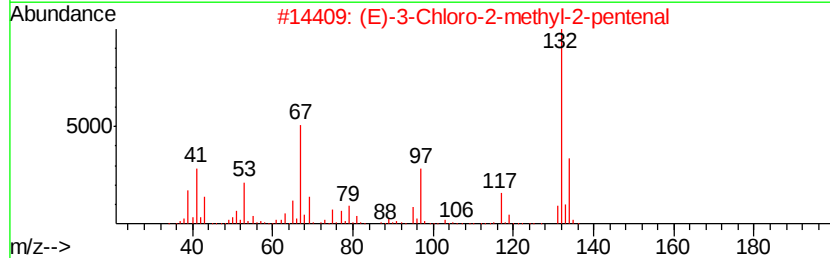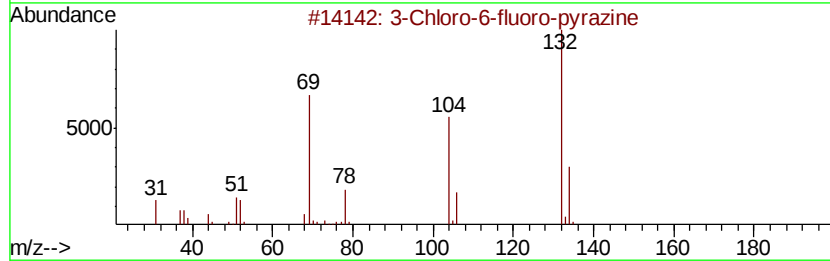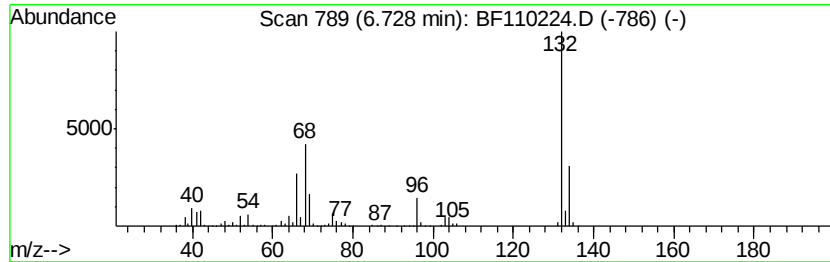

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102618\
Data File : BF110224.D
Acq On : 26 Oct 2018 21:52
Operator : JU/SJ
Sample : J5204-15 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-01-102518-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.73	6.73	21.0	ng	797363	1	6.97	758382	20.0