


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102618\
 Data File : BF110232.D
 Acq On : 27 Oct 2018 1:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 23 15:06:18 2018

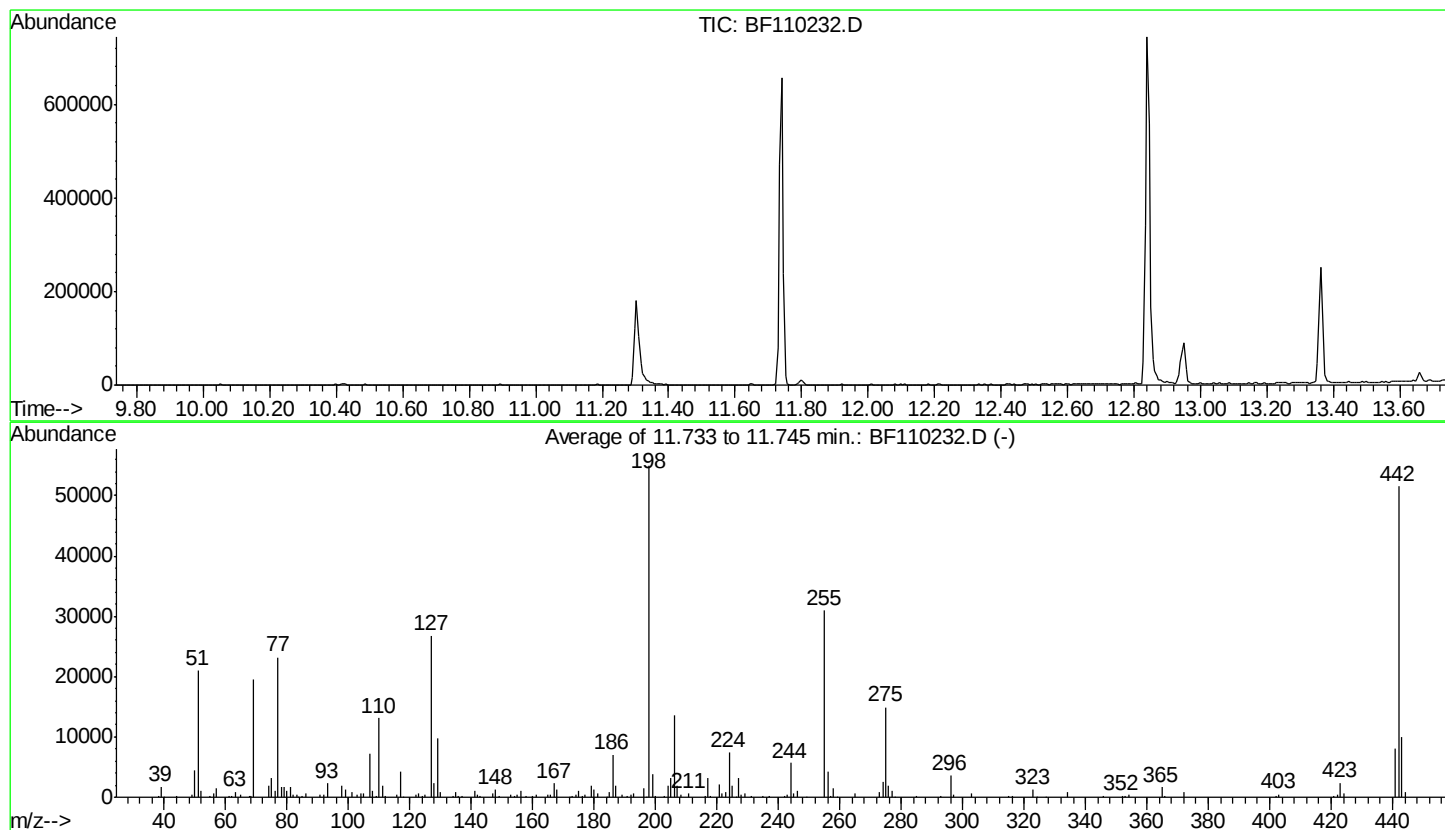

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	20957	PASS
68	69	0.00	2	0.9	178	PASS
69	198	0.00	100	35.7	19599	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	26832	PASS
197	198	0.00	2	0.2	106	PASS
198	198	100	100	100.0	54965	PASS
199	198	5	9	6.9	3800	PASS
275	198	10	60	27.1	14918	PASS
365	198	1	100	3.1	1695	PASS
441	198	0.01	100	14.8	8123	PASS
442	198	50	100	93.7	51509	PASS
443	442	15	24	19.2	9888	PASS