
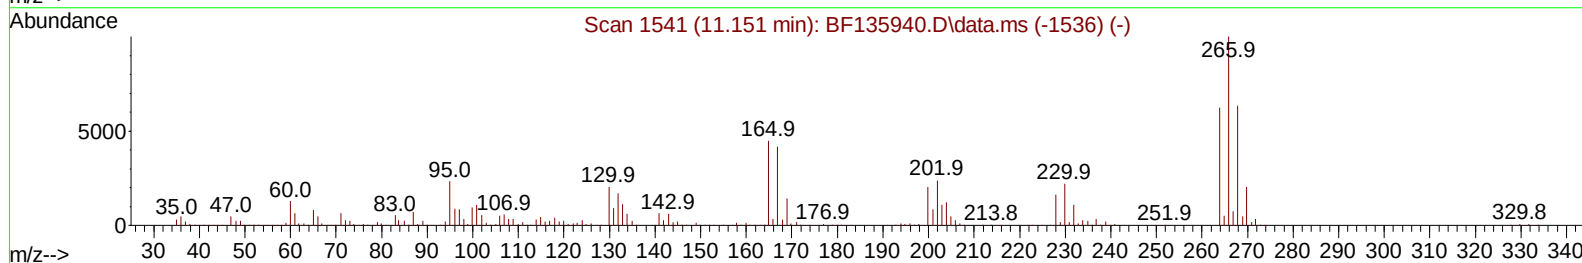
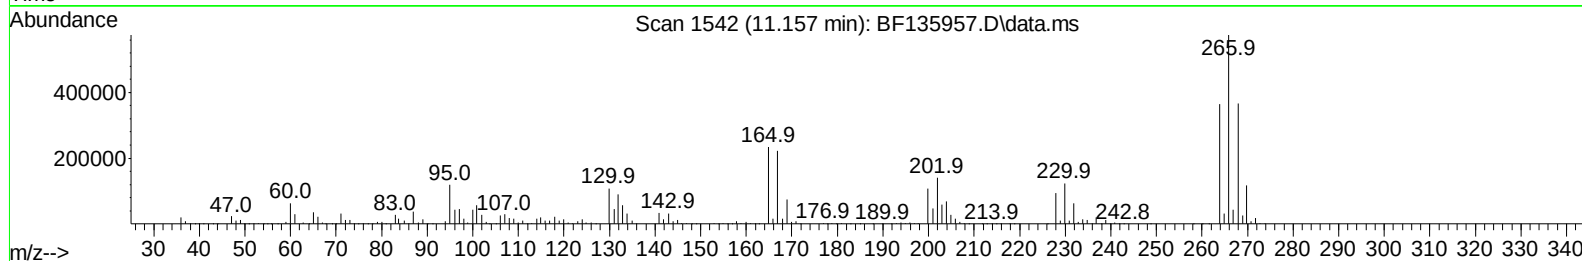


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102623\
Data File : BF135957.D
Acq On : 26 Oct 2023 09:40
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 19:54:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

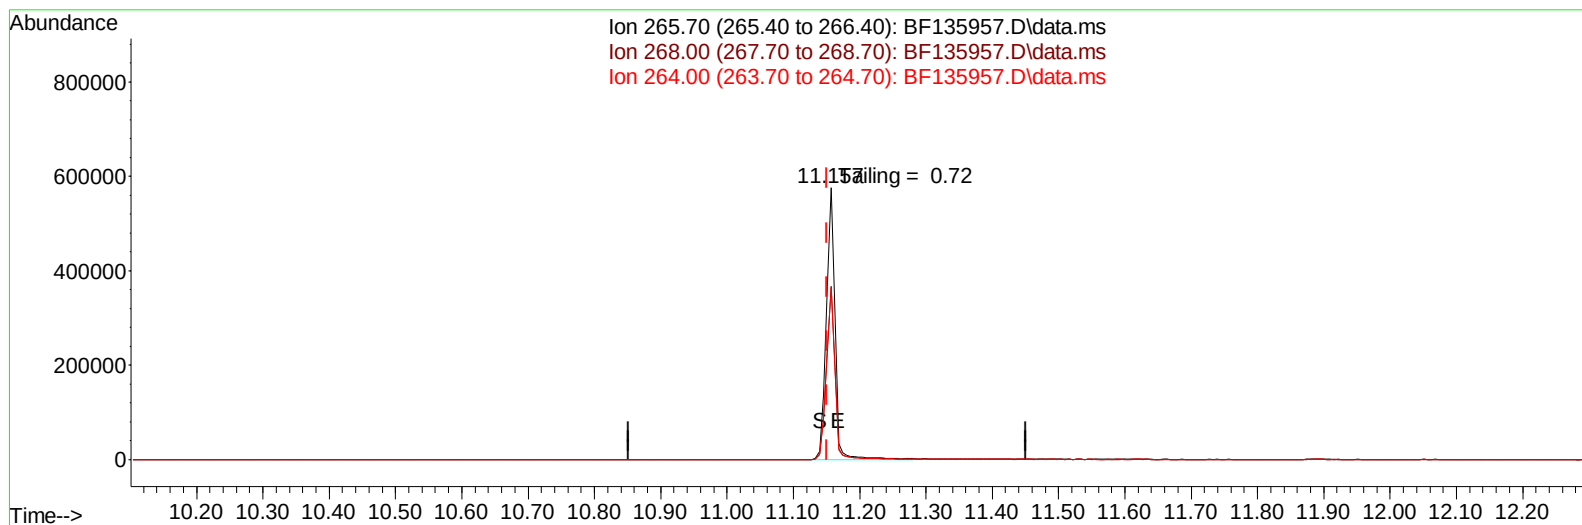

TIC: BF135957.D\data.ms

(70) Pentachlorophenol (C)




11.157min (+ 0.006) 38821.46 ng

response 534971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.90
264.00	62.20	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102623\
Data File : BF135957.D
Acq On : 26 Oct 2023 09:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 19:54:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

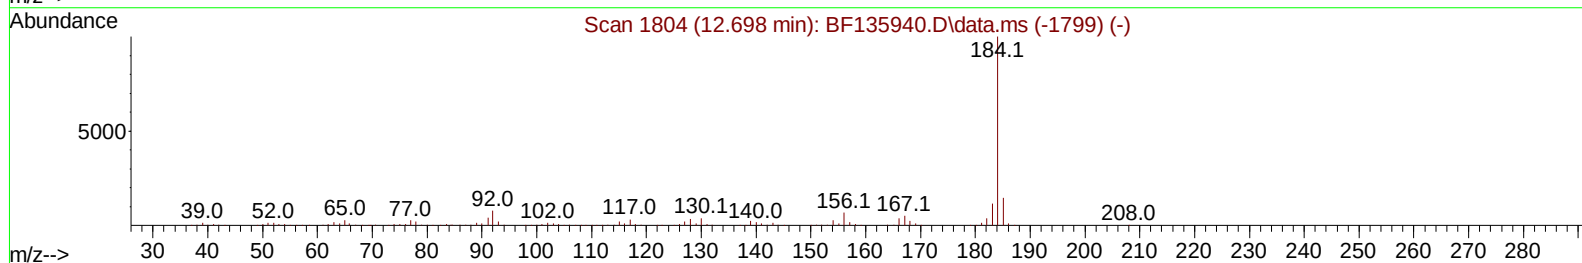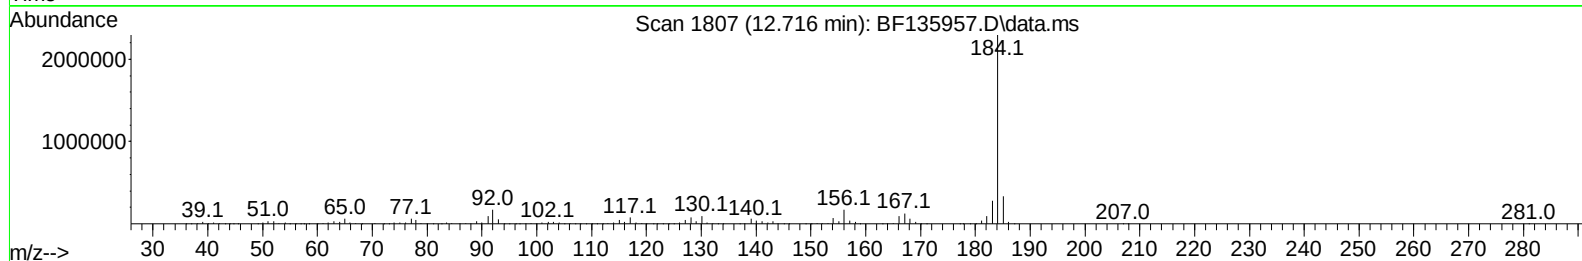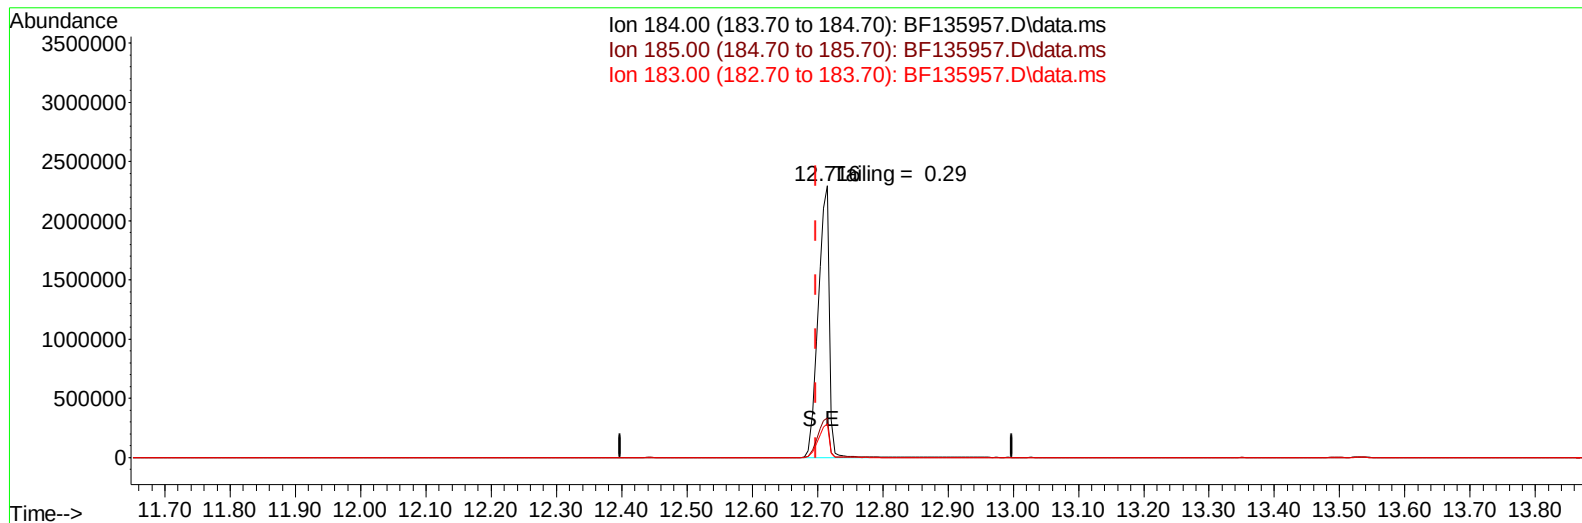

TIC: BF135957.D\data.ms

(77) Benzidine**12.716min (+ 0.018) 59082.95 ng****response 2787746**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.59
183.00	11.50	12.30
0.00	0.00	0.00