


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102623\
 Data File : BF135957.D
 Acq On : 26 Oct 2023 09:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 26 03:58:01 2023



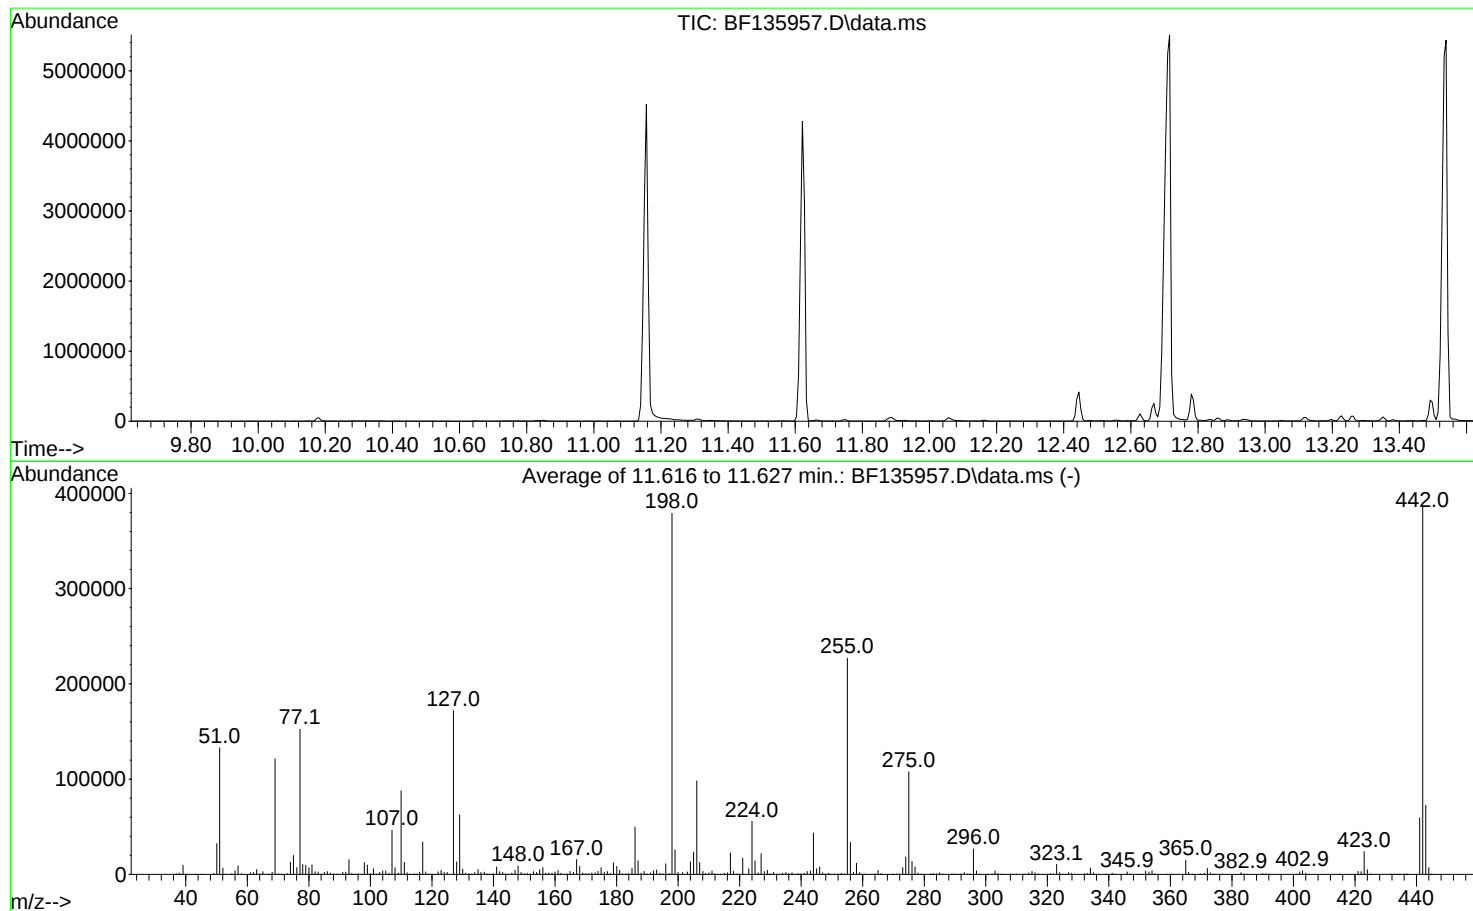


AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	132848	PASS
68	69	0.00	2	1.9	2285	PASS
69	198	0.00	100	32.0	121280	PASS
70	69	0.00	2	0.6	717	PASS
127	198	10	80	45.3	171840	PASS
197	198	0.00	2	0.2	883	PASS
198	198	100	100	100.0	379115	PASS
199	198	5	9	6.8	25845	PASS
275	198	10	60	28.4	107661	PASS
365	198	1	100	3.9	14725	PASS
441	198	0.01	100	15.7	59352	PASS
442	442	50	100	100.0	386155	PASS
443	442	15	24	18.8	72629	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 26 19:54:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

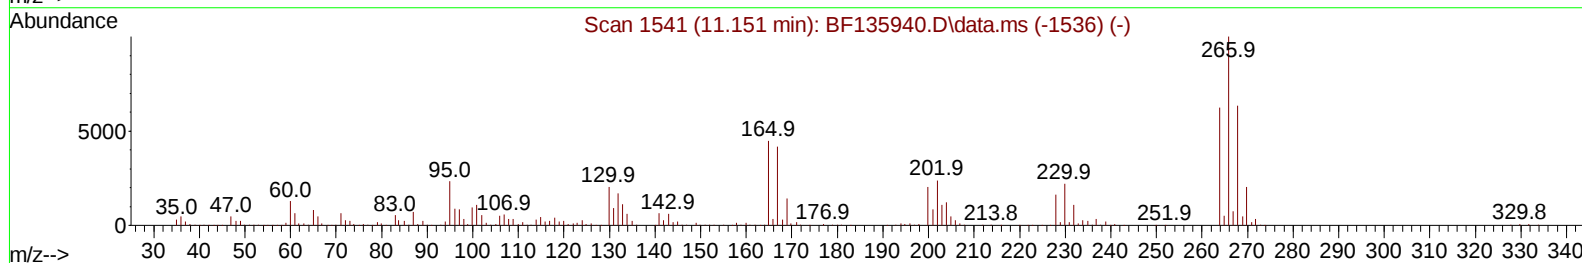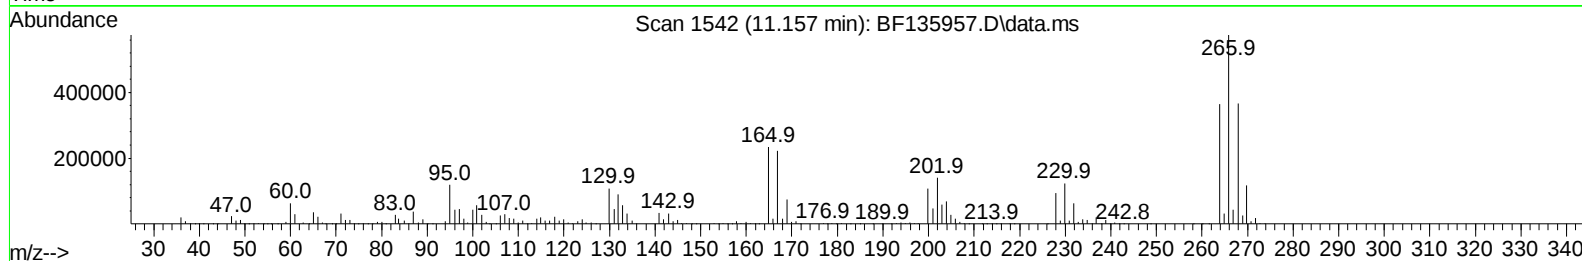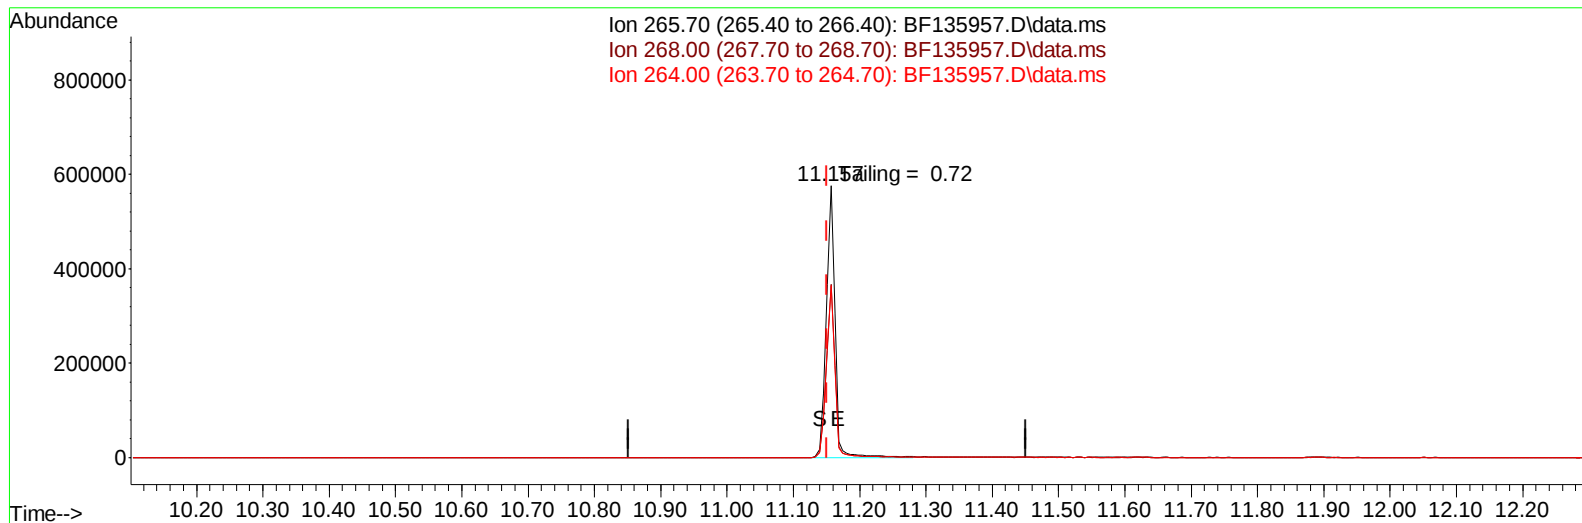

TIC: BF135957.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.006) 38821.46 ng




response 534971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.90
264.00	62.20	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102623\
Data File : BF135957.D
Acq On : 26 Oct 2023 09:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 26 19:54:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

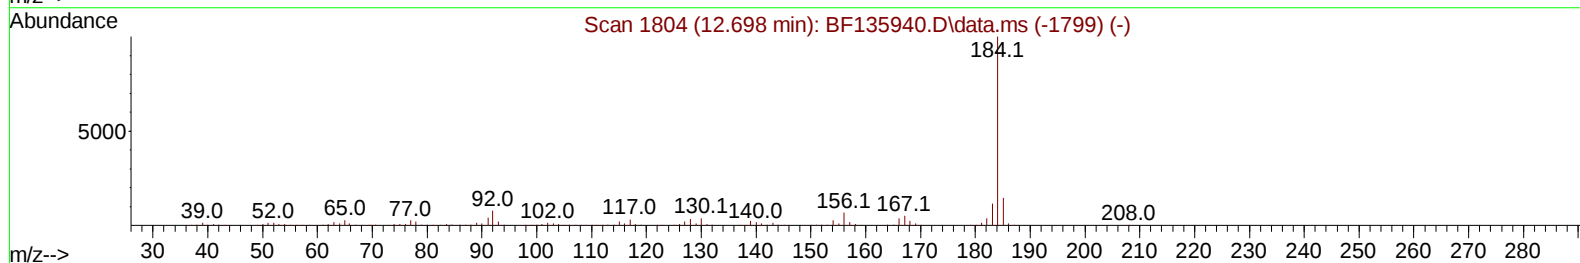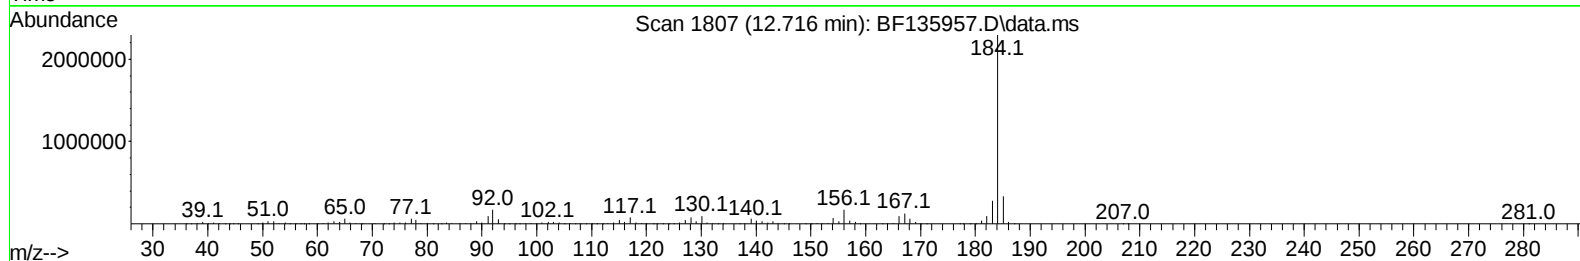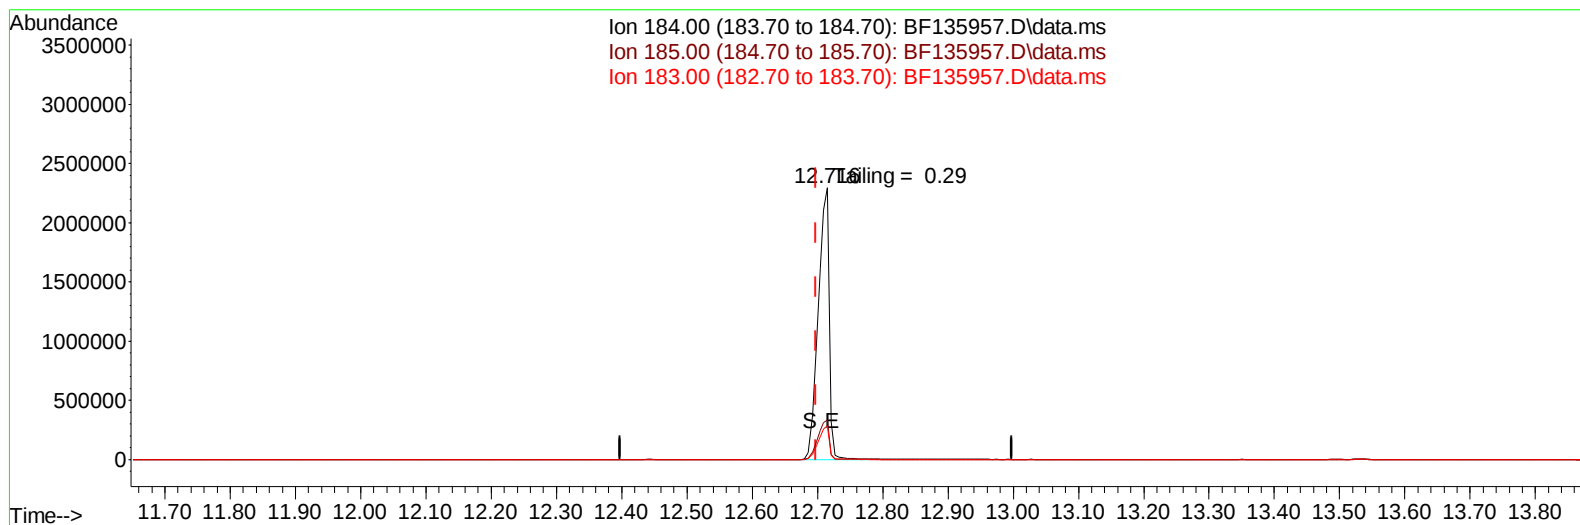

TIC: BF135957.D\data.ms

(77) Benzidine

12.716min (+ 0.018) 59082.95 ng

response 2787746

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.59
183.00	11.50	12.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2023	BNA_F	<u>BF135957.D</u>
Compound Name	Response	Retention Time
DDT	1127273	13.539
DDD	23865	13.227
DDE	2055	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25920	1153193	2.25

Instrument :
BNA_F
ClientSampleId :
DFTPP