

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102723\
 Data File : BF135991.D
 Acq On : 27 Oct 2023 18:34
 Operator : CG\JU
 Sample : 04767-01DL 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D-1(0-5)DL

Quant Time: Oct 27 22:34:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 26 03:58:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.828	152	174061	20.000	ng	0.00
21) Naphthalene-d8	8.104	136	688716	20.000	ng	0.00
39) Acenaphthene-d10	9.863	164	340902	20.000	ng	0.00
64) Phenanthrene-d10	11.351	188	520375	20.000	ng	0.00
76) Chrysene-d12	14.010	240	333579	20.000	ng	0.00
86) Perylene-d12	15.498	264	349329	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.451	112	624321	55.386	ng	0.00
7) Phenol-d6	6.451	99	766978	54.654	ng	0.00
23) Nitrobenzene-d5	7.381	82	436284	45.985	ng	-0.01
42) 2,4,6-Tribromophenol	10.651	330	162867	54.582	ng	0.00
45) 2-Fluorobiphenyl	9.181	172	850879	39.967	ng	0.00
79) Terphenyl-d14	12.951	244	617373	30.922	ng	0.00
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.381	70	56670	7.101	ng	# 79
24) Nitrobenzene	7.404	77	59	2.587	ng	# 36
25) Isophorone	7.381	82	435326	19.997	ng	# 64
32) Benzoic acid	7.881	122	146	5.760	ng	# 54
48) 2-Nitroaniline	9.381	65	556	4.322	ng	# 4
49) Acenaphthylene	9.722	152	113694	3.772	ng	98
50) Dimethylphthalate	9.863	163	71571	3.237	ng	# 1
51) 2,6-Dinitrotoluene	9.863	165	46526	13.985	ng	# 21
53) 3-Nitroaniline	9.816	138	108	4.580	ng	# 1
56) 4-Nitrophenol	9.969	139	1509	6.496	ng	# 78
57) 2,4-Dinitrotoluene	10.063	165	1764	6.101	ng	# 54
58) Fluorene	10.410	166	44906	2.151	ng	95
62) 4-Nitroaniline	10.381	138	334	4.705	ng	82
65) 4,6-Dinitro-2-methylph...	10.481	198	56	6.957	ng	# 1
71) Phenanthrene	11.381	178	747660	28.399	ng	100
72) Anthracene	11.428	178	173879	6.450	ng	100
75) Fluoranthene	12.575	202	912495	32.945	ng	99
78) Pyrene	12.804	202	1166902	41.662	ng	100
80) Butylbenzylphthalate	13.439	149	664	3.885	ng	# 45
81) Benzo(a)anthracene	14.033	228	555102	24.474	ng	96
83) Chrysene	14.033	228	555102	25.128	ng	98
87) Indeno(1,2,3-cd)pyrene	16.998	276	173980	8.783	ng	95
88) Benzo(b)fluoranthene	15.063	252	805823	38.761	ng	98
89) Benzo(k)fluoranthene	15.063	252	805823	39.467	ng	98
90) Benzo(a)pyrene	15.433	252	477644	24.929	ng	98
91) Dibenzo(a,h)anthracene	17.021	278	48740	2.877	ng	96
92) Benzo(g,h,i)perylene	17.457	276	164299	11.619	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102723\
Data File : BF135991.D
Acq On : 27 Oct 2023 18:34
Operator : CG\JU
Sample : 04767-01DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL

Quant Time: Oct 27 22:34:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration




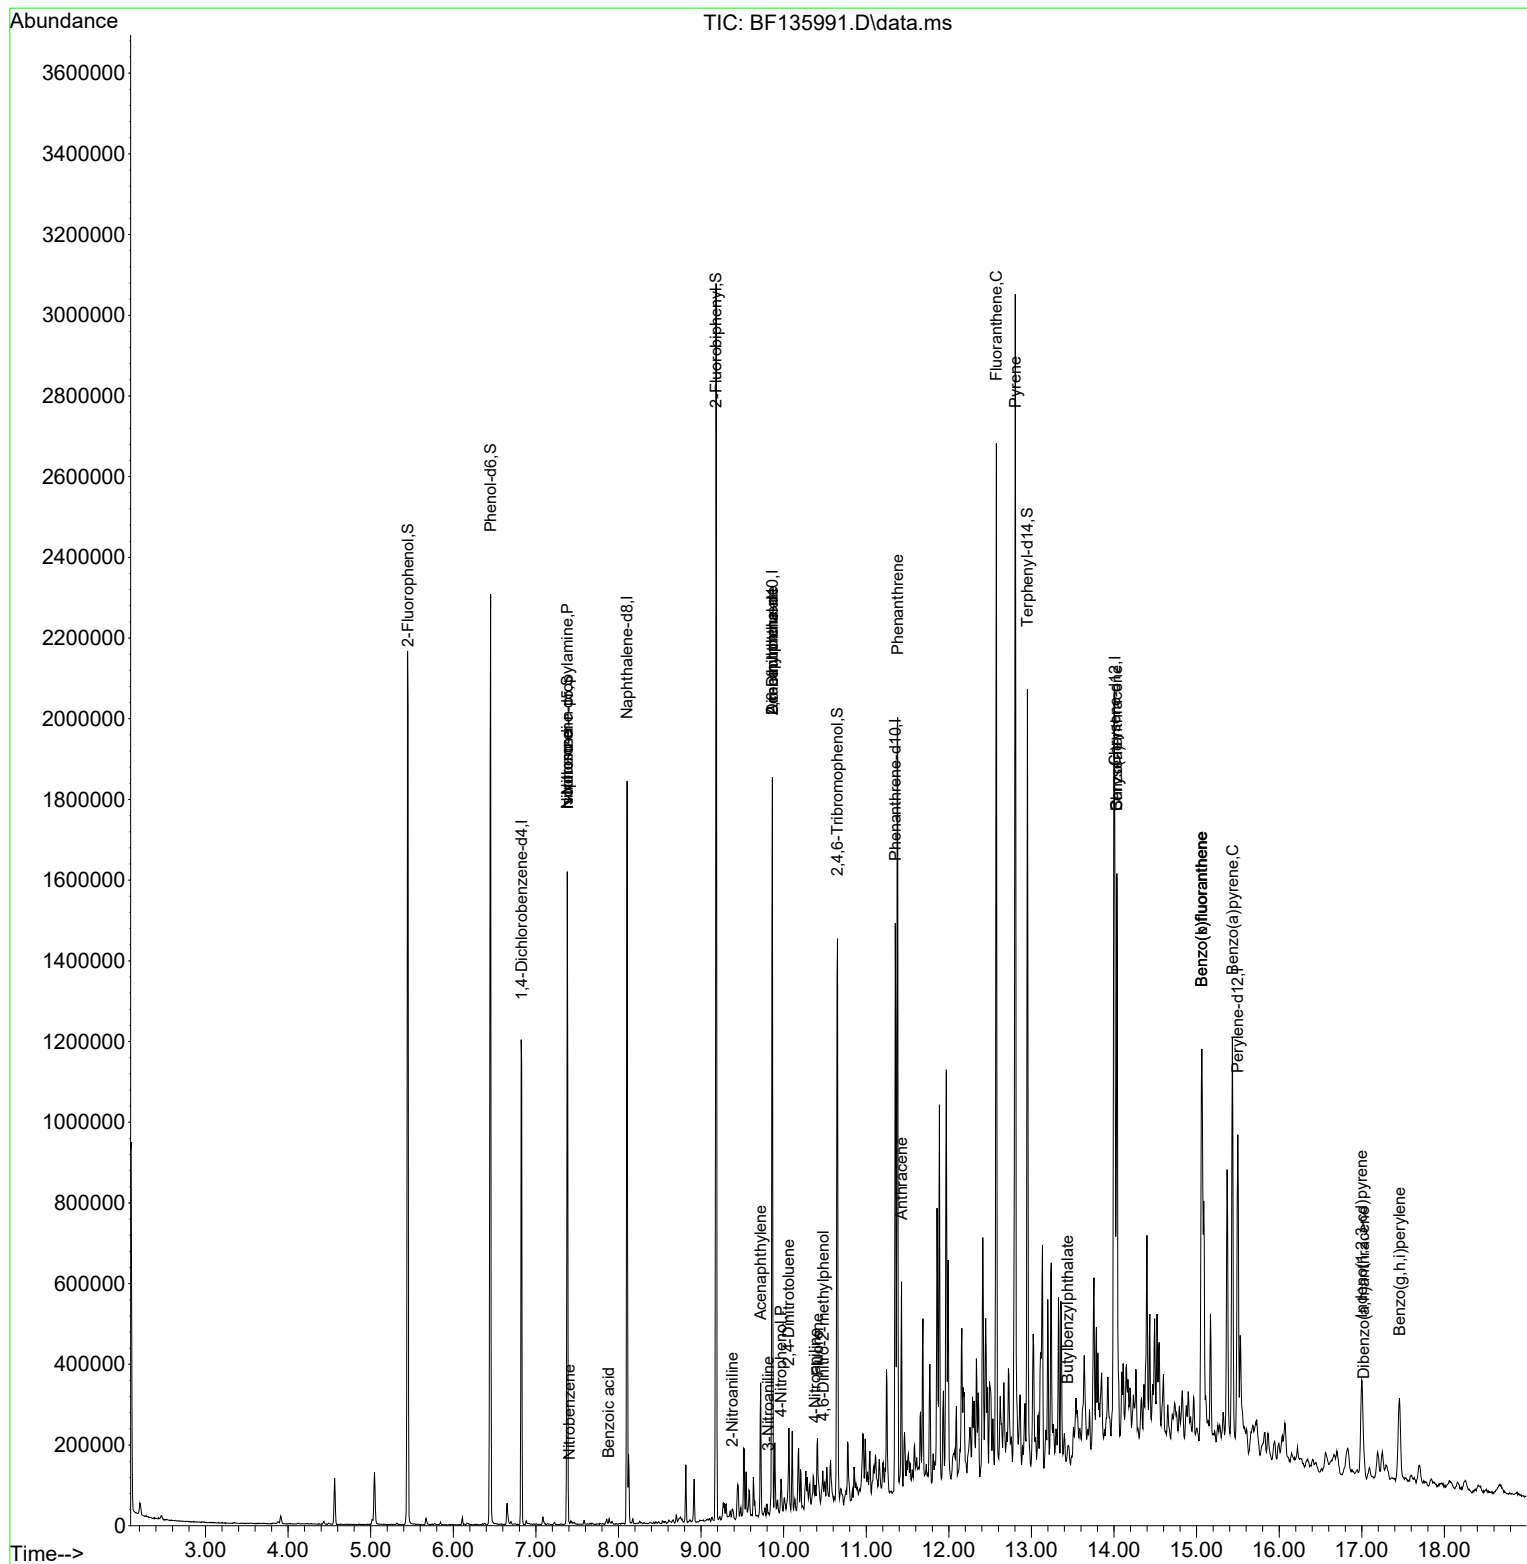




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.828 min Scan# 806
Delta R.T. -0.000 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:152 Resp: 174061
Ion Ratio Lower Upper
152 100
150 156.7 124.6 186.8
115 60.6 46.6 69.8

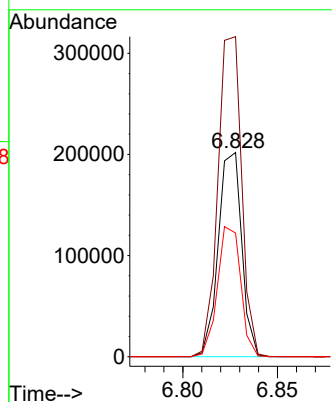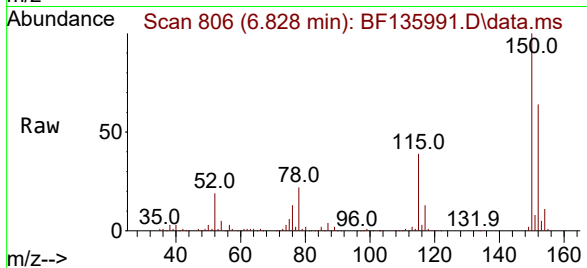

#5
2-Fluorophenol
Concen: 55.386 ng
RT: 5.451 min Scan# 572
Delta R.T. 0.000 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion:112 Resp: 624321
Ion Ratio Lower Upper
112 100
64 55.0 45.1 67.7
63 27.1 23.0 34.4




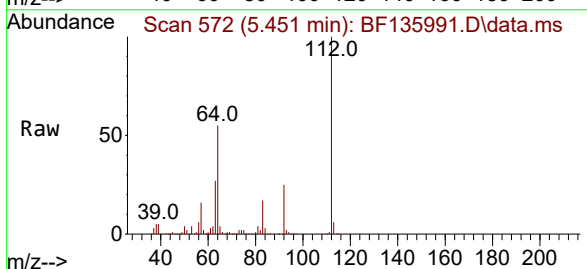




#7
Phenol-d6
Concen: 54.654 ng
RT: 6.451 min Scan# 74
Delta R.T. -0.006 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion: 99 Resp: 766978
Ion Ratio Lower Upper
99 100
42 16.9 13.8 20.8
71 31.2 25.1 37.7

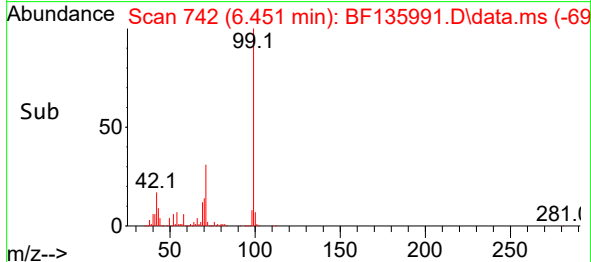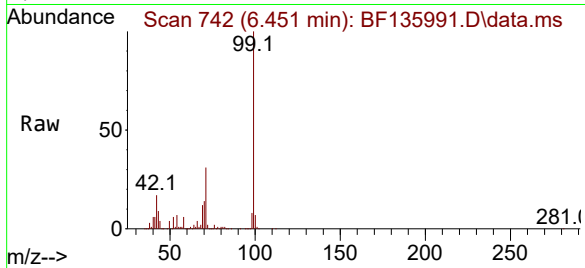

#19
n-Nitroso-di-n-propylamine
Concen: 7.101 ng
RT: 7.381 min Scan# 900
Delta R.T. 0.141 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion: 70 Resp: 56670
Ion Ratio Lower Upper
70 100
42 48.9 47.3 70.9
101 0.0 7.8 11.8#
130 2.8 16.9 25.3#


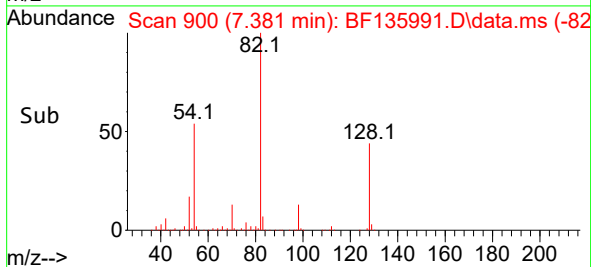

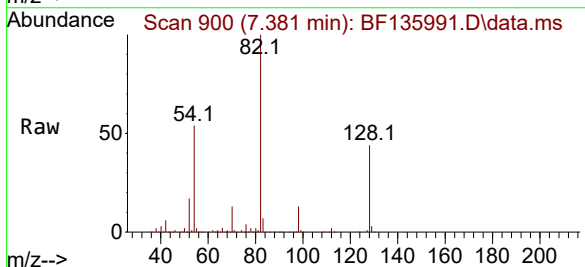




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.104 min Scan# 1
Delta R.T. 0.000 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:136 Resp: 688716
Ion Ratio Lower Upper
136 100
137 10.9 9.0 13.6
54 7.8 7.1 10.7
68 6.0 5.2 7.8

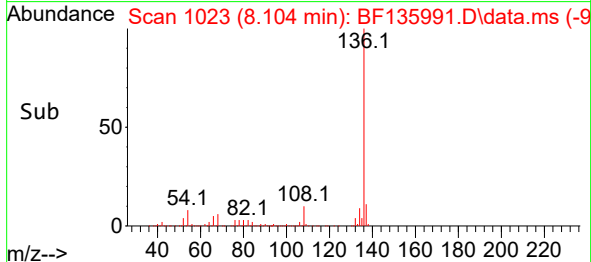

#23
Nitrobenzene-d5
Concen: 45.985 ng
RT: 7.381 min Scan# 900
Delta R.T. -0.011 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion: 82 Resp: 436284
Ion Ratio Lower Upper
82 100
128 44.3 36.8 55.2
54 53.9 43.4 65.0


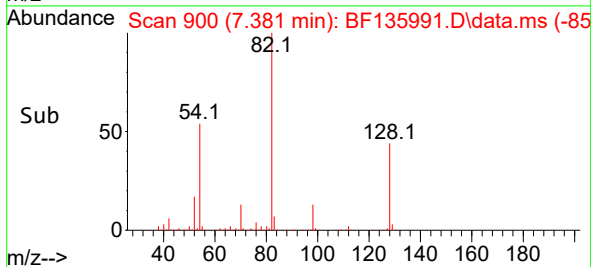

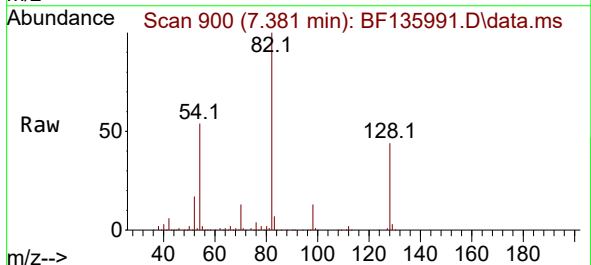




#24
Nitrobenzene
Concen: 2.587 ng
RT: 7.404 min Scan# 904
Delta R.T. -0.006 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion: 77 Resp: 59
Ion Ratio Lower Upper
77 100
123 0.0 40.2 60.2#
65 0.0 11.0 16.4#

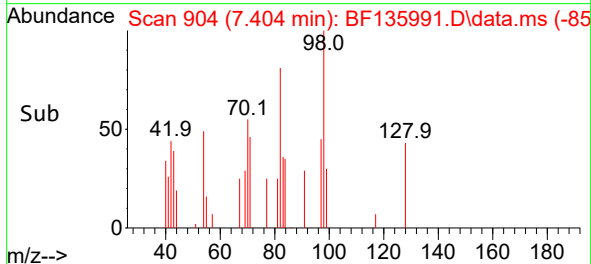

#25
Isophorone
Concen: 19.997 ng
RT: 7.381 min Scan# 900
Delta R.T. -0.265 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion: 82 Resp: 435326
Ion Ratio Lower Upper
82 100
95 0.0 5.6 8.4#
138 0.0 14.8 22.2#

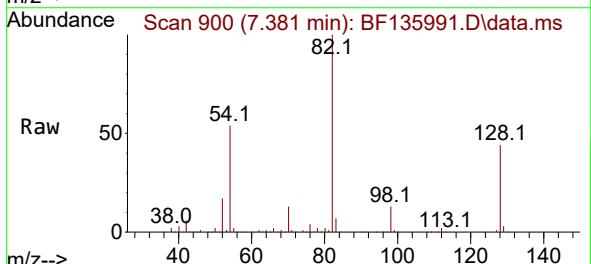



#32

Benzoic acid

Concen: 5.760 ng

RT: 7.881 min Scan# 91

Delta R.T. 0.012 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion:122 Resp: 146

Ion Ratio Lower Upper

122 100

105 66.4 113.1 153.1#

77 125.7 75.2 115.2#

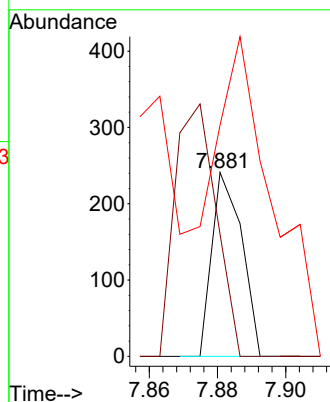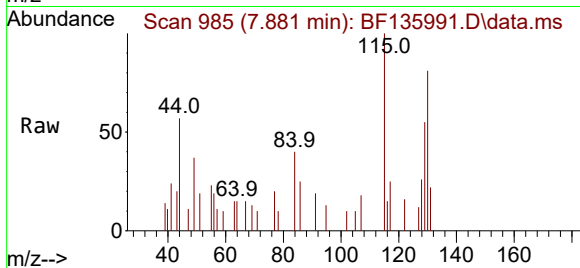

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.863 min Scan# 1322

Delta R.T. -0.000 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:164 Resp: 340902


Ion Ratio Lower Upper

164 100

162 100.1 82.0 123.0

160 44.2 35.6 53.4

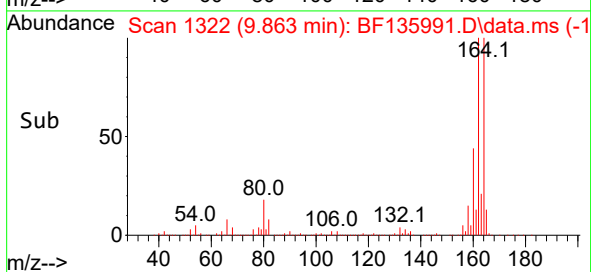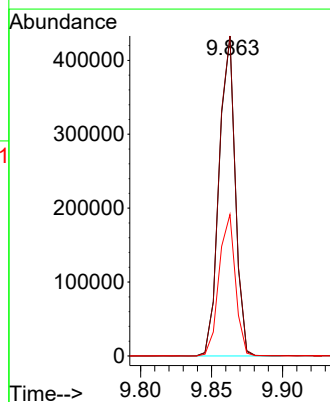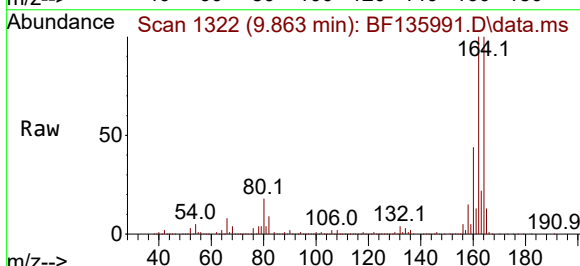



#42

2,4,6-Tribromophenol

Concen: 54.582 ng

RT: 10.651 min Scan# 1457

Delta R.T. -0.006 min

Lab File: BF135991.D


Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL






Tgt Ion:330 Resp: 162867

Ion Ratio Lower Upper

330 100

332 96.3 77.4 116.2

141 31.3 24.9 37.3

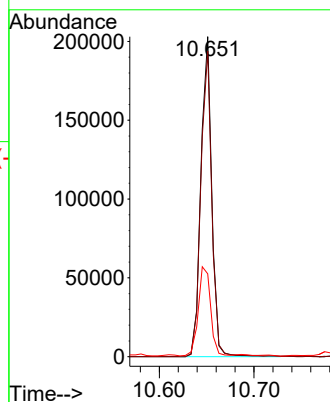

#45

2-Fluorobiphenyl

Concen: 39.967 ng

RT: 9.181 min Scan# 1206

Delta R.T. -0.006 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:172 Resp: 850879


Ion Ratio Lower Upper

172 100

171 35.3 28.6 43.0

170 23.7 18.6 28.0

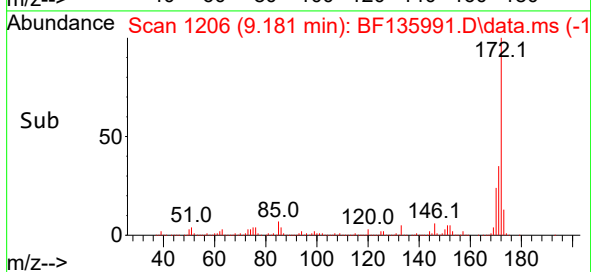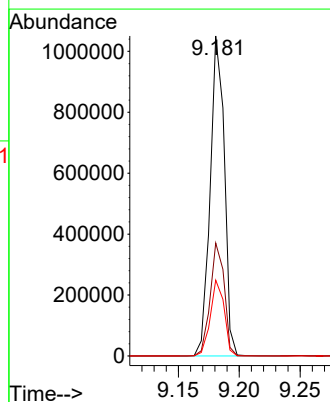



#48

2-Nitroaniline

Concen: 4.322 ng

RT: 9.381 min Scan# 11

Delta R.T. -0.023 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion: 65 Resp: 556

Ion Ratio Lower Upper

65 100

92 0.0 54.9 82.3#

138 0.0 85.2 127.8#

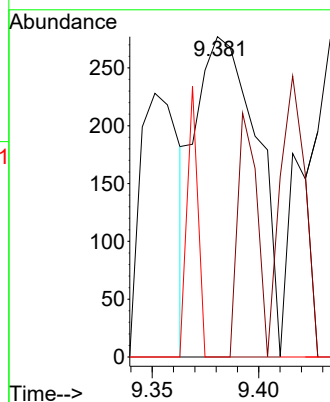

#49

Acenaphthylene

Concen: 3.772 ng

RT: 9.722 min Scan# 1298

Delta R.T. -0.006 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion: 152 Resp: 113694


Ion Ratio Lower Upper

152 100

151 19.1 16.0 24.0

153 14.4 11.0 16.6



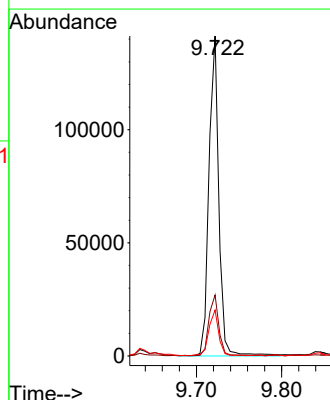





#50
Dimethylphthalate
Concen: 3.237 ng
RT: 9.863 min Scan# 1322
Delta R.T. 0.271 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:163 Resp: 71571
Ion Ratio Lower Upper
163 100
194 0.0 3.4 5.0#
164 464.4 8.3 12.5#

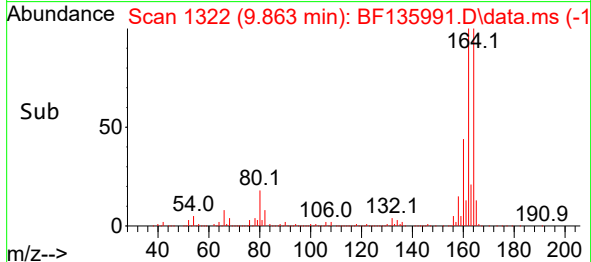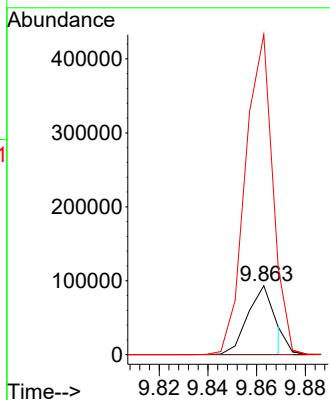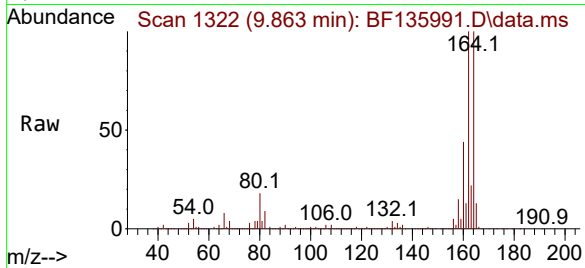

#51
2,6-Dinitrotoluene
Concen: 13.985 ng
RT: 9.863 min Scan# 1322
Delta R.T. 0.218 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion:165 Resp: 46526
Ion Ratio Lower Upper
165 100
63 1.4 51.7 77.5#
89 1.1 48.3 72.5#

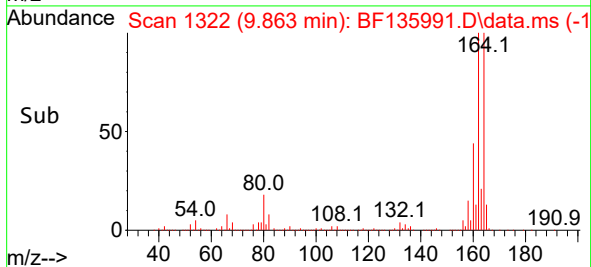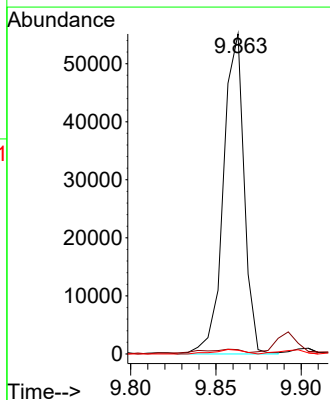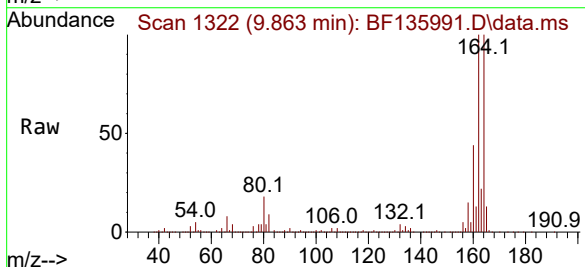



#53

3-Nitroaniline

Concen: 4.580 ng

RT: 9.816 min Scan# 1314

Delta R.T. -0.000 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion:138 Resp: 108

Ion Ratio Lower Upper

138 100

108 0.0 11.3 16.9#

92 0.0 95.0 142.6#

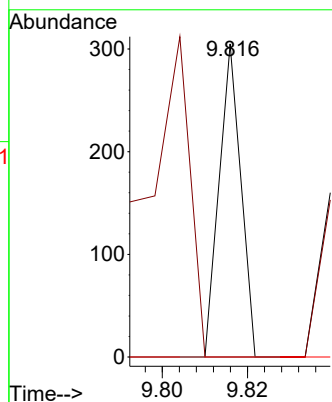

#56

4-Nitrophenol

Concen: 6.496 ng

RT: 9.969 min Scan# 1340

Delta R.T. -0.000 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:139 Resp: 1509


Ion Ratio Lower Upper

139 100

109 68.2 45.2 85.2

65 51.8 65.1 105.1#









#57
2,4-Dinitrotoluene
Concen: 6.101 ng
RT: 10.063 min Scan# 11
Delta R.T. 0.012 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:165 Resp: 1764
Ion Ratio Lower Upper
165 100
63 114.6 33.7 50.5#
89 72.5 54.6 81.8
182 0.0 2.1 3.1#

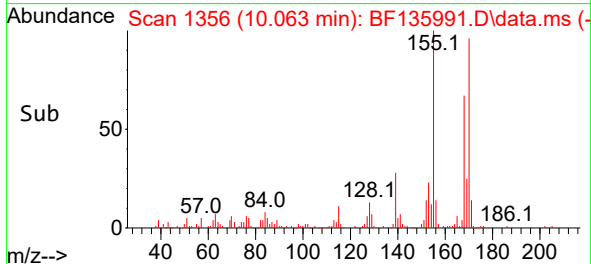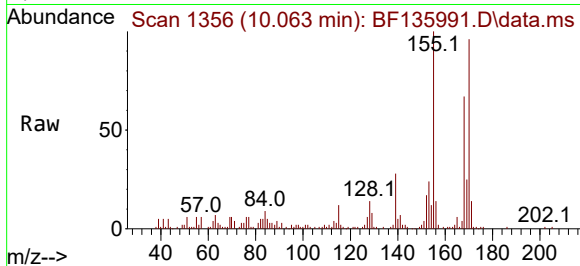

#58
Fluorene
Concen: 2.151 ng
RT: 10.410 min Scan# 1415
Delta R.T. -0.006 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion:166 Resp: 44906
Ion Ratio Lower Upper
166 100
165 91.8 78.0 117.0
167 13.2 10.6 16.0


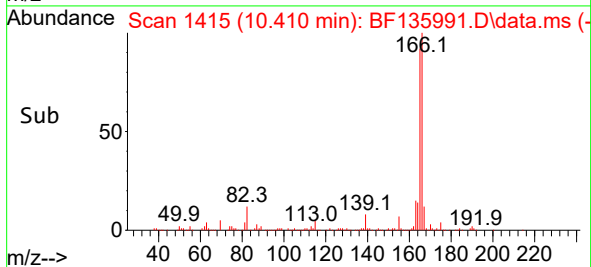

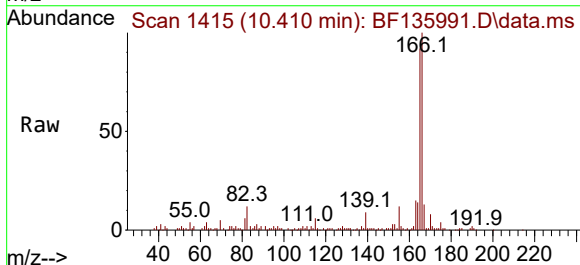


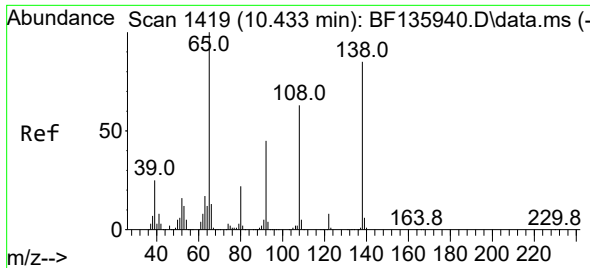

#62
4-Nitroaniline
Concen: 4.705 ng
RT: 10.381 min Scan# 1419
Delta R.T. -0.052 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:138 Resp: 334
Ion Ratio Lower Upper
138 100
92 63.2 32.9 72.9
108 56.1 53.5 93.5

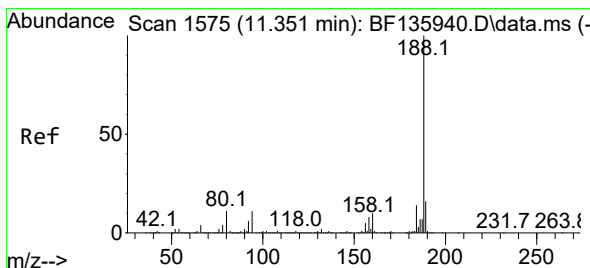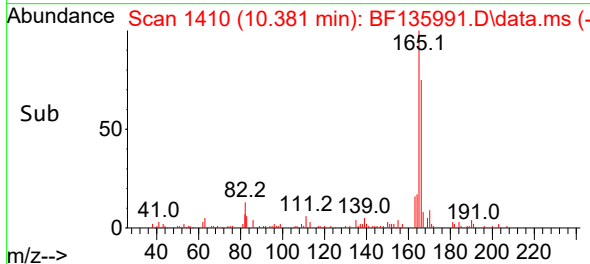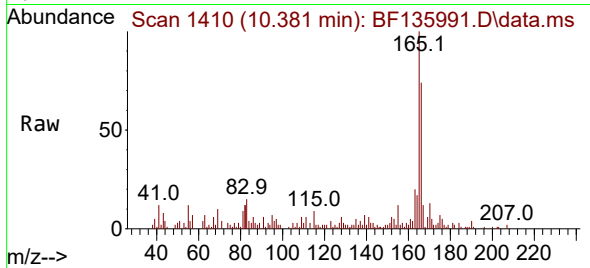

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.351 min Scan# 1575
Delta R.T. 0.000 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion:188 Resp: 520375
Ion Ratio Lower Upper
188 100
94 10.5 8.6 13.0
80 10.8 9.0 13.6


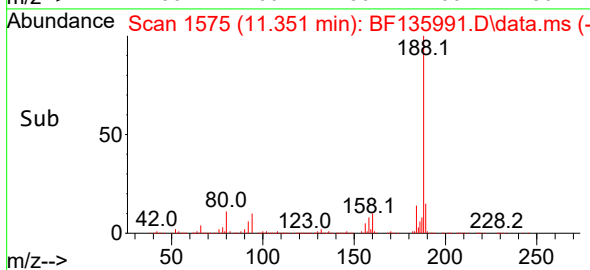

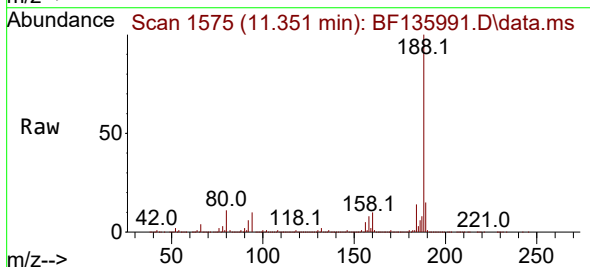




#65
4,6-Dinitro-2-methylphenol
Concen: 6.957 ng
RT: 10.481 min Scan# 1427
Delta R.T. 0.024 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:198 Resp: 56
Ion Ratio Lower Upper
198 100
51 457.9 28.7 68.7#
105 328.3 27.2 67.2#

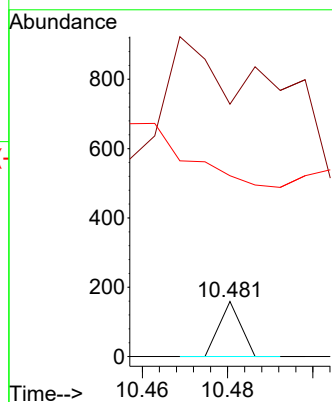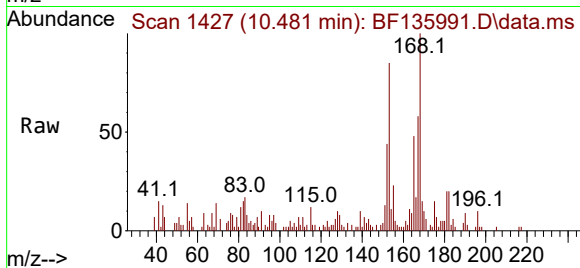

#71
Phenanthrene
Concen: 28.399 ng
RT: 11.381 min Scan# 1580
Delta R.T. 0.000 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion:178 Resp: 747660
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.2
179 15.3 12.5 18.7

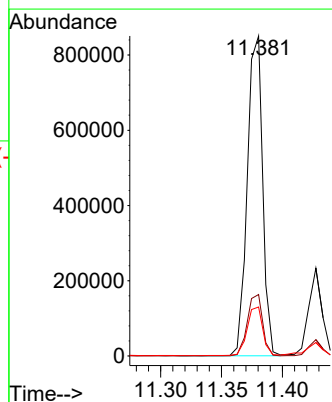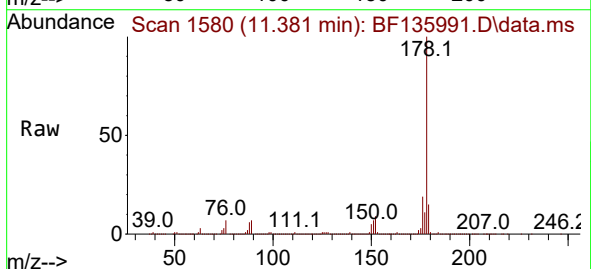



#72

Anthracene

Concen: 6.450 ng

RT: 11.428 min Scan# 1588

Delta R.T. -0.006 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion:178 Resp: 173879

Ion Ratio Lower Upper

178 100

176 18.6 14.9 22.3

179 15.3 12.5 18.7

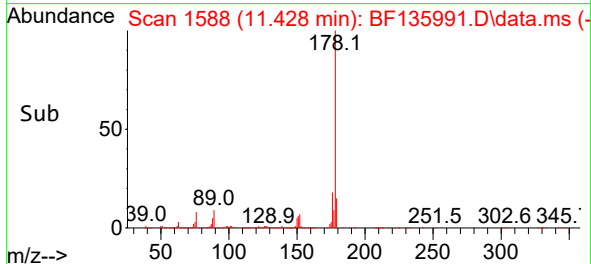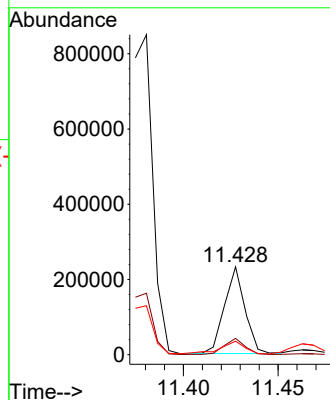

#75

Fluoranthene

Concen: 32.945 ng

RT: 12.575 min Scan# 1783

Delta R.T. 0.000 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:202 Resp: 912495


Ion Ratio Lower Upper

202 100

101 11.0 0.0 30.6

203 17.6 0.0 37.5

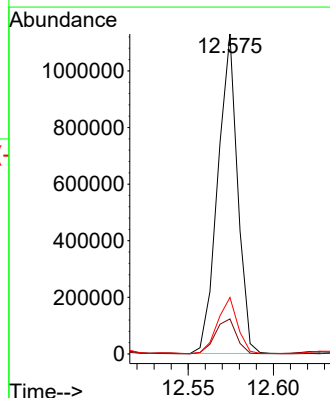



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.010 min Scan# 2027

Delta R.T. 0.000 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion:240 Resp: 333579

Ion Ratio Lower Upper

240 100

120 11.2 8.6 13.0

236 25.5 20.6 30.8

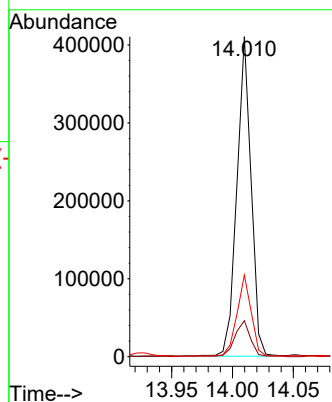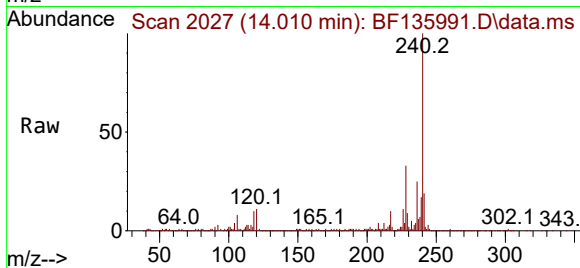

#78

Pyrene

Concen: 41.662 ng

RT: 12.804 min Scan# 1822

Delta R.T. 0.000 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:202 Resp: 1166902


Ion Ratio Lower Upper

202 100

200 21.3 17.0 25.6

203 18.2 14.5 21.7

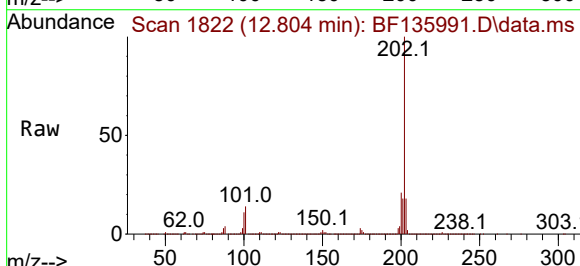



#79

Terphenyl-d14

Concen: 30.922 ng

RT: 12.951 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion:244 Resp: 617373

Ion Ratio Lower Upper

244 100

212 6.2 5.0 7.6

122 11.4 8.0 12.0

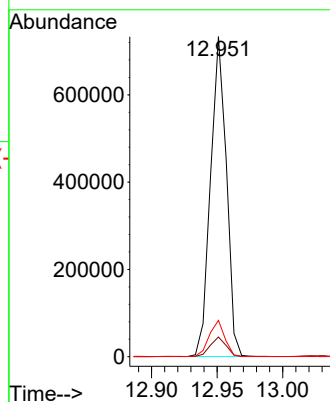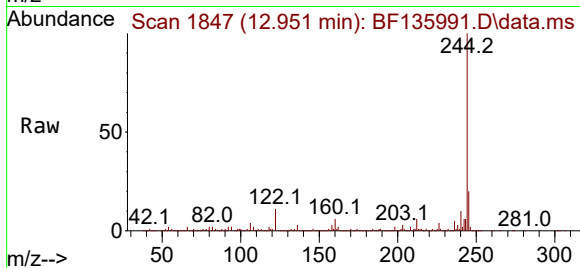

#80

Butylbenzylphthalate

Concen: 3.885 ng

RT: 13.439 min Scan# 1930

Delta R.T. 0.000 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:149 Resp: 664


Ion Ratio Lower Upper

149 100

91 96.6 53.4 80.0#

206 73.7 17.5 26.3#



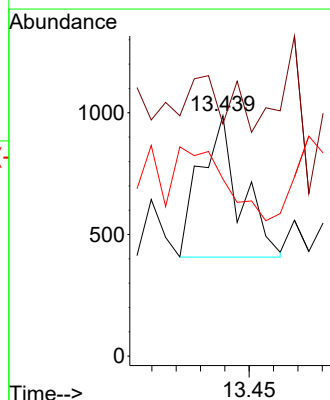
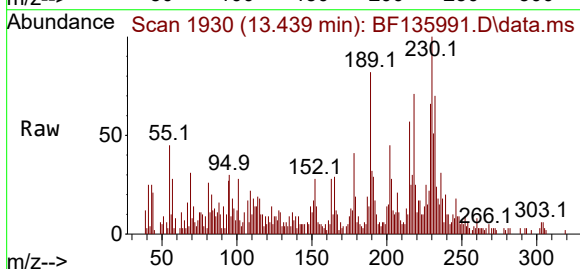




#81
Benzo(a)anthracene
Concen: 24.474 ng
RT: 14.033 min Scan# 2031
Delta R.T. 0.035 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:228 Resp: 555102
Ion Ratio Lower Upper
228 100
226 29.6 21.8 32.6
229 22.0 16.2 24.4

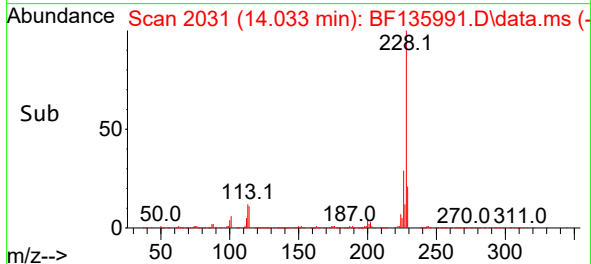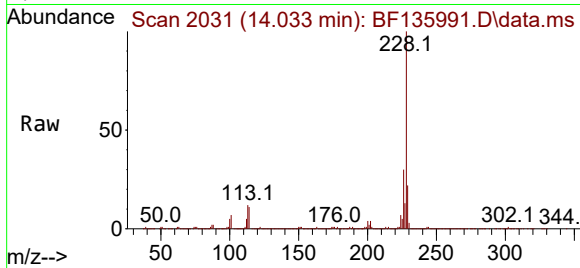

#83
Chrysene
Concen: 25.128 ng
RT: 14.033 min Scan# 2031
Delta R.T. 0.000 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34

Tgt Ion:228 Resp: 555102
Ion Ratio Lower Upper
228 100
226 29.6 23.9 35.9
229 22.0 16.2 24.2

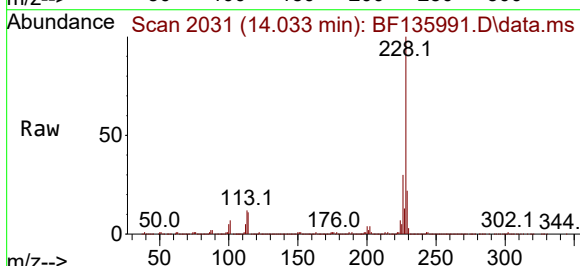



#86

Perylene-d12

Concen: 20.000 ng

RT: 15.498 min Scan# 21

Delta R.T. 0.006 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion:264 Resp: 349329

Ion Ratio Lower Upper

264 100

260 22.7 18.6 28.0

265 24.2 17.3 25.9

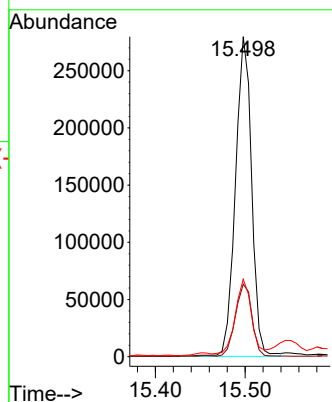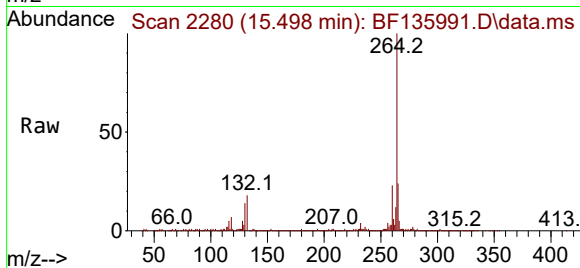

#87

Indeno(1,2,3-cd)pyrene

Concen: 8.783 ng

RT: 16.998 min Scan# 2535

Delta R.T. 0.006 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:276 Resp: 173980


Ion Ratio Lower Upper

276 100

138 22.8 21.8 32.6

277 24.5 20.0 30.0

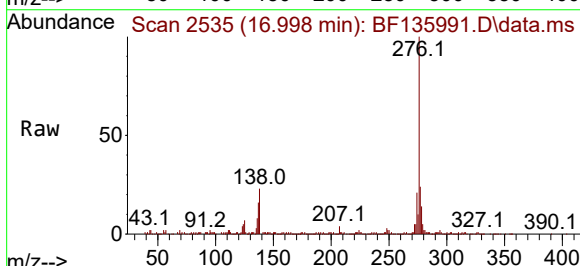



#88

Benzo(b)fluoranthene

Concen: 38.761 ng

RT: 15.063 min Scan# 2206

Delta R.T. 0.006 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34

Instrument :

BNA_F

ClientSampleId :

D-1(0-5)DL





Tgt Ion:252 Resp: 805823

Ion Ratio Lower Upper

252 100

253 23.0 18.0 27.0

125 11.5 8.2 12.4

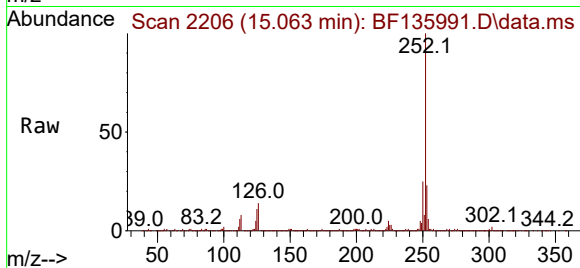

#89

Benzo(k)fluoranthene

Concen: 39.467 ng

RT: 15.063 min Scan# 2206

Delta R.T. -0.023 min

Lab File: BF135991.D

Acq: 27 Oct 2023 18:34




Tgt Ion:252 Resp: 805823


Ion Ratio Lower Upper

252 100

253 23.0 17.7 26.5

125 11.5 8.5 12.7




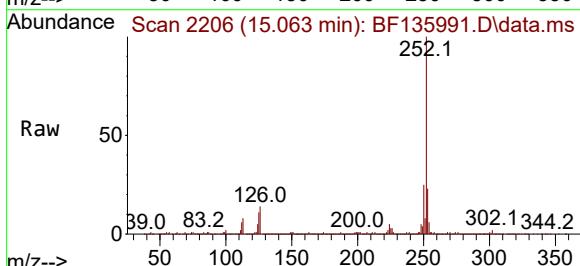


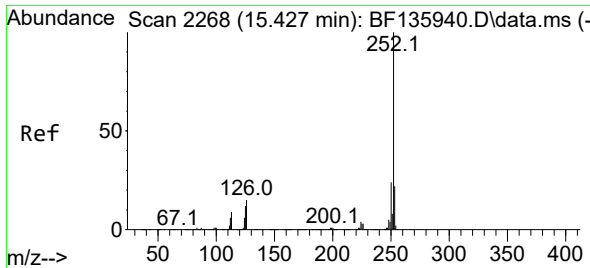

#90
Benzo(a)pyrene
Concen: 24.929 ng
RT: 15.433 min Scan# 2269
Delta R.T. 0.006 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34




Instrument :
BNA_F
ClientSampleId :
D-1(0-5)DL


Tgt Ion:252 Resp: 477644
Ion Ratio Lower Upper
252 100
253 22.6 17.4 26.2
125 11.4 9.6 14.4

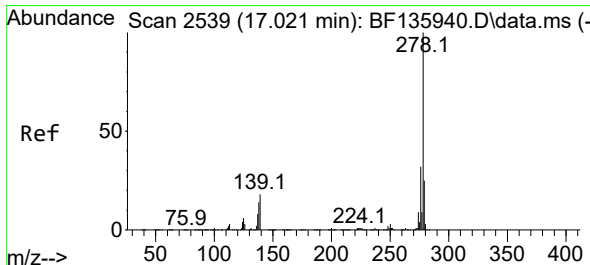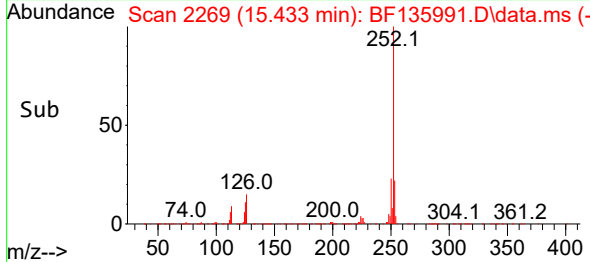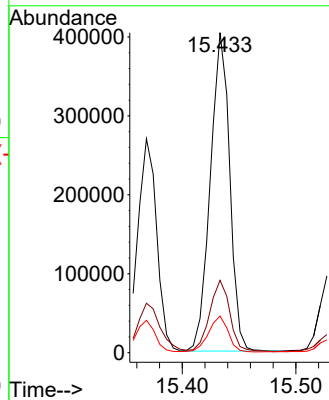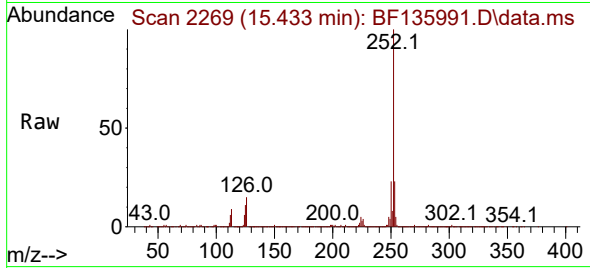

#91
Dibenzo(a,h)anthracene
Concen: 2.877 ng
RT: 17.021 min Scan# 2539
Delta R.T. 0.000 min
Lab File: BF135991.D
Acq: 27 Oct 2023 18:34


Tgt Ion:278 Resp: 48740
Ion Ratio Lower Upper
278 100
139 19.3 14.0 21.0
279 27.0 19.7 29.5

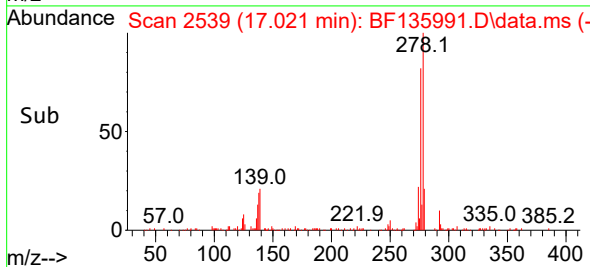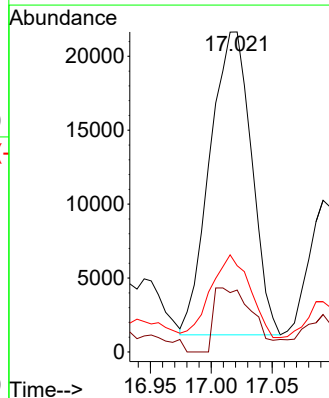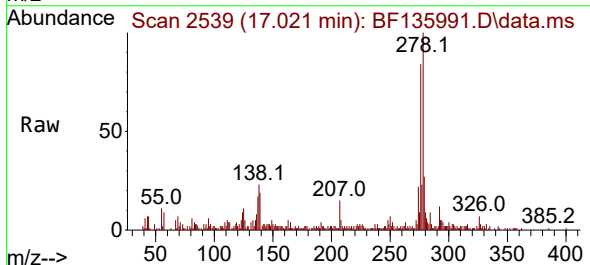



#92
 Benzo(g,h,i)perylene
 Concen: 11.619 ng
 RT: 17.457 min Scan# 20
 Delta R.T. 0.001 min
 Lab File: BF135991.D
 Acq: 27 Oct 2023 18:34

Instrument :
 BNA_F
 ClientSampleId :
 D-1(0-5)DL



Tgt Ion:276 Resp: 164299
 Ion Ratio Lower Upper
 276 100
 277 23.7 18.6 28.0
 138 24.0 18.4 27.6

