


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102723\
 Data File : BF135976.D
 Acq On : 27 Oct 2023 10:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 26 03:58:01 2023

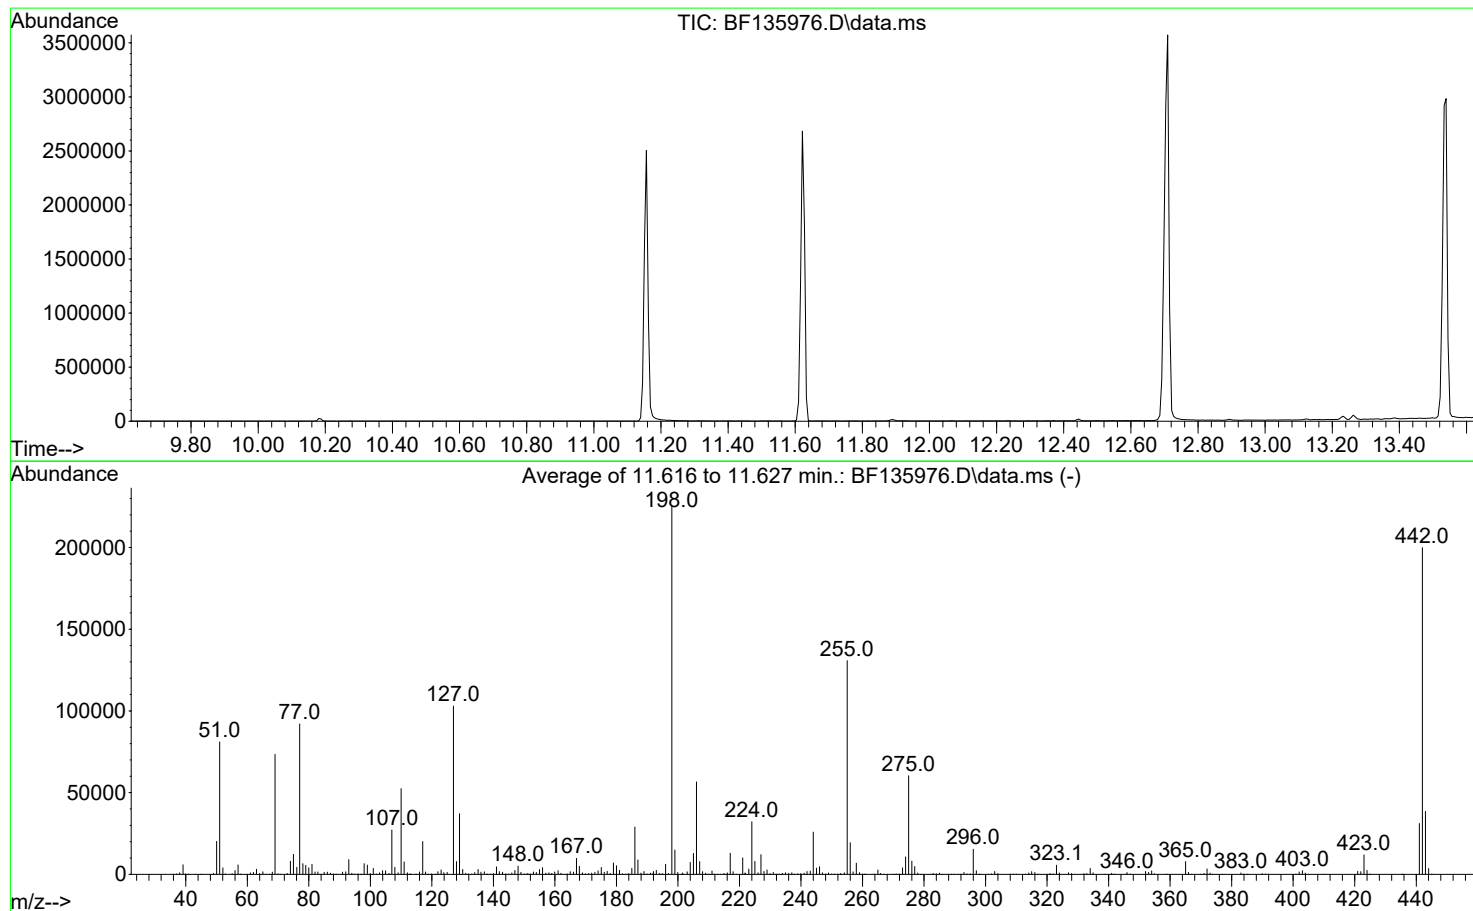

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	81029	PASS
68	69	0.00	2	1.9	1414	PASS
69	198	0.00	100	32.6	73413	PASS
70	69	0.00	2	0.6	418	PASS
127	198	10	80	45.8	103024	PASS
197	198	0.00	2	0.2	500	PASS
198	198	100	100	100.0	225088	PASS
199	198	5	9	6.6	14933	PASS
275	198	10	60	26.8	60296	PASS
365	198	1	100	3.5	7862	PASS
441	198	0.01	100	13.8	31112	PASS
442	442	50	100	100.0	199933	PASS
443	442	15	24	19.3	38571	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/27/2023	BNA_F	<u>BF135975.D</u>
Compound Name	Response	Retention Time
DDT	574333	13.539
DDD	10338	13.263
DDE	1086	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11424	585757	1.95

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102723\
 Data File : BF135976.D
 Acq On : 27 Oct 2023 10:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 27 10:40:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 26 03:58:01 2023
 Response via : Initial Calibration

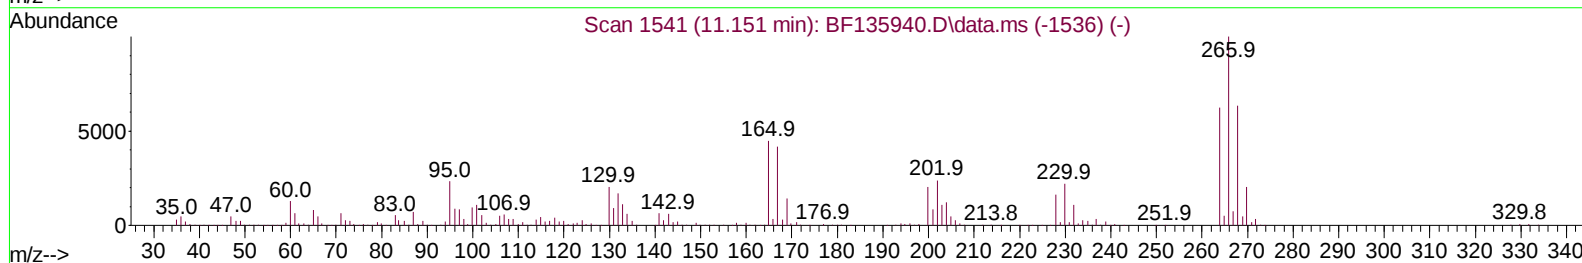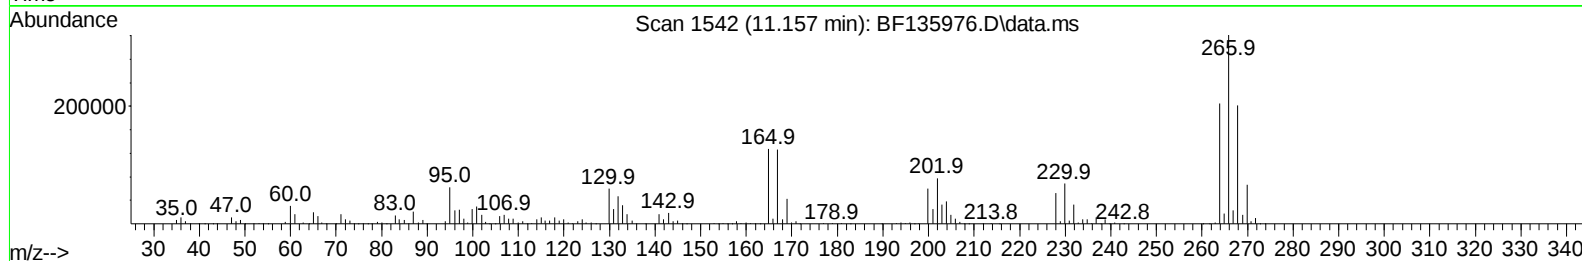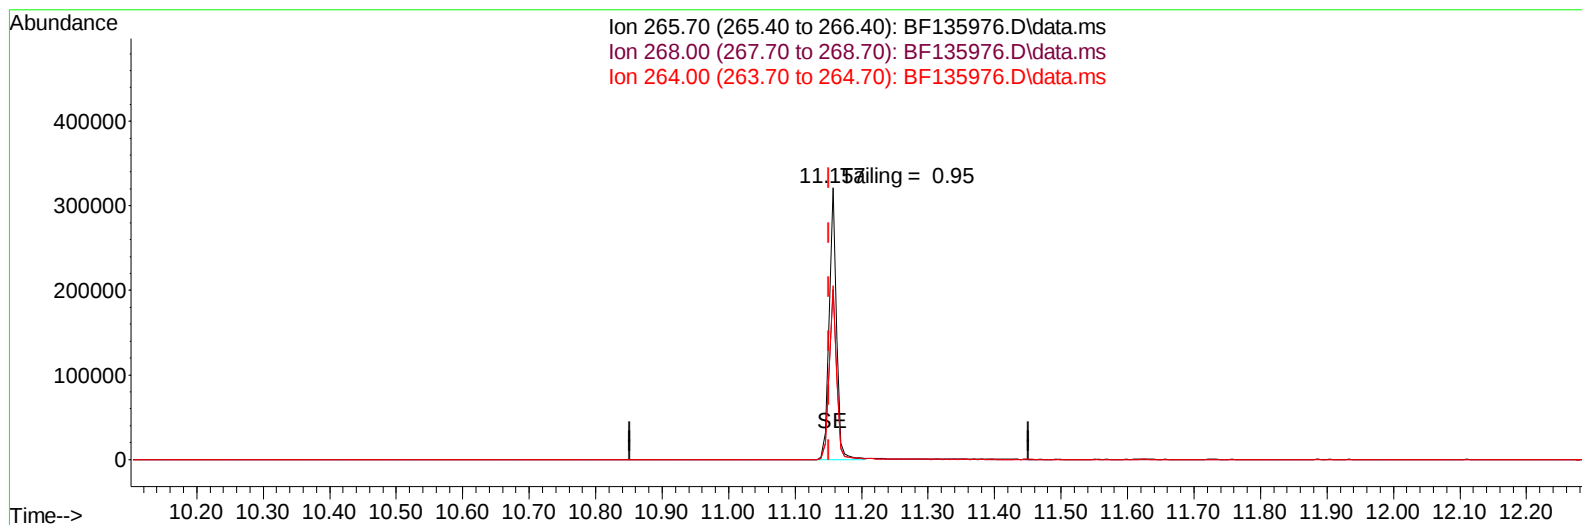

TIC: BF135976.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.006) 40037.24 ng




response 253290

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.67
264.00	62.20	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102723\
Data File : BF135976.D
Acq On : 27 Oct 2023 10:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 27 10:40:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

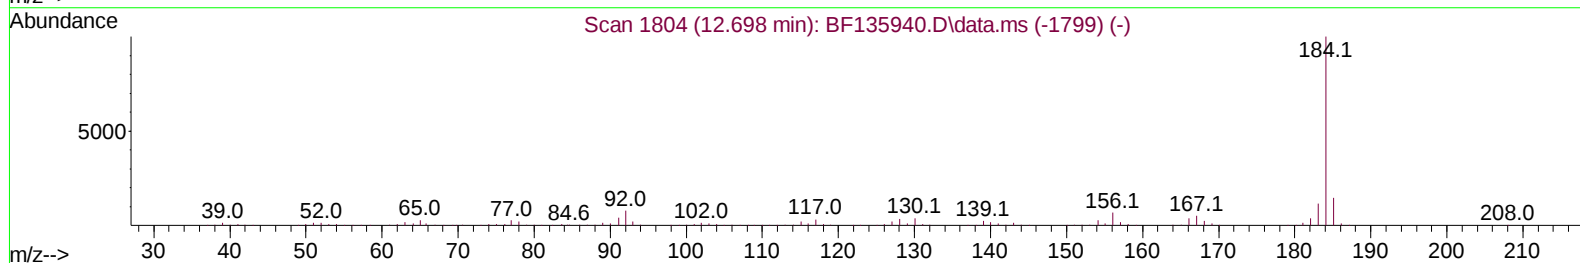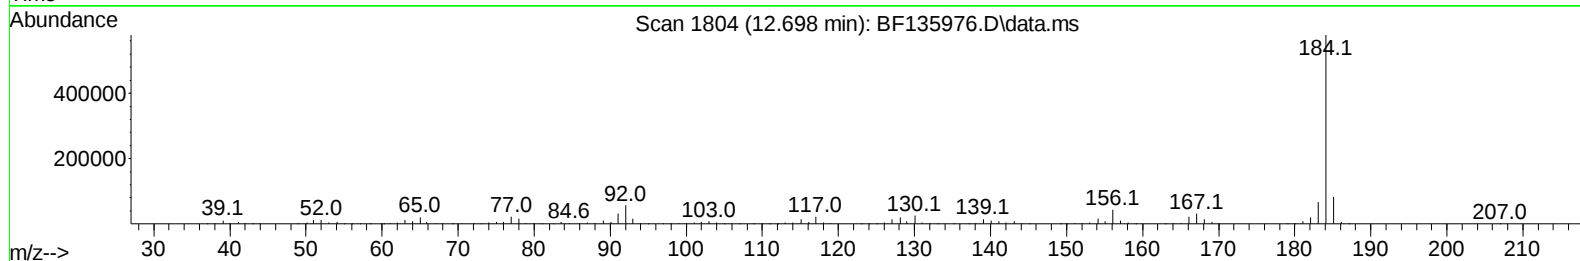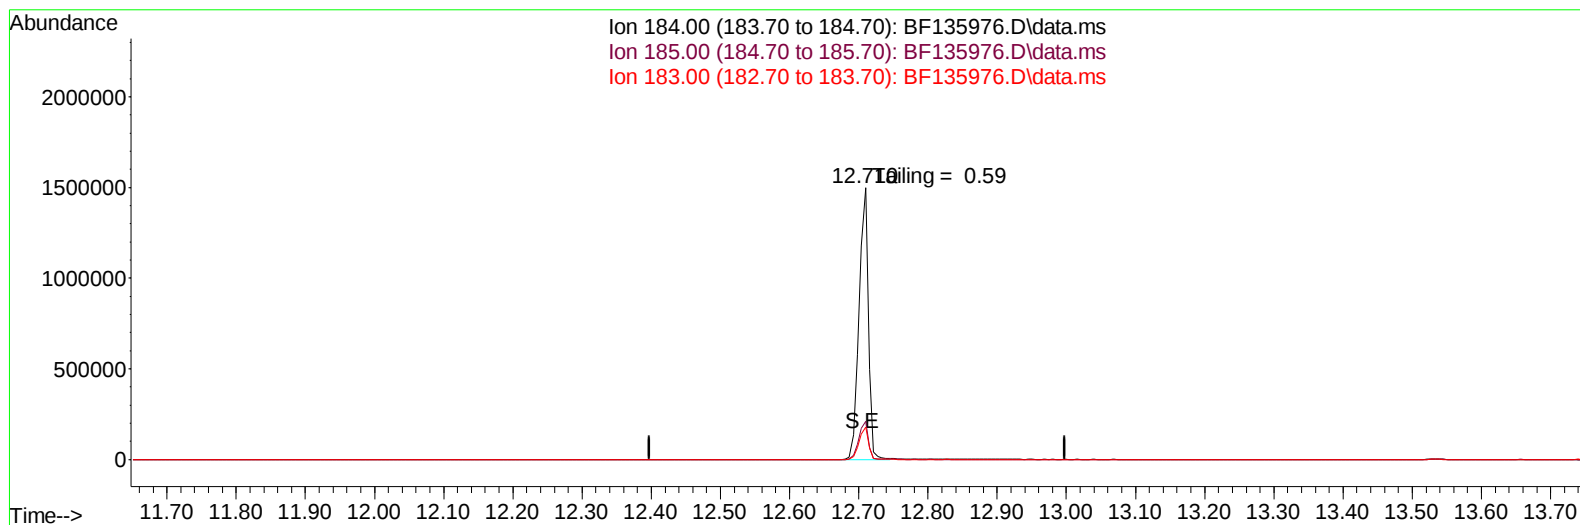

TIC: BF135976.D\data.ms

(77) Benzidine

12.698min (-12.698) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.60	0.00#
183.00	11.50	0.00#
0.00	0.00	0.00