
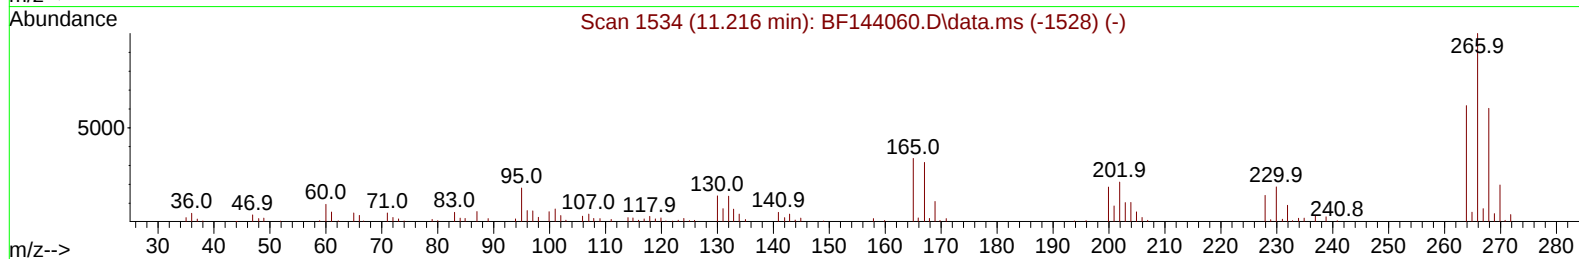
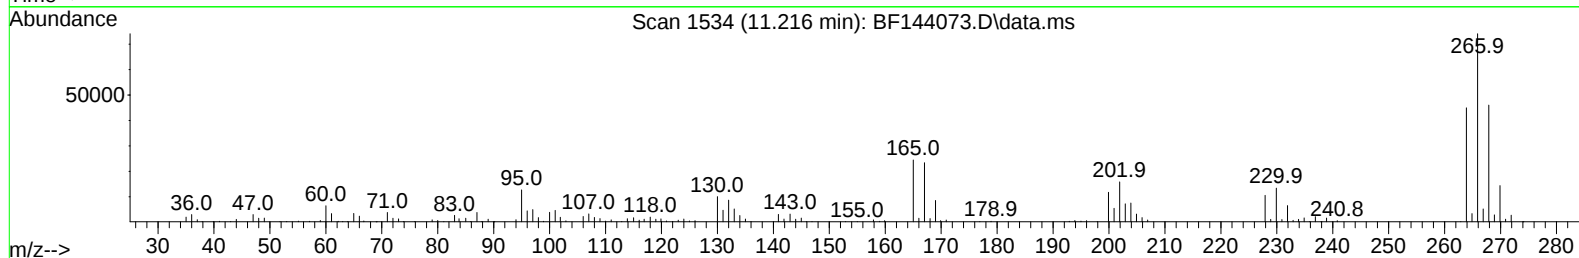


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102725\
Data File : BF144073.D
Acq On : 27 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 11:44:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

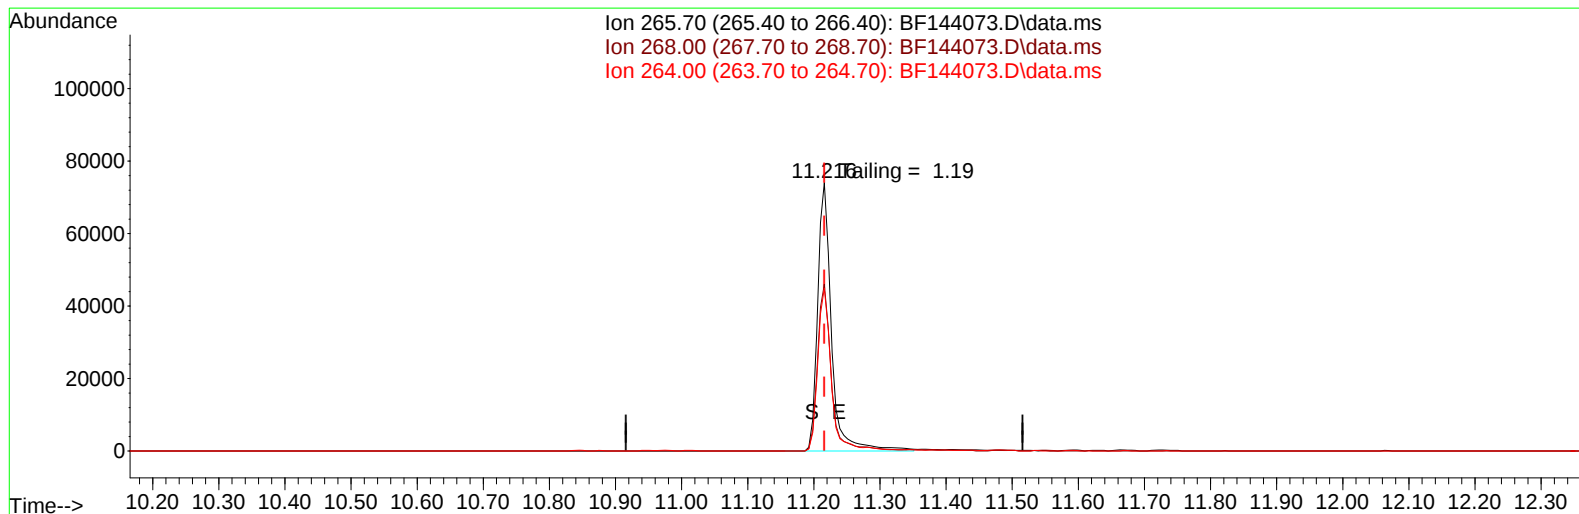

TIC: BF144073.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.000) 52871.76 ng

response 108593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	62.12
264.00	61.70	60.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102725\
Data File : BF144073.D
Acq On : 27 Oct 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 11:44:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

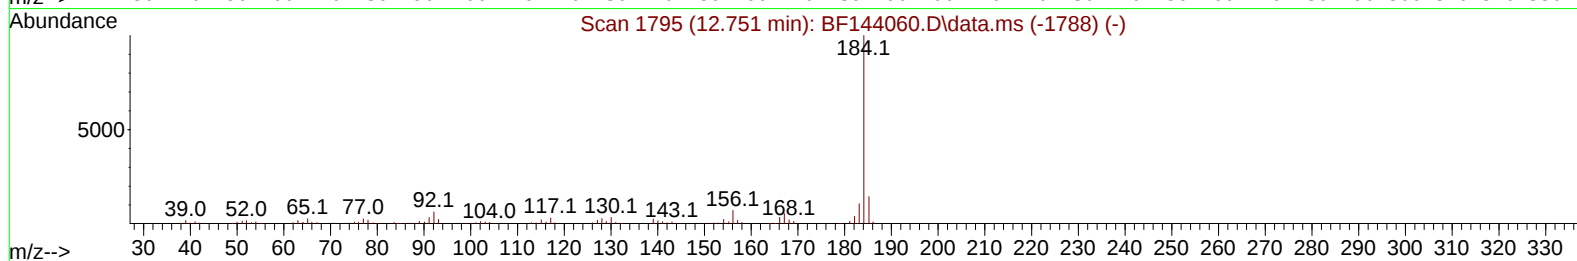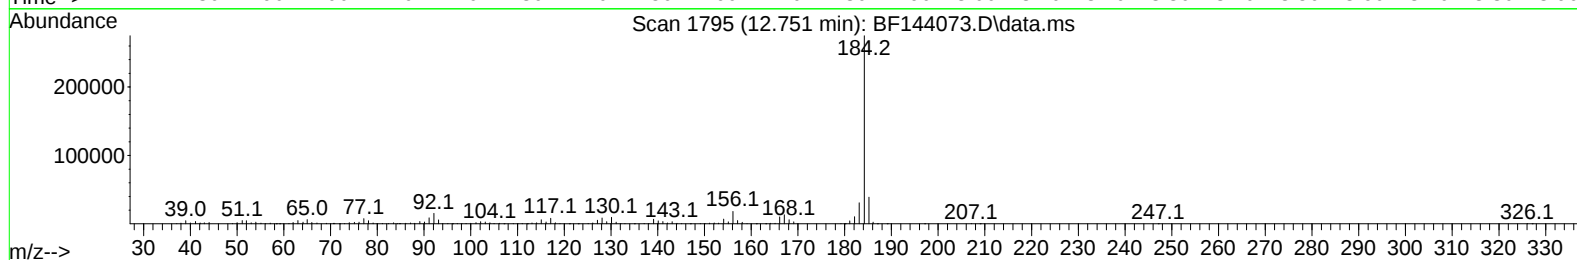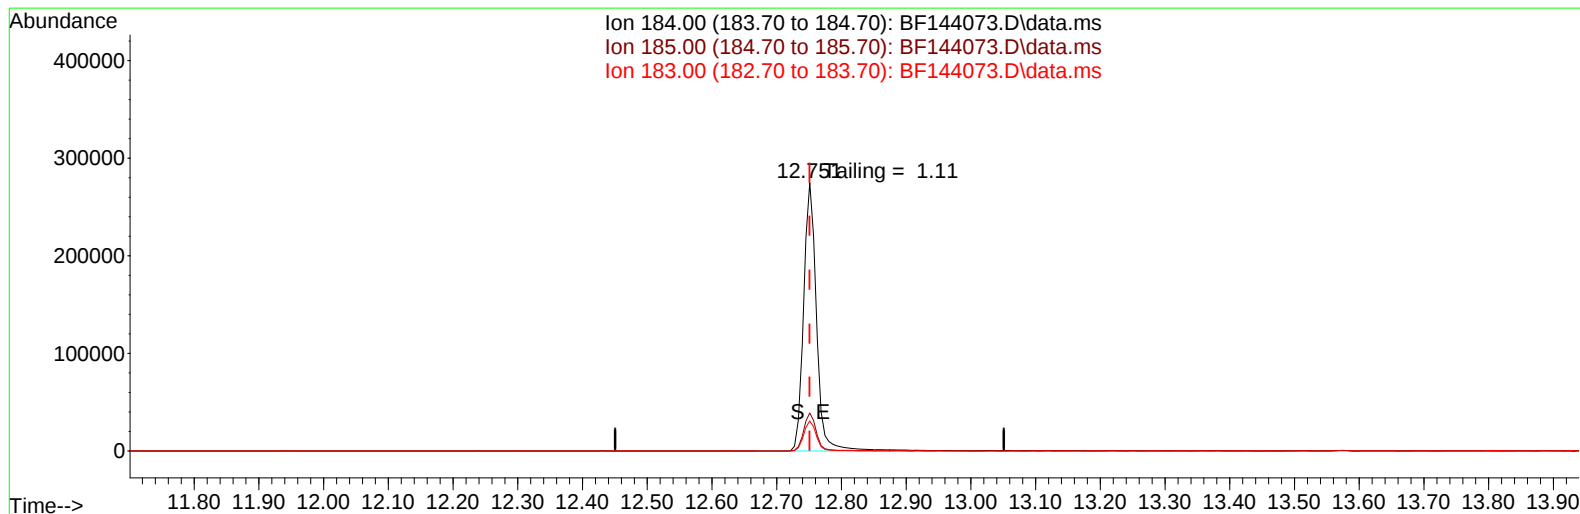

TIC: BF144073.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 21247.29 ng m

response 380221

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.21
183.00	10.60	11.20
0.00	0.00	0.00